

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
 Data File : PL050480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2019 19:10
 Operator : SM\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:29:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 18 03:18:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.931	283.8E6	69730449	24.623	24.453
28)	SA Decachlor...	7.980	8.963	264.3E6	72774700	25.415	25.999
Target Compounds							
23)	Chlordane-1	4.158	4.916	90425118	26806032	245.705	242.954
24)	Chlordane-2	4.648	5.383	111.2E6	29158395	252.869	250.080
25)	Chlordane-3	5.202	6.027	348.9E6	116.4E6	249.692	240.817
26)	Chlordane-4	5.257	6.100	336.0E6	141.8E6	254.308	243.477
27)	Chlordane-5	6.079	6.902	122.2E6	23699746	237.910	248.090



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
Data File : PL050480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2019 19:10
Operator : SM\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:29:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Thu Jul 18 03:18:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

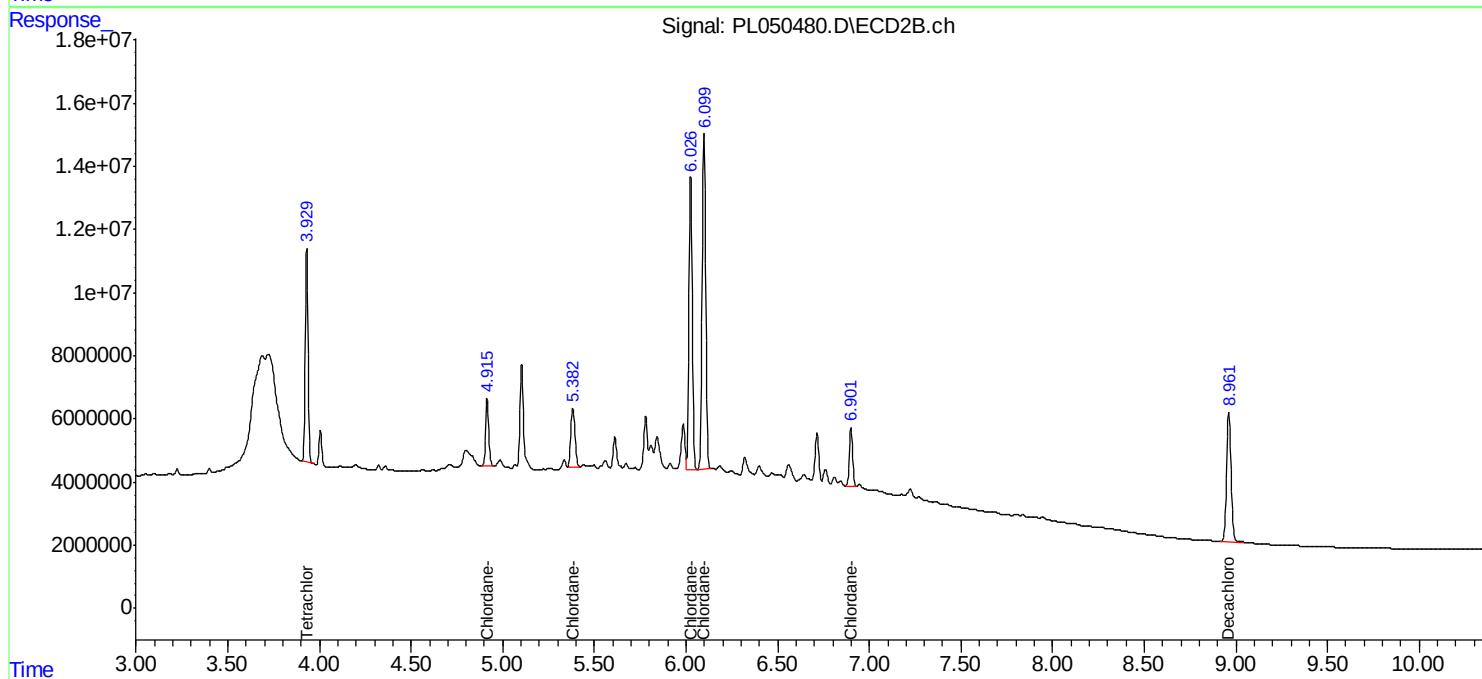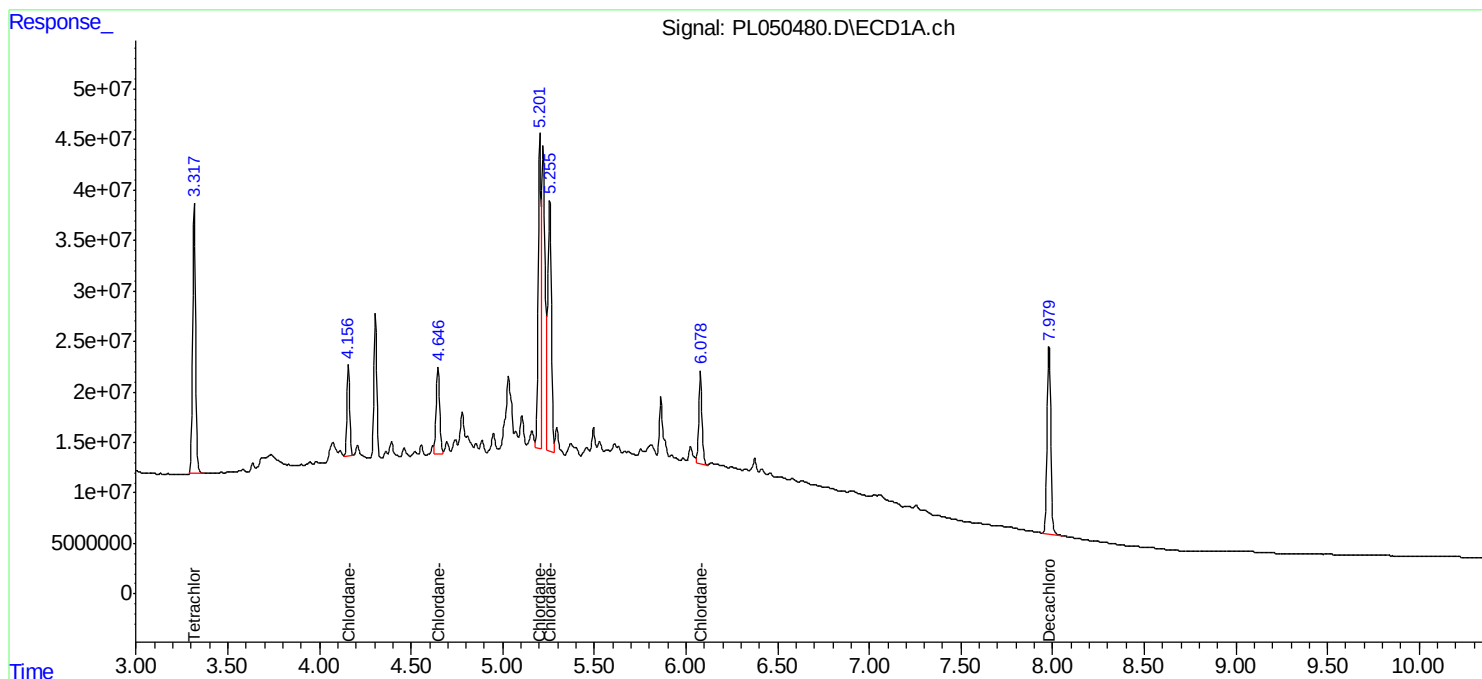


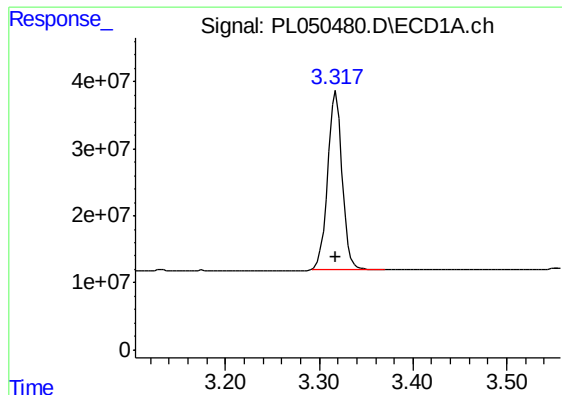

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 283808656
Conc: 24.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

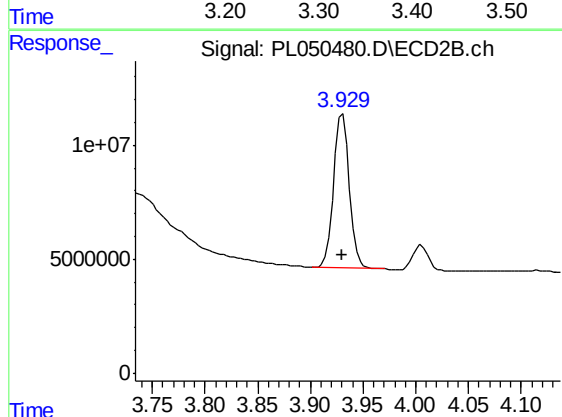


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 69730449
Conc: 24.45 ng/ml

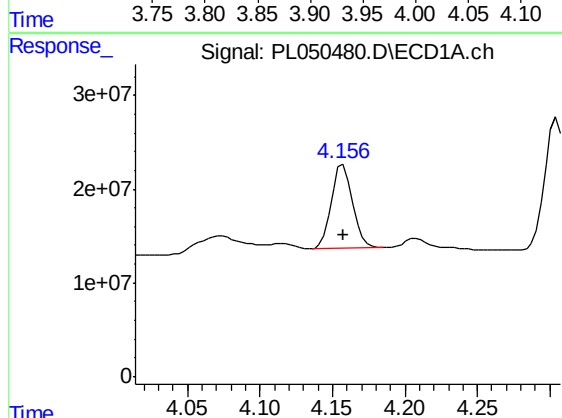


#23 Chlordane-1

R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 90425118
Conc: 245.70 ng/ml

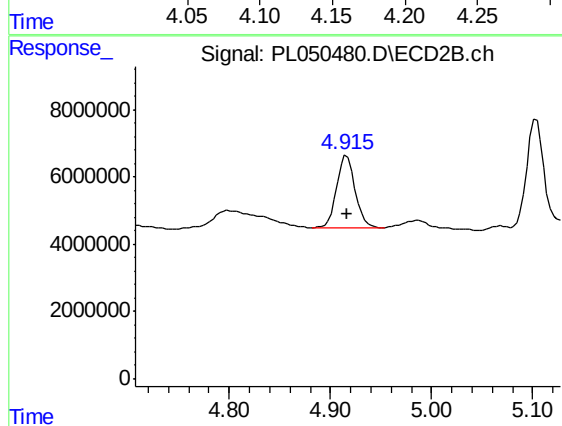

#23 Chlordane-1


R.T.: 4.916 min
Delta R.T.: 0.000 min
Response: 26806032
Conc: 242.95 ng/ml

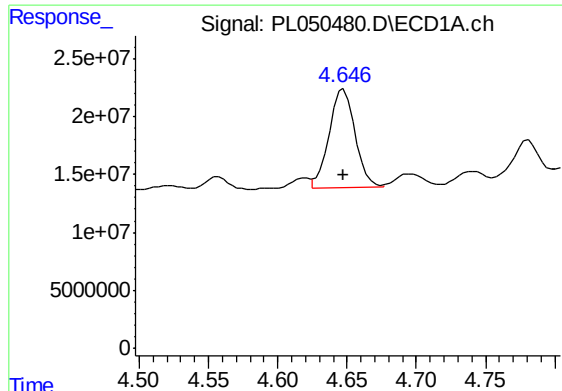

#24 Chlordane-2


R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 111180734
Conc: 252.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

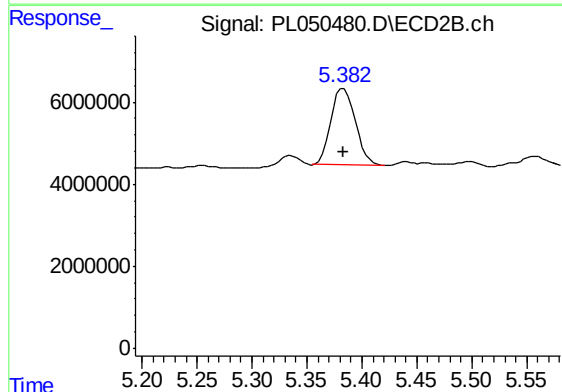


#24 Chlordane-2

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 29158395
Conc: 250.08 ng/ml

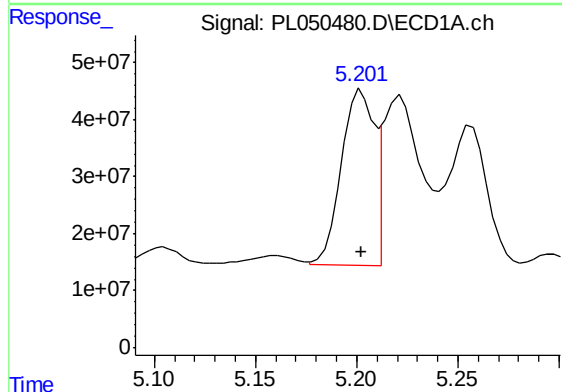


#25 Chlordane-3

R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 348862044
Conc: 249.69 ng/ml

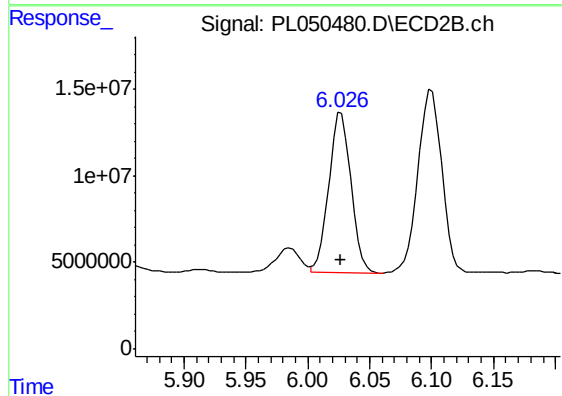

#25 Chlordane-3


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 116418486
Conc: 240.82 ng/ml

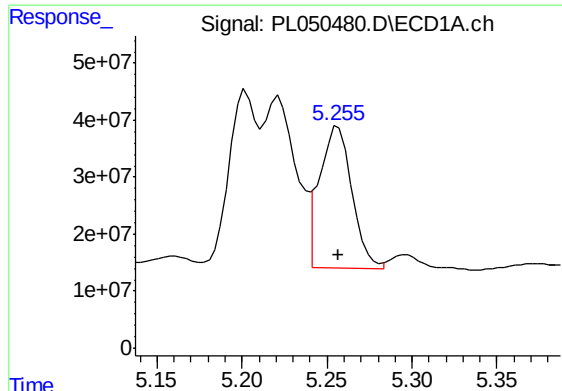

#26 Chlordane-4


R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 336001652
Conc: 254.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

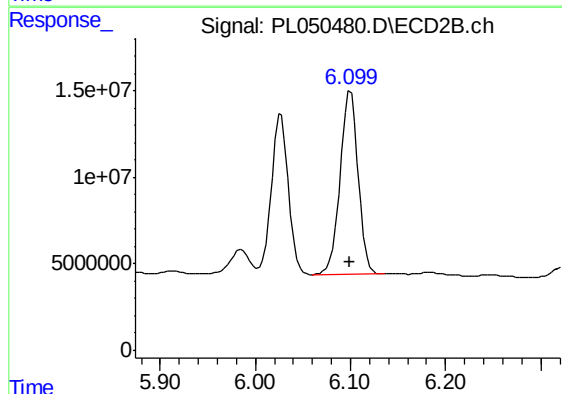


#26 Chlordane-4

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 141806657
Conc: 243.48 ng/ml

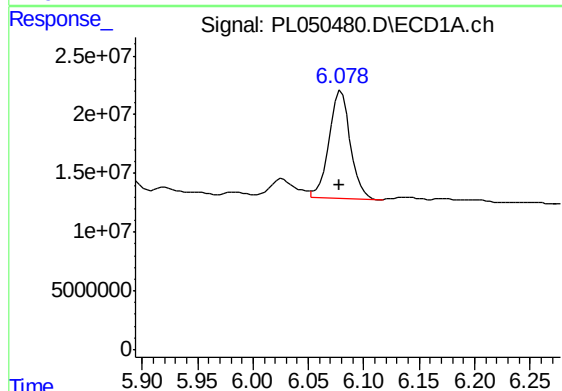


#27 Chlordane-5

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 122177064
Conc: 237.91 ng/ml

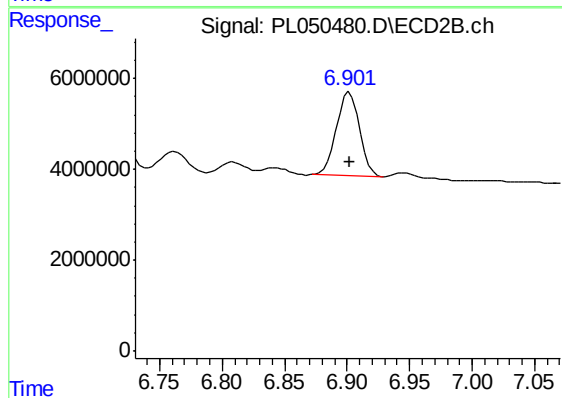

#27 Chlordane-5


R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 23699746
Conc: 248.09 ng/ml

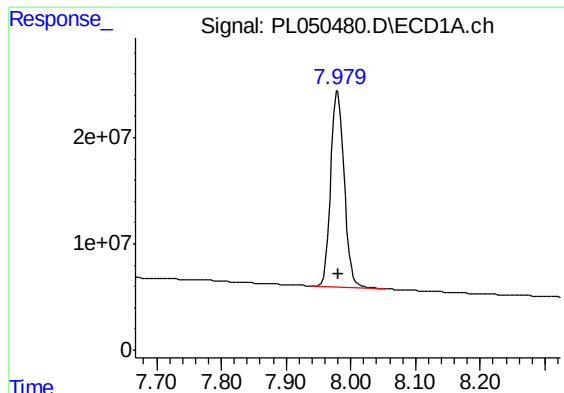

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 264277177
Conc: 25.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

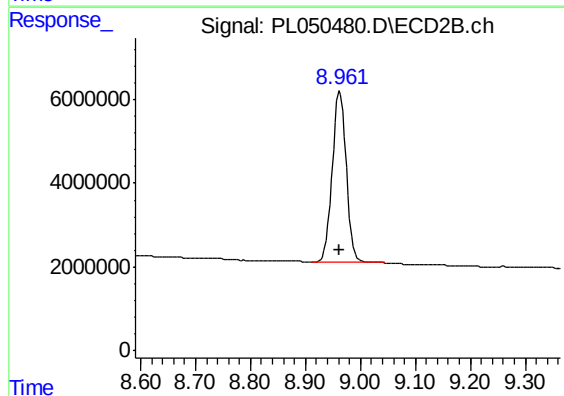

#28 Decachlorobiphenyl

R.T.: 8.963 min
Delta R.T.: 0.000 min
Response: 72774700
Conc: 26.00 ng/ml