

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
 Data File : PL050488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2019 21:04
 Operator : SM\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL071719CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 09:09:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 18 09:08:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.931	583.1E6	142.3E6	50.239	49.694
28)	SA Decachlor...	7.980	8.962	537.1E6	140.0E6	50.923	48.924
Target Compounds							
23)	Chlordane-1	4.157	4.916	187.2E6	55217015	508.732	508.962
24)	Chlordane-2	4.647	5.383	221.9E6	57873522	495.814	492.740
25)	Chlordane-3	5.202	6.027	704.9E6	240.1E6	503.551	499.088
26)	Chlordane-4	5.256	6.099	669.6E6	289.1E6	507.686	497.705
27)	Chlordane-5	6.079	6.902	249.1E6	47506599	490.324	498.146



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
Data File : PL050488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2019 21:04
Operator : SM\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL071719CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 09:09:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Thu Jul 18 09:08:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

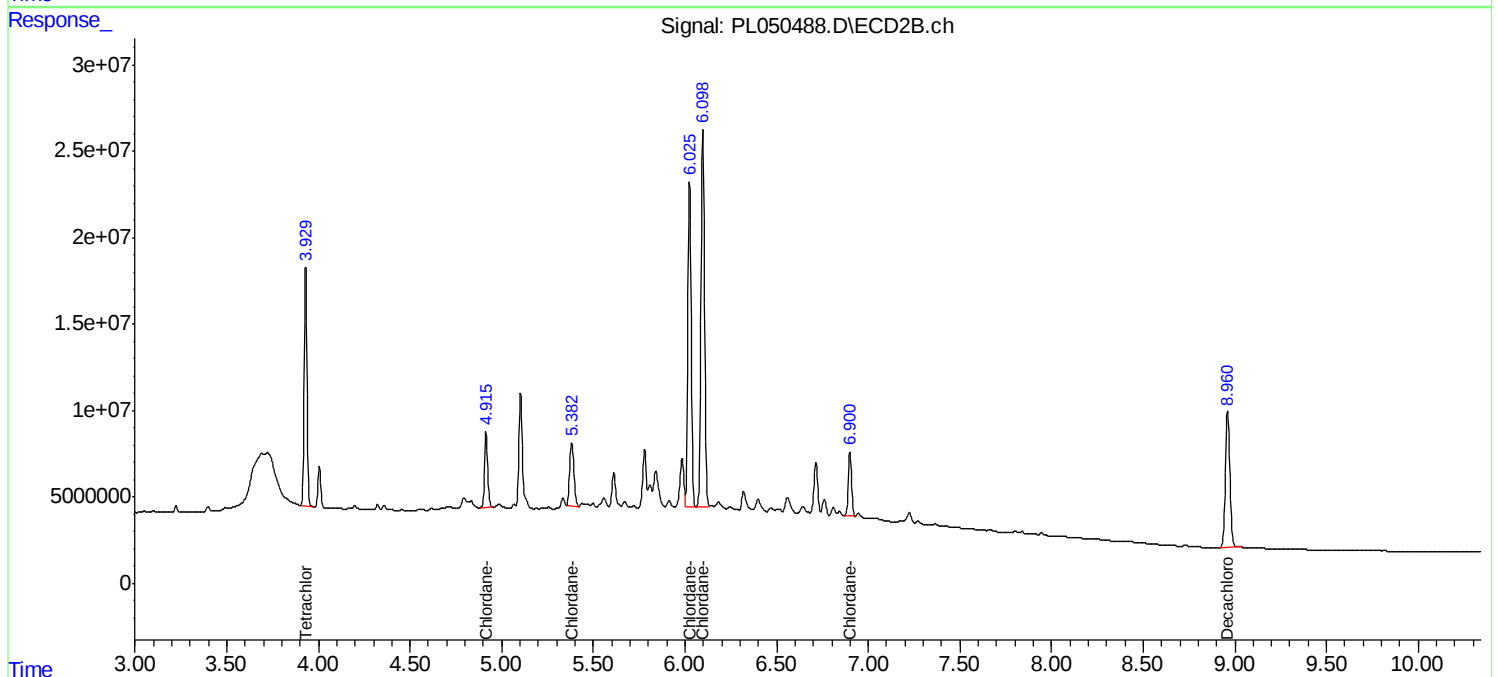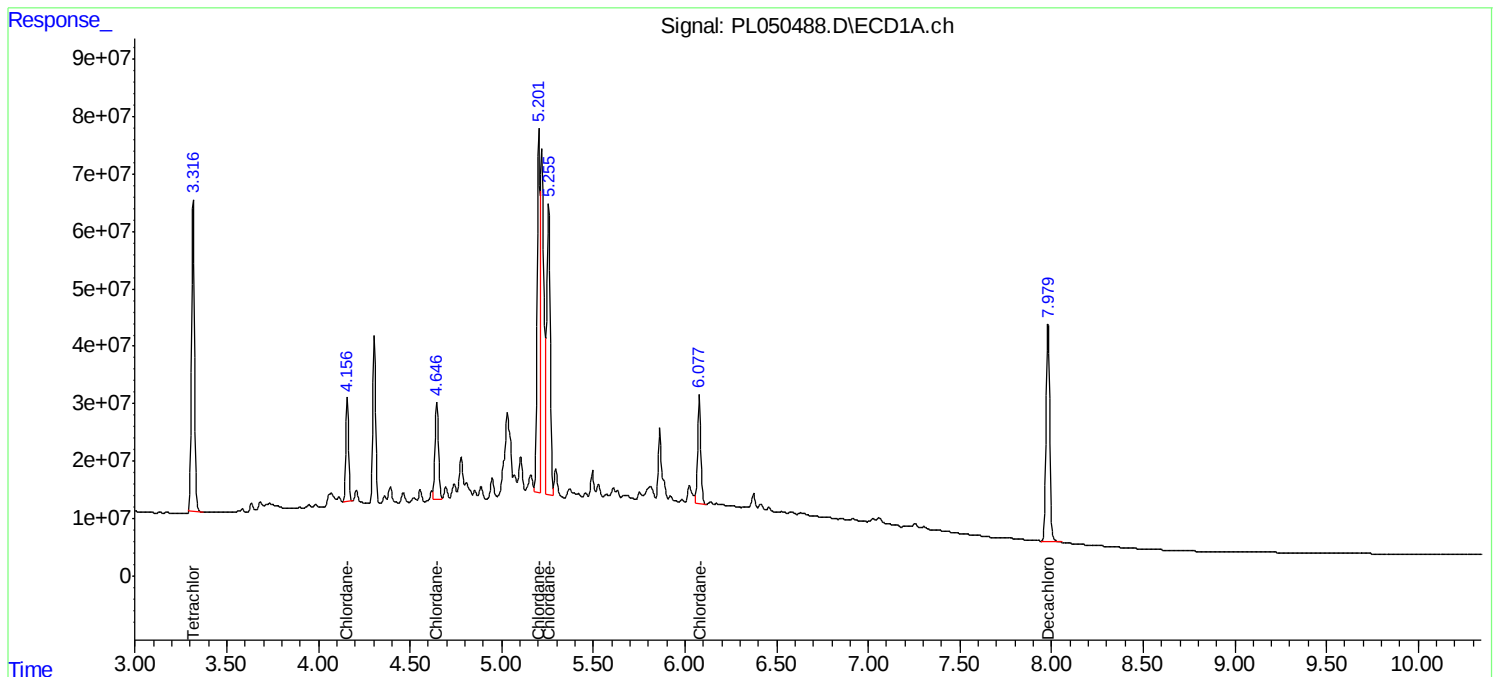


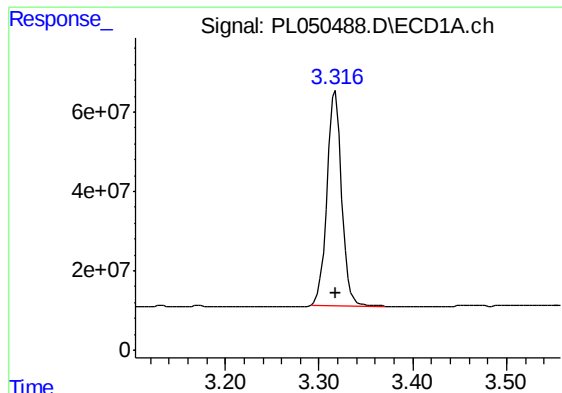

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 583082663
Conc: 50.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL071719CHLOR

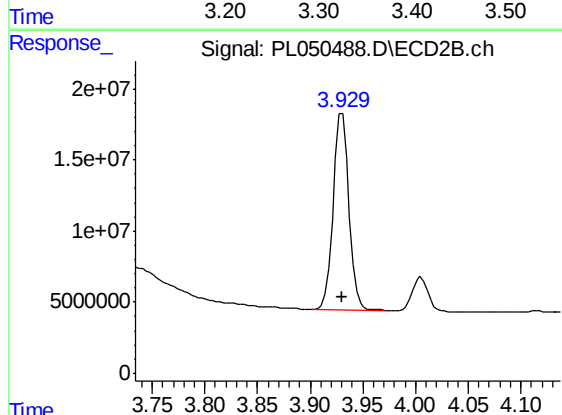


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 142279894
Conc: 49.69 ng/ml

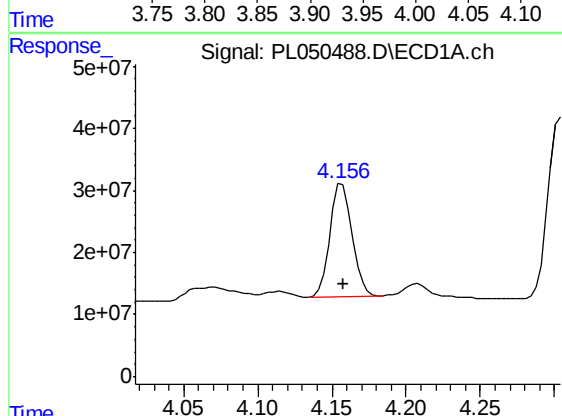


#23 Chlordane-1

R.T.: 4.157 min
Delta R.T.: 0.000 min
Response: 187189112
Conc: 508.73 ng/ml

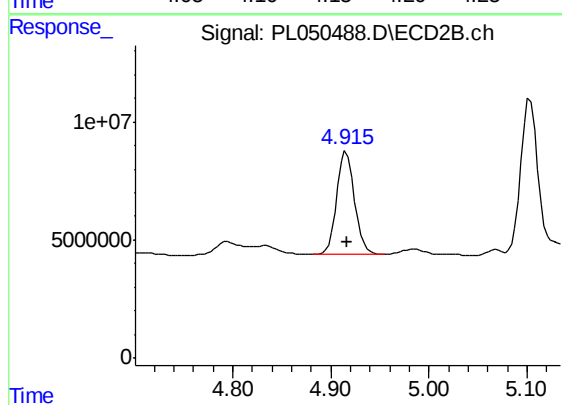

#23 Chlordane-1


R.T.: 4.916 min
Delta R.T.: 0.000 min
Response: 55217015
Conc: 508.96 ng/ml

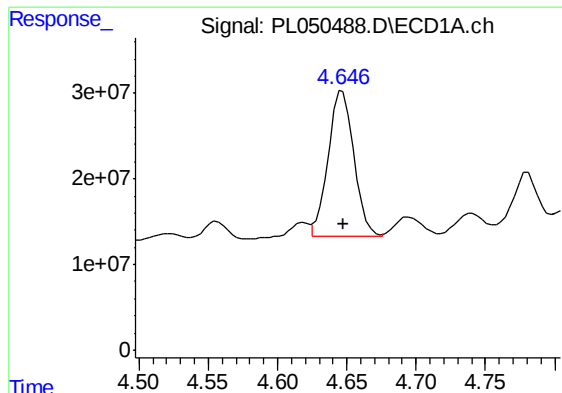

#24 Chlordane-2


R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 221929139
Conc: 495.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL071719CHLOR

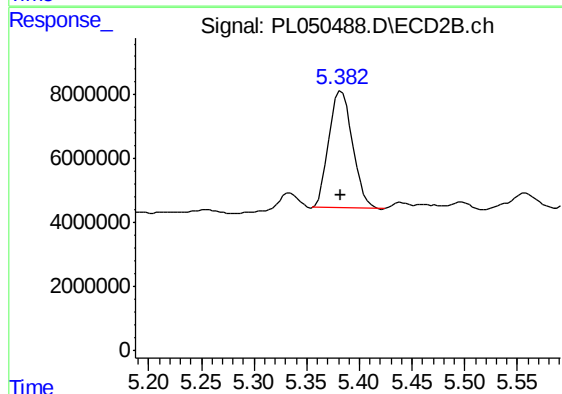


#24 Chlordane-2

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 57873522
Conc: 492.74 ng/ml

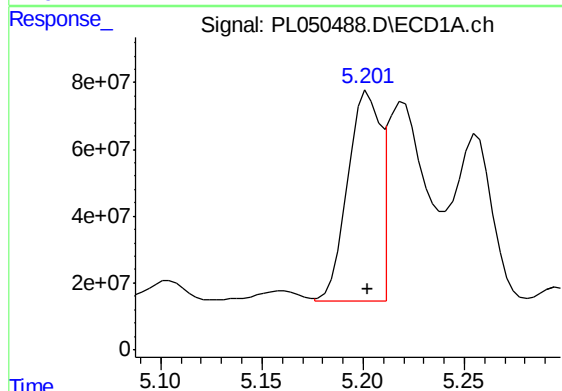


#25 Chlordane-3

R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 704864525
Conc: 503.55 ng/ml

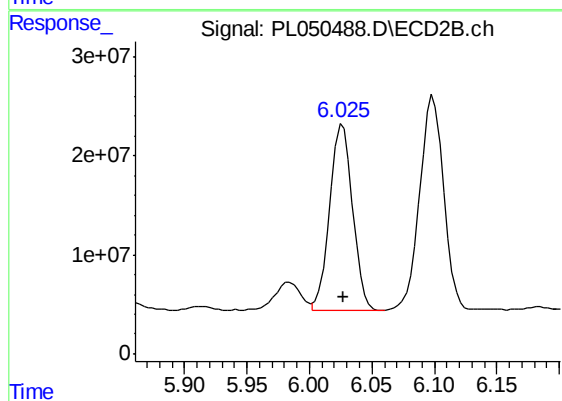

#25 Chlordane-3


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 240051473
Conc: 499.09 ng/ml

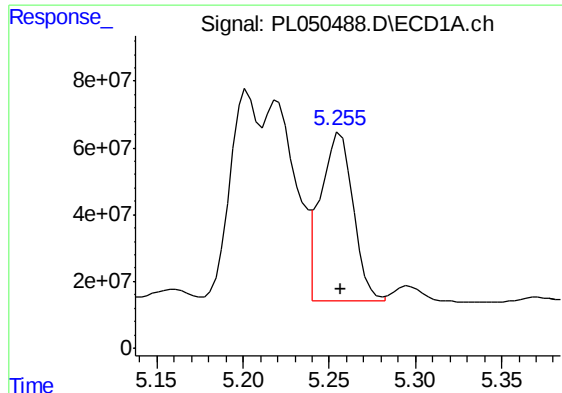

#26 Chlordane-4


R.T.: 5.256 min
Delta R.T.: 0.000 min
Response: 669627735
Conc: 507.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL071719CHLOR

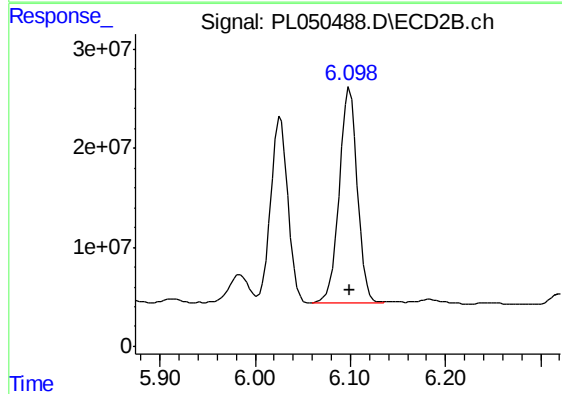


#26 Chlordane-4

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 289125929
Conc: 497.70 ng/ml

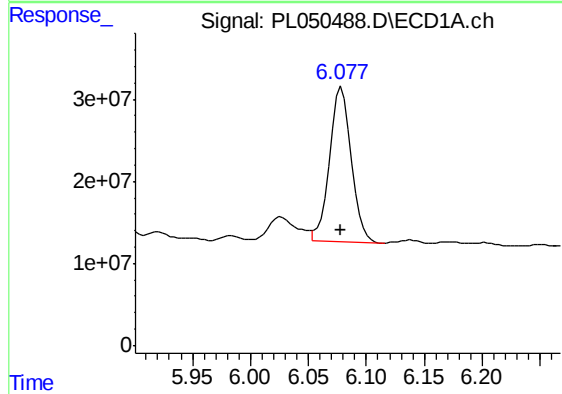


#27 Chlordane-5

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 249053640
Conc: 490.32 ng/ml

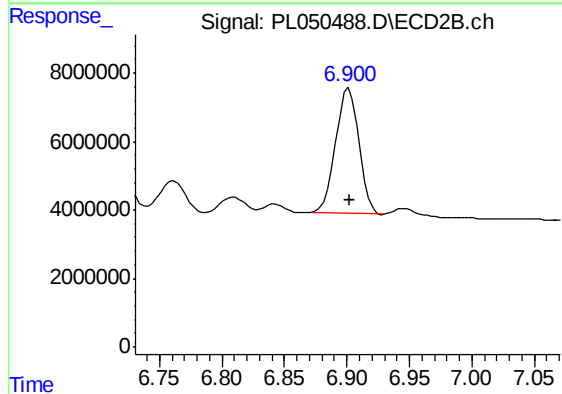

#27 Chlordane-5


R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 47506599
Conc: 498.15 ng/ml

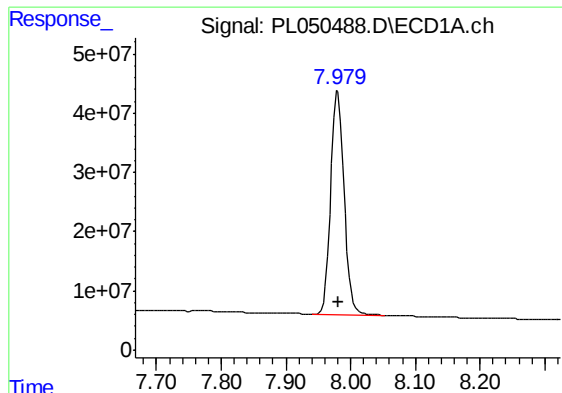

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 537104800
Conc: 50.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL071719CHLOR

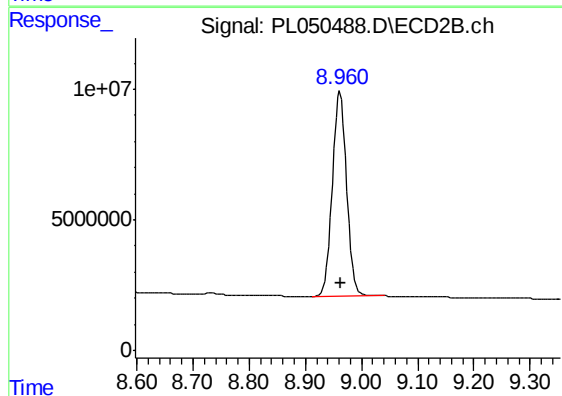

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: 0.000 min
Response: 139977839
Conc: 48.92 ng/ml