

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
 Data File : PL050513.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 03:01
 Operator : SM\AJ
 Sample : K3591-08
 Misc : CHLOR LOQ 50 PPB
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LOQ-WATER-02-QT3-2019

Manual Integrations
 APPROVED

Ankita
 7/18/2019 2:56:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 06:41:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 18 04:12:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.930	248.2E6	68384279	24.700	23.968
28)	SA Decachlor...	7.980	8.960	291.2E6	76769920	28.757	27.147
Target Compounds							
23)	Chlordane-1	4.157	4.915	27005014	7465862	73.393	68.816
24)	Chlordane-2	4.646	5.383	32232701	8781951	72.011m	74.770
25)	Chlordane-3	5.200	6.026	102.9E6	28326654	73.482m	58.894
26)	Chlordane-4	5.257	6.099	92749493	35403670	70.319	60.944
27)	Chlordane-5	6.078	6.901	32780443	5955633	64.536	62.450

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
Data File : PL050513.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 03:01
Operator : SM\AJ
Sample : K3591-08
Misc : CHLOR LOQ 50 PPB
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT3-2019


Manual Integrations
APPROVED

Ankita
7/18/2019 2:56:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 06:41:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Thu Jul 18 04:12:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

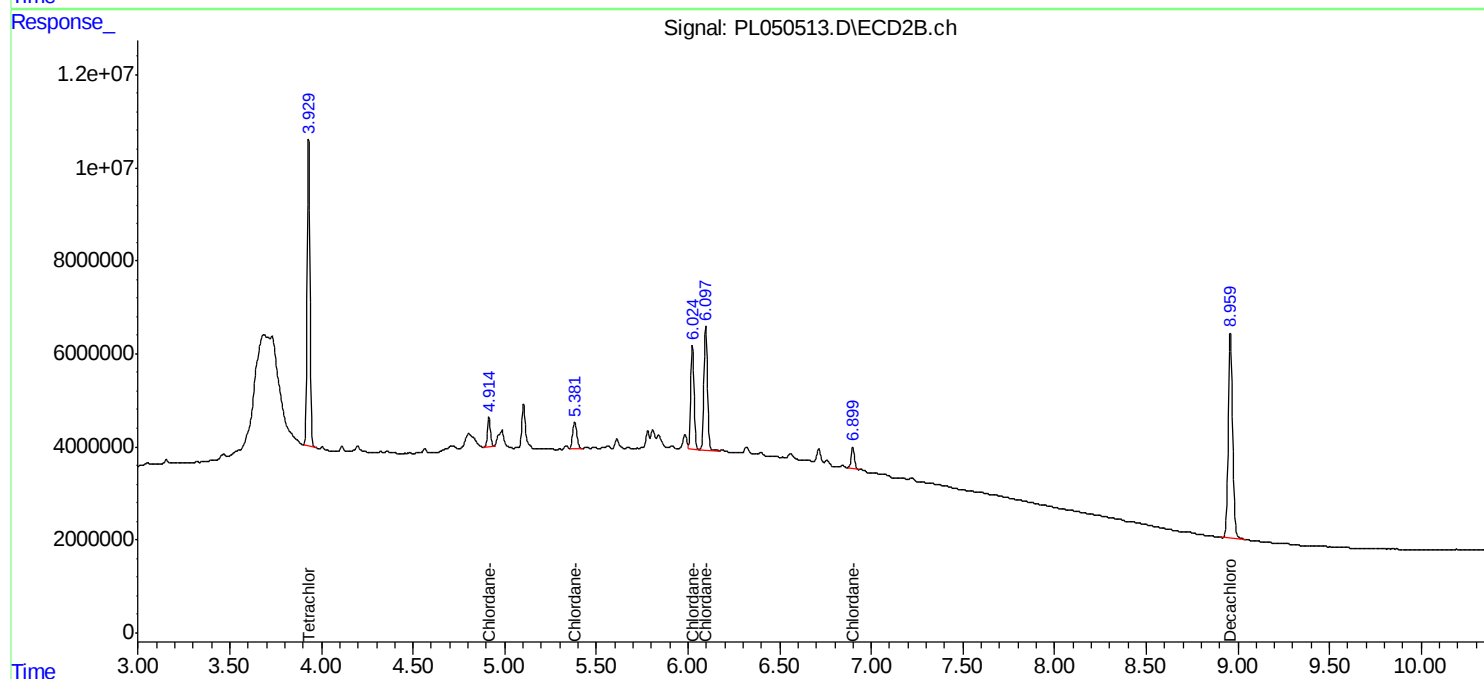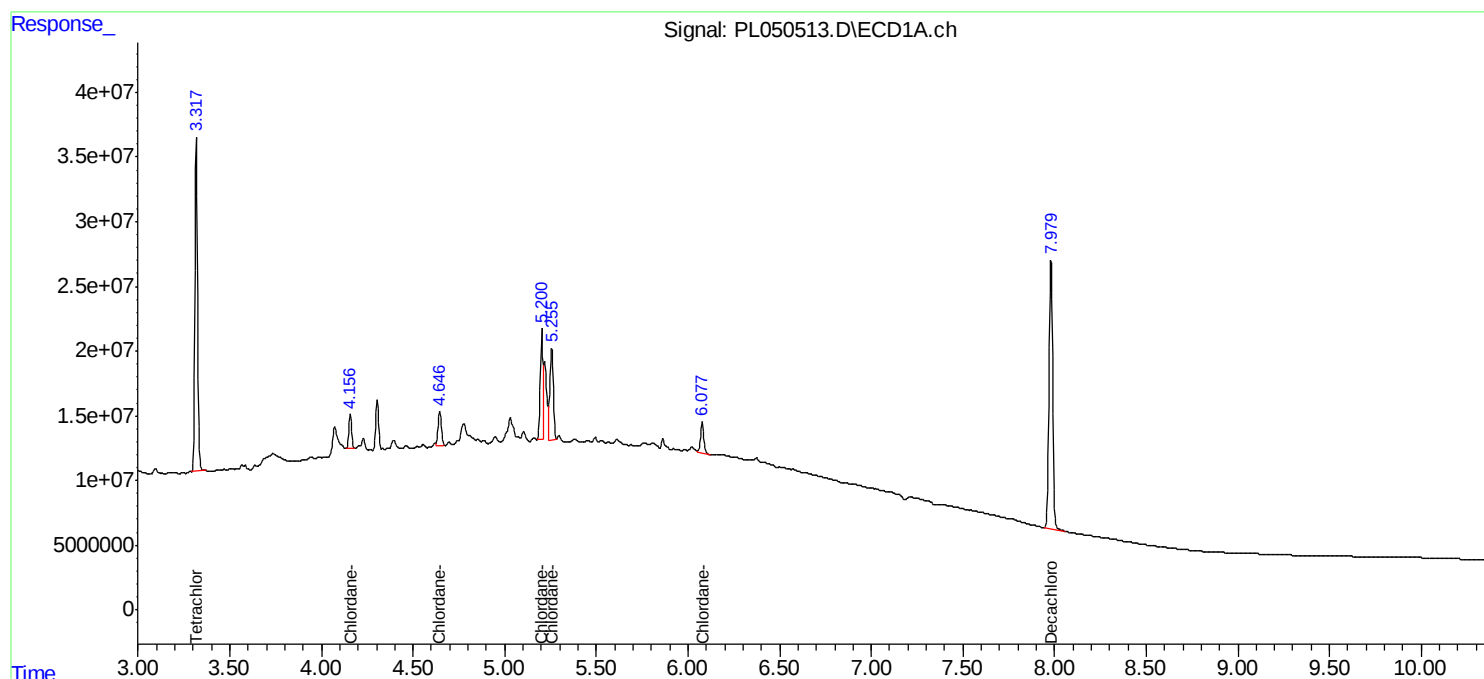

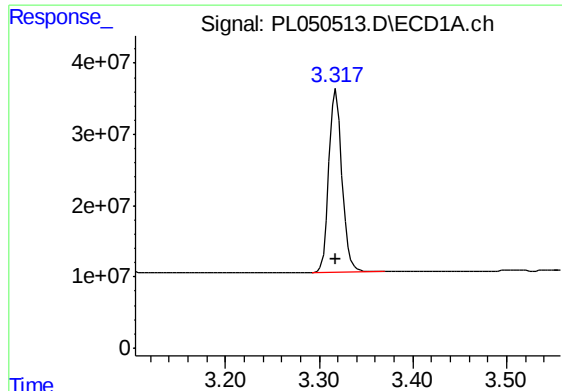


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 248176852
Conc: 24.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT3-2019


Manual Integrations
APPROVED

Ankita
7/18/2019 2:56:40 PM

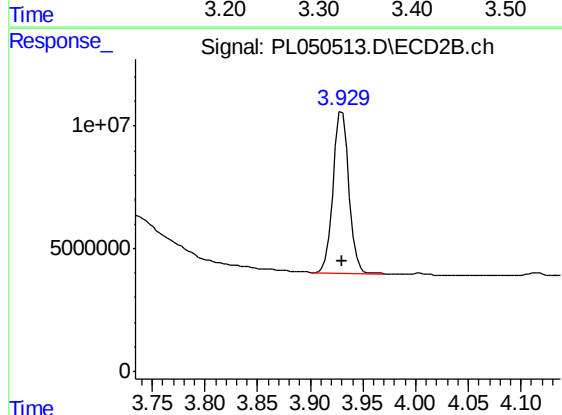


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 68384279
Conc: 23.97 ng/ml

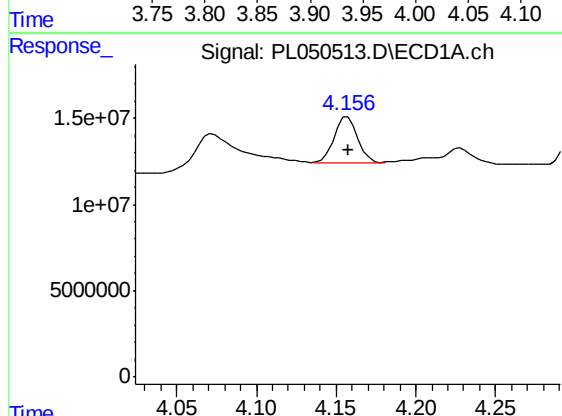


#23 Chlordane-1

R.T.: 4.157 min
Delta R.T.: 0.000 min
Response: 27005014
Conc: 73.39 ng/ml

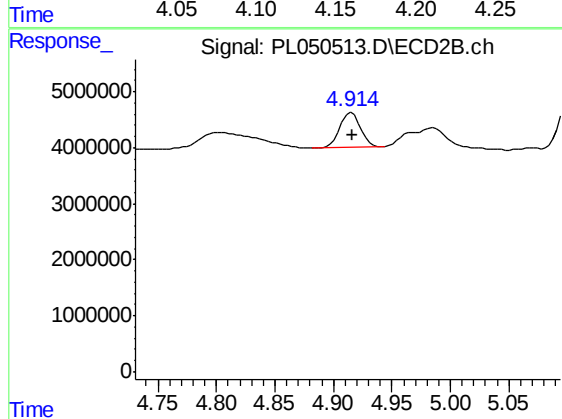

#23 Chlordane-1

R.T.: 4.915 min
Delta R.T.: 0.000 min
Response: 7465862
Conc: 68.82 ng/ml

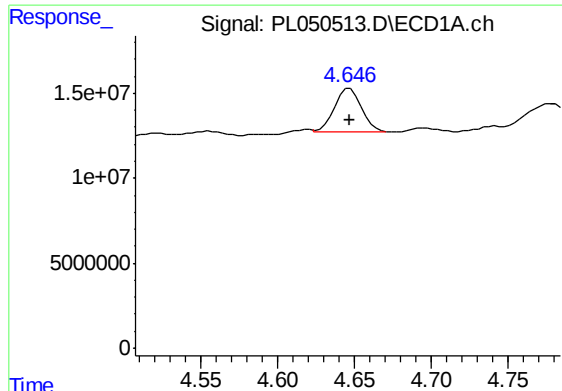


#24 Chlordane-2

R.T.: 4.646 min
Delta R.T.: -0.002 min
Response: 32232701
Conc: 72.01 ng/ml m

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT3-2019


Manual Integrations
APPROVED

Ankita
7/18/2019 2:56:40 PM

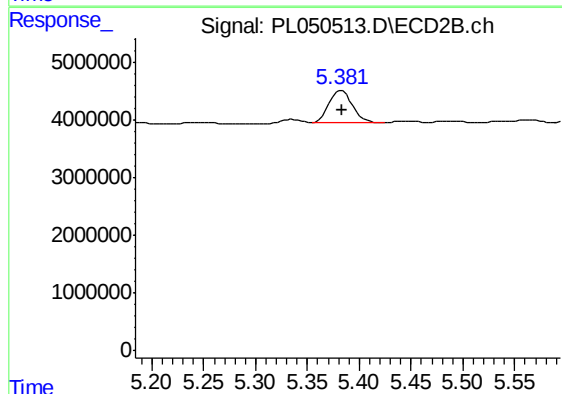


#24 Chlordane-2

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 8781951
Conc: 74.77 ng/ml

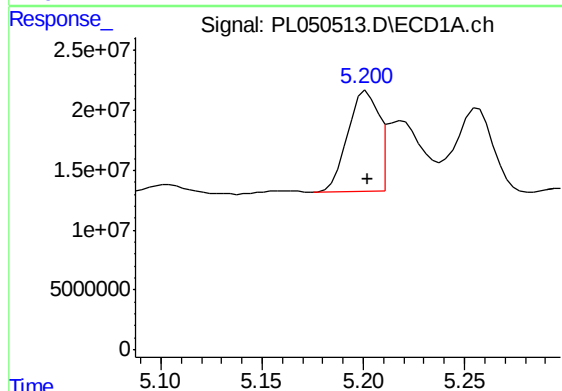


#25 Chlordane-3

R.T.: 5.200 min
Delta R.T.: -0.002 min
Response: 102859202
Conc: 73.48 ng/ml m

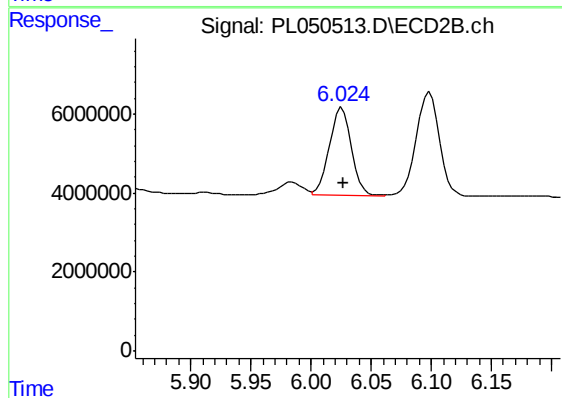

#25 Chlordane-3

R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 28326654
Conc: 58.89 ng/ml

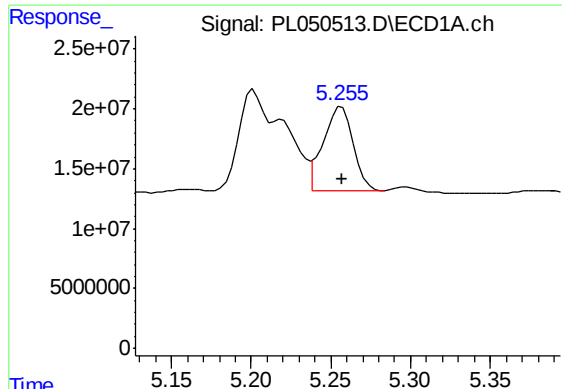


#26 Chlordane-4

R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 92749493
Conc: 70.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT3-2019


Manual Integrations
APPROVED

Ankita
7/18/2019 2:56:40 PM

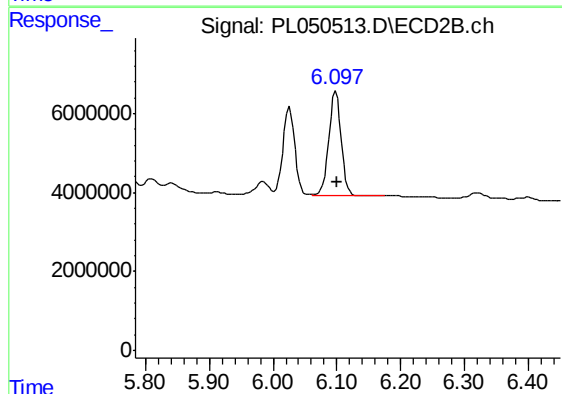


#26 Chlordane-4

R.T.: 6.099 min
Delta R.T.: -0.002 min
Response: 35403670
Conc: 60.94 ng/ml

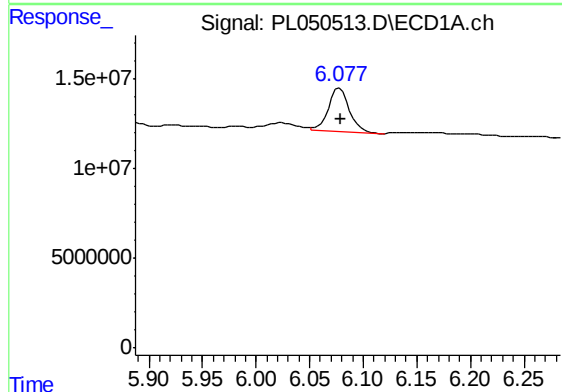


#27 Chlordane-5

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 32780443
Conc: 64.54 ng/ml

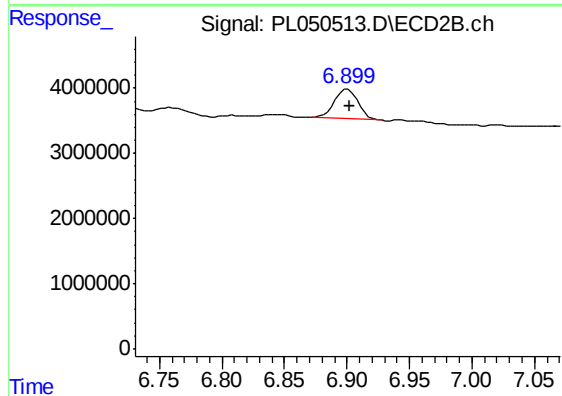

#27 Chlordane-5

R.T.: 6.901 min
Delta R.T.: -0.002 min
Response: 5955633
Conc: 62.45 ng/ml

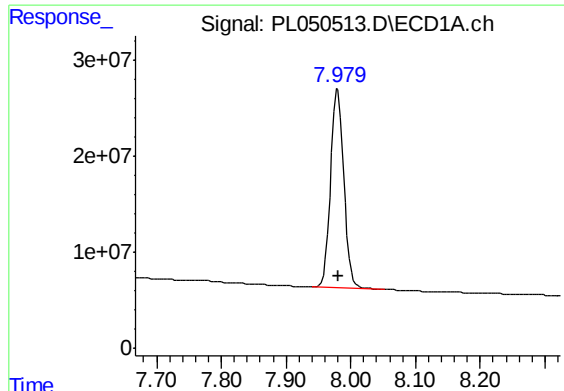


#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 291177374
Conc: 28.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT3-2019

Manual Integrations
APPROVED

Ankita
7/18/2019 2:56:40 PM

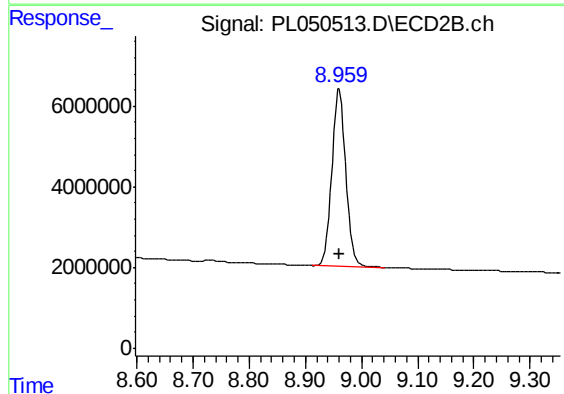

#28 Decachlorobiphenyl

R.T.: 8.960 min
Delta R.T.: -0.001 min
Response: 76769920
Conc: 27.15 ng/ml