

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071720\
 Data File : PL060001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2020 08:43
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 16:32:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.010	48446278	63482046	25.047	23.954
28)	SA Decachlor...	8.228	9.101	34379621	43657849	20.898	20.875
Target Compounds							
8)	B Heptachlo...	0.000	5.884	0	36926621	N.D.	13.711 #
9)	A Endosulfan I	0.000	6.249	0	11331044	N.D.	4.248 #
11)	B alpha-Chl...	0.000	6.176f	0	19176222	N.D.	6.707 #
12)	B 4,4'-DDE	0.000	6.339f	0	5720639	N.D.	2.137 #
14)	MA Endrin	6.023	0.000	1355811	0	0.931	N.D. #
15)	B Endosulfa...	0.000	6.948	0	11797241	N.D.	4.697 #
16)	A 4,4'-DDD	0.000	6.872f	0	7997355	N.D.	3.484 #
18)	B Endrin al...	0.000	7.063	0	9243005	N.D.	4.256 #
26)	Chlordane-4	0.000	6.176f	0	19176222	N.D.	41.426 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071720\
Data File : PL060001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2020 08:43
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 16:32:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

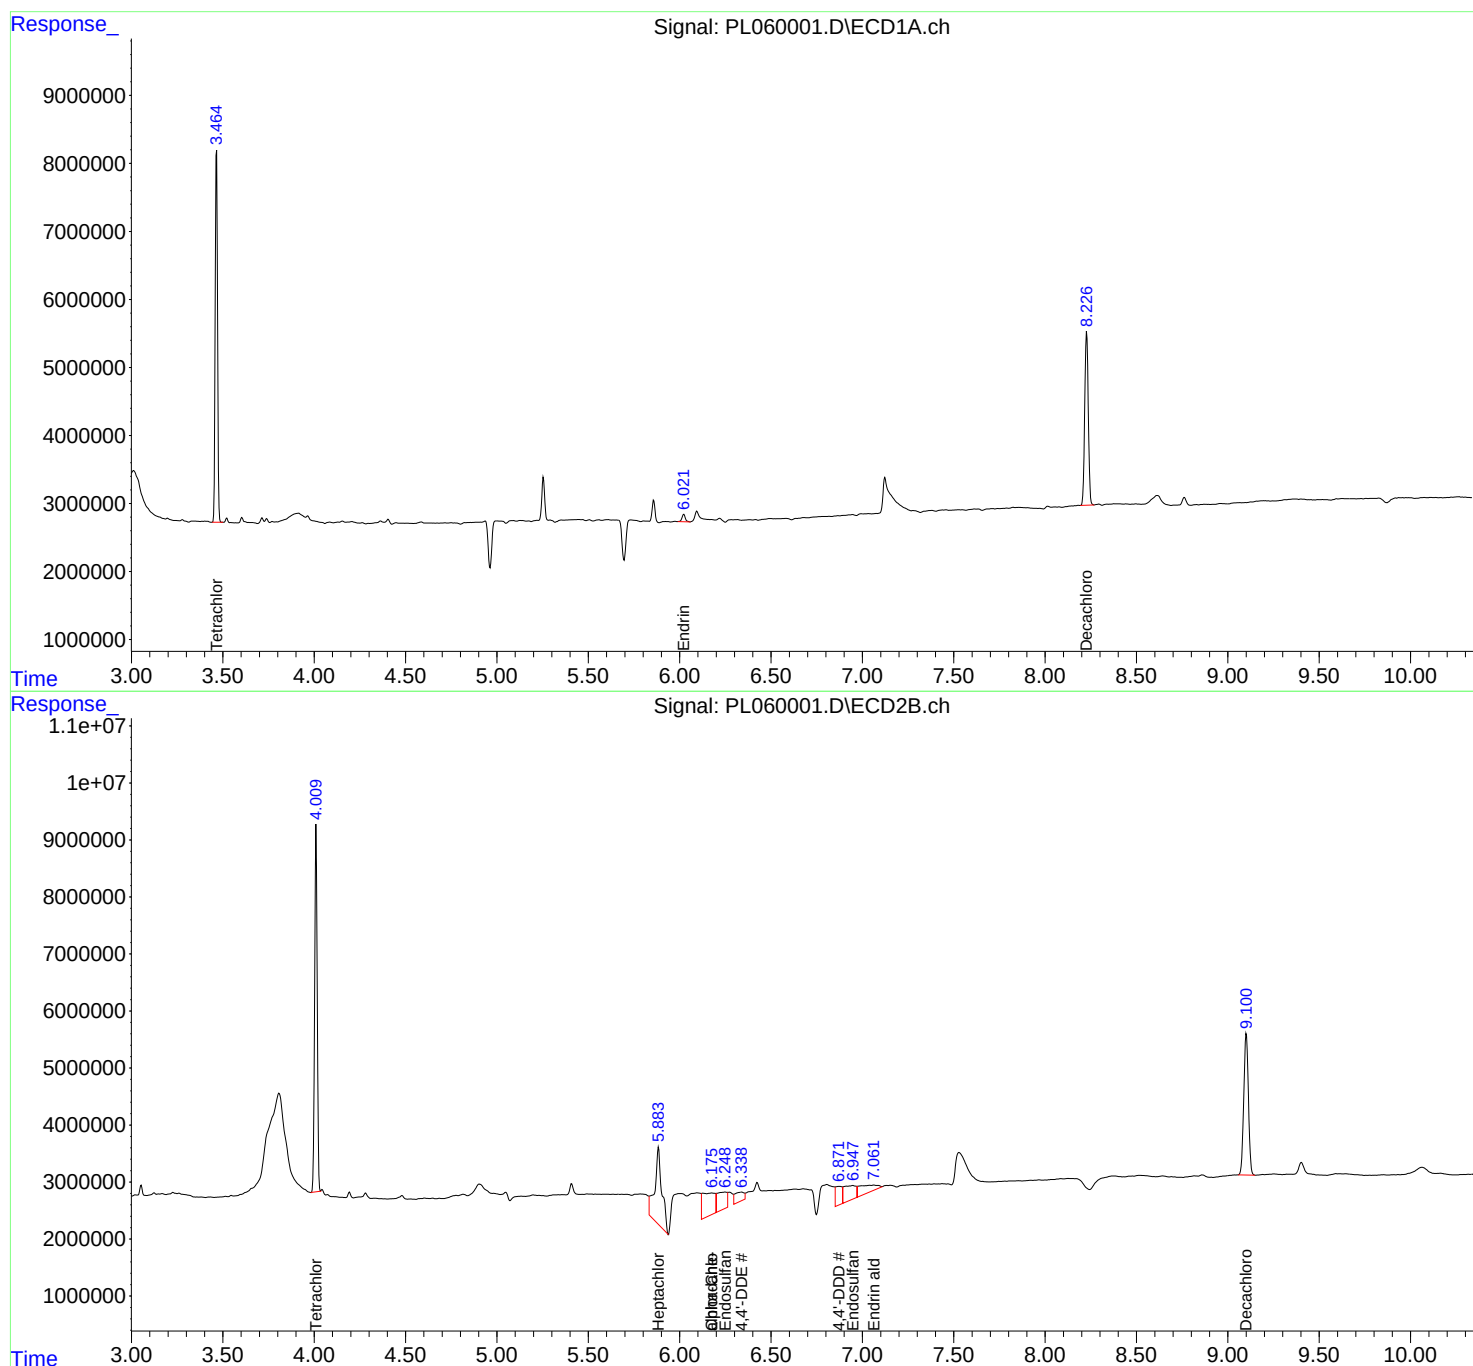


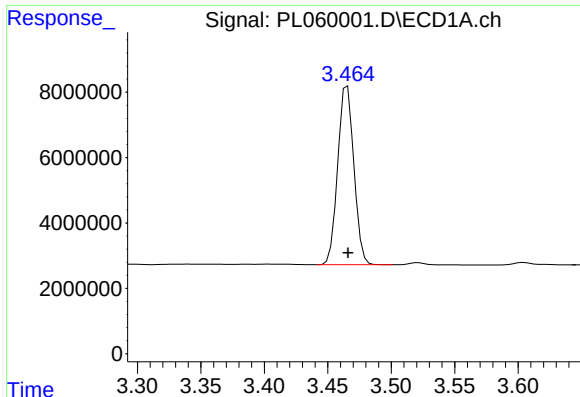

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 48446278
Conc: 25.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

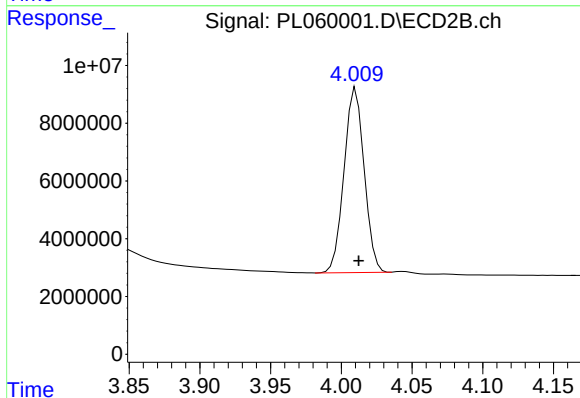


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: -0.002 min
Response: 63482046
Conc: 23.95 ng/ml

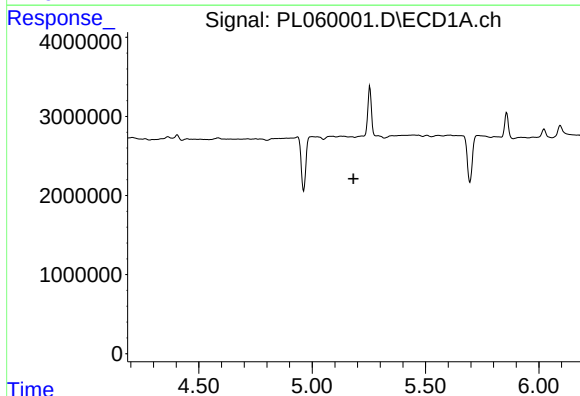


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.183 min
Response: 0
Conc: N.D.

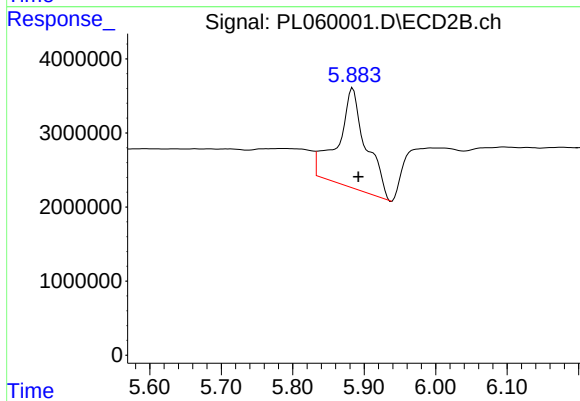

#8 Heptachlor epoxide


R.T.: 5.884 min
Delta R.T.: -0.008 min
Response: 36926621
Conc: 13.71 ng/ml

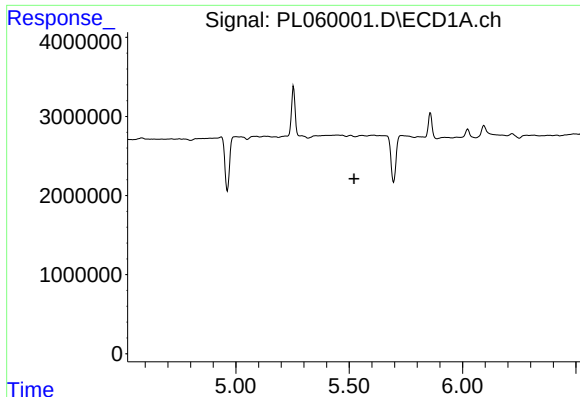

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

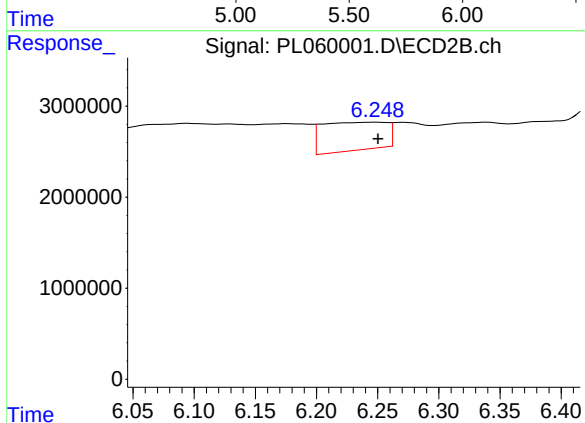


#9 Endosulfan I

R.T.: 6.249 min
Delta R.T.: -0.002 min
Response: 11331044
Conc: 4.25 ng/ml

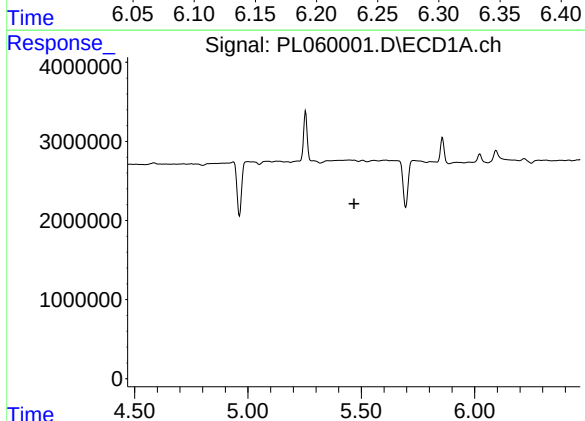


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.469 min
Response: 0
Conc: N.D.

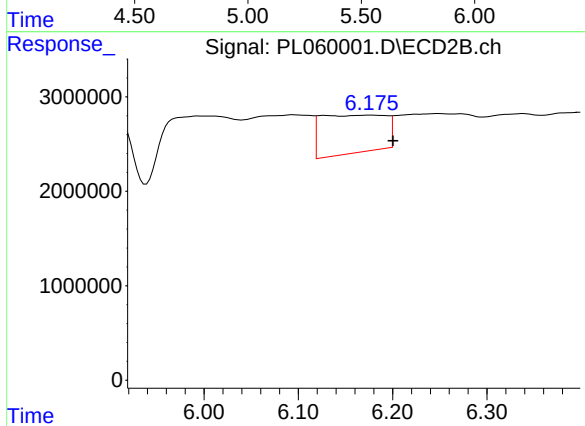

#11 alpha-Chlordane


R.T.: 6.176 min
Delta R.T.: -0.024 min
Response: 19176222
Conc: 6.71 ng/ml

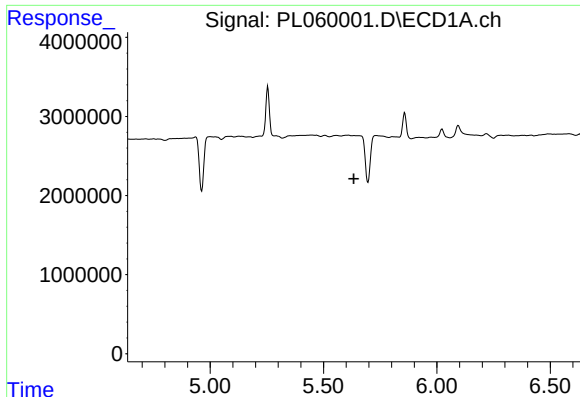

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

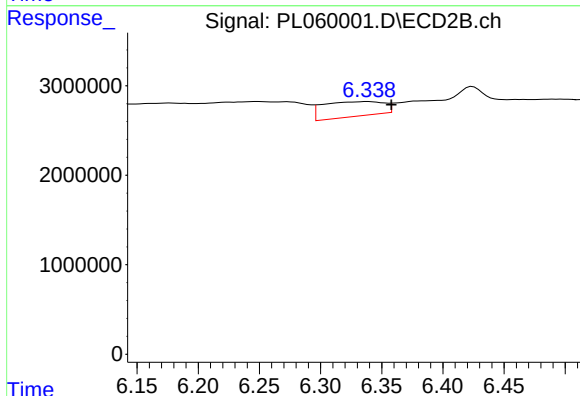


#12 4,4'-DDE

R.T.: 6.339 min
Delta R.T.: -0.019 min
Response: 5720639
Conc: 2.14 ng/ml

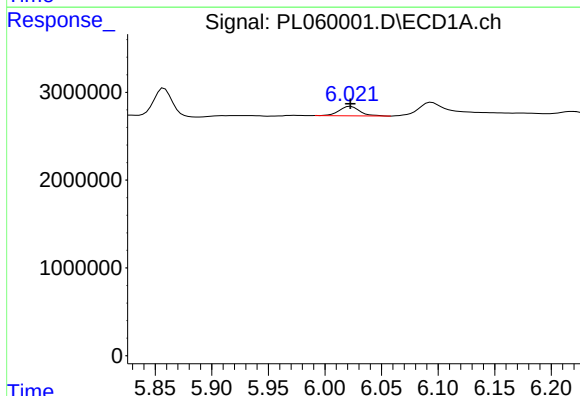


#14 Endrin

R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 1355811
Conc: 0.93 ng/ml

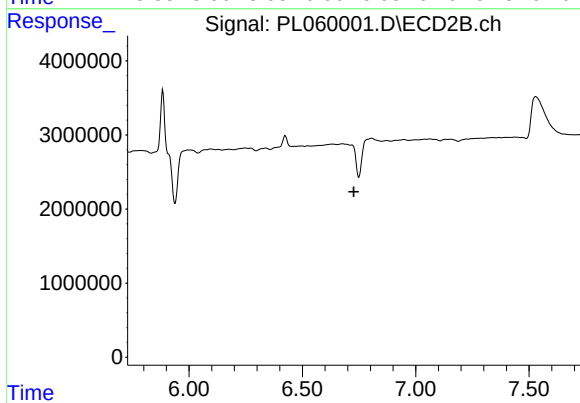

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.727 min
Response: 0
Conc: N.D.

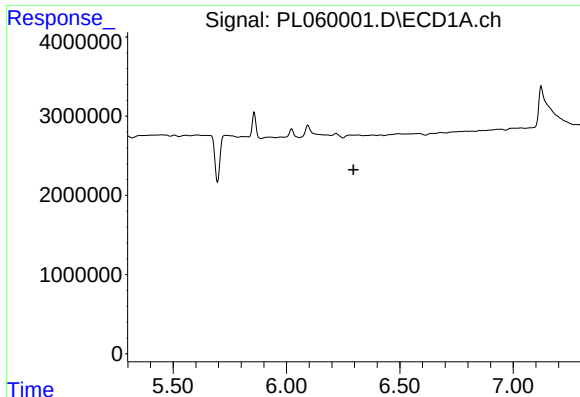

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

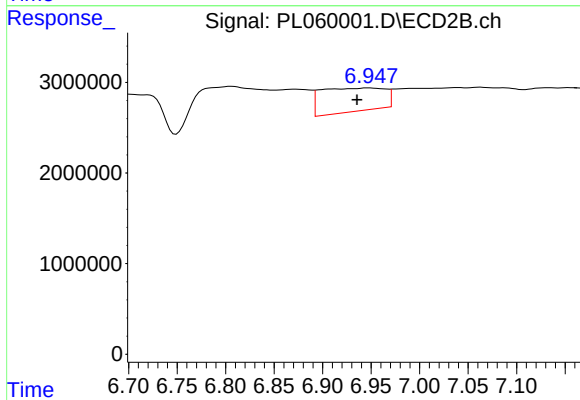


#15 Endosulfan II

R.T.: 6.948 min
Delta R.T.: 0.012 min
Response: 11797241
Conc: 4.70 ng/ml

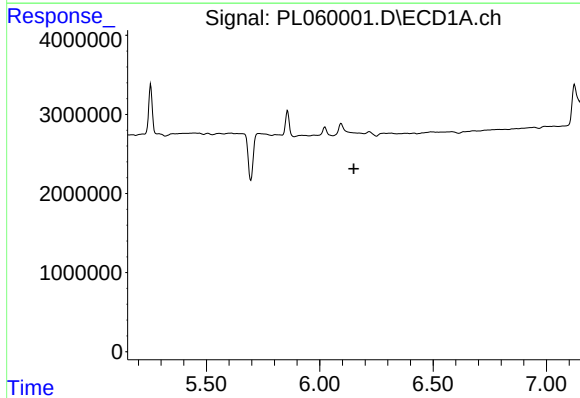


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

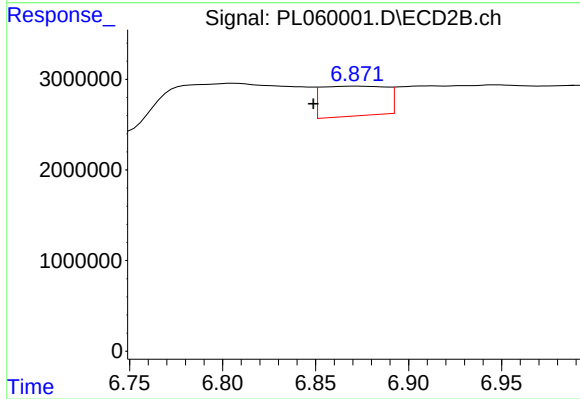

#16 4,4'-DDD


R.T.: 6.872 min
Delta R.T.: 0.023 min
Response: 7997355
Conc: 3.48 ng/ml

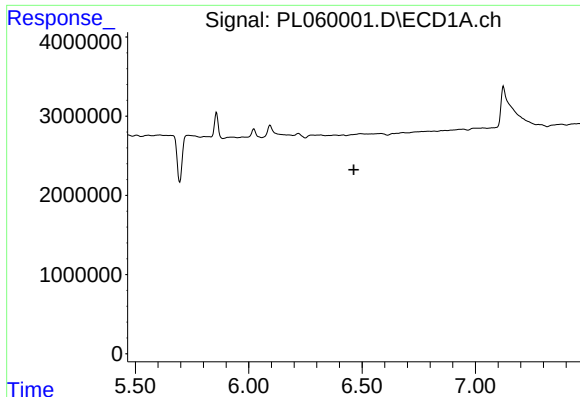

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

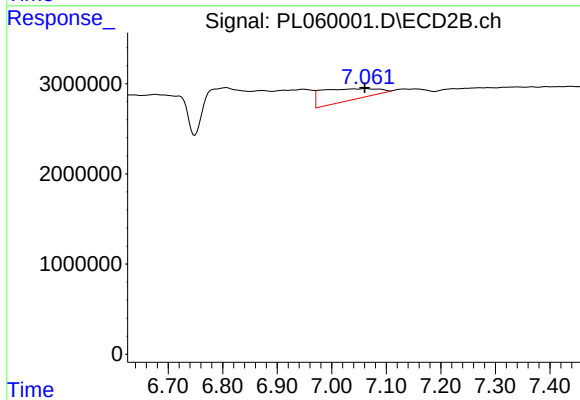


#18 Endrin aldehyde

R.T.: 7.063 min
Delta R.T.: 0.002 min
Response: 9243005
Conc: 4.26 ng/ml

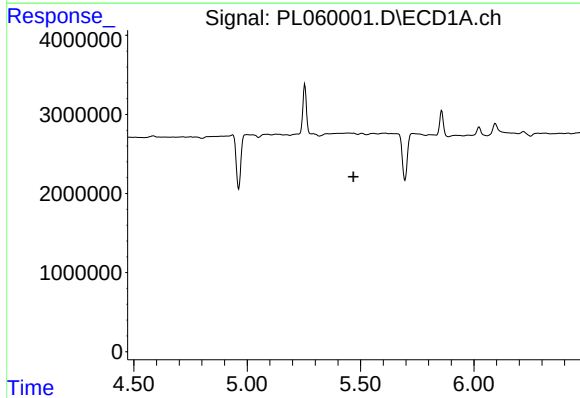


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

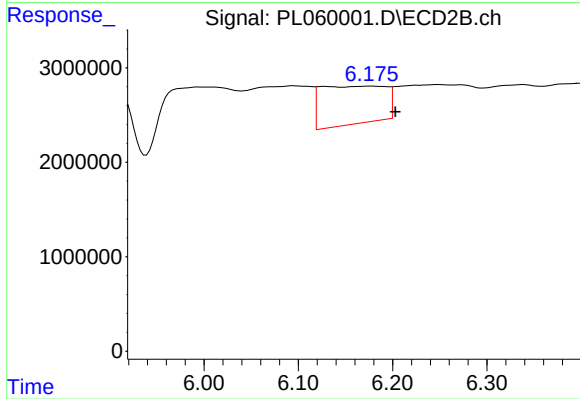

#26 Chlordane-4


R.T.: 6.176 min
Delta R.T.: -0.026 min
Response: 19176222
Conc: 41.43 ng/ml

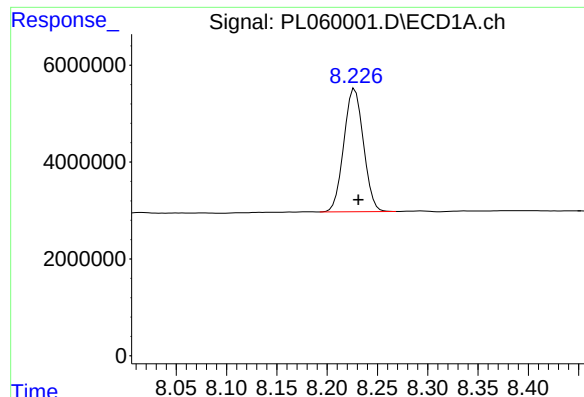

#28 Decachlorobiphenyl

R.T.: 8.228 min
Delta R.T.: -0.004 min
Response: 34379621
Conc: 20.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

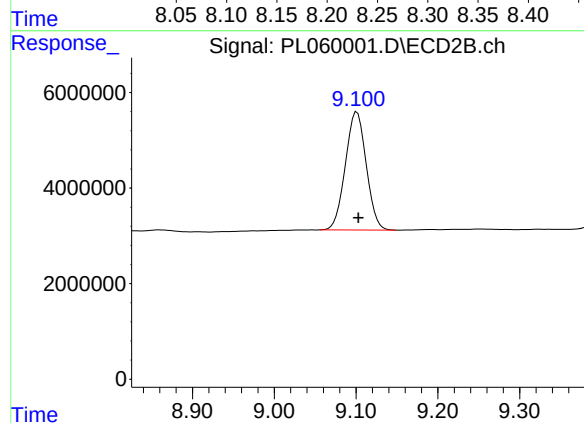

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: -0.002 min
Response: 43657849
Conc: 20.87 ng/ml