

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071720\
 Data File : PL060013.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2020 14:45
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 16:35:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.011	45811188	60097548	23.684	22.677
28)	SA Decachlor...	8.225	9.101	34857956	44870547	21.189	21.455
Target Compounds							
4)	MA Heptachlor	0.000	5.200	0	1326774	N.D.	0.394 #
8)	B Heptachlo...	0.000	5.883	0	14835956	N.D.	5.509 #
9)	A Endosulfan I	0.000	6.263	0	6165907	N.D.	2.312 #
10)	B gamma-Chl...	0.000	6.148f	0	33520866	N.D.	11.706 #
11)	B alpha-Chl...	0.000	6.199	0	2896917	N.D.	1.013 #
14)	MA Endrin	6.020	0.000	1837825	0	1.263	N.D. #
15)	B Endosulfa...	0.000	6.949	0	478478	N.D.	0.191 #
25)	Chlordane-3	0.000	6.148f	0	33520866	N.D.	86.636 #
26)	Chlordane-4	0.000	6.199	0	2896917	N.D.	6.258 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071720\
Data File : PL060013.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2020 14:45
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 16:35:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

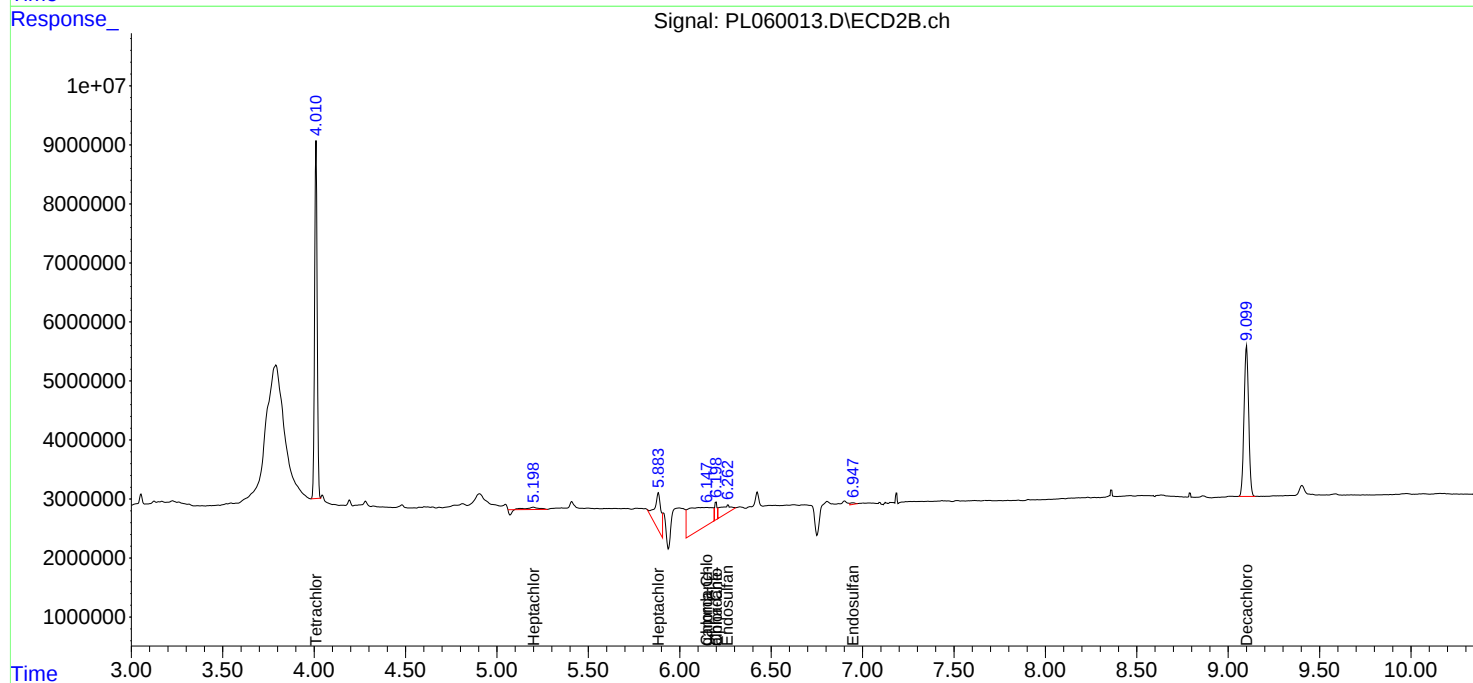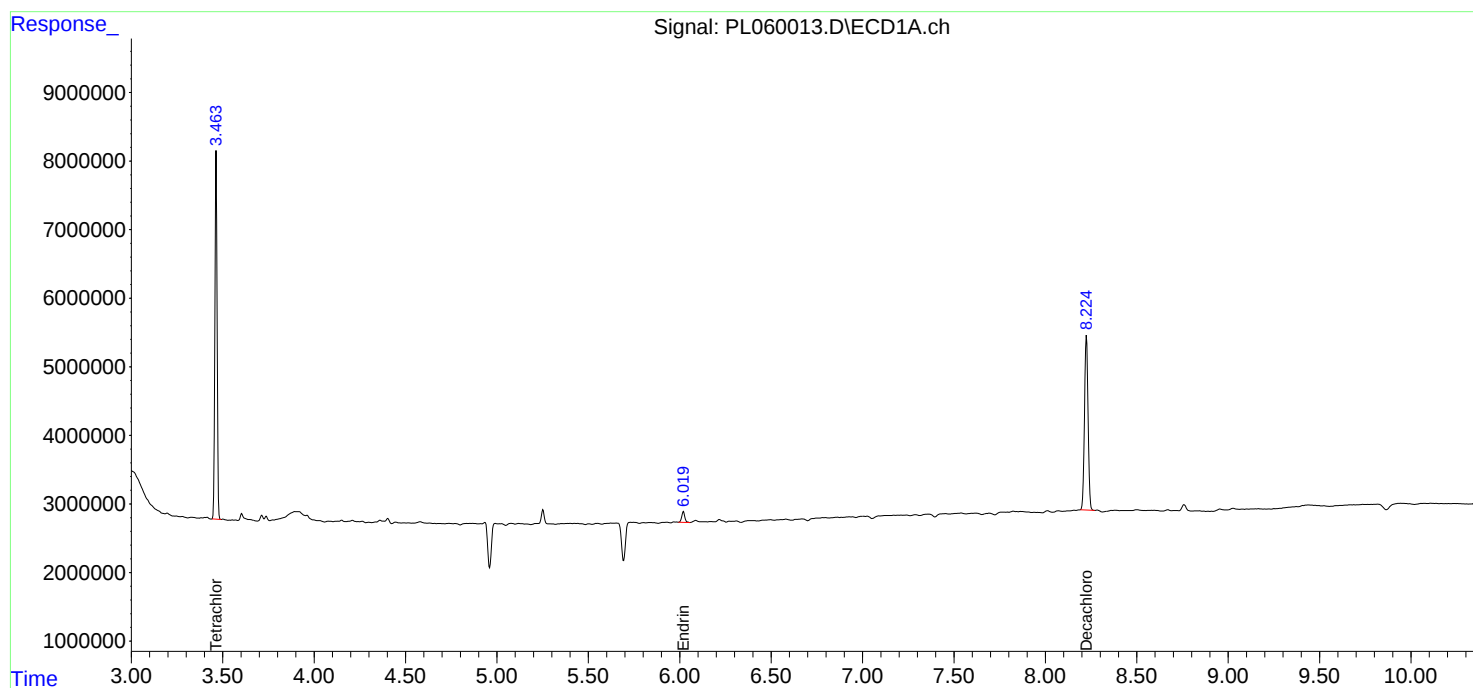


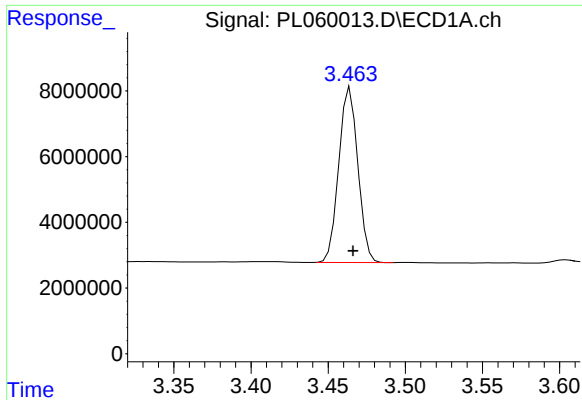

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: -0.002 min
Response: 45811188
Conc: 23.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

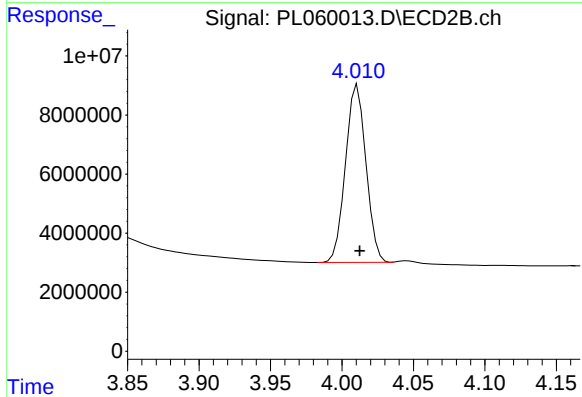


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.001 min
Response: 60097548
Conc: 22.68 ng/ml

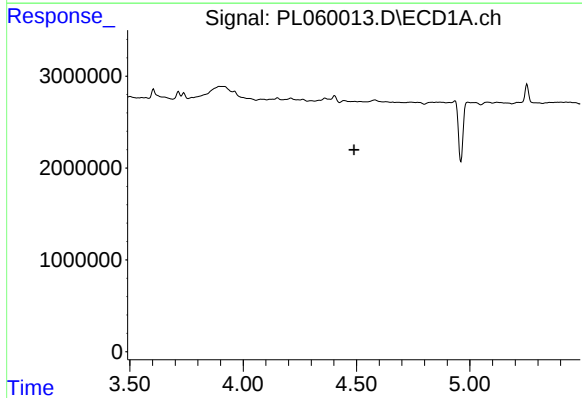


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

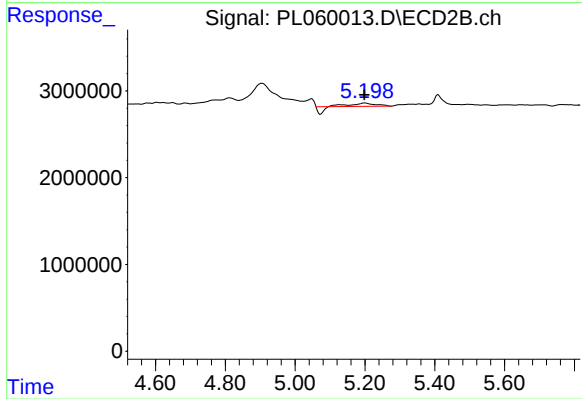

#4 Heptachlor


R.T.: 5.200 min
Delta R.T.: 0.001 min
Response: 1326774
Conc: 0.39 ng/ml

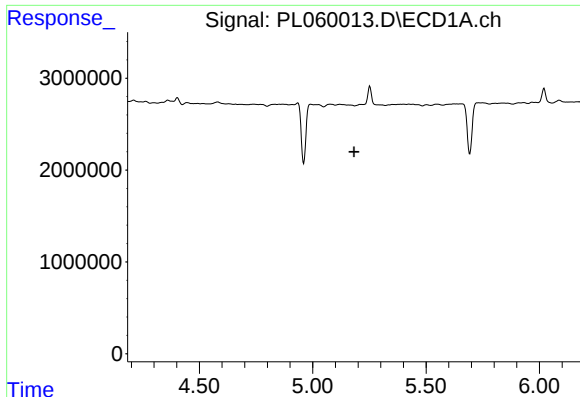

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

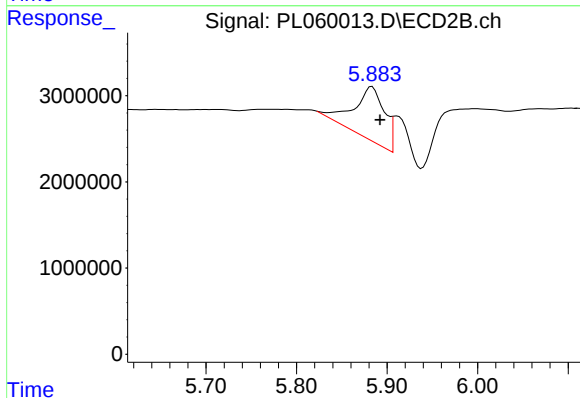


#8 Heptachlor epoxide

R.T.: 5.883 min
Delta R.T.: -0.009 min
Response: 14835956
Conc: 5.51 ng/ml

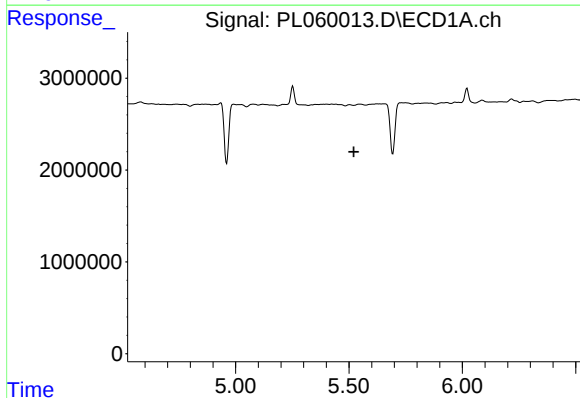


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.522 min
Response: 0
Conc: N.D.

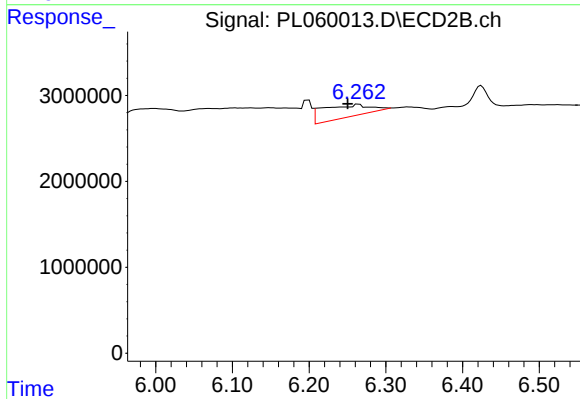

#9 Endosulfan I


R.T.: 6.263 min
Delta R.T.: 0.013 min
Response: 6165907
Conc: 2.31 ng/ml

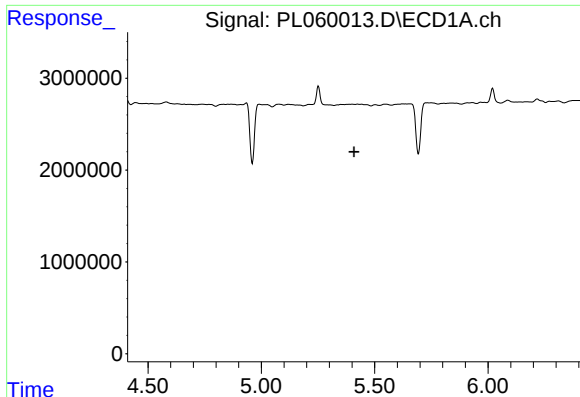

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

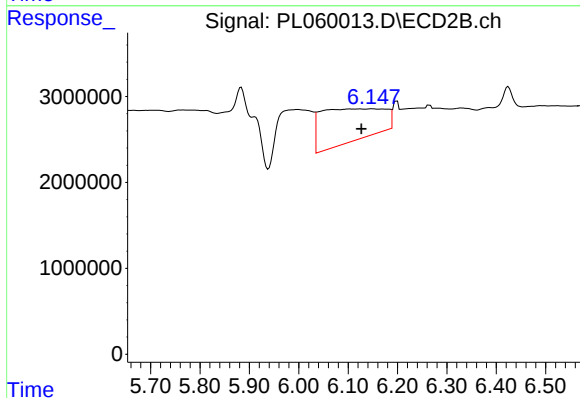


#10 gamma-Chlordane

R.T.: 6.148 min
Delta R.T.: 0.021 min
Response: 33520866
Conc: 11.71 ng/ml

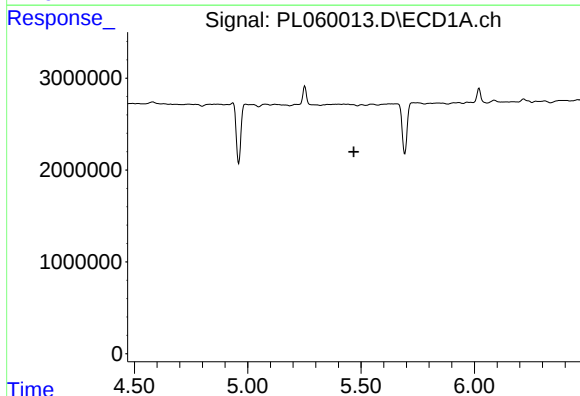


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

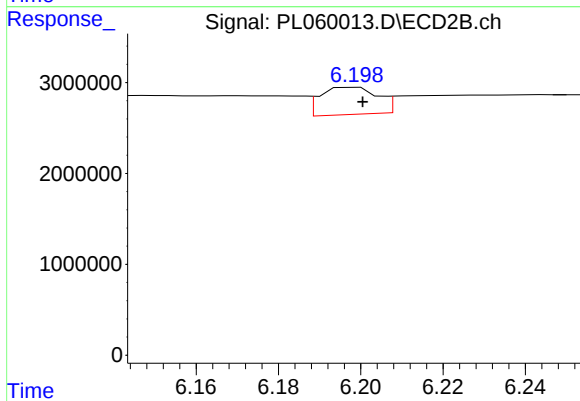

#11 alpha-Chlordane


R.T.: 6.199 min
Delta R.T.: -0.002 min
Response: 2896917
Conc: 1.01 ng/ml

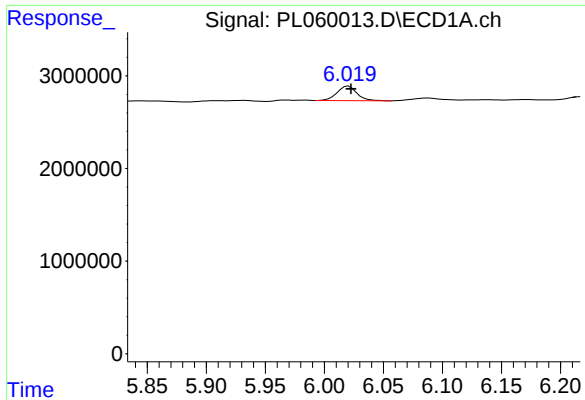

#14 Endrin


R.T.: 6.020 min
Delta R.T.: -0.002 min
Response: 1837825
Conc: 1.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

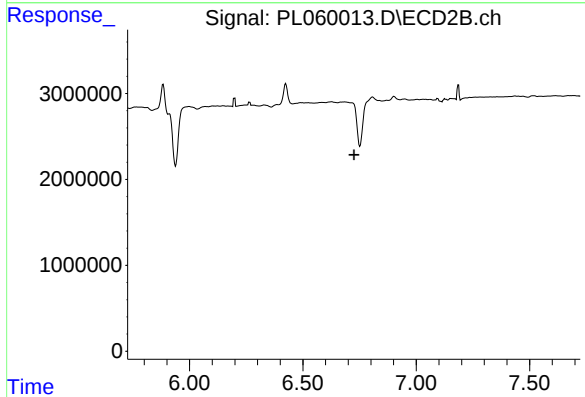


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.727 min
Response: 0
Conc: N.D.

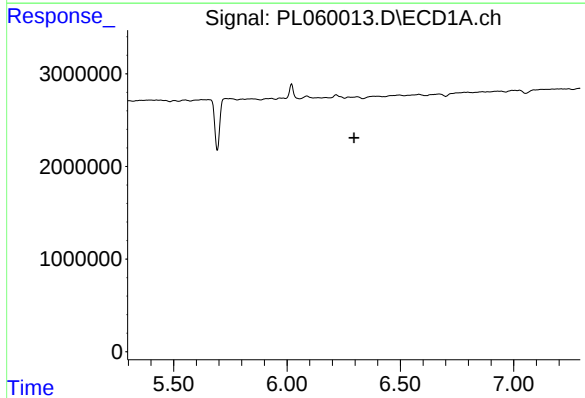


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.296 min
Response: 0
Conc: N.D.

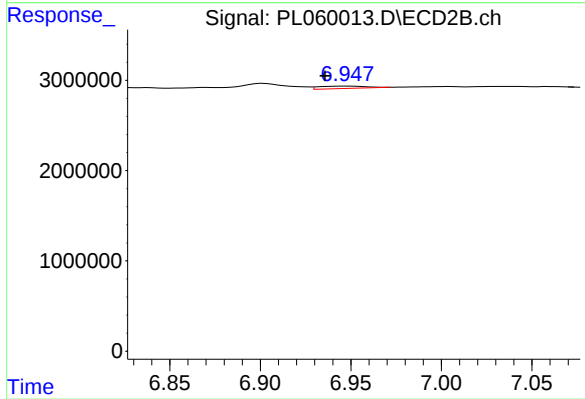

#15 Endosulfan II


R.T.: 6.949 min
Delta R.T.: 0.013 min
Response: 478478
Conc: 0.19 ng/ml

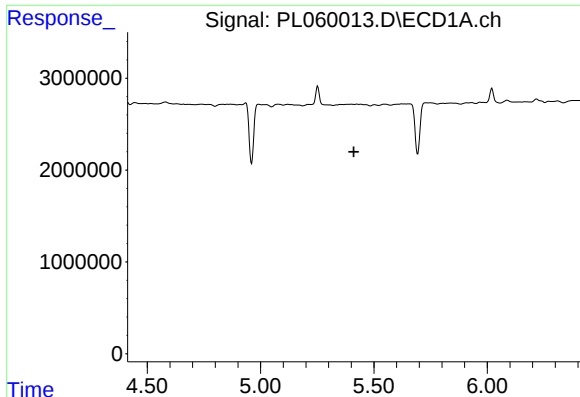

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

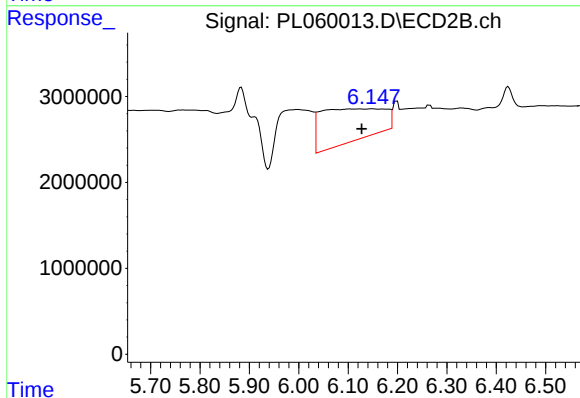


#25 Chlordane-3

R.T.: 6.148 min
Delta R.T.: 0.020 min
Response: 33520866
Conc: 86.64 ng/ml

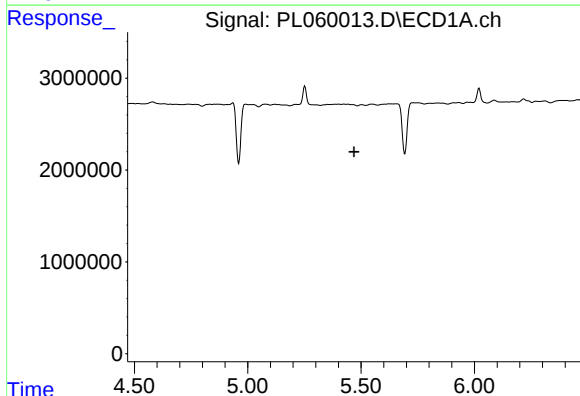


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

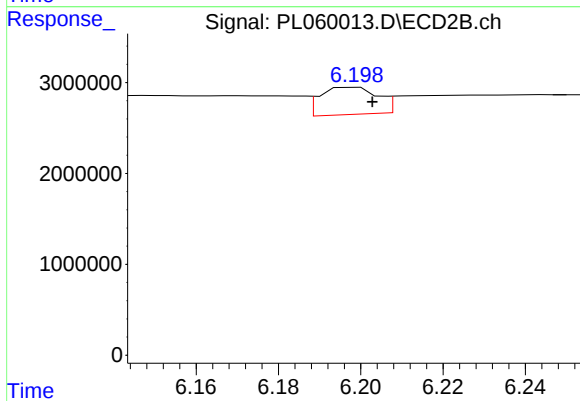

#26 Chlordane-4


R.T.: 6.199 min
Delta R.T.: -0.004 min
Response: 2896917
Conc: 6.26 ng/ml

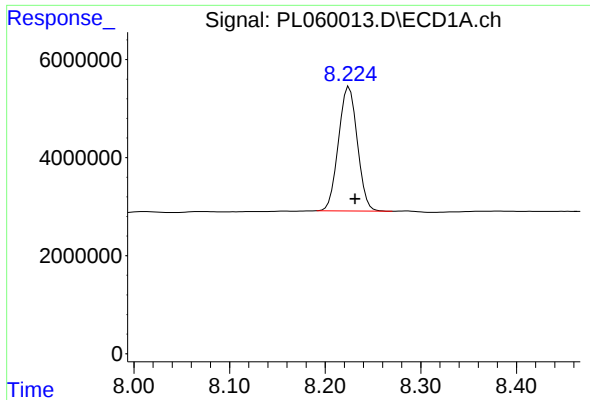

#28 Decachlorobiphenyl

R.T.: 8.225 min
Delta R.T.: -0.006 min
Response: 34857956
Conc: 21.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

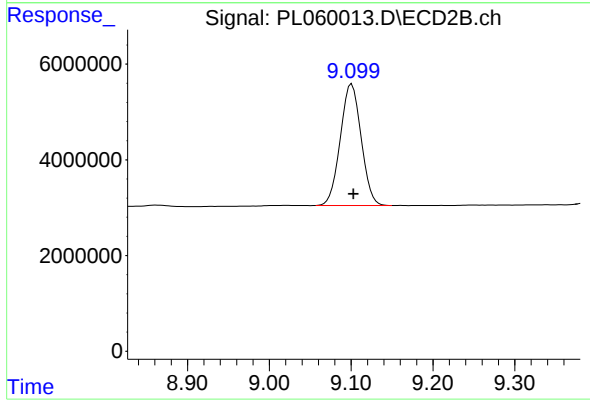

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: -0.002 min
Response: 44870547
Conc: 21.45 ng/ml