

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071720\
 Data File : PL060016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2020 15:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 16:35:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.011	48096143	62933250	24.866	23.747
28)	SA Decachlor...	8.226	9.101	35607900	45431805	21.645	21.723
Target Compounds							
8)	B Heptachlo...	0.000	5.884	0	33705081	N.D.	12.515 #
14)	MA Endrin	6.021	0.000	1704711	0	1.171	N.D. #
15)	B Endosulfa...	0.000	6.946	0	1837073	N.D.	0.731 #
17)	MA 4,4'-DDT	0.000	7.154	0	1320662	N.D.	0.671 #
18)	B Endrin al...	0.000	7.034f	0	3759000	N.D.	1.731 #
27)	Chlordane-5	0.000	7.034f	0	3759000	N.D.	48.400 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071720\
Data File : PL060016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2020 15:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 16:35:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

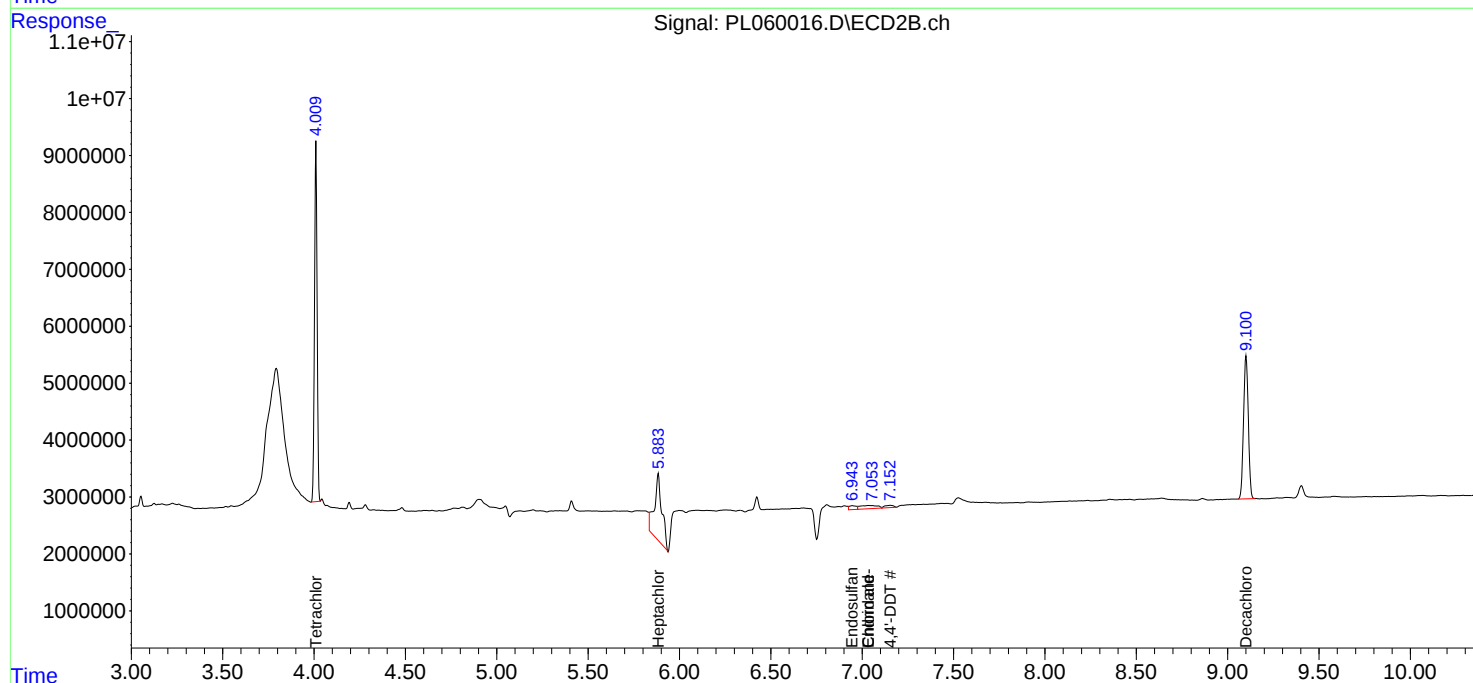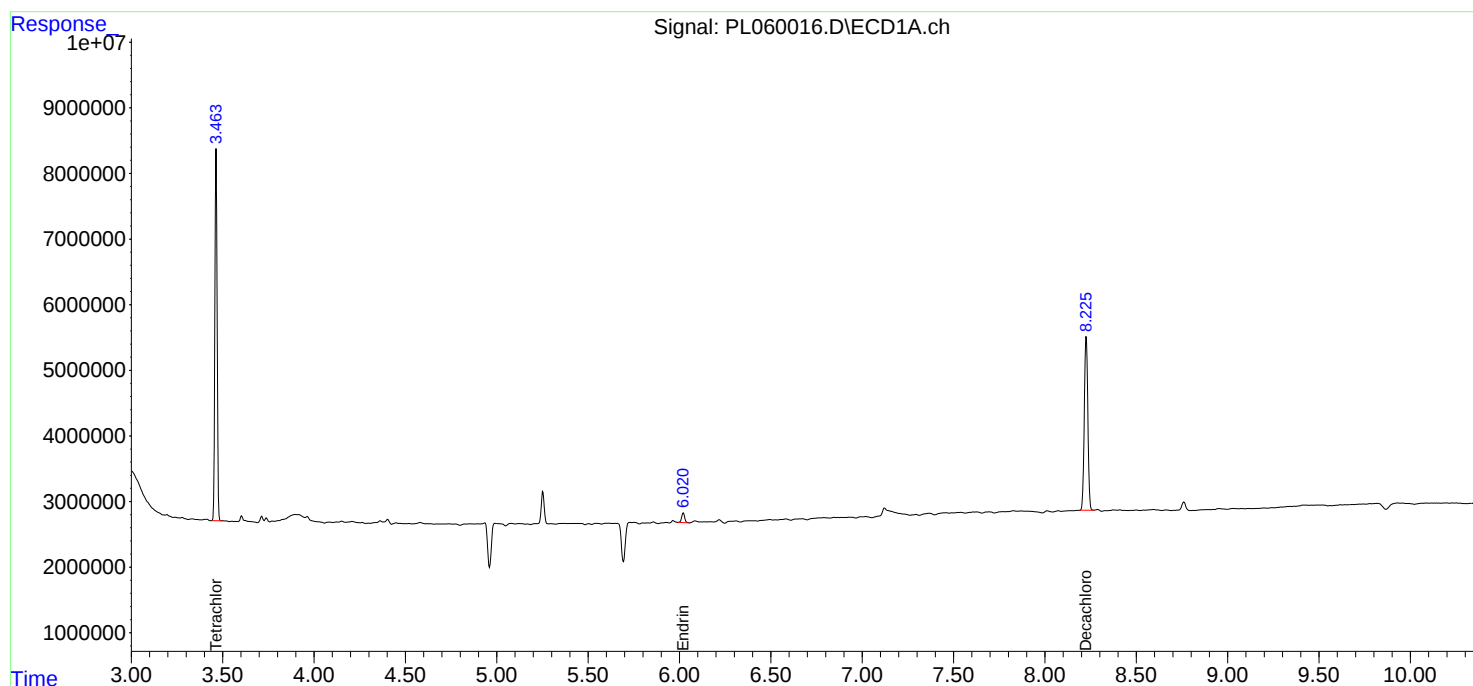


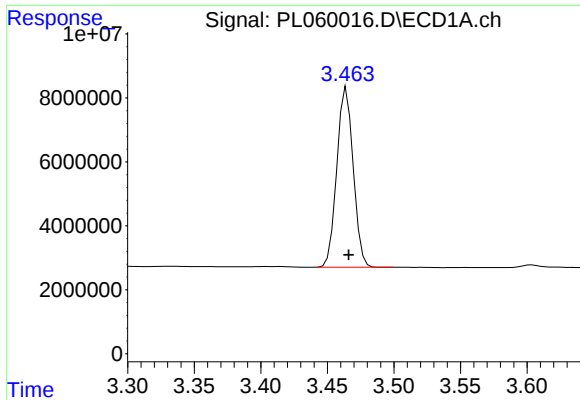

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: -0.001 min
Response: 48096143
Conc: 24.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

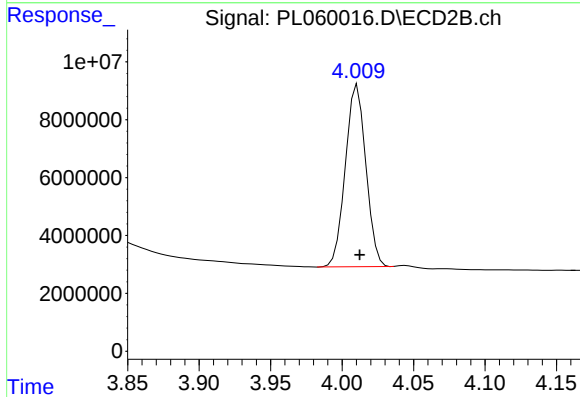


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.002 min
Response: 62933250
Conc: 23.75 ng/ml

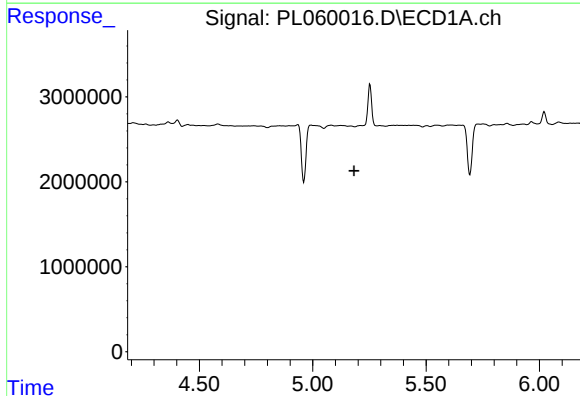


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.183 min
Response: 0
Conc: N.D.

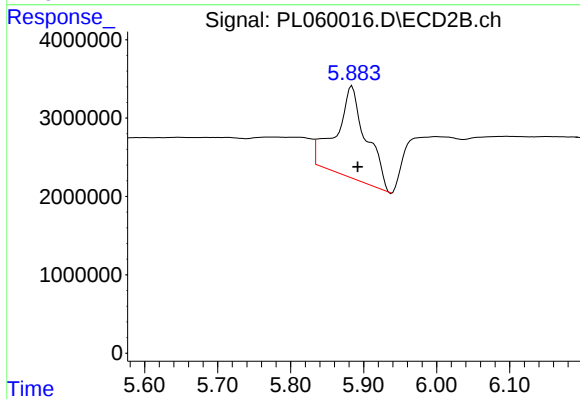

#8 Heptachlor epoxide


R.T.: 5.884 min
Delta R.T.: -0.008 min
Response: 33705081
Conc: 12.51 ng/ml

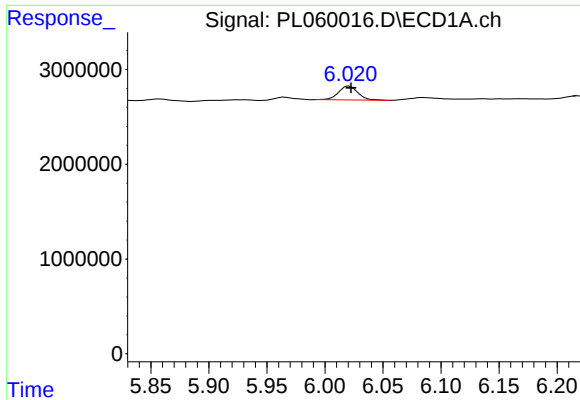

#14 Endrin


R.T.: 6.021 min
Delta R.T.: -0.001 min
Response: 1704711
Conc: 1.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

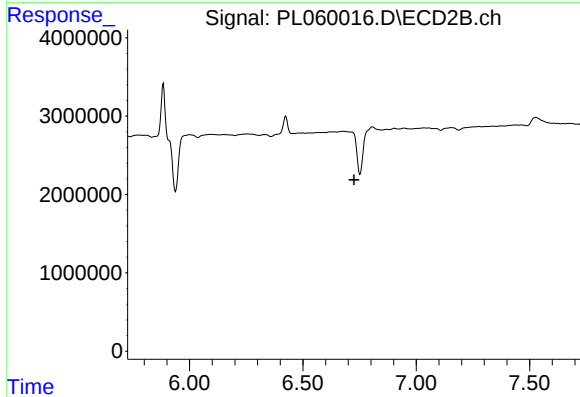


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.727 min
Response: 0
Conc: N.D.

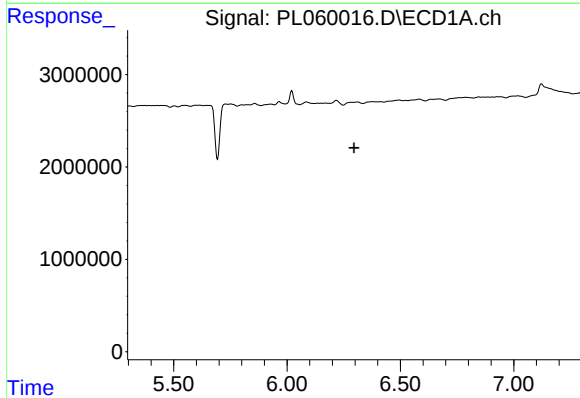


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.296 min
Response: 0
Conc: N.D.

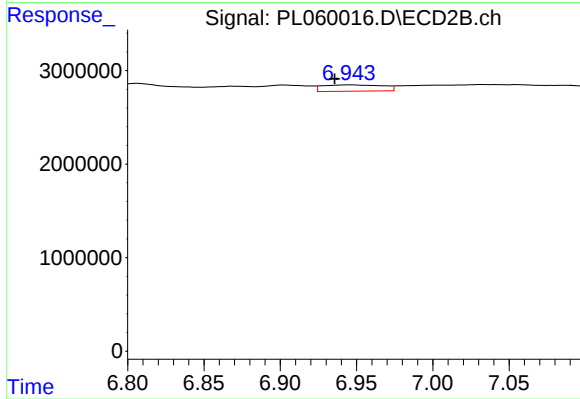

#15 Endosulfan II

R.T.: 6.946 min
Delta R.T.: 0.010 min
Response: 1837073
Conc: 0.73 ng/ml

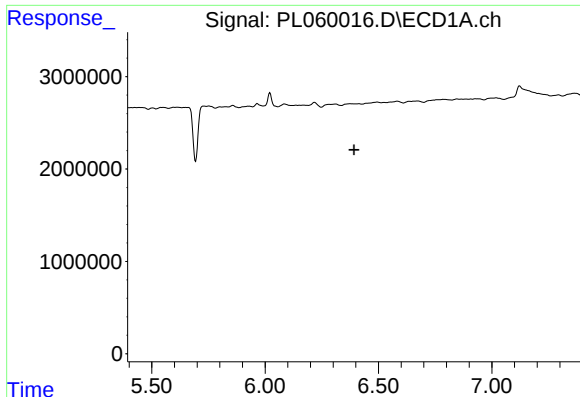

#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#17 4,4'-DDT


R.T.: 7.154 min
Delta R.T.: 0.005 min
Response: 1320662
Conc: 0.67 ng/ml

#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.464 min
Response: 0
Conc: N.D.

#18 Endrin aldehyde


R.T.: 7.034 min
Delta R.T.: -0.026 min
Response: 3759000
Conc: 1.73 ng/ml

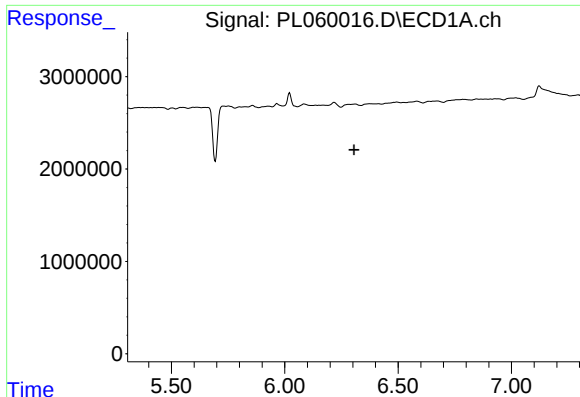

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

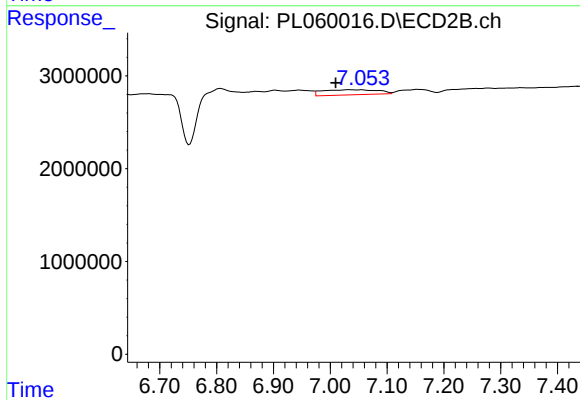


#27 Chlordane-5

R.T.: 7.034 min
Delta R.T.: 0.024 min
Response: 3759000
Conc: 48.40 ng/ml

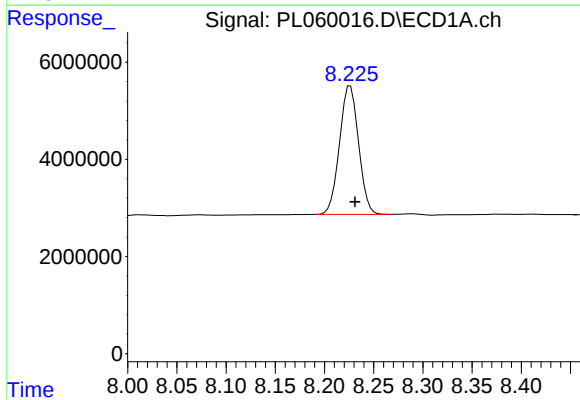

#28 Decachlorobiphenyl

R.T.: 8.226 min
Delta R.T.: -0.005 min
Response: 35607900
Conc: 21.64 ng/ml

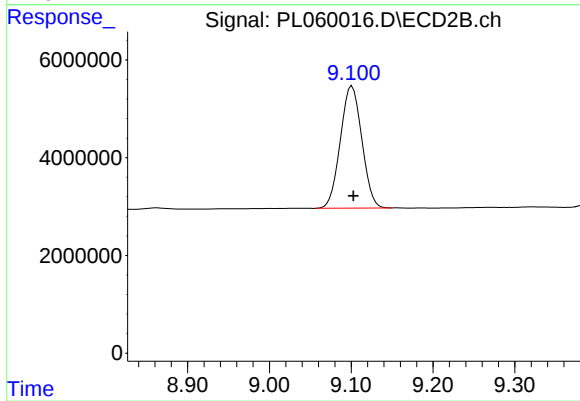

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: -0.002 min
Response: 45431805
Conc: 21.72 ng/ml