

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071721\
 Data File : PL068204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2021 16:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 22:39:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.655	5.586	8291727	20955407	20.569	20.320
28)	SA Decachlor...	10.432	11.511	9903696	16719780	24.000	18.583
Target Compounds							
3)	MA gamma-BHC...	5.785	0.000	781554	0	1.505	N.D. #
4)	MA Heptachlor	6.174f	0.000	259449	0	0.470	N.D. #
6)	B beta-BHC	6.174	0.000	259449	0	0.998	N.D. #
23)	Chlordane-1	0.000	6.987f	0	1246734	N.D.	32.389 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071721\
Data File : PL068204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2021 16:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 22:39:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

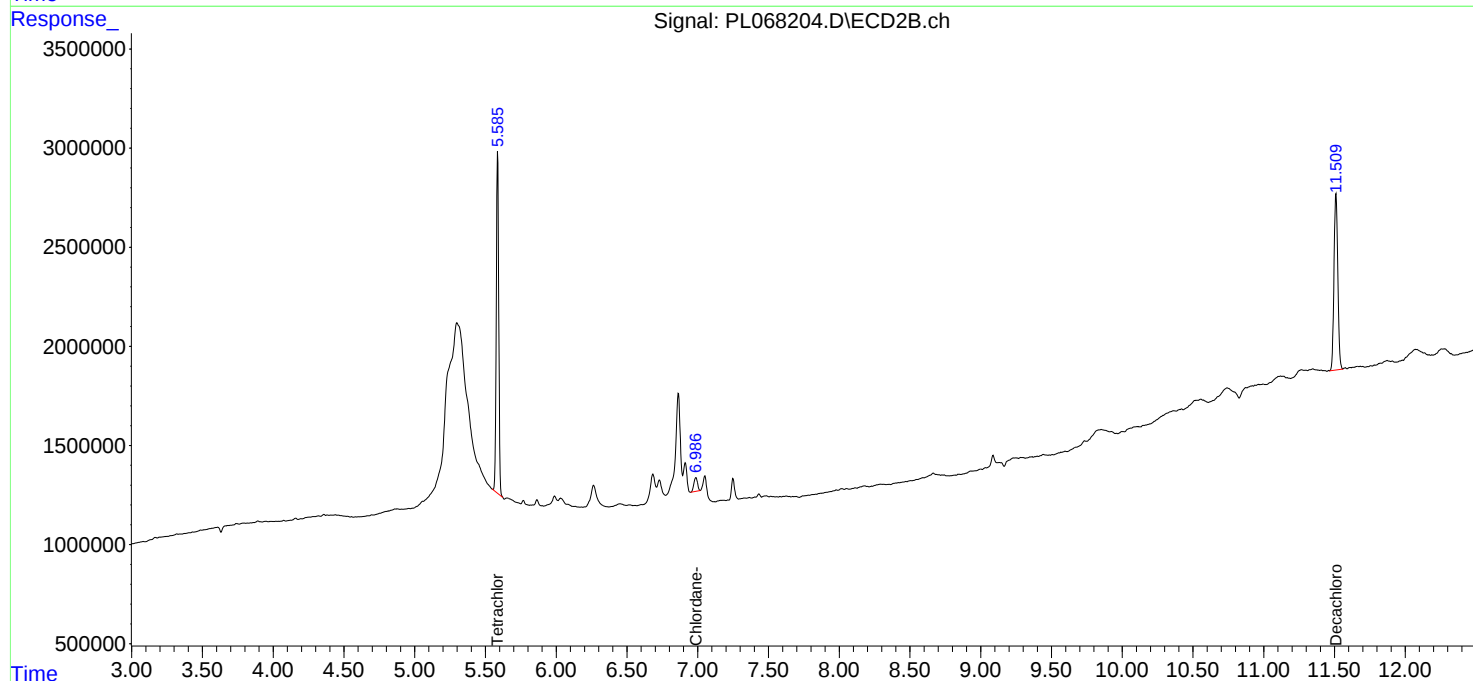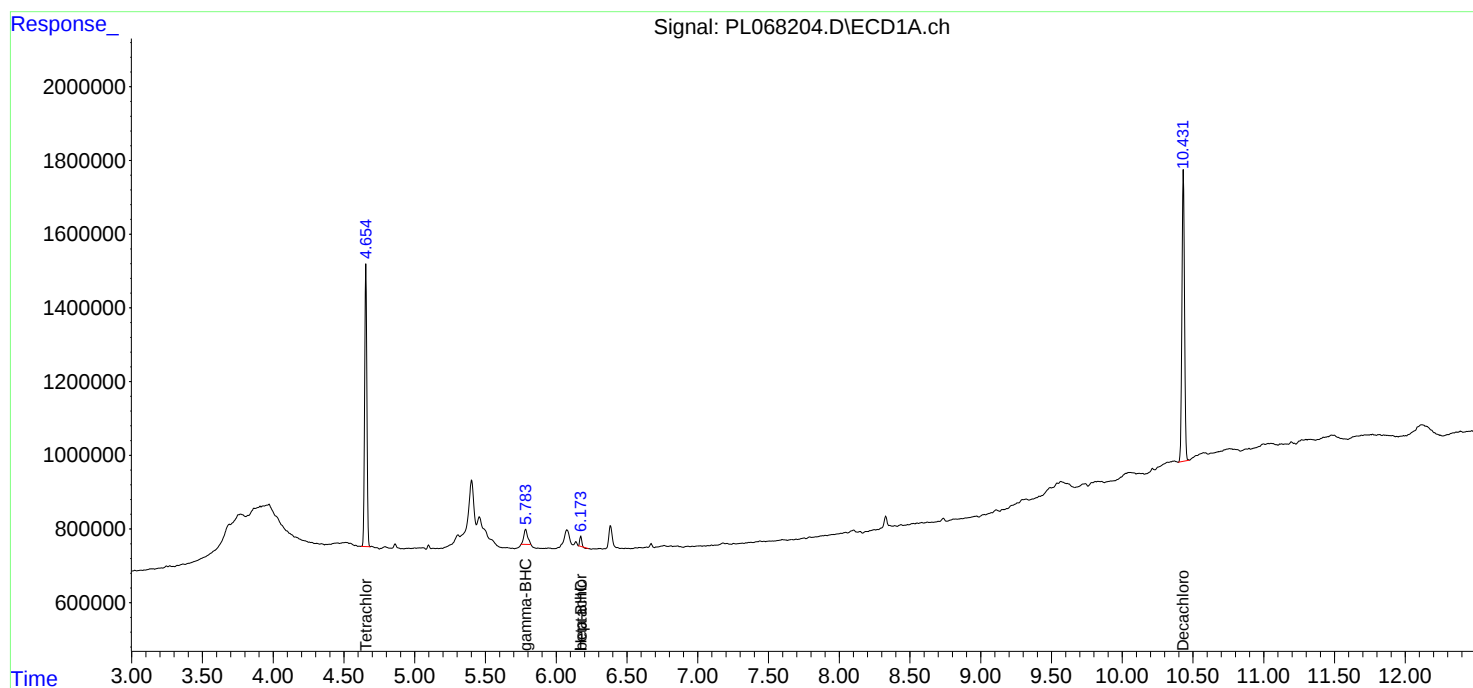


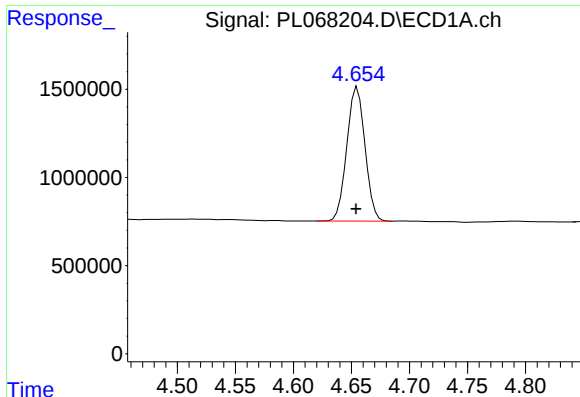

#1 Tetrachloro-m-xylene


R.T.: 4.655 min
Delta R.T.: 0.001 min
Response: 8291727
Conc: 20.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

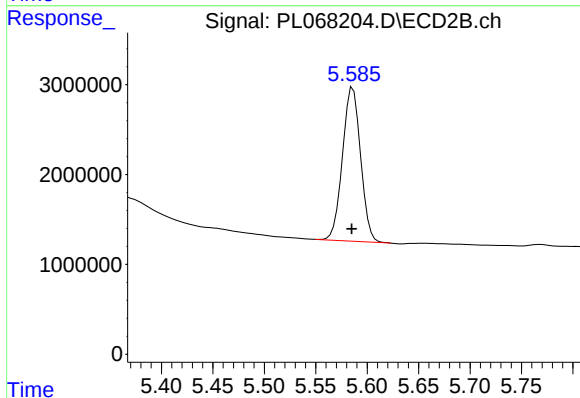


#1 Tetrachloro-m-xylene

R.T.: 5.586 min
Delta R.T.: 0.001 min
Response: 20955407
Conc: 20.32 ng/ml

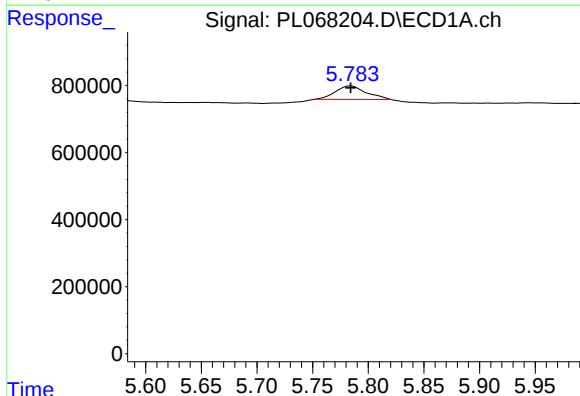


#3 gamma-BHC (Lindane)

R.T.: 5.785 min
Delta R.T.: 0.000 min
Response: 781554
Conc: 1.51 ng/ml

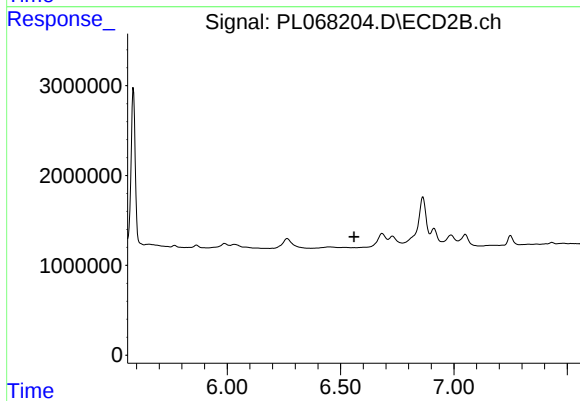

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 6.560 min
Response: 0
Conc: N.D.

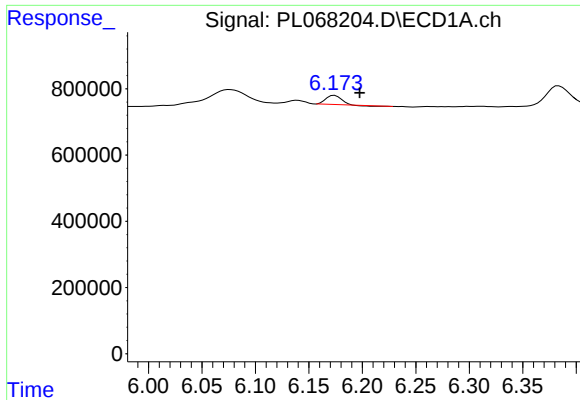

#4 Heptachlor


R.T.: 6.174 min
Delta R.T.: -0.023 min
Response: 259449
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

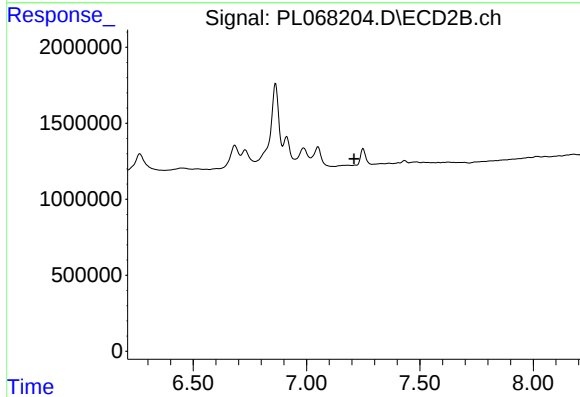


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.210 min
Response: 0
Conc: N.D.

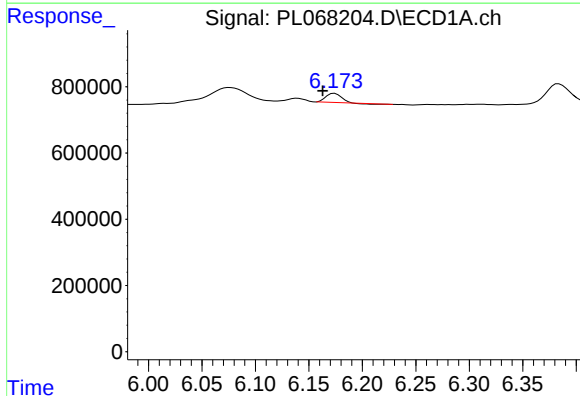


#6 beta-BHC

R.T.: 6.174 min
Delta R.T.: 0.011 min
Response: 259449
Conc: 1.00 ng/ml

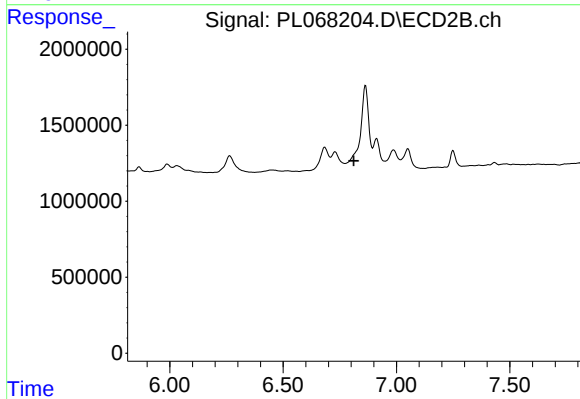

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.812 min
Response: 0
Conc: N.D.

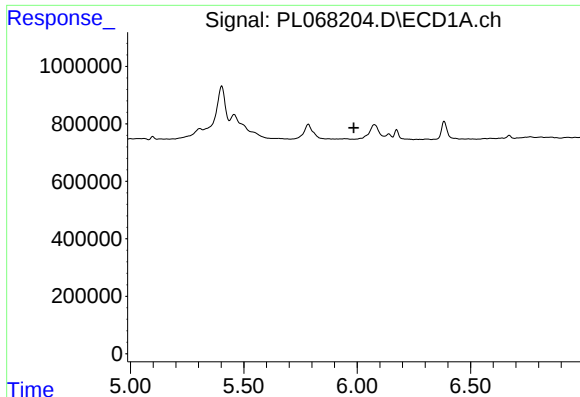

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.986 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

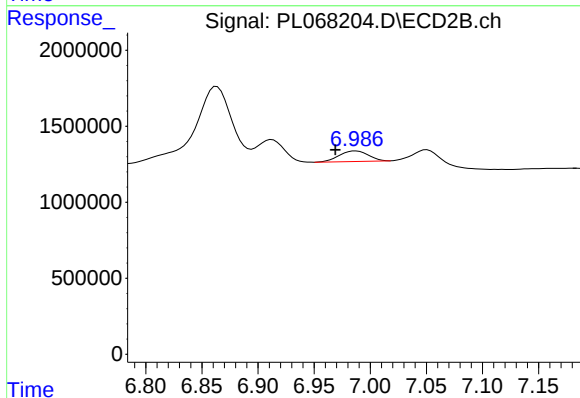


#23 Chlordane-1

R.T.: 6.987 min
Delta R.T.: 0.018 min
Response: 1246734
Conc: 32.39 ng/ml

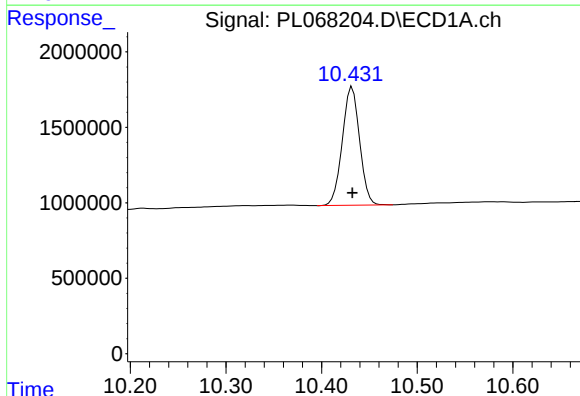

#28 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 9903696
Conc: 24.00 ng/ml

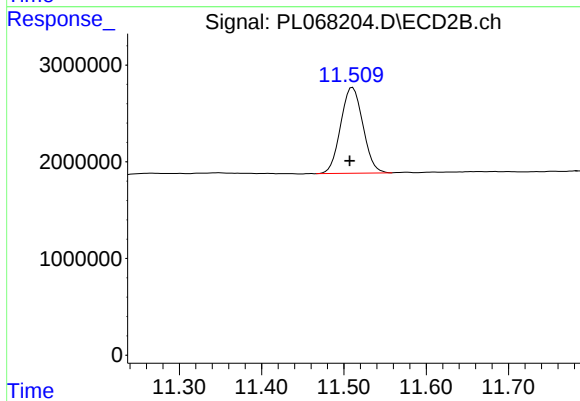

#28 Decachlorobiphenyl

R.T.: 11.511 min
Delta R.T.: 0.003 min
Response: 16719780
Conc: 18.58 ng/ml