

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
 Data File : PL083972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 13:26
 Operator : AR\AJ
 Sample : 03501-16MS
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A46X7MS

Manual Integrations APPROVED

Reviewed By :Abdul Mirza 07/21/2023
 Supervised By :Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 00:46:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 05:26:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	2.688	2569.9E6	10854233	1239.184m	10.572 #
27)	SA Decachlor...	9.025	7.871	44628581	23300601	33.954	21.053 #
Target Compounds							
2)	A alpha-BHC	3.928	3.192	234.0E6	58838081	77.442m	40.711m#
3)	MA gamma-BHC...	4.274	3.505	2395.9E6	1656.0E6	849.225m	1199.091m#
4)	MA Heptachlor	4.857	3.869	49631084	794.9E6	15.770m	603.395m#
5)	MB Aldrin	5.201	4.128	98255486	728.2E6	33.070m	557.793m#
6)	B beta-BHC	4.448	3.822	6751.1E6	31203031	5038.085	46.317m#
7)	B delta-BHC	4.736	4.061	1725.1E6	236.5E6	609.230m	165.348m#
8)	B Heptachlo...	5.627	4.652	782.2E6	320.7E6	282.776m	256.165
9)	A Endosulfan I	6.010	5.021	192.7E6	26056917	79.856m	23.014m#
10)	B trans-Chl...	5.913	4.889	288.8E6	275.8E6	110.436m	223.016m#
11)	B cis-Chlor...	5.971	4.962	238.6E6	84287782	89.864m	65.798m#
12)	B 4,4'-DDE	6.145	5.168	316.3E6	99928491	152.737	82.823 #
13)	MA Dieldrin	6.295	5.294	287.1E6	440.8E6	118.228m	337.060m#
14)	MA Endrin	6.525	5.563	498.7E6	156.6E6	257.239m	137.512m#
15)	B Endosulfa...	6.743	5.861	183.2E6	148.7E6	95.987m	130.347 #
16)	A 4,4'-DDD	6.670	5.725	296.7E6	77902791	201.610m	80.429 #
17)	MA 4,4'-DDT	6.951	5.972	316.3E6	251.9E6	204.785m	241.802
18)	B Endrin al...	6.874	6.041	135.0E6	39564652	102.229m	48.215m#
19)	B Endosulfa...	7.109	6.270	188.2E6	107.5E6	107.284	97.404
20)	A Methoxychlor	7.463	6.561	329.4E6	242.4E6	431.990	432.463m
21)	B Endrin ke...	7.585	6.773	339.1E6	102.6E6	199.881	78.299 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
 Data File : PL083972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 13:26
 Operator : AR\AJ
 Sample : 03501-16MS
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 00:46:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 05:26:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

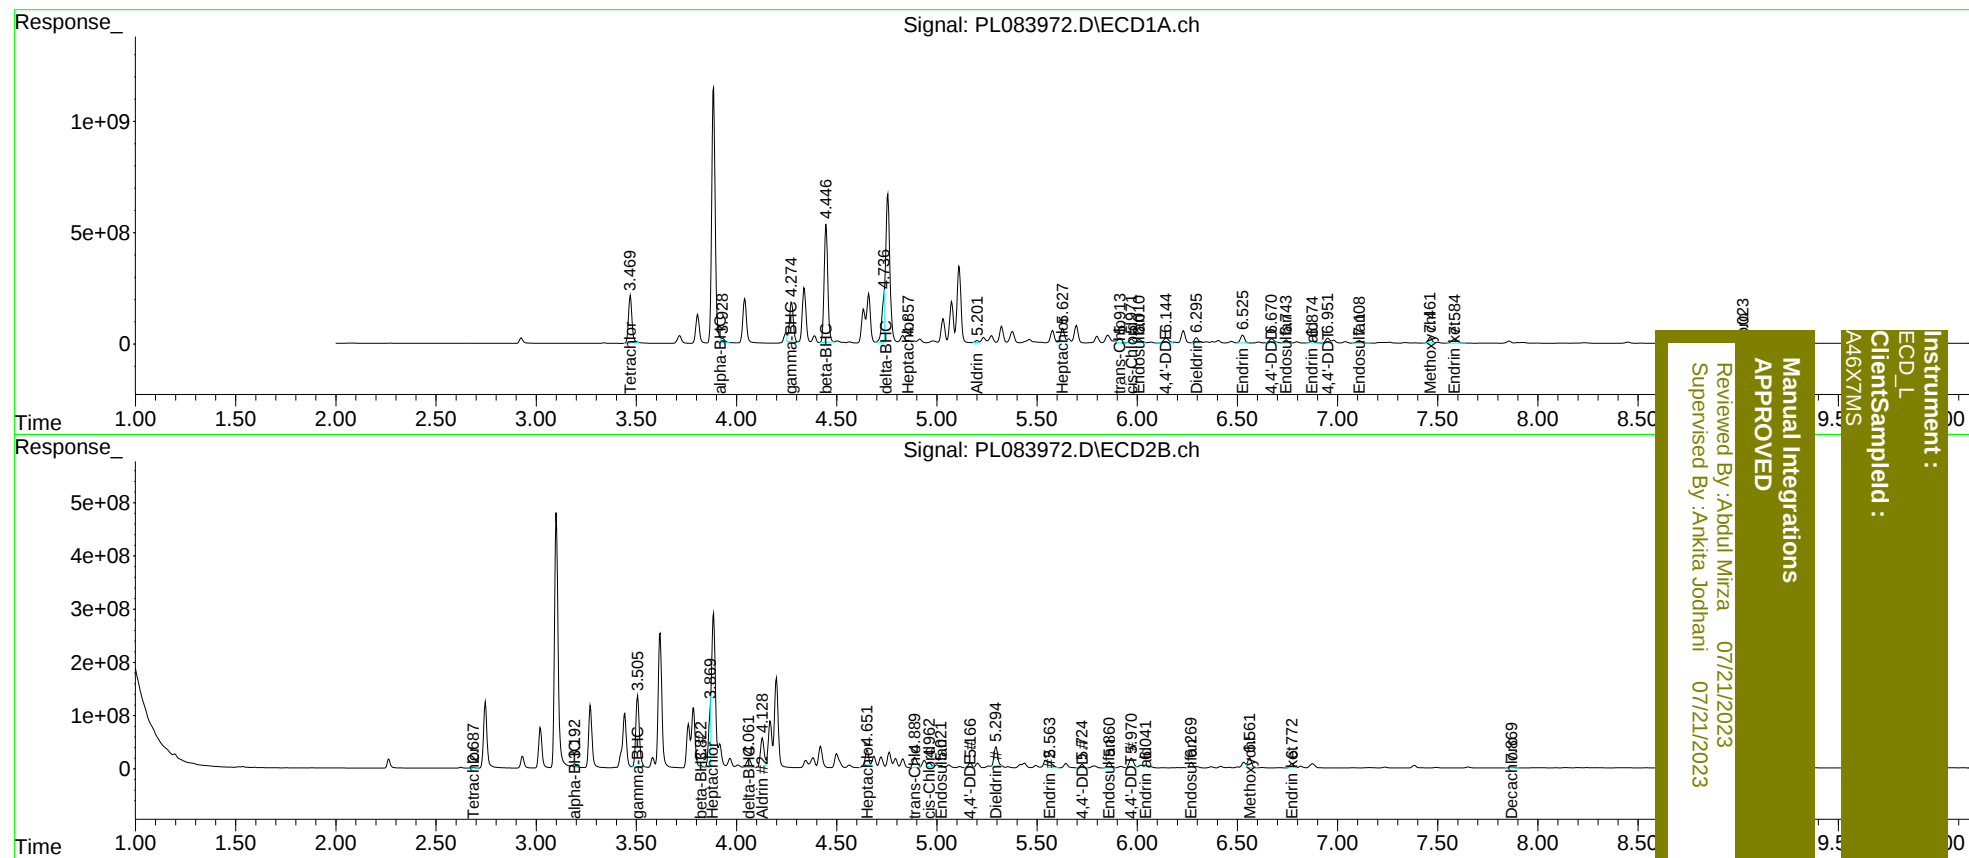

Instrument :
 ECD_L
 Client Sampled :
 A46XTMS
 Manual Integrations
 APPROVED
 Reviewed By: Abdul Miza 07/21/2023
 Supervised By: Ankita Jodhani 07/21/2023