

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
 Data File : PL083983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 16:03
 Operator : AR\AJ
 Sample : 03540-08MSD
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A4738MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/18/2023
 Supervised By : Ankita Jodhani 07/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 00:49:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 05:26:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	2.689	39835047	11844760	19.208	11.537 #
27)	SA Decachlor...	9.023	7.872	38674026	19657085	29.424m	17.761 #
Target Compounds							
2)	A alpha-BHC	3.934	3.194	116.1E6	56504454	38.440	39.097
3)	MA gamma-BHC...	4.271	3.523	240.2E6	64411893	85.127m	46.641m#
4)	MA Heptachlor	4.859	3.870	113.3E6	125.4E6	35.994m	95.194m#
5)	MB Aldrin	5.201	4.133	108.1E6	127.2E6	36.380m	97.433m#
6)	B beta-BHC	4.447	3.825	204.4E6	20553079	152.563	30.509m#
7)	B delta-BHC	4.719	4.061	114.3E6	123.7E6	40.375m	86.493 #
8)	B Heptachlo...	5.629	4.651	186.6E6	58320860	67.459m	46.592m#
9)	A Endosulfan I	6.018	5.023	79461395	35462797	32.923	31.321
10)	B trans-Chl...	5.888	4.903	132.0E6	66040030	50.459m	53.393m
11)	B cis-Chlor...	5.970	4.969	88375424	65117860	33.285	50.833m#
12)	B 4,4'-DDE	6.146	5.168	185.2E6	88397260	89.429m	73.266
13)	MA Dieldrin	6.294	5.291	178.6E6	137.9E6	73.557m	105.427m#
14)	MA Endrin	6.524	5.563	180.6E6	110.2E6	93.158m	96.788m
15)	B Endosulfa...	6.743	5.862	124.8E6	99982907	65.408m	87.647 #
16)	A 4,4'-DDD	6.667	5.726	123.3E6	78668192	83.788	81.220
17)	MA 4,4'-DDT	6.981	5.977	130.8E6	101.1E6	84.698m	97.023
18)	B Endrin al...	6.873	6.044	102.8E6	58401088	77.833m	71.170
19)	B Endosulfa...	7.111	6.269	118.8E6	82822942	67.695	75.072
20)	A Methoxychlor	7.464	6.562	306.5E6	218.1E6	402.006	389.067
21)	B Endrin ke...	7.596	6.774	186.1E6	96001968	109.689	73.261 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
Data File : PL083983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 16:03
Operator : AR\AJ
Sample : 03540-08MSD
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 00:49:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 05:26:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

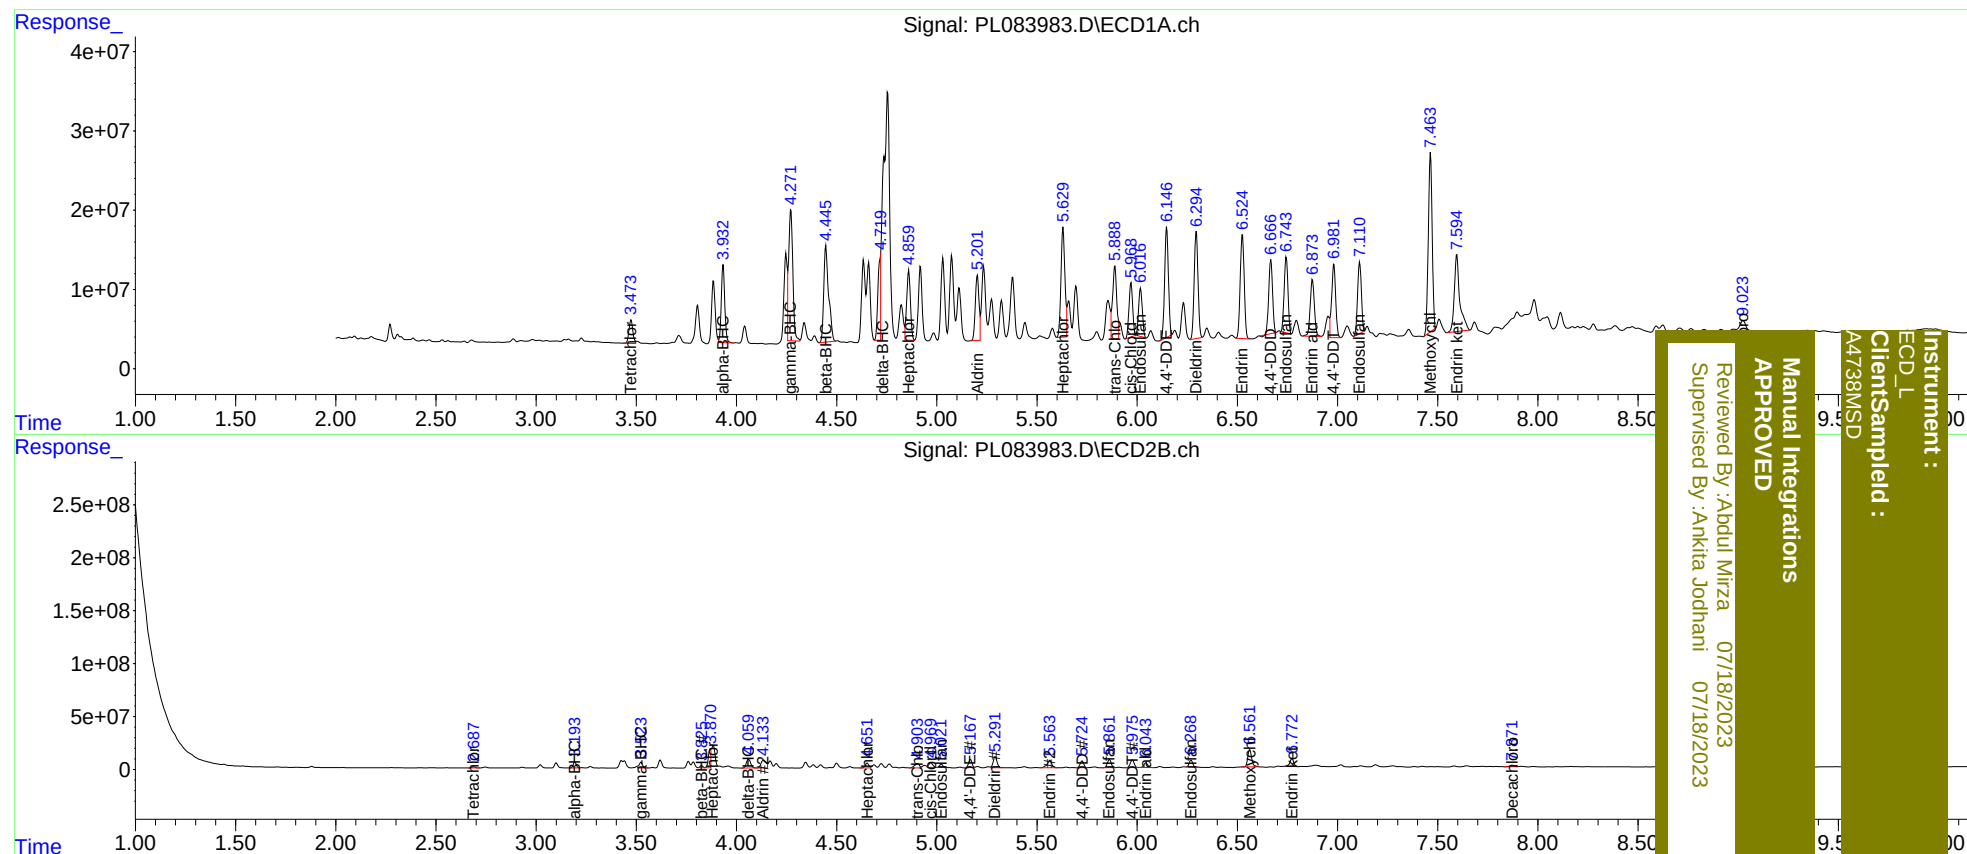

Reviewed By: Abdul Mirza 07/18/2023
Supervised By: Ankita Jodhani 07/18/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
Client/Sampled :
A4738MSD