

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
Data File : PL083963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 09:34
Operator : AR\AJ
Sample : 03501-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
A46X3

Manual IntegrationsAPPROVED



Reviewed By :Abdul Mirza 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023

07/21/2023
Supervised By :Ankita
Jodhani

07/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 00:43:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 05:26:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

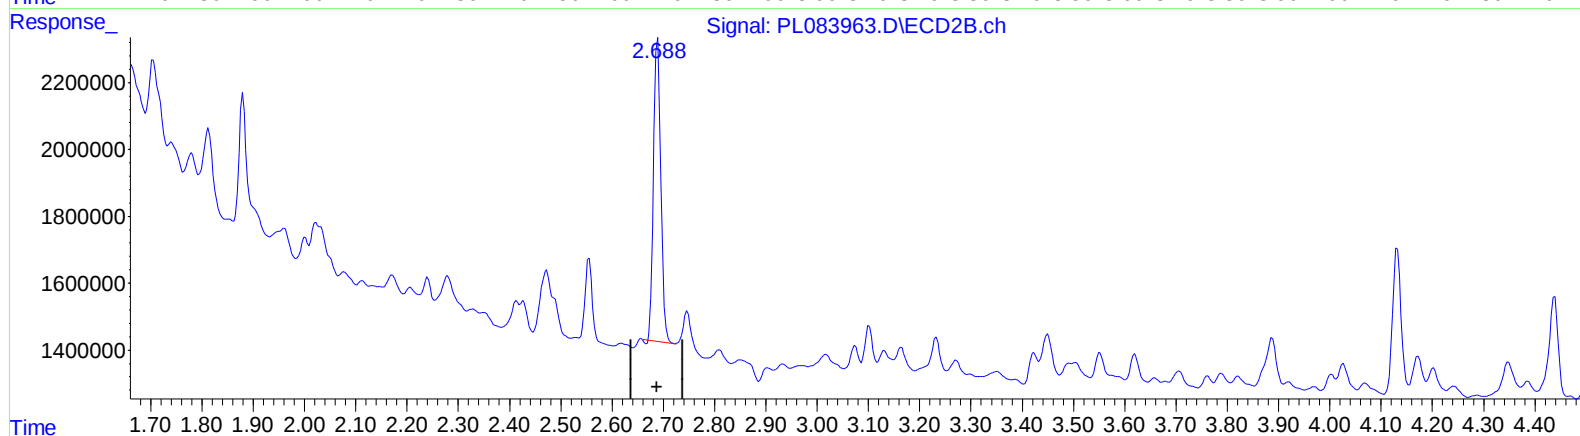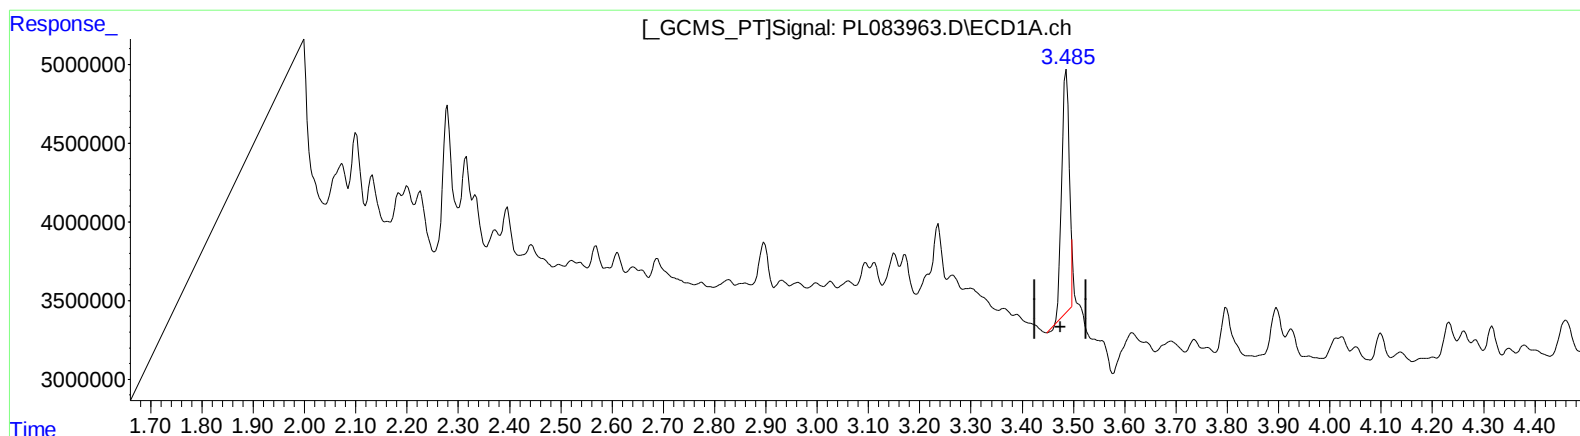

QEdit

(1) Tetrachloro-m-xylene (SA)

3.486min 7.492 ng/ml

response 15537745

(1) Tetrachloro-m-xylene #2 (SA)

2.689min 8.779 ng/ml

response 9013008

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
 Data File : PL083963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 09:34
 Operator : AR\AJ
 Sample : 03501-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A46X3

Manual IntegrationsAPPROVED


Reviewed By :Abdul Mirza 07/21/2023
 Supervised By :Ankita Jodhani 07/21/2023

07/21/2023
 Supervised By :Ankita
 Jodhani

07/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 00:43:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 05:26:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

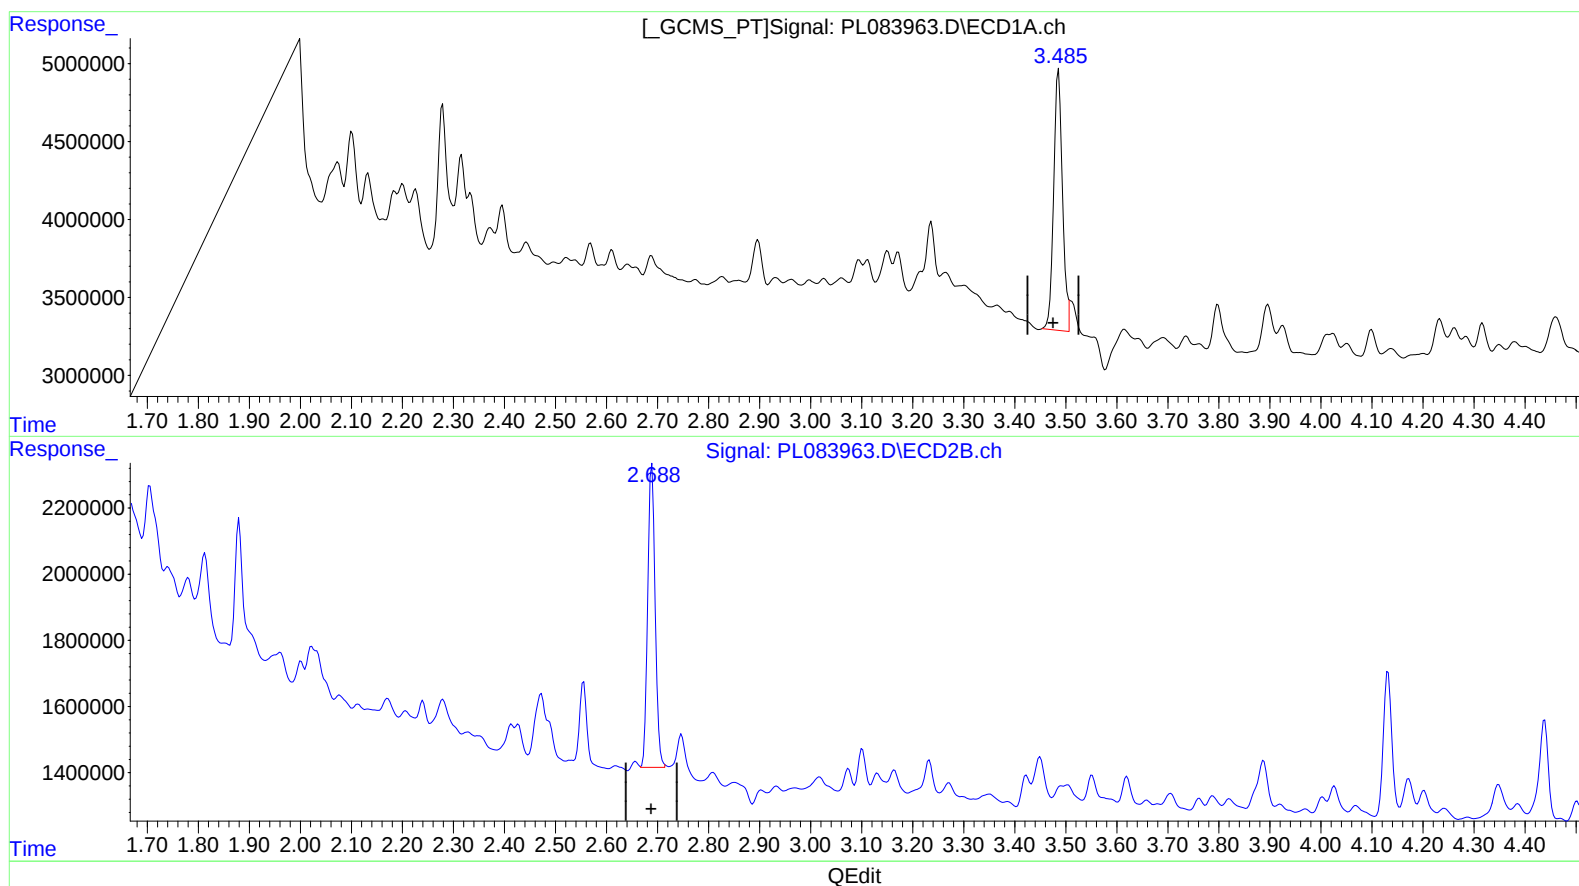

(1) Tetrachloro-m-xylene (SA)

3.485min 9.779 ng/ml m

response 20279264

(1) Tetrachloro-m-xylene #2 (SA)

2.688min 9.038 ng/ml m

response 9279048

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
Data File : PL083963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 09:34
Operator : AR\AJ
Sample : 03501-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
A46X3

Manual IntegrationsAPPROVED


Reviewed By :Abdul Mirza 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023

07/21/2023
Supervised By :Ankita
Jodhani

07/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 00:43:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 05:26:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

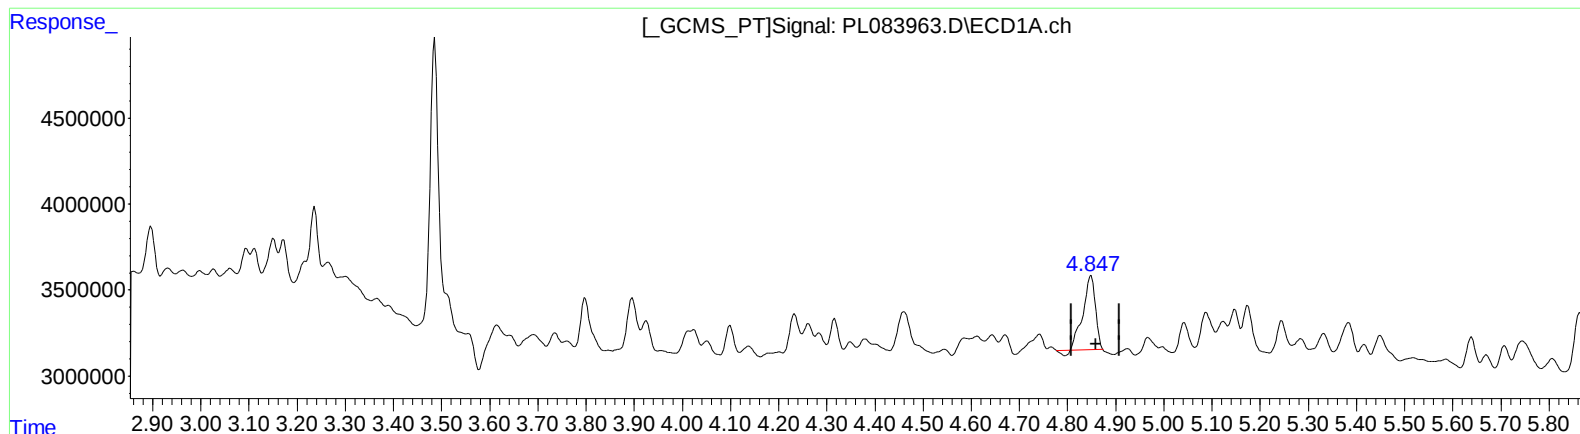

(4) Heptachlor (MA)

4.849min 2.402 ng/ml

response 7560088

(4) Heptachlor #2 (MA)

3.888min 1.501 ng/ml

response 1977179

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
Data File : PL083963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 09:34
Operator : AR\AJ
Sample : 03501-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
A46X3

Manual IntegrationsAPPROVED


Reviewed By :Abdul Mirza 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023

07/21/2023
Supervised By :Ankita
Jodhani

07/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 00:43:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 05:26:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

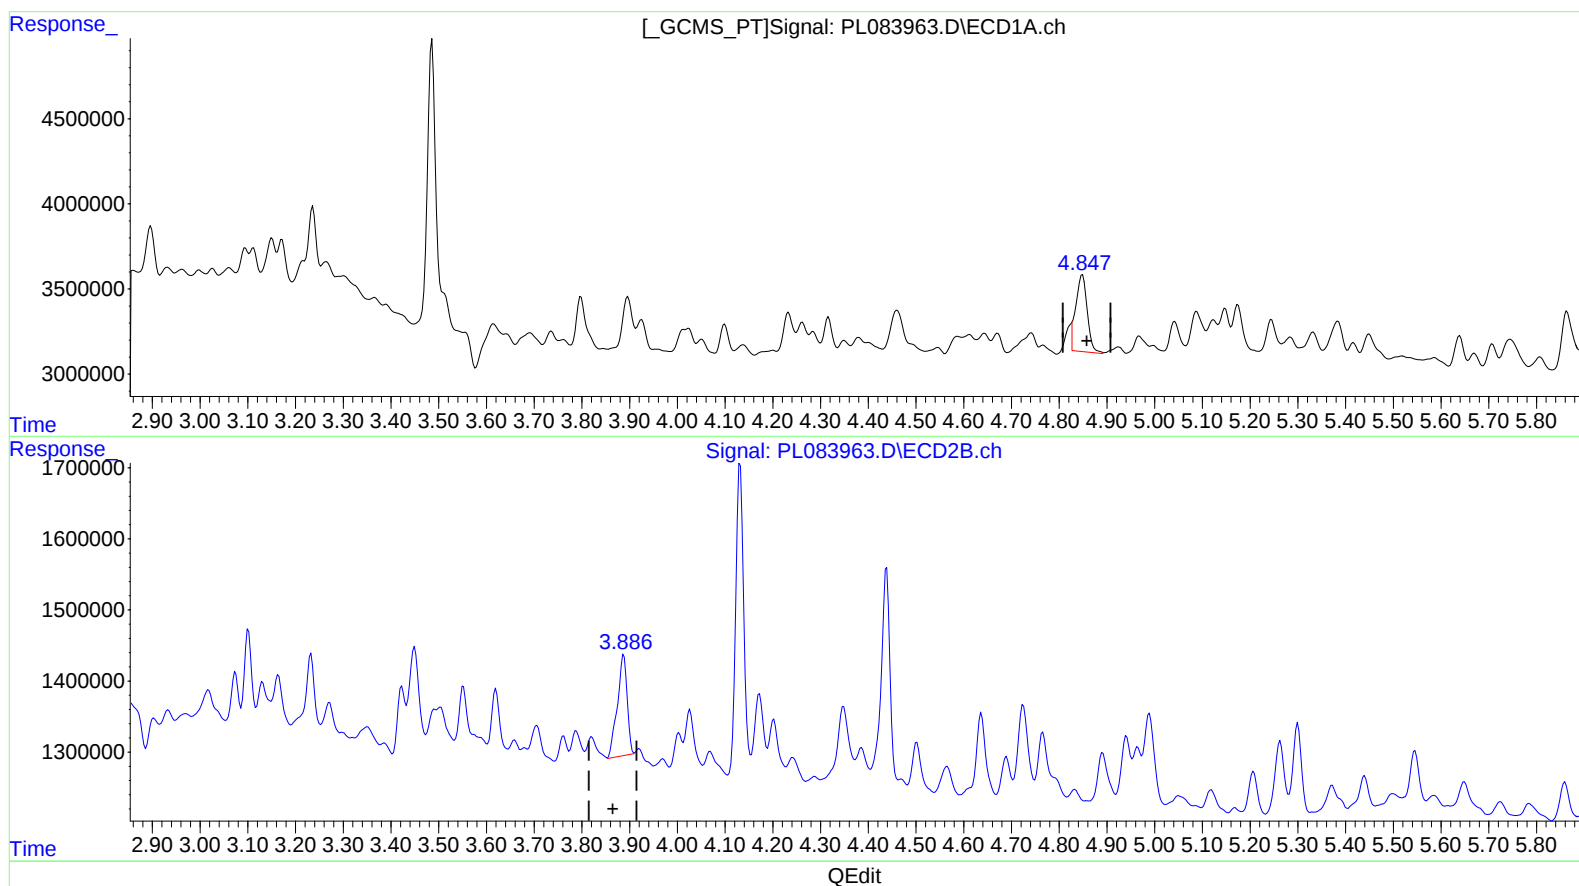

(4) Heptachlor (MA)

4.847min 2.364 ng/ml m
response 7439707

(4) Heptachlor #2 (MA)

3.886min 1.532 ng/ml m
response 2018917

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
Data File : PL083963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 09:34
Operator : AR\AJ
Sample : 03501-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
A46X3

Manual IntegrationsAPPROVED



Reviewed By :Abdul Mirza 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023

07/21/2023
Supervised By :Ankita
Jodhani

07/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 00:43:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 05:26:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

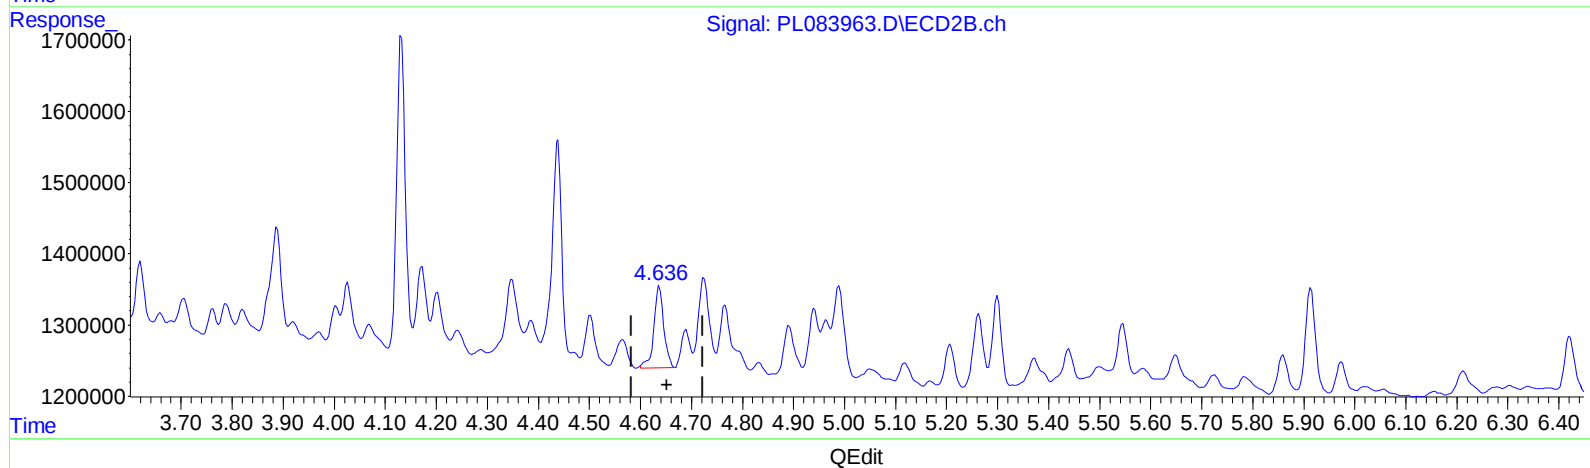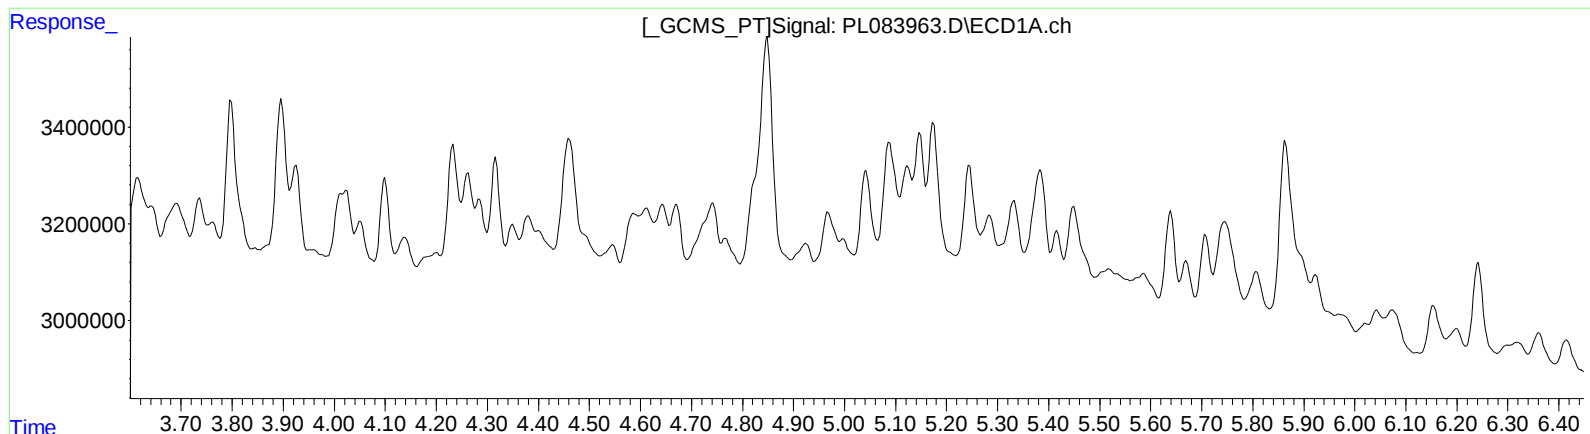

(8) Heptachlor epoxide (B)

0.000min 0.000 ng/ml

response 0

(8) Heptachlor epoxide #2 (B)

4.637min 1.233 ng/ml

response 1543406

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
 Data File : PL083963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 09:34
 Operator : AR\AJ
 Sample : 03501-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A46X3

Manual IntegrationsAPPROVED



Reviewed By :Abdul Mirza 07/21/2023
 Supervised By :Ankita Jodhani 07/21/2023

07/21/2023
 Supervised By :Ankita
 Jodhani

07/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 00:43:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 05:26:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

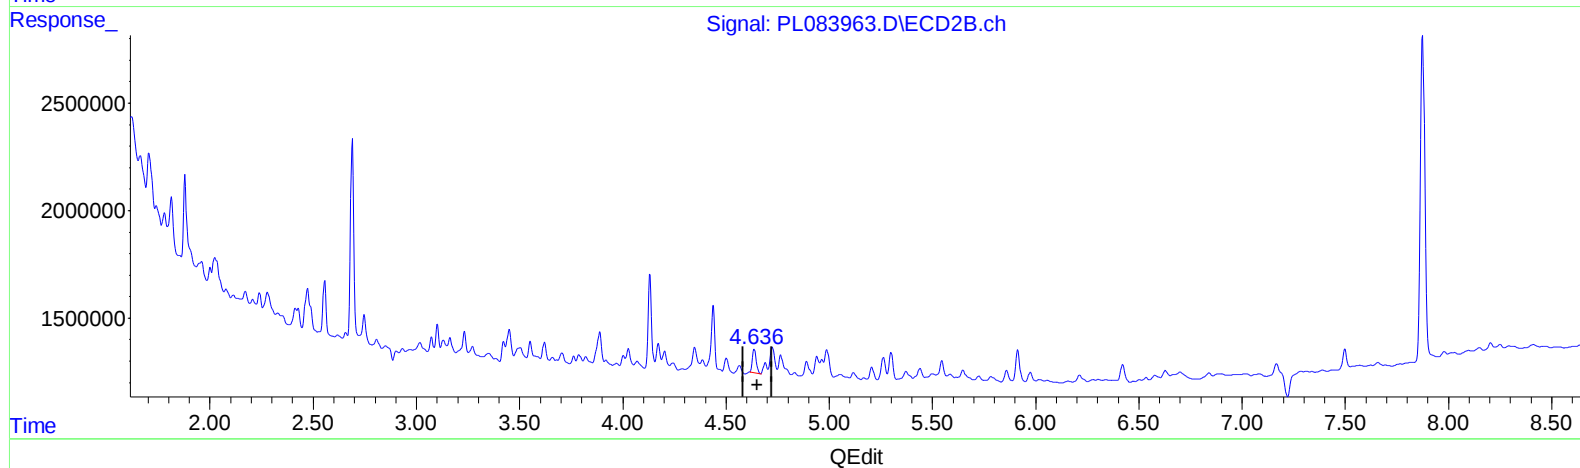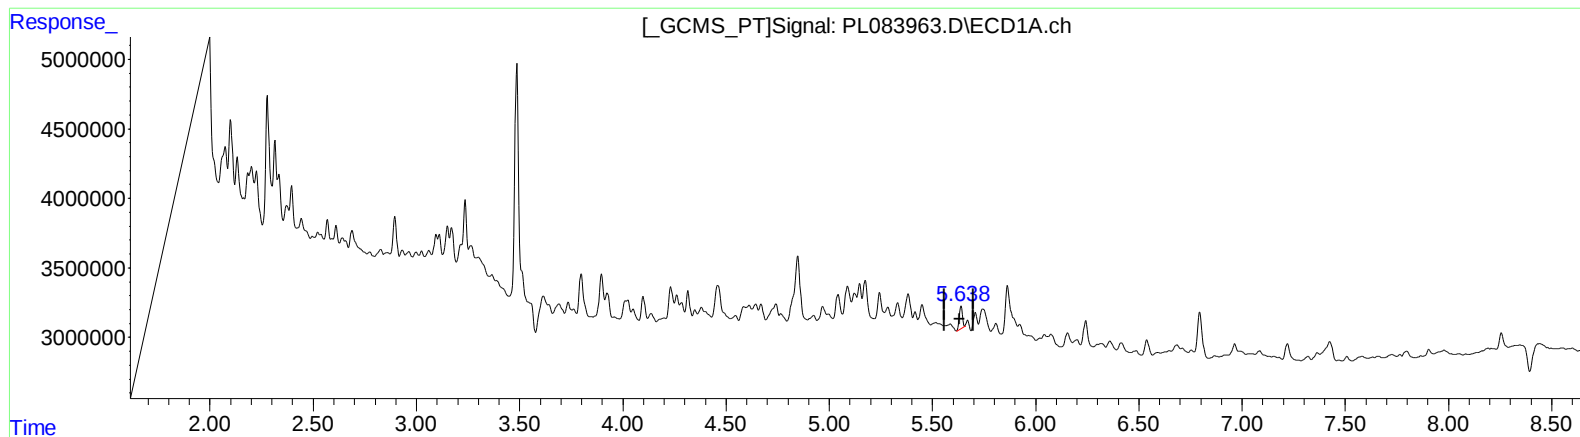

(8) Heptachlor epoxide (B)

5.638min 0.661 ng/ml m

response 1827800

(8) Heptachlor epoxide #2 (B)

4.636min 1.073 ng/ml m

response 1342822

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
Data File : PL083963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 09:34
Operator : AR\AJ
Sample : 03501-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
A46X3

Manual IntegrationsAPPROVED


Reviewed By :Abdul Mirza 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023

07/21/2023
Supervised By :Ankita
Jodhani

07/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 00:43:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 05:26:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

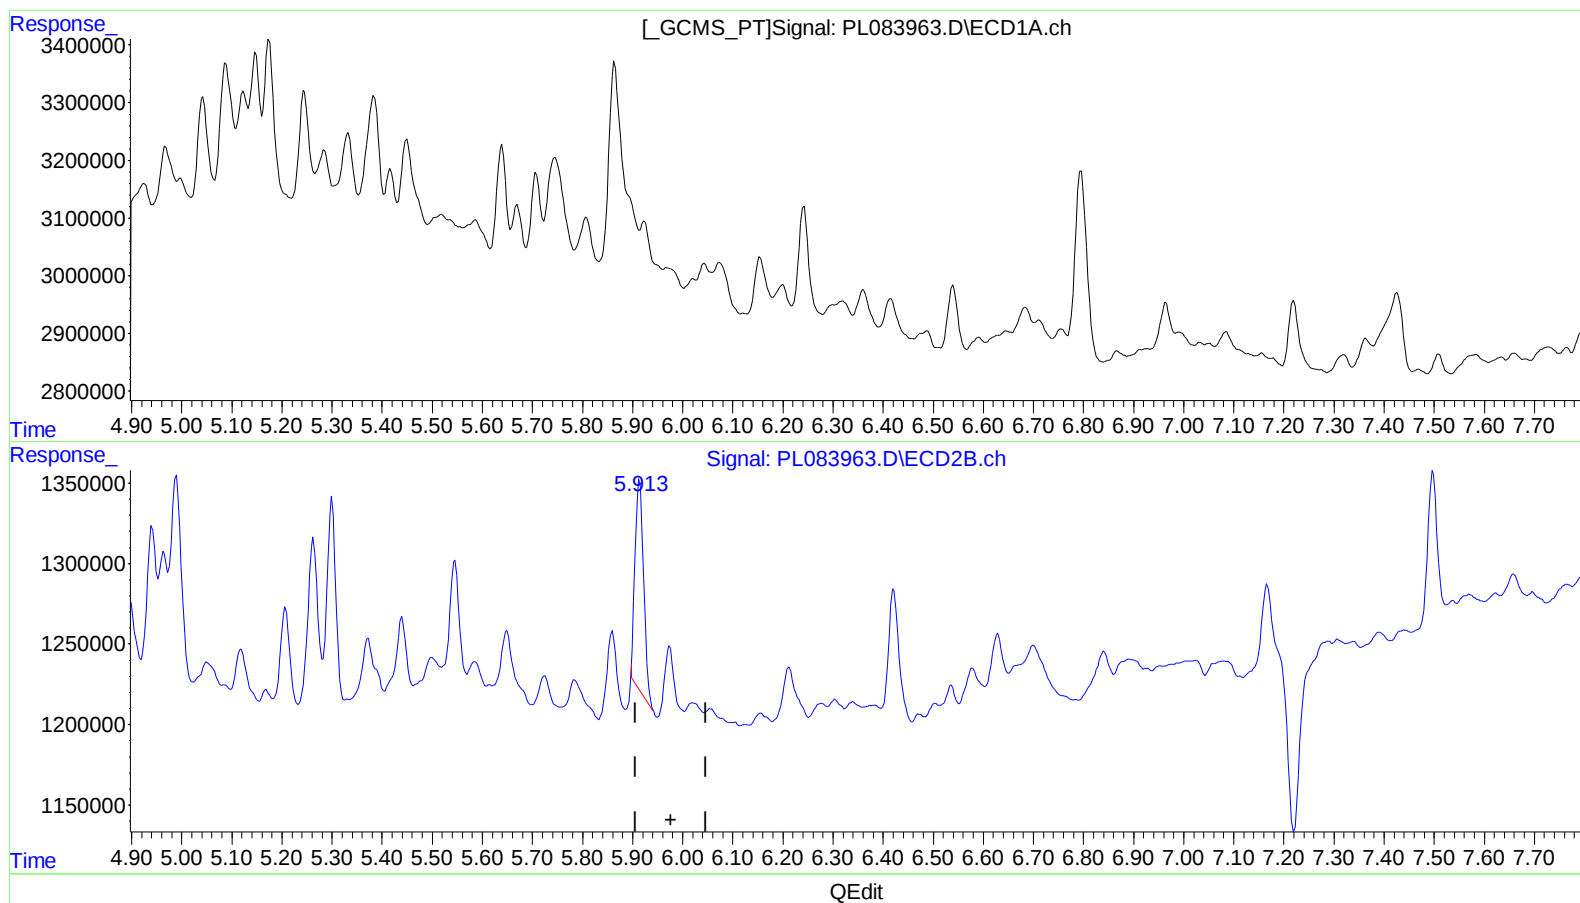

(17) 4,4'-DDT (MA)
0.000min 0.000 ng/ml
response 0

(17) 4,4'-DDT #2 (MA)
5.914min 1.483 ng/ml
response 1544456

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
Data File : PL083963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 09:34
Operator : AR\AJ
Sample : 03501-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
A46X3

Manual IntegrationsAPPROVED


Reviewed By :Abdul Mirza 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023

07/21/2023
Supervised By :Ankita
Jodhani

07/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 00:43:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 05:26:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

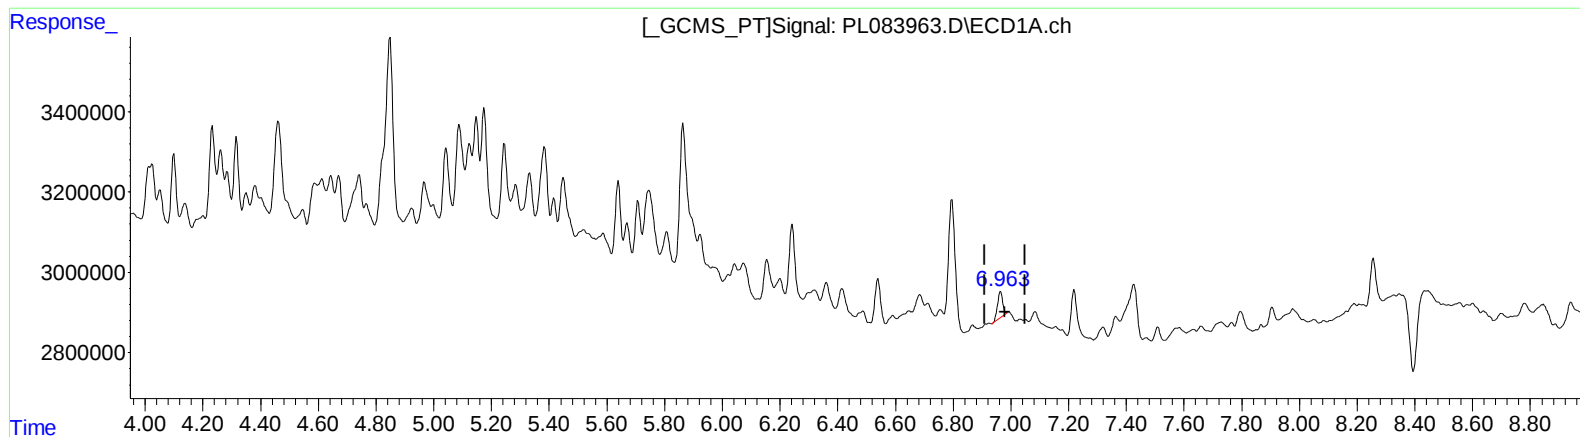

(17) 4,4'-DDT (MA)

6.963min 0.514 ng/ml m

response 793821

(17) 4,4'-DDT #2 (MA)

5.973min 0.509 ng/ml m

response 530422