

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
 Data File : PL083976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 14:22
 Operator : AR\AJ
 Sample : 03540-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A4728

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/18/2023
 Supervised By : Ankita Jodhani 07/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 00:47:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 05:26:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	2.688	15433522	8036739	7.442m	7.828
27)	SA Decachlor...	9.023	7.870	27282361	18958276	20.757m	17.129
Target Compounds							
3)	MA gamma-BHC...	4.273	3.522	31687823	3521356	11.232m	2.550m#
10)	B trans-Chl...	5.912	4.887	68925675	48625959	26.356m	39.314m#
17)	MA 4,4'-DDT	6.953	5.970	44179004	32667522	28.605	31.360

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071723\
Data File : PL083976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 14:22
Operator : AR\AJ
Sample : 03540-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 00:47:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 05:26:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

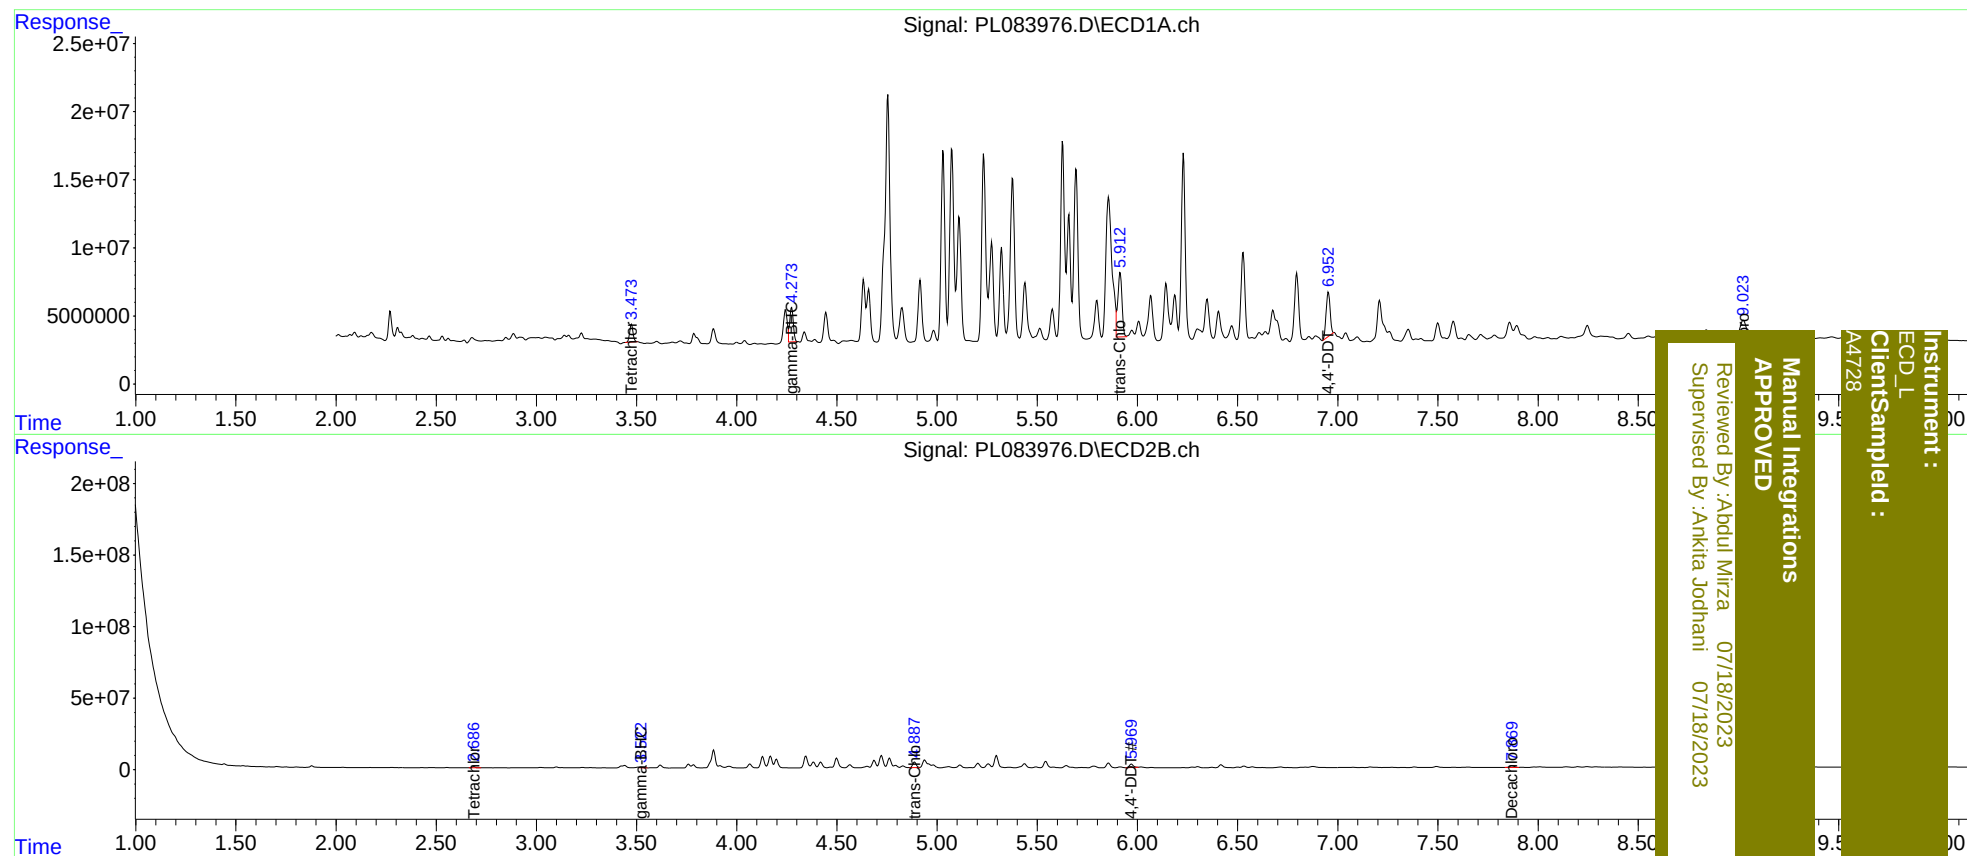

Reviewed By: Abdul Mirza 07/18/2023
Supervised By: Ankita Jodhani 07/18/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
A4728