

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071724\
 Data File : PL090557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2024 17:53
 Operator : AR\AJ
 Sample : P3257-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-W-03-202407

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/18/2024
 Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 01:24:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 15 14:16:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.788	35547608	39035498	17.072m	23.194m#
28) SA Decachlor...	9.058	7.931	29740961	34234788	22.381	23.479

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071724\
Data File : PL090557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2024 17:53
Operator : AR\AJ
Sample : P3257-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-W-03-202407


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/18/2024
Supervised By : Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 01:24:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 14:16:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

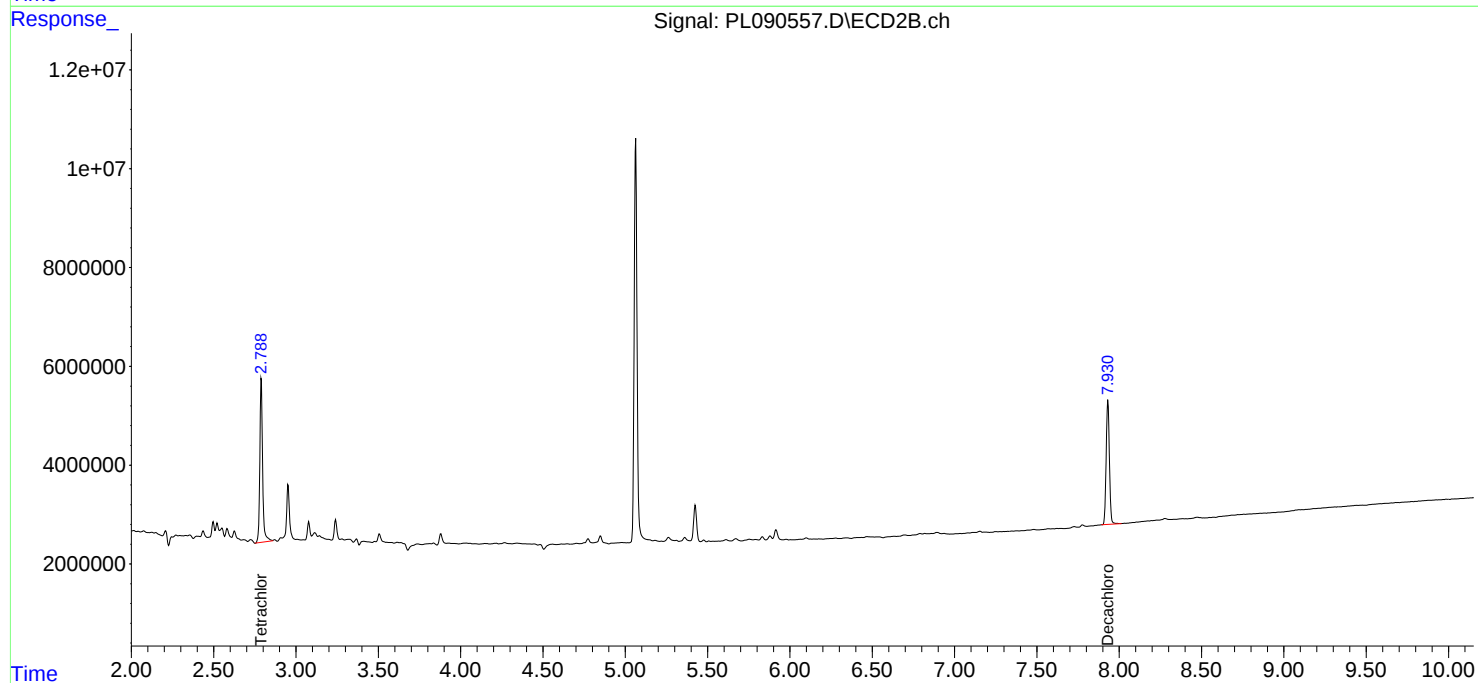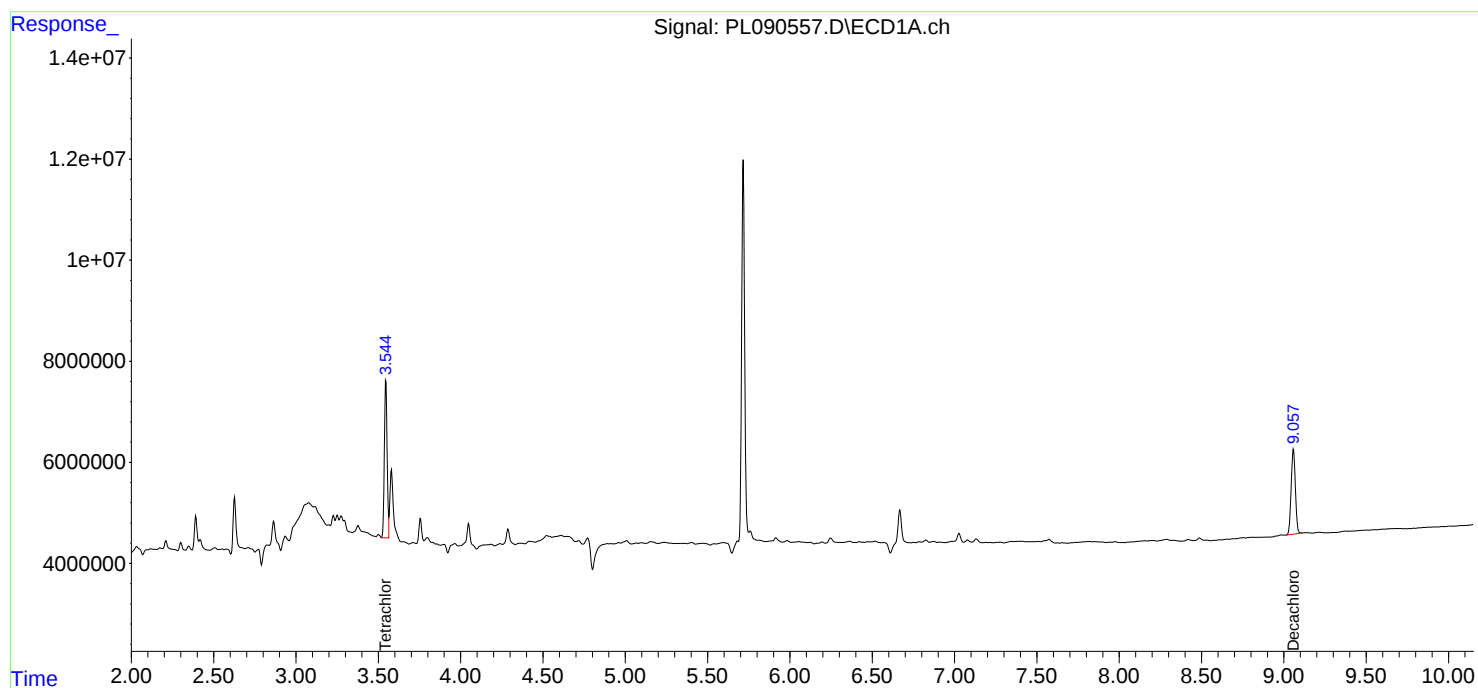

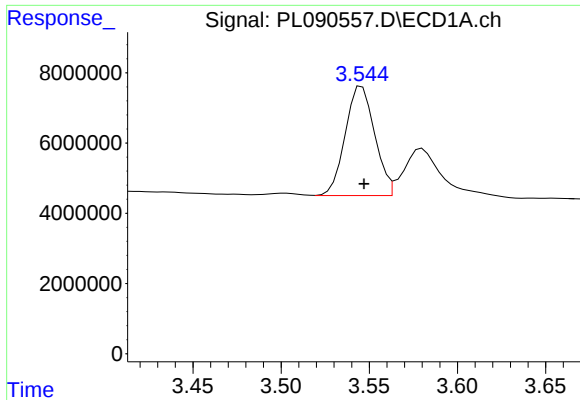


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.003 min
Response: 35547608
Conc: 17.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-W-03-202407


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/18/2024
Supervised By :Ankita Jodhani 07/19/2024

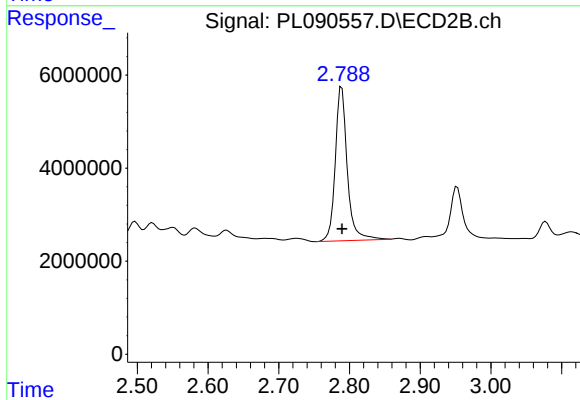


#1 Tetrachloro-m-xylene

R.T.: 2.788 min
Delta R.T.: -0.002 min
Response: 39035498
Conc: 23.19 ng/ml m

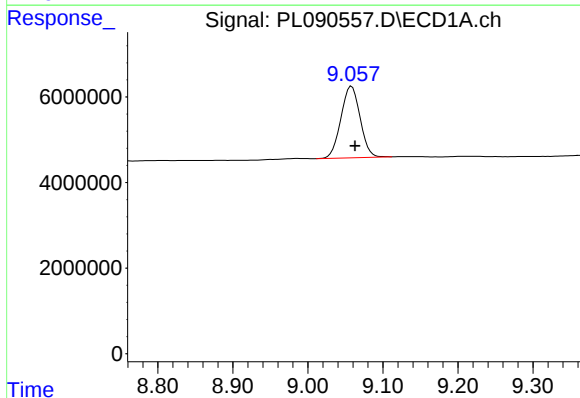

#28 Decachlorobiphenyl

R.T.: 9.058 min
Delta R.T.: -0.004 min
Response: 29740961
Conc: 22.38 ng/ml

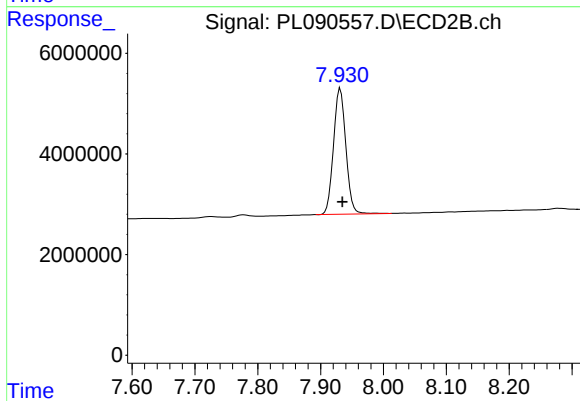

#28 Decachlorobiphenyl

R.T.: 7.931 min
Delta R.T.: -0.003 min
Response: 34234788
Conc: 23.48 ng/ml