

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071725\
 Data File : PL096438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2025 19:39
 Operator : AR\AJ
 Sample : Q2622-01 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2819

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 02:36:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.829	0	12109317	N.D.	2.098 #
28)	SA Decachlor...	0.000	7.994	0	10274528	N.D.	2.060 #
Target Compounds							
9)	A Endosulfan I	0.000	5.191f	0	17747279	N.D.	2.474 #
18)	B Endrin al...	0.000	6.177	0	9956521	N.D.	2.235 #
20)	A Methoxychlor	0.000	6.708f	0	2739899	N.D.	0.902 #
27)	Chlordane-5	0.000	6.046f	0	5155310	N.D.	18.188 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071725\
Data File : PL096438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2025 19:39
Operator : AR\AJ
Sample : Q2622-01 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
2819

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 02:36:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

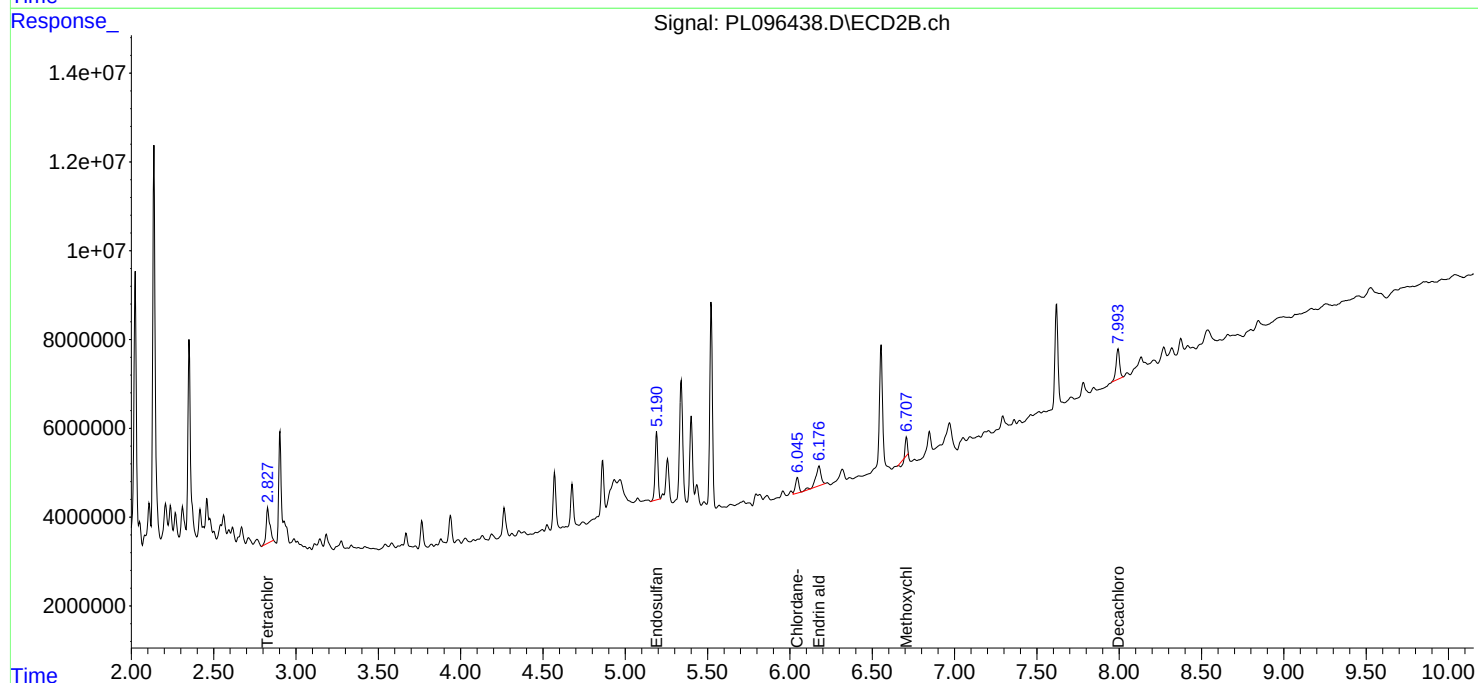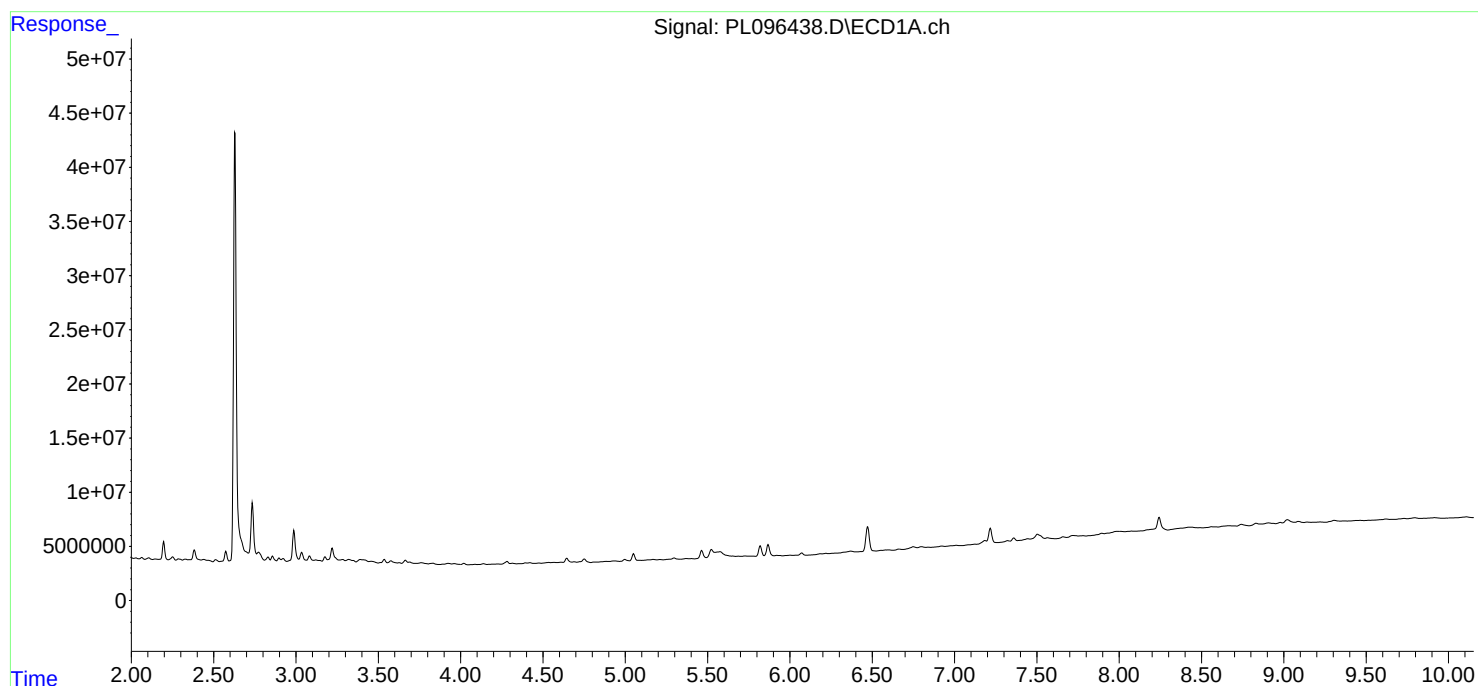


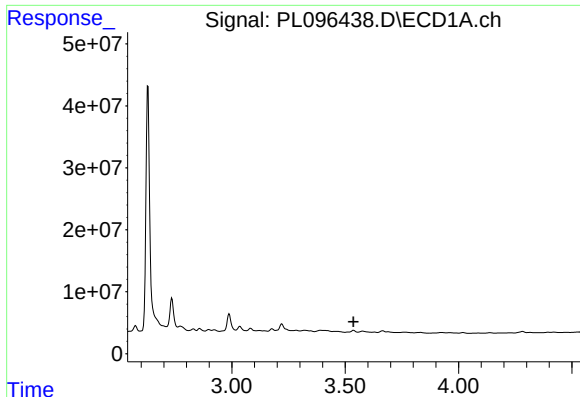

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2819

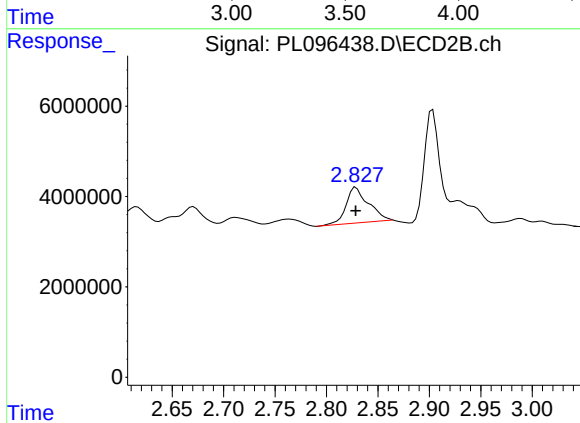


#1 Tetrachloro-m-xylene

R.T.: 2.829 min
Delta R.T.: 0.000 min
Response: 12109317
Conc: 2.10 ng/ml

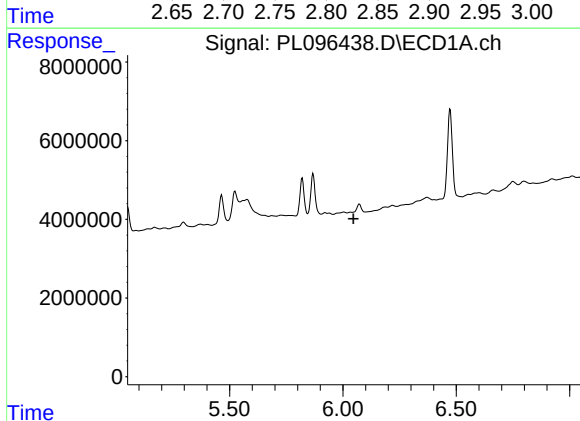


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.047 min
Response: 0
Conc: N.D.

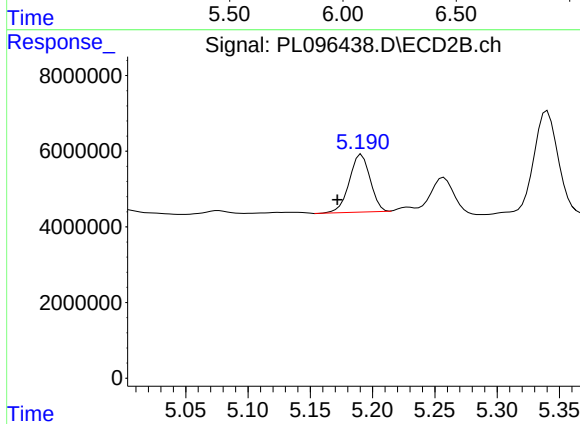

#9 Endosulfan I


R.T.: 5.191 min
Delta R.T.: 0.020 min
Response: 17747279
Conc: 2.47 ng/ml

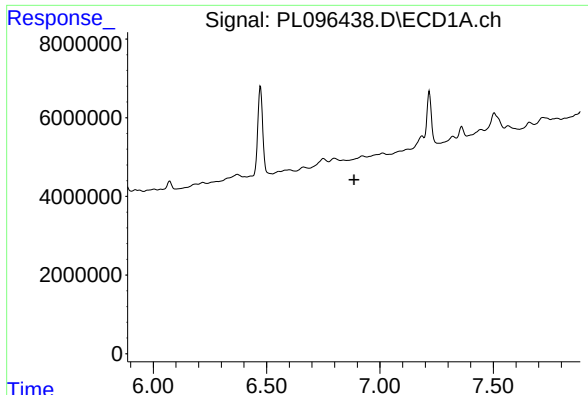

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2819

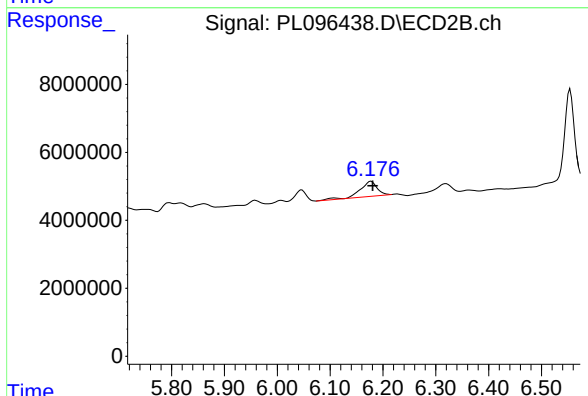


#18 Endrin aldehyde

R.T.: 6.177 min
Delta R.T.: -0.003 min
Response: 9956521
Conc: 2.24 ng/ml

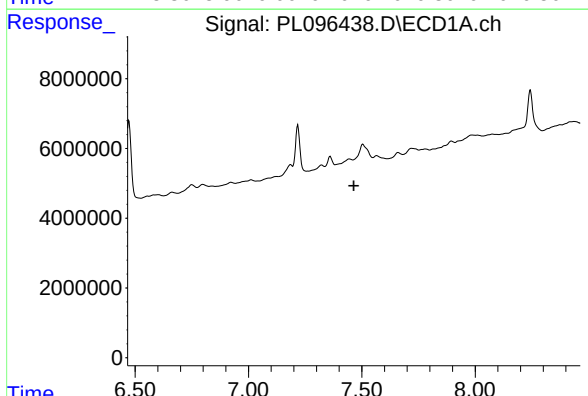


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.465 min
Response: 0
Conc: N.D.

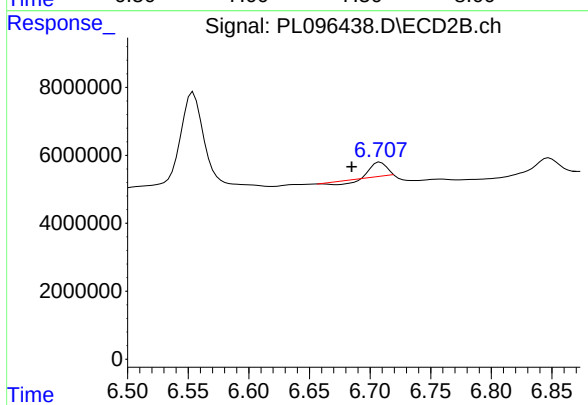

#20 Methoxychlor


R.T.: 6.708 min
Delta R.T.: 0.024 min
Response: 2739899
Conc: 0.90 ng/ml

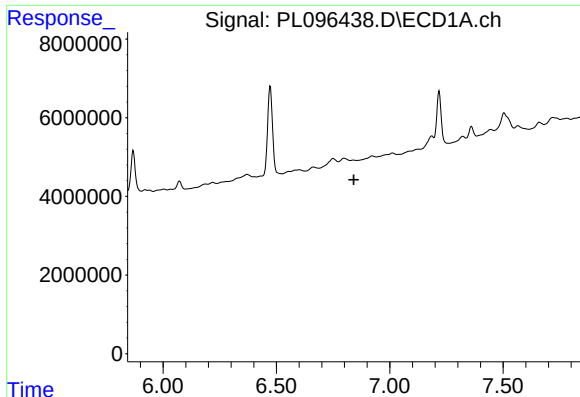

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.841 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2819

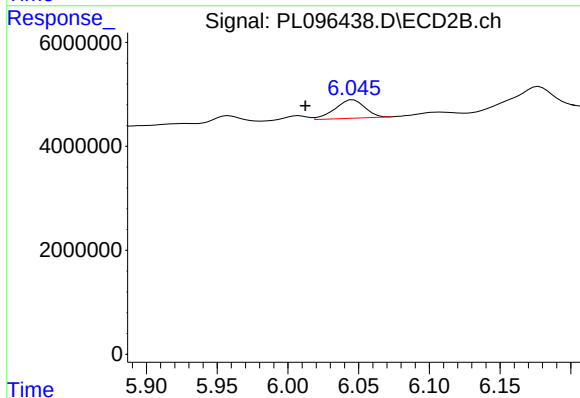


#27 Chlordane-5

R.T.: 6.046 min
Delta R.T.: 0.034 min
Response: 5155310
Conc: 18.19 ng/ml

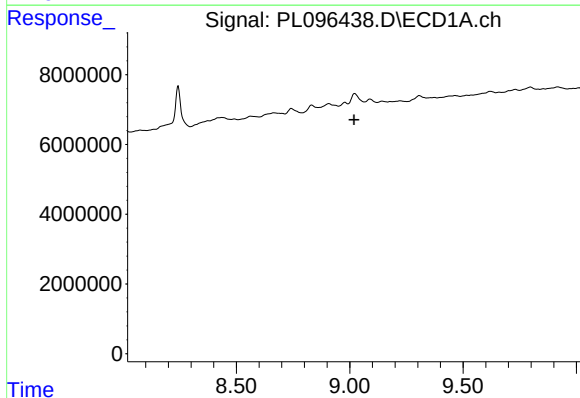

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.020 min
Response: 0
Conc: N.D.

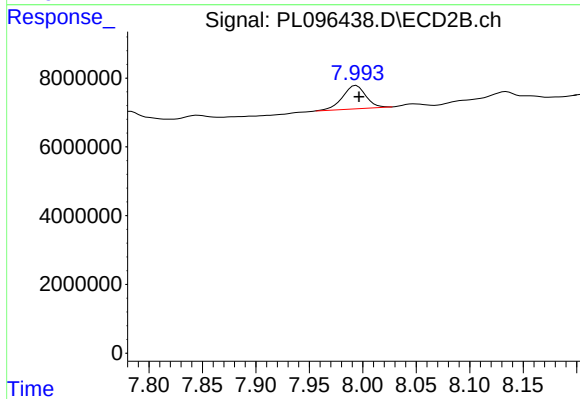

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: -0.003 min
Response: 10274528
Conc: 2.06 ng/ml