

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
 Data File : PL038220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2018 19:02
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:52:27 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.930	139.5E6	55853259	18.735	21.278
28)	SA Decachlor...	8.000	8.939	144.6E6	53707954	19.065	21.971
Target Compounds							
6)	B beta-BHC	4.245f	0.000	14221561	0	3.013	N.D. #
7)	B delta-BHC	0.000	4.960	0	4243111	N.D.	1.279 #
15)	B Endosulfa...	6.035f	0.000	22827464	0	2.879	N.D. #
16)	A 4,4'-DDD	0.000	6.678f	0	7598014	N.D.	3.550 #
23)	Chlordane-1	0.000	4.960	0	4243111	N.D.	36.615 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
Data File : PL038220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2018 19:02
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:52:27 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

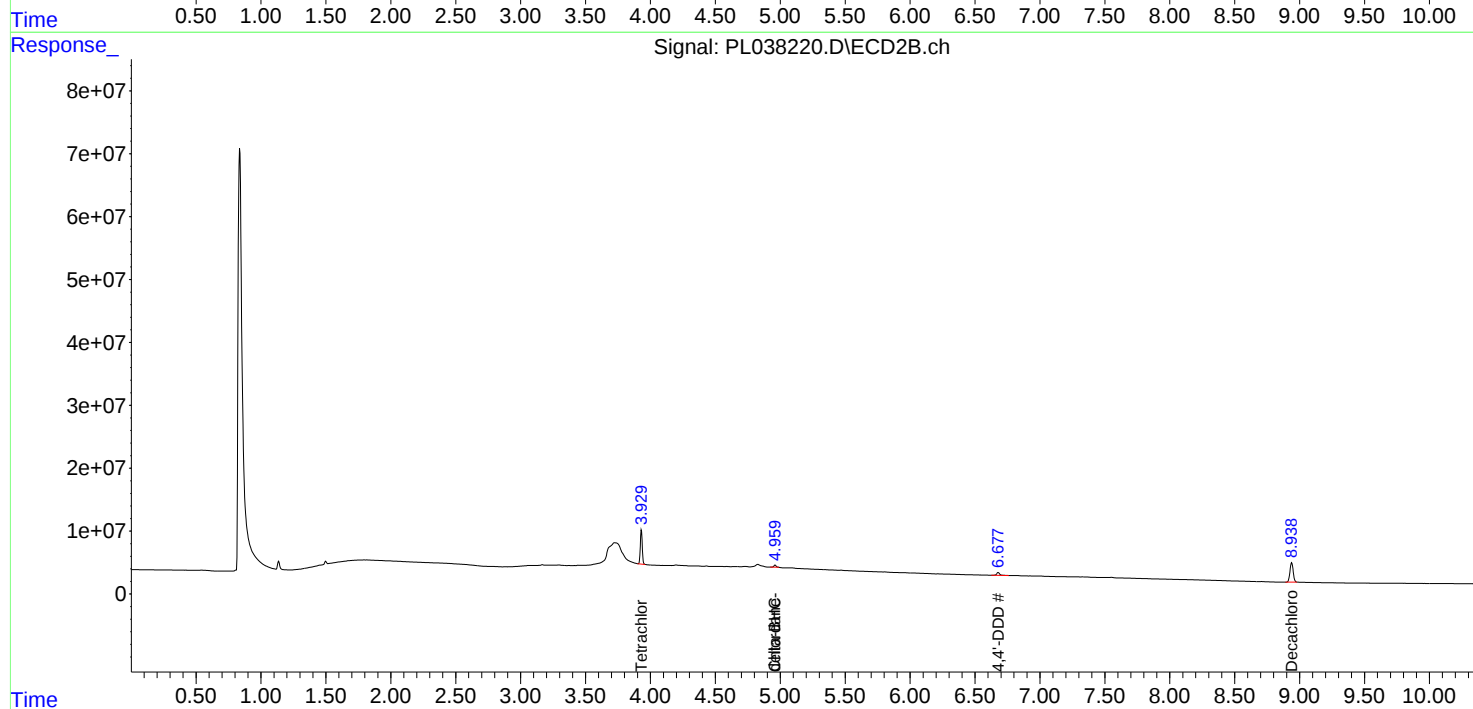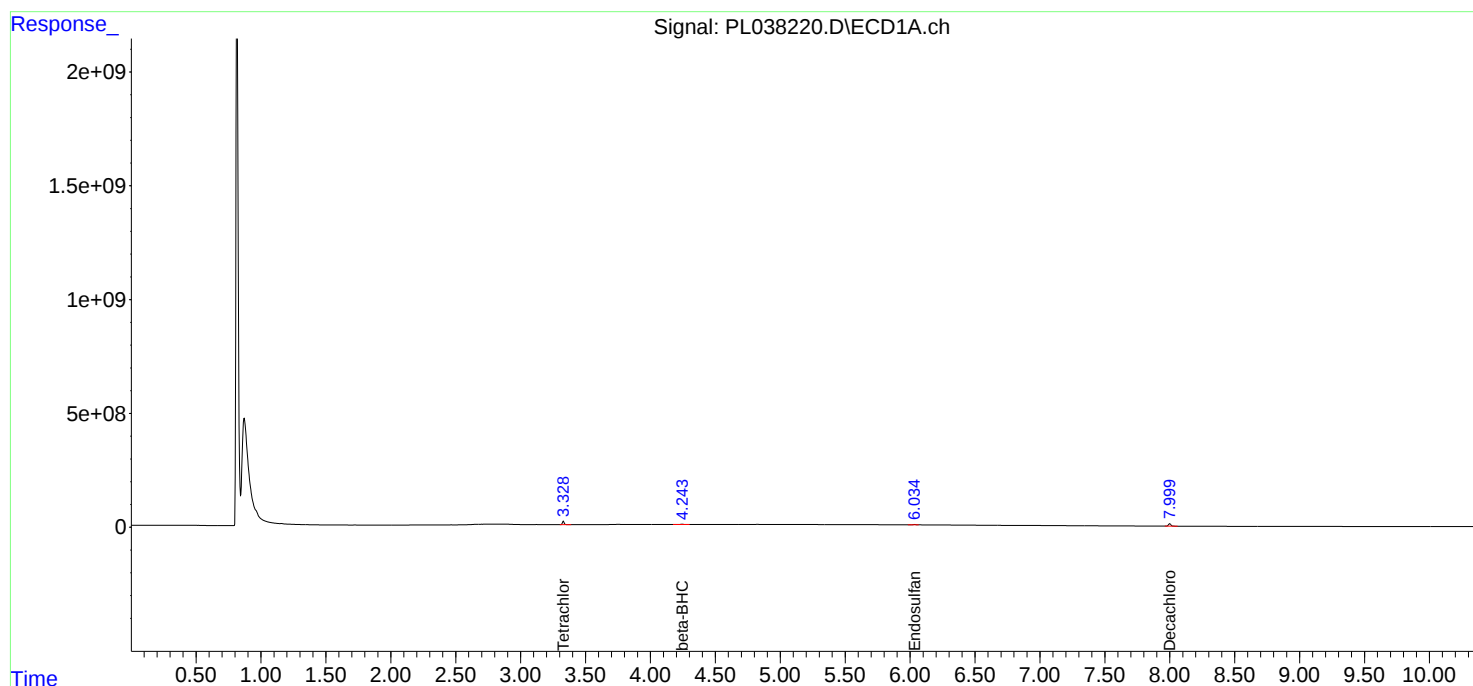


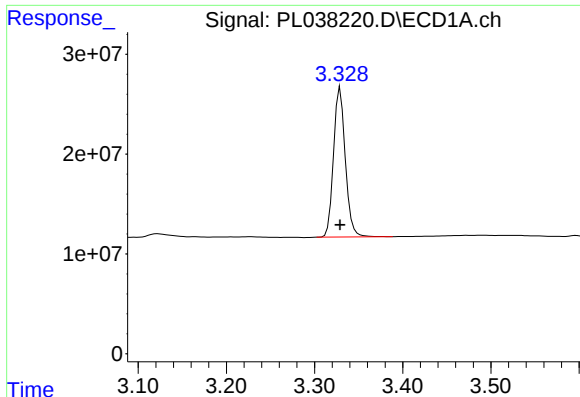

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 139509094
Conc: 18.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

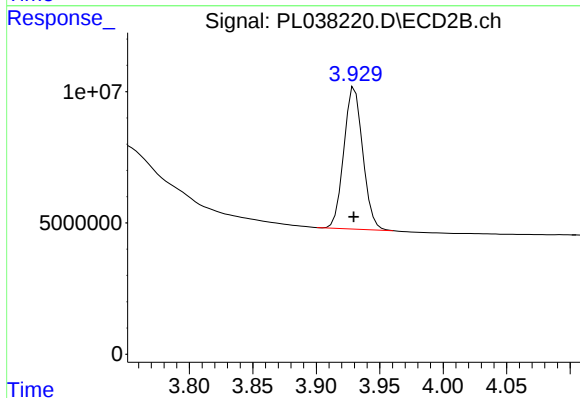


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 55853259
Conc: 21.28 ng/ml

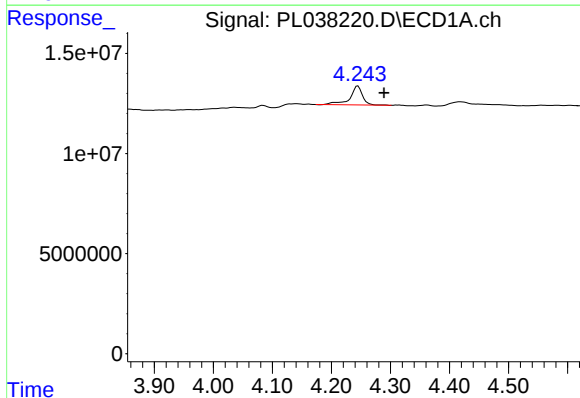


#6 beta-BHC

R.T.: 4.245 min
Delta R.T.: -0.044 min
Response: 14221561
Conc: 3.01 ng/ml

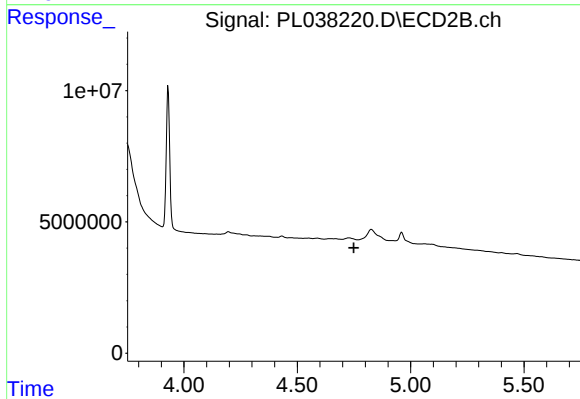

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

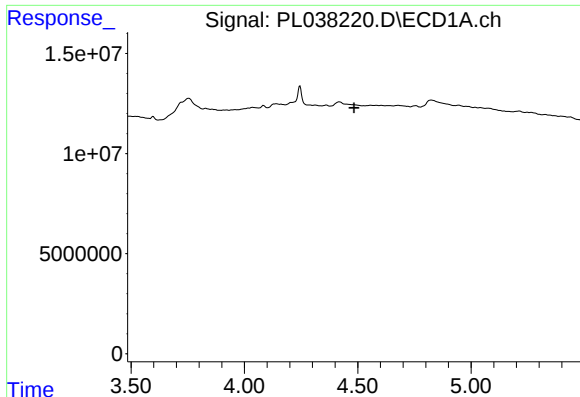

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

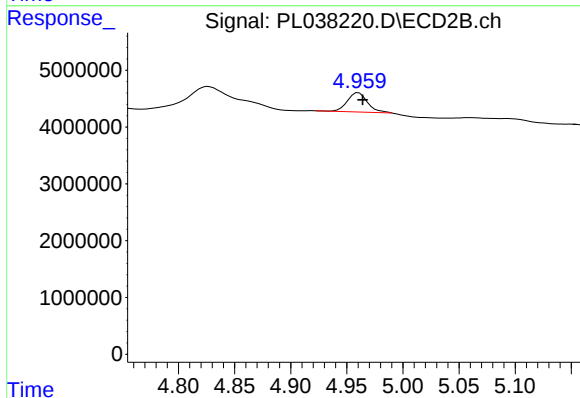


#7 delta-BHC

R.T.: 4.960 min
Delta R.T.: -0.004 min
Response: 4243111
Conc: 1.28 ng/ml

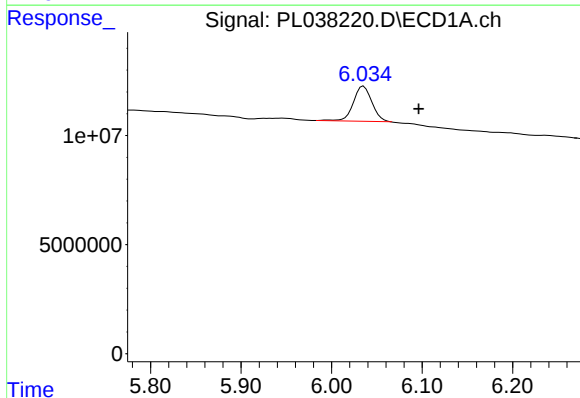


#15 Endosulfan II

R.T.: 6.035 min
Delta R.T.: -0.061 min
Response: 22827464
Conc: 2.88 ng/ml

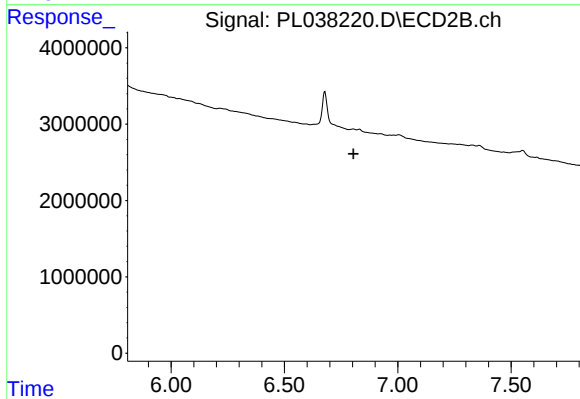

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.805 min
Response: 0
Conc: N.D.

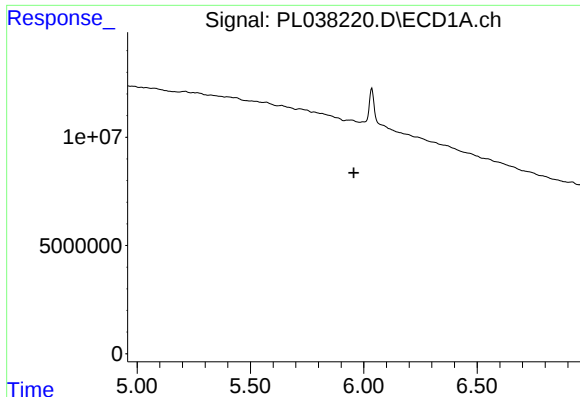

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

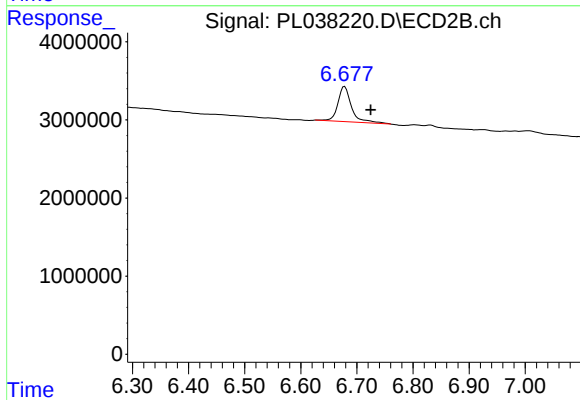


#16 4,4'-DDD

R.T.: 6.678 min
Delta R.T.: -0.046 min
Response: 7598014
Conc: 3.55 ng/ml

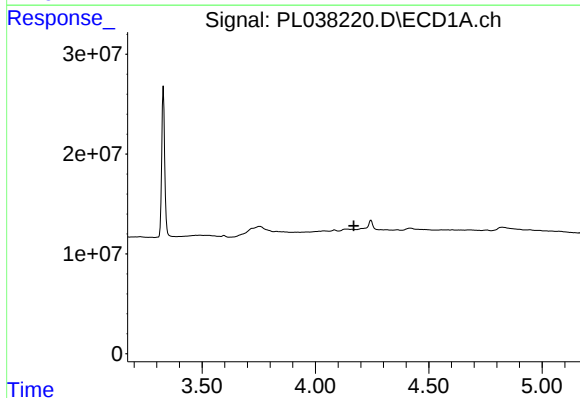


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.169 min
Response: 0
Conc: N.D.

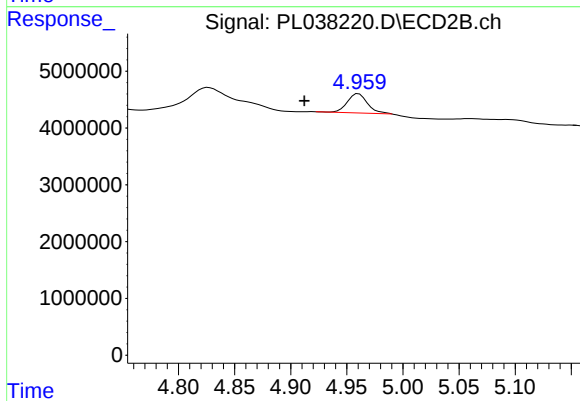

#23 Chlordane-1

R.T.: 4.960 min
Delta R.T.: 0.048 min
Response: 4243111
Conc: 36.61 ng/ml

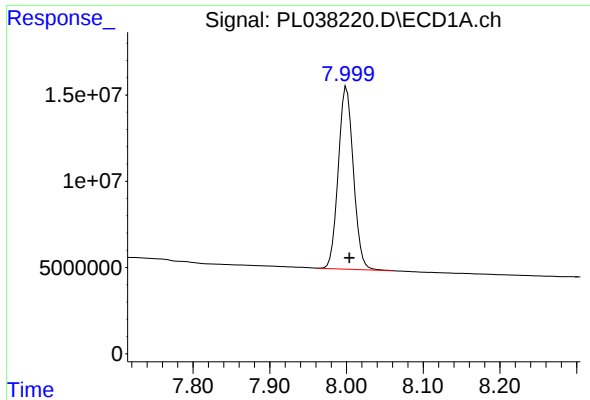

#28 Decachlorobiphenyl


R.T.: 8.000 min

Delta R.T.: -0.003 min

Response: 144623999

Conc: 19.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

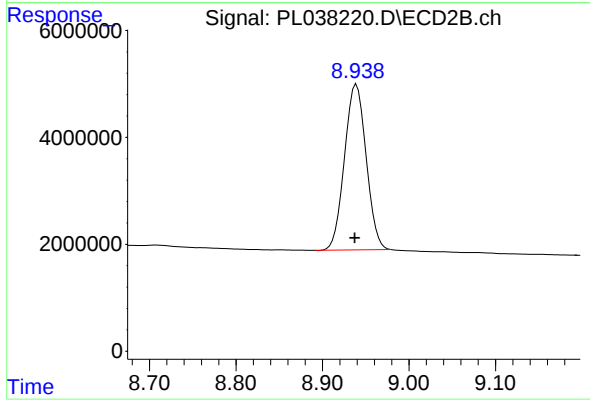

#28 Decachlorobiphenyl

R.T.: 8.939 min

Delta R.T.: 0.002 min

Response: 53707954

Conc: 21.97 ng/ml