

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
 Data File : PL038230.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2018 21:23
 Operator : AJ\SJ
 Sample : J4016-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:54:00 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.930	141.5E6	57060062	19.001	21.738
28)	SA Decachlor...	8.000	8.939	133.2E6	48945878	17.565	20.023
Target Compounds							
3)	MA gamma-BHC...	0.000	4.552f	0	2664964	N.D.	0.738 #
6)	B beta-BHC	4.245f	0.000	26164638	0	5.543	N.D. #
7)	B delta-BHC	0.000	4.959	0	6206634	N.D.	1.871 #
12)	B 4,4'-DDE	5.398f	0.000	6060450	0	0.632	N.D. #
15)	B Endosulfa...	6.035f	0.000	21896588	0	2.761	N.D. #
16)	A 4,4'-DDD	0.000	6.679f	0	8334621	N.D.	3.894 #
20)	A Methoxychlor	6.673f	0.000	6917140	0	1.798	N.D. #
23)	Chlordane-1	4.102	4.959	37646246	6206634	108.725	53.559 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
Data File : PL038230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2018 21:23
Operator : AJ\SJ
Sample : J4016-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:54:00 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

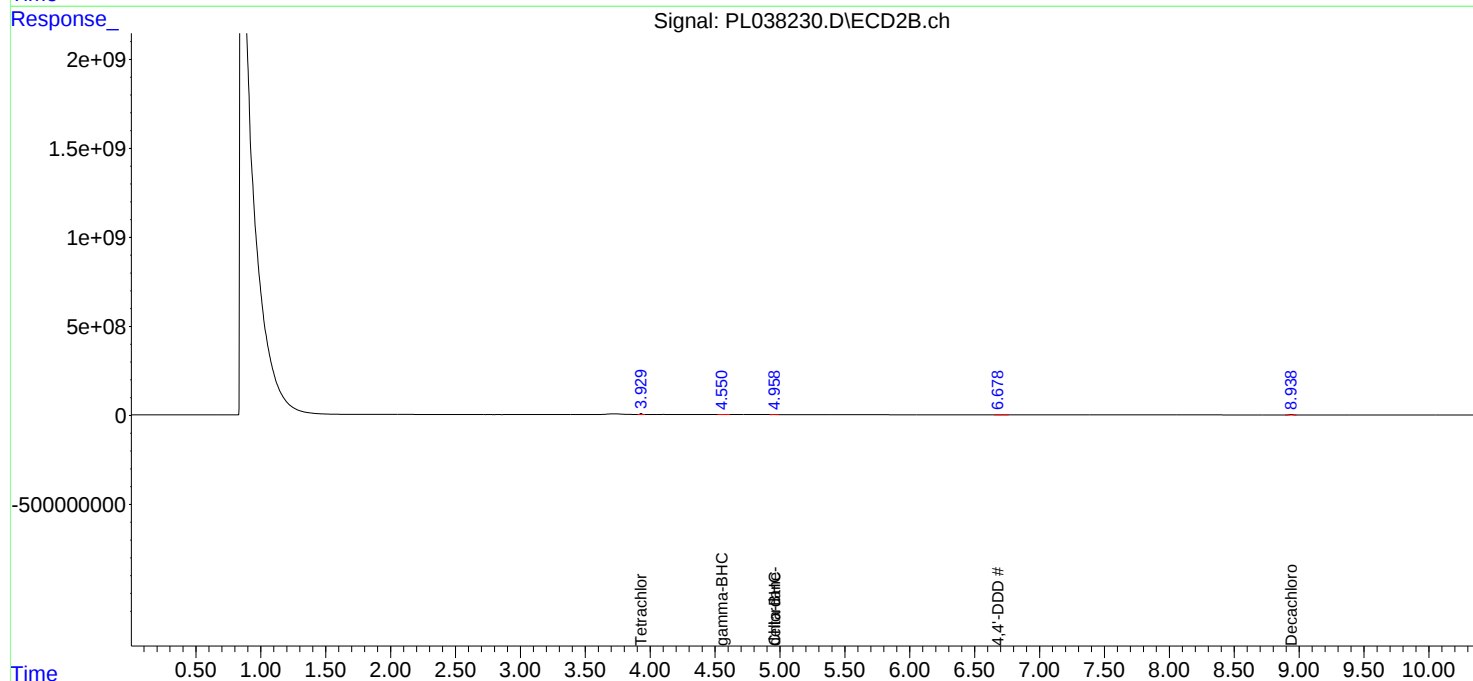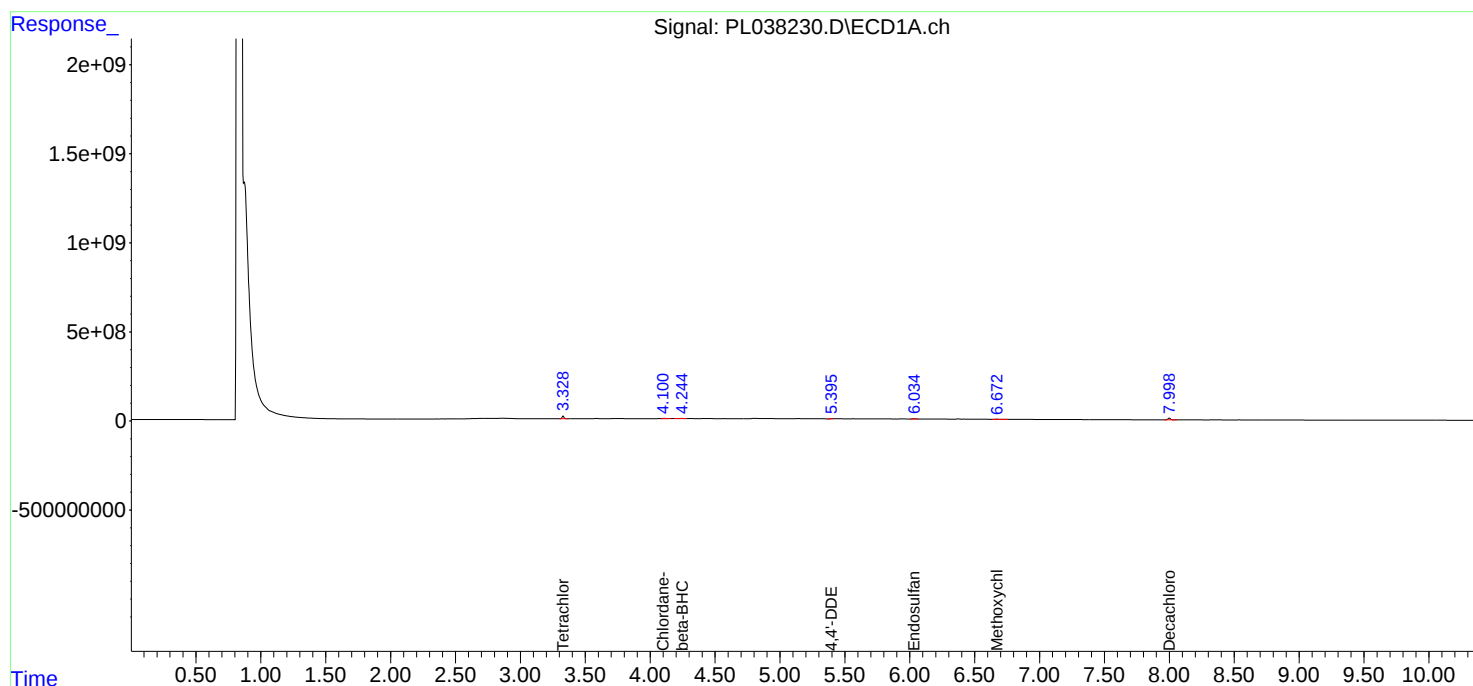


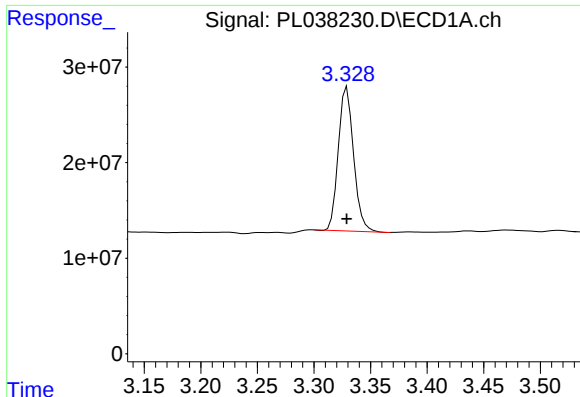

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 141491147
Conc: 19.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

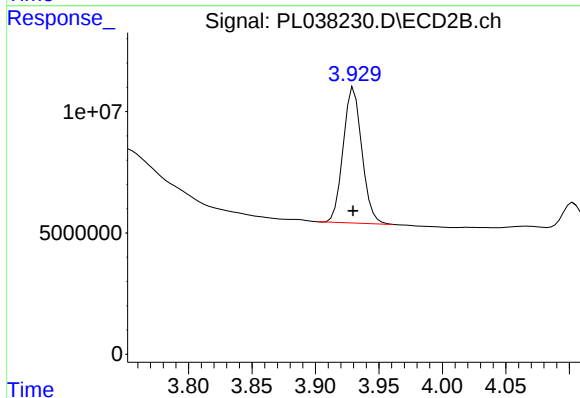


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 57060062
Conc: 21.74 ng/ml

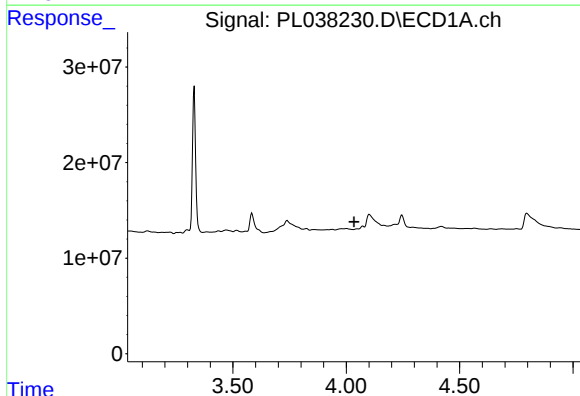


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

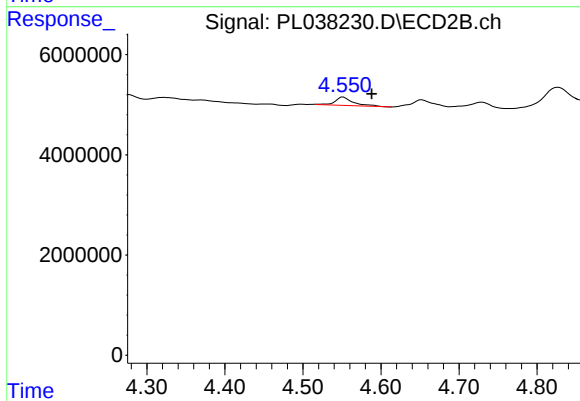

#3 gamma-BHC (Lindane)


R.T.: 4.552 min
Delta R.T.: -0.036 min
Response: 2664964
Conc: 0.74 ng/ml

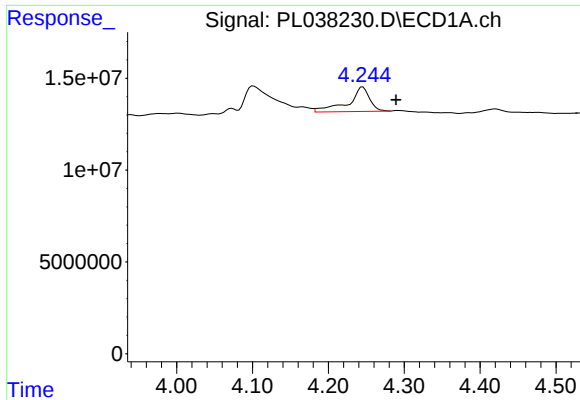

#6 beta-BHC


R.T.: 4.245 min
Delta R.T.: -0.044 min
Response: 26164638
Conc: 5.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

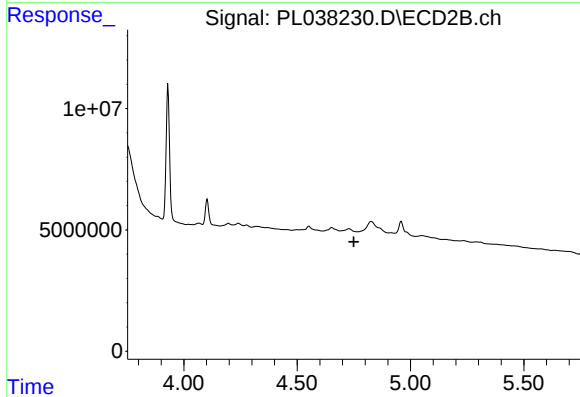


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

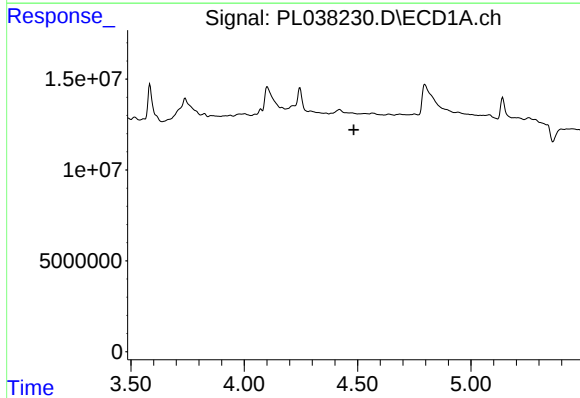


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

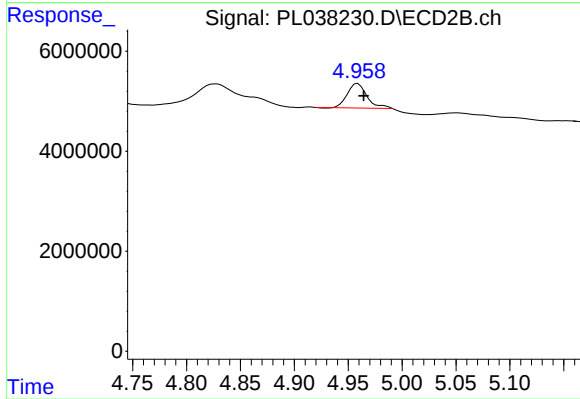

#7 delta-BHC


R.T.: 4.959 min
Delta R.T.: -0.005 min
Response: 6206634
Conc: 1.87 ng/ml

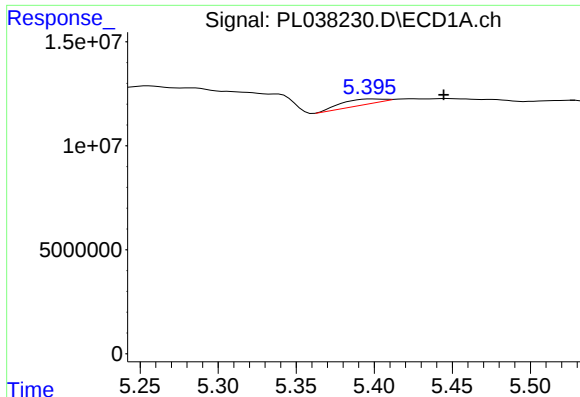

#12 4,4'-DDE


R.T.: 5.398 min
Delta R.T.: -0.046 min
Response: 6060450
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

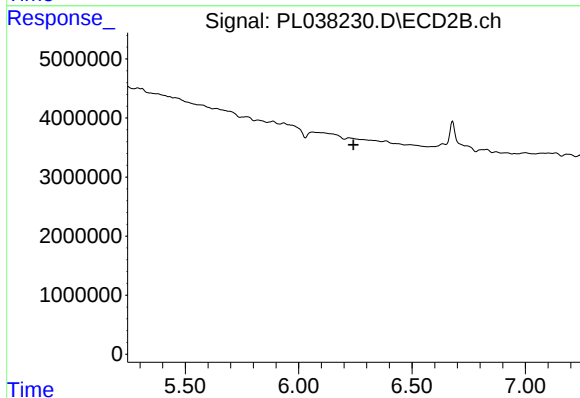


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

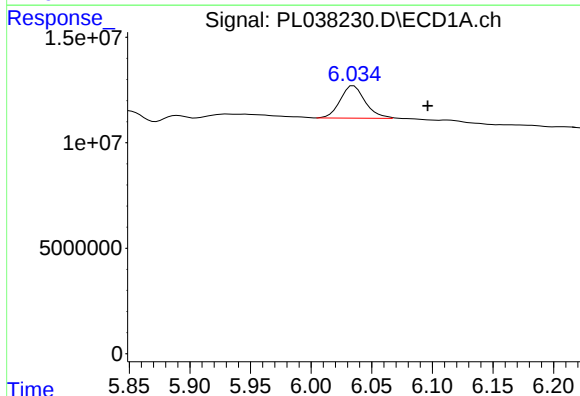


#15 Endosulfan II

R.T.: 6.035 min
Delta R.T.: -0.061 min
Response: 21896588
Conc: 2.76 ng/ml

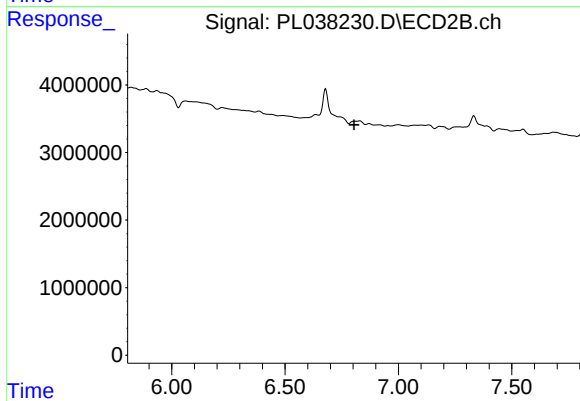

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.805 min
Response: 0
Conc: N.D.

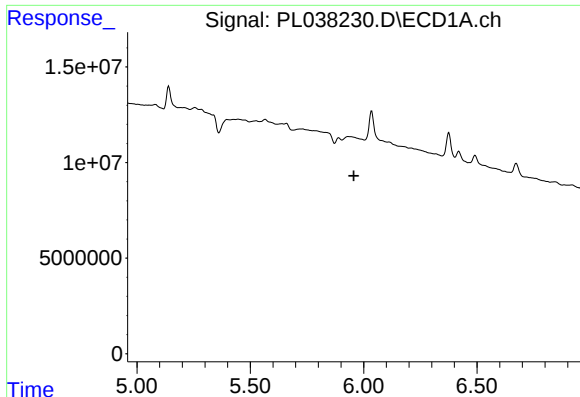

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

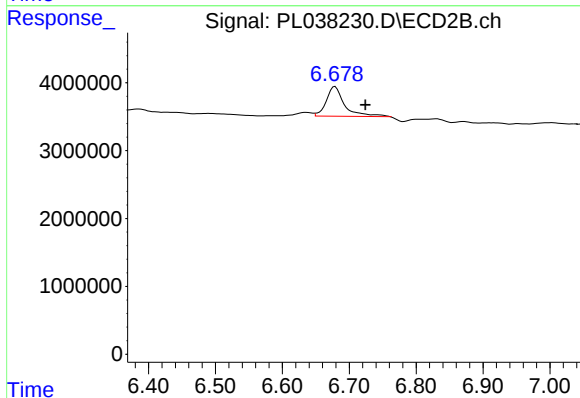


#16 4,4'-DDD

R.T.: 6.679 min
Delta R.T.: -0.046 min
Response: 8334621
Conc: 3.89 ng/ml

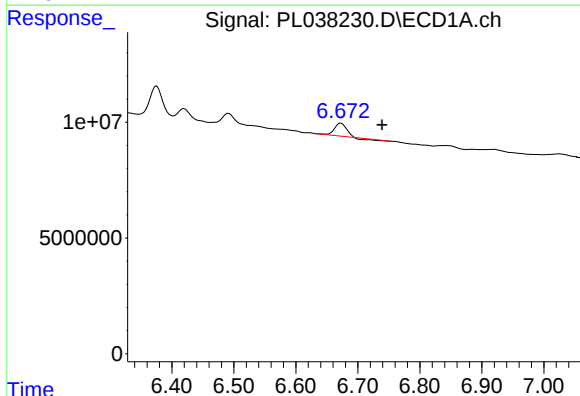


#20 Methoxychlor

R.T.: 6.673 min
Delta R.T.: -0.067 min
Response: 6917140
Conc: 1.80 ng/ml

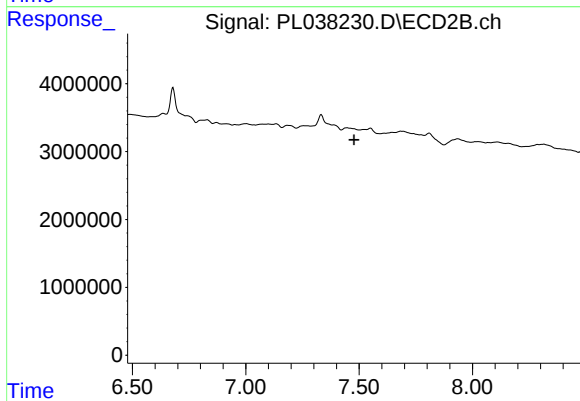

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.478 min
Response: 0
Conc: N.D.

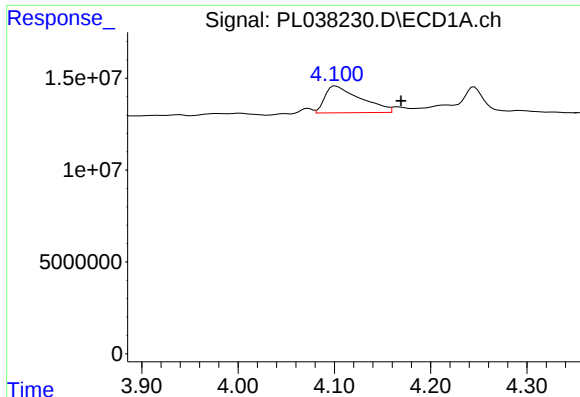

#23 Chlordane-1


R.T.: 4.102 min
Delta R.T.: -0.068 min
Response: 37646246
Conc: 108.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

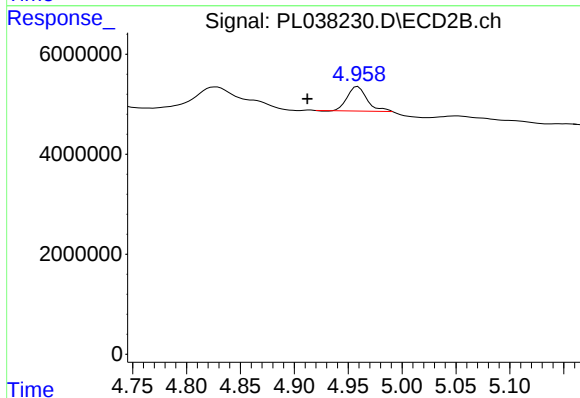


#23 Chlordane-1

R.T.: 4.959 min
Delta R.T.: 0.047 min
Response: 6206634
Conc: 53.56 ng/ml

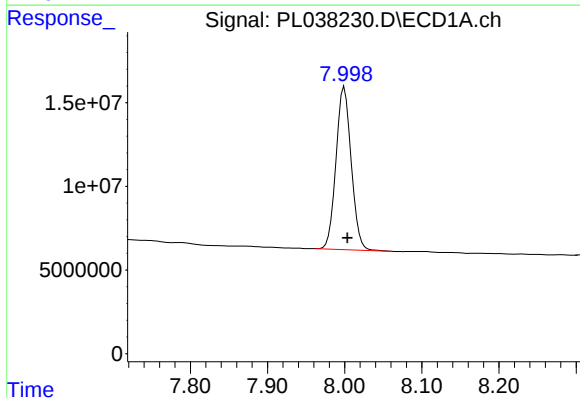

#28 Decachlorobiphenyl

R.T.: 8.000 min
Delta R.T.: -0.004 min
Response: 133242345
Conc: 17.56 ng/ml

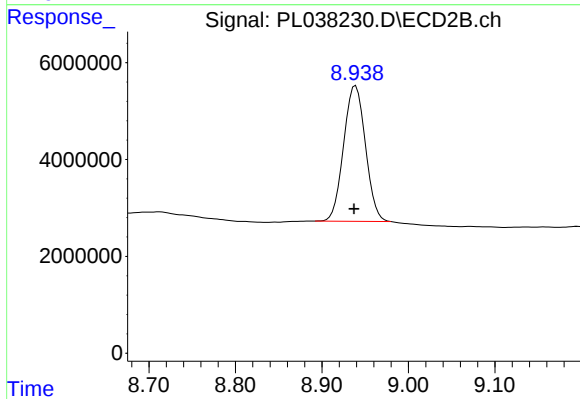

#28 Decachlorobiphenyl

R.T.: 8.939 min
Delta R.T.: 0.002 min
Response: 48945878
Conc: 20.02 ng/ml