

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
 Data File : PL038232.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2018 21:51
 Operator : AJ\SJ
 Sample : J4016-15
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:54:18 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.931	138.4E6	56470779	18.592	21.513
28)	SA Decachlor...	8.000	8.939	138.8E6	50865086	18.301	20.808
Target Compounds							
3)	MA gamma-BHC...	0.000	4.554f	0	4118568	N.D.	1.140 #
6)	B beta-BHC	4.247f	0.000	26885775	0	5.696	N.D. #
7)	B delta-BHC	0.000	4.959	0	10098357	N.D.	3.045 #
15)	B Endosulfa...	6.034f	0.000	24480418	0	3.087	N.D. #
16)	A 4,4'-DDD	0.000	6.678f	0	6926817	N.D.	3.236 #
19)	B Endosulfa...	6.492	0.000	9289384	0	1.230	N.D. #
20)	A Methoxychlor	6.673f	0.000	14695588	0	3.820	N.D. #
23)	Chlordane-1	0.000	4.959	0	10098357	N.D.	87.141 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
Data File : PL038232.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2018 21:51
Operator : AJ\SJ
Sample : J4016-15
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:54:18 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

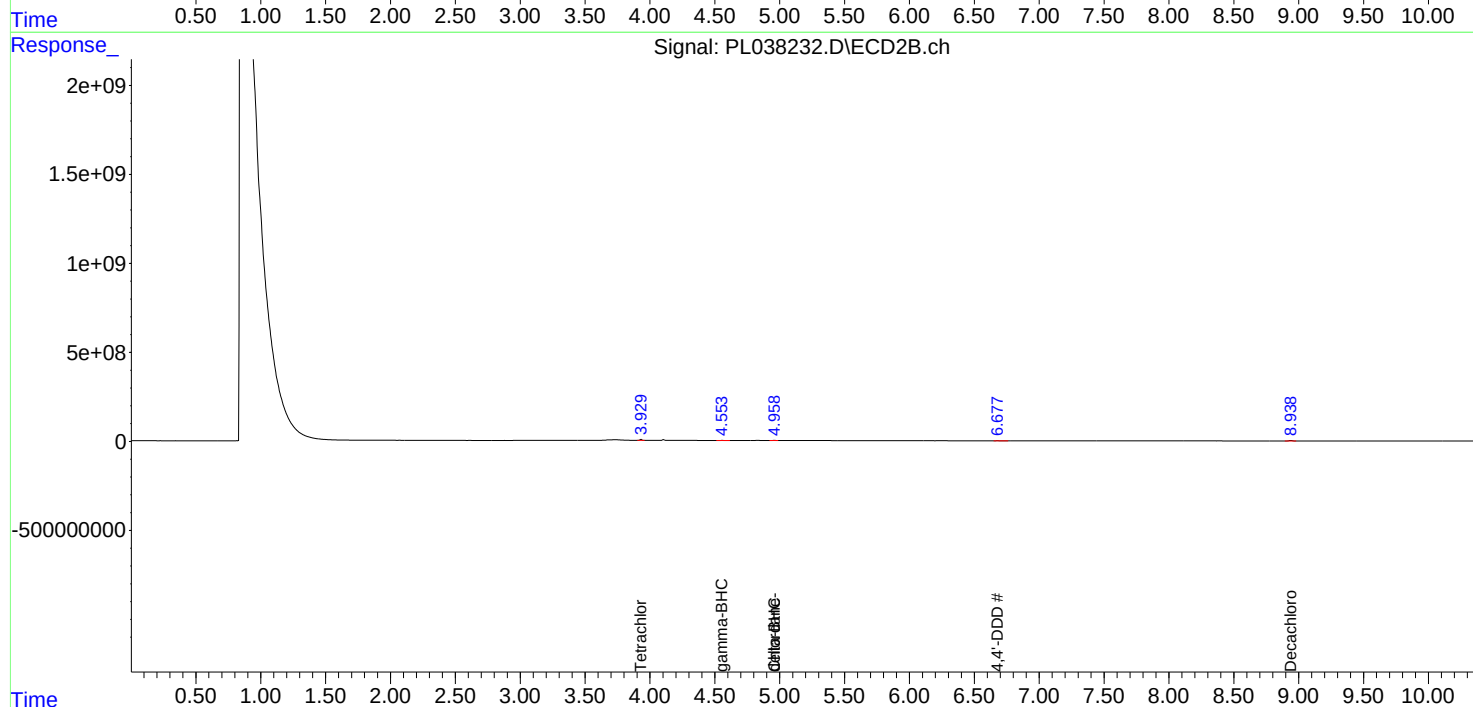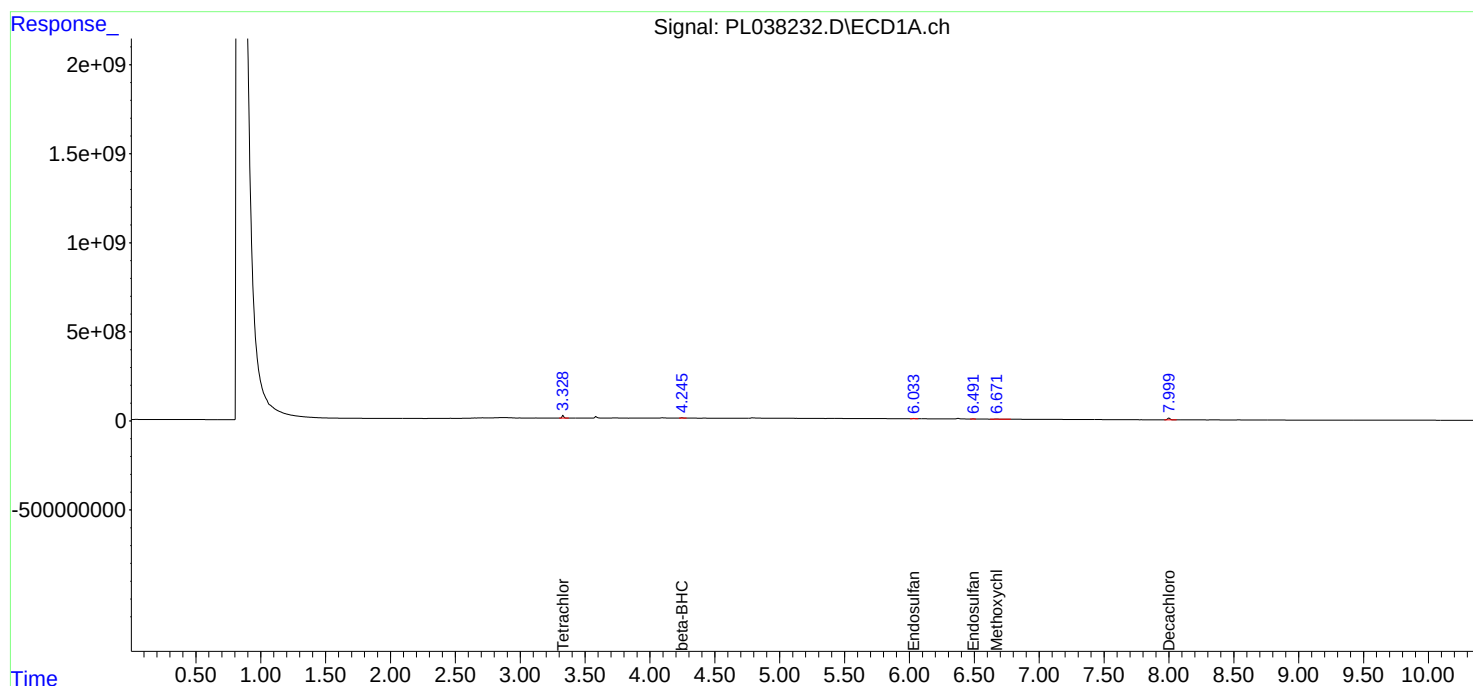


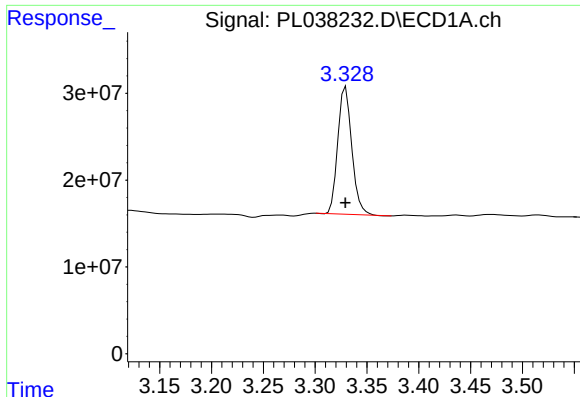

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 138441973
Conc: 18.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

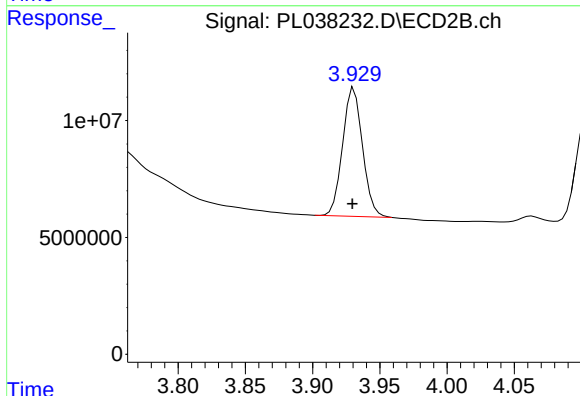


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.001 min
Response: 56470779
Conc: 21.51 ng/ml

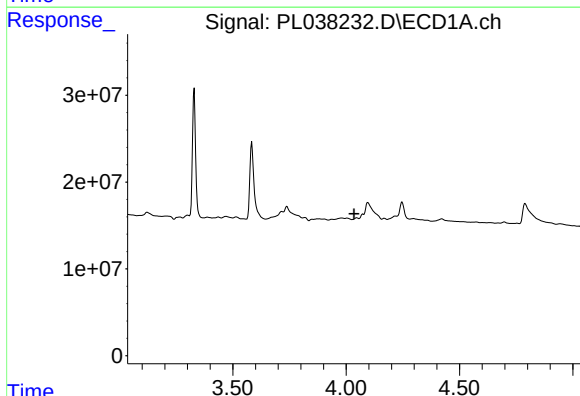


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

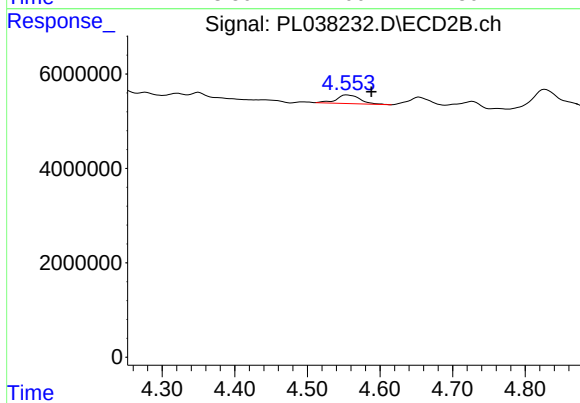

#3 gamma-BHC (Lindane)


R.T.: 4.554 min
Delta R.T.: -0.034 min
Response: 4118568
Conc: 1.14 ng/ml

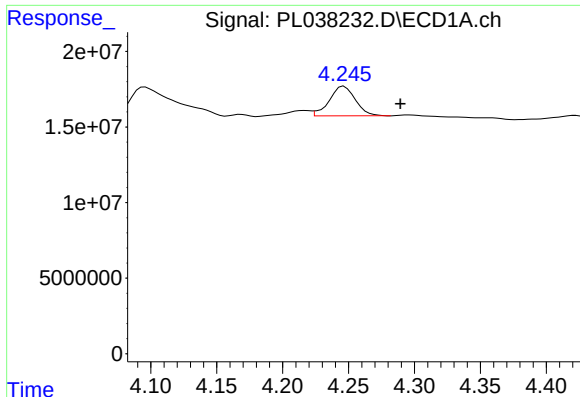

#6 beta-BHC


R.T.: 4.247 min
Delta R.T.: -0.043 min
Response: 26885775
Conc: 5.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

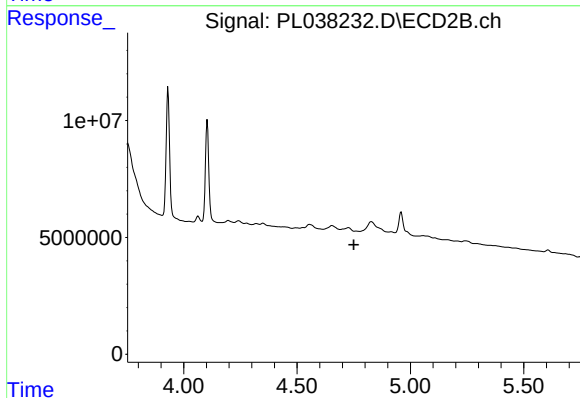


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

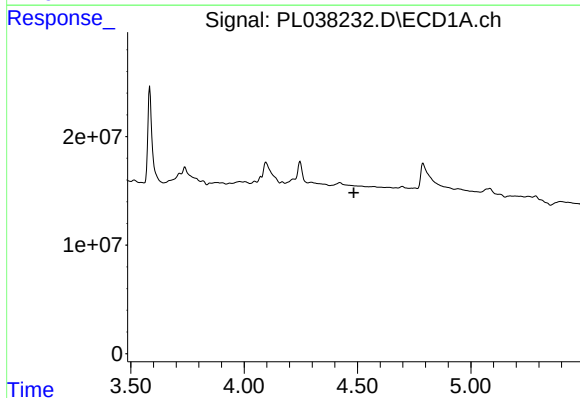


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

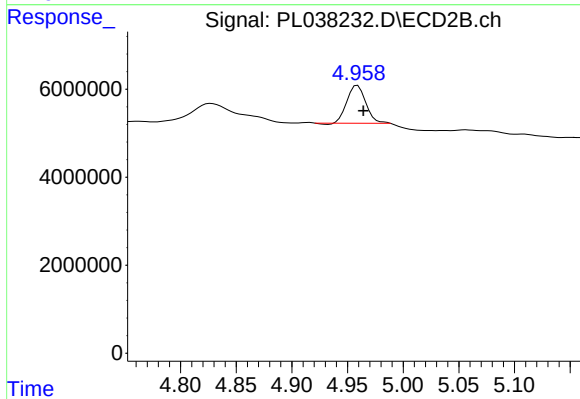

#7 delta-BHC


R.T.: 4.959 min
Delta R.T.: -0.005 min
Response: 10098357
Conc: 3.04 ng/ml

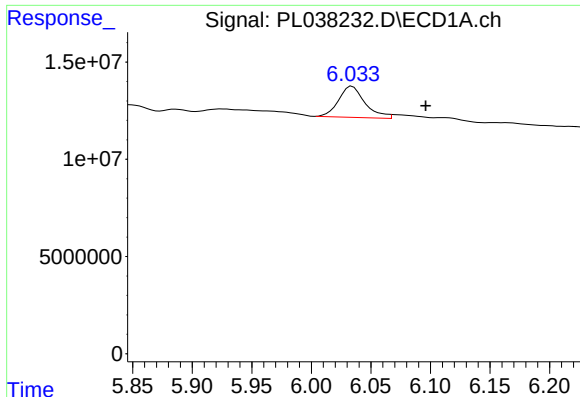

#15 Endosulfan II


R.T.: 6.034 min
Delta R.T.: -0.062 min
Response: 24480418
Conc: 3.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

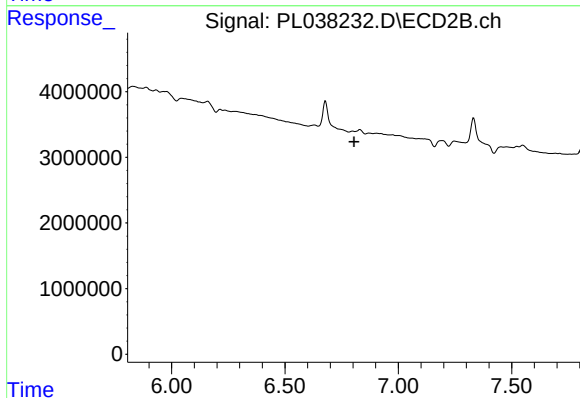


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.805 min
Response: 0
Conc: N.D.

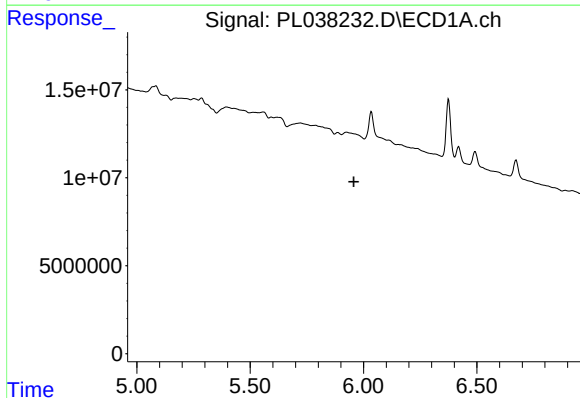


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.956 min
Response: 0
Conc: N.D.

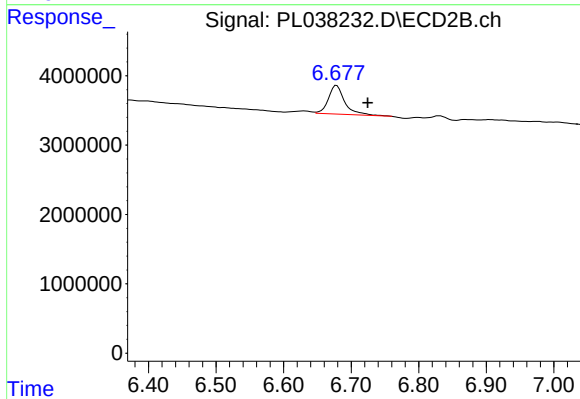

#16 4,4'-DDD


R.T.: 6.678 min
Delta R.T.: -0.046 min
Response: 6926817
Conc: 3.24 ng/ml

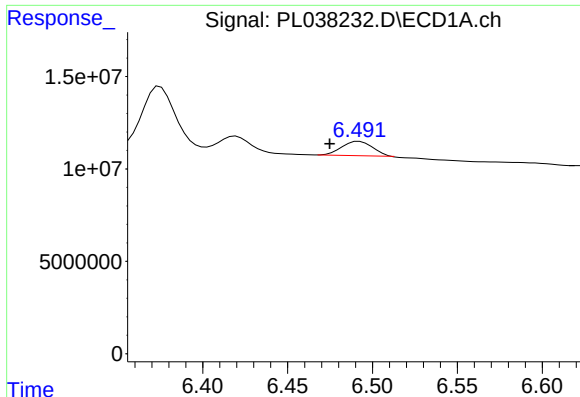

#19 Endosulfan Sulfate


R.T.: 6.492 min
Delta R.T.: 0.017 min
Response: 9289384
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

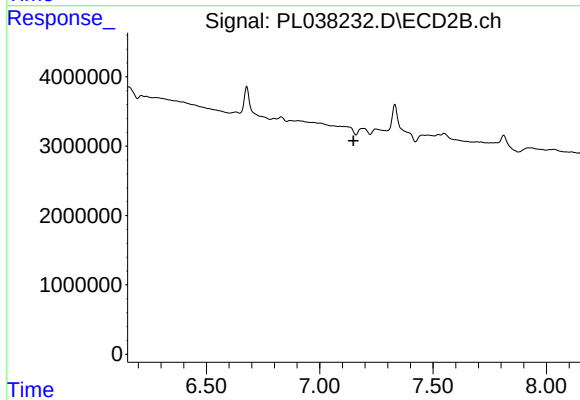


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

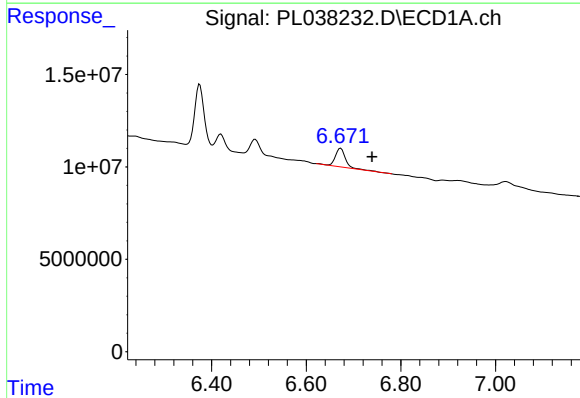


#20 Methoxychlor

R.T.: 6.673 min
Delta R.T.: -0.067 min
Response: 14695588
Conc: 3.82 ng/ml

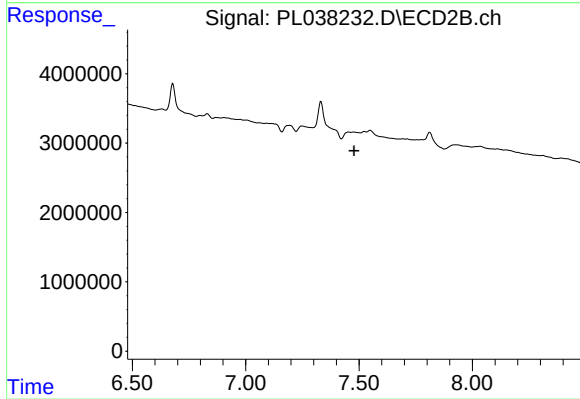

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.478 min
Response: 0
Conc: N.D.

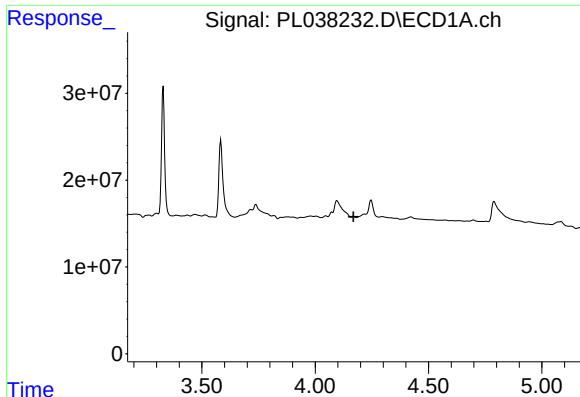

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

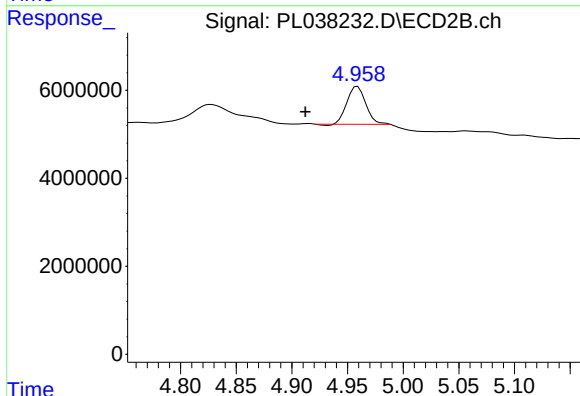


#23 Chlordane-1

R.T.: 4.959 min
Delta R.T.: 0.047 min
Response: 10098357
Conc: 87.14 ng/ml

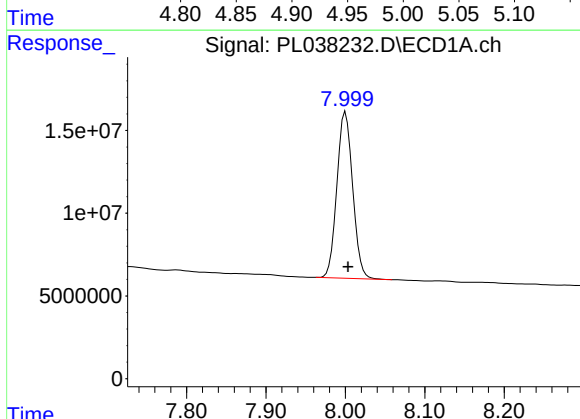

#28 Decachlorobiphenyl

R.T.: 8.000 min
Delta R.T.: -0.003 min
Response: 138826772
Conc: 18.30 ng/ml

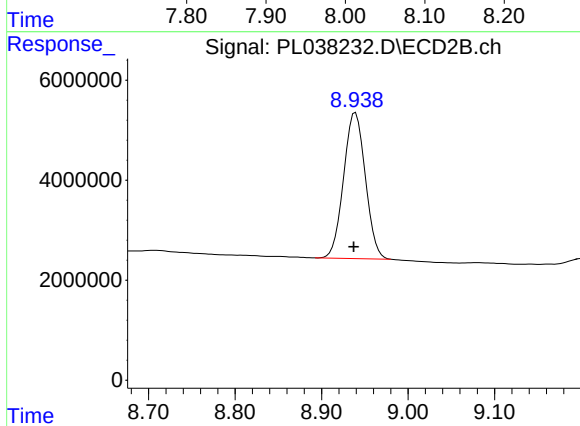

#28 Decachlorobiphenyl

R.T.: 8.939 min
Delta R.T.: 0.002 min
Response: 50865086
Conc: 20.81 ng/ml