

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
 Data File : PL038247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2018 01:23
 Operator : AJ\SJ
 Sample : J4028-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:56:56 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.930	174.2E6	74206459	23.388	28.270
28)	SA Decachlor...	8.000	8.939	142.8E6	51987787	18.826	21.268
Target Compounds							
3)	MA gamma-BHC...	4.049	0.000	24534310	0	2.340	N.D. #
6)	B beta-BHC	4.244f	0.000	16492218	0	3.494	N.D. #
7)	B delta-BHC	0.000	4.960	0	4367110	N.D.	1.317 #
15)	B Endosulfa...	6.034f	6.837	22502204	659767	2.838	0.275 #
16)	A 4,4'-DDD	0.000	6.678f	0	7266431	N.D.	3.395 #
23)	Chlordane-1	0.000	4.960	0	4367110	N.D.	37.685 #
24)	Chlordane-2	0.000	5.312	0	9216272	N.D.	76.963 #
27)	Chlordane-5	0.000	6.837	0	659767	N.D.	7.365 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
Data File : PL038247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2018 01:23
Operator : AJ\SJ
Sample : J4028-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:56:56 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

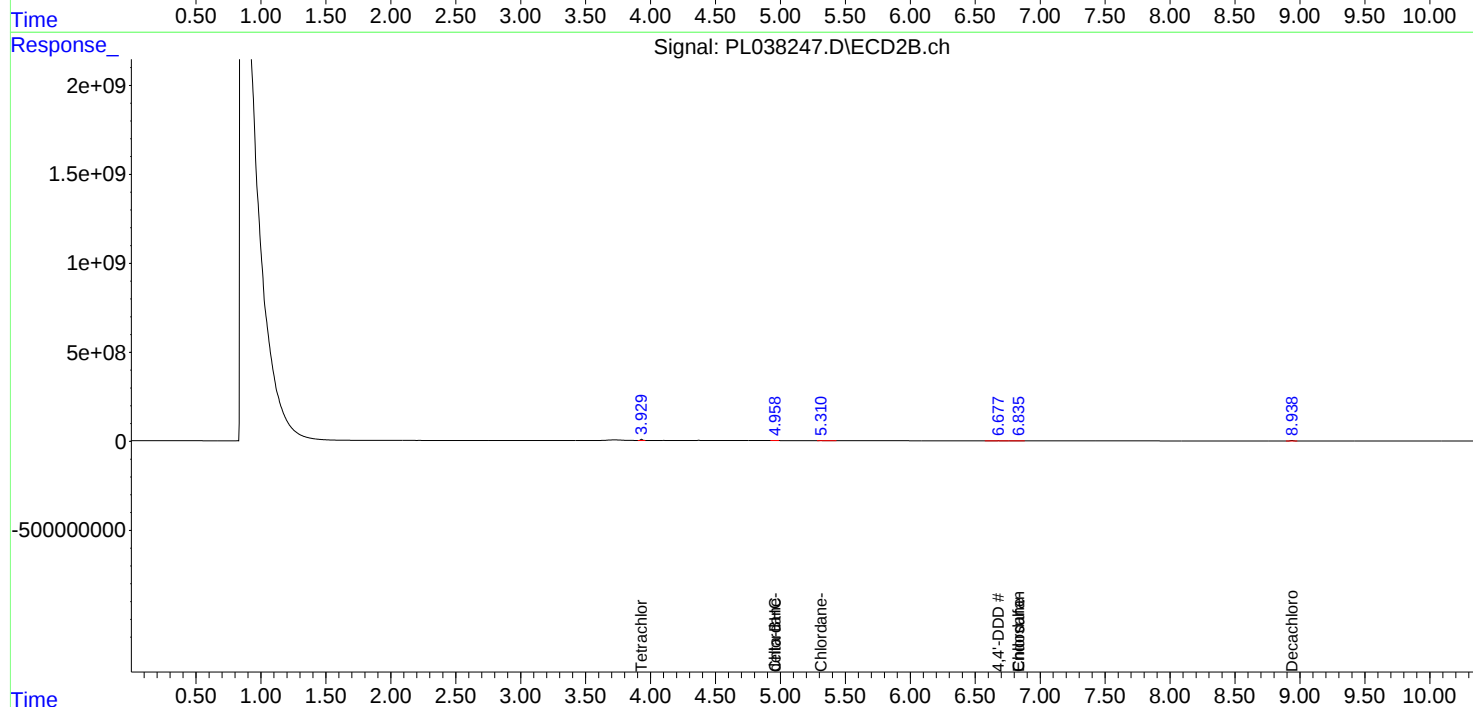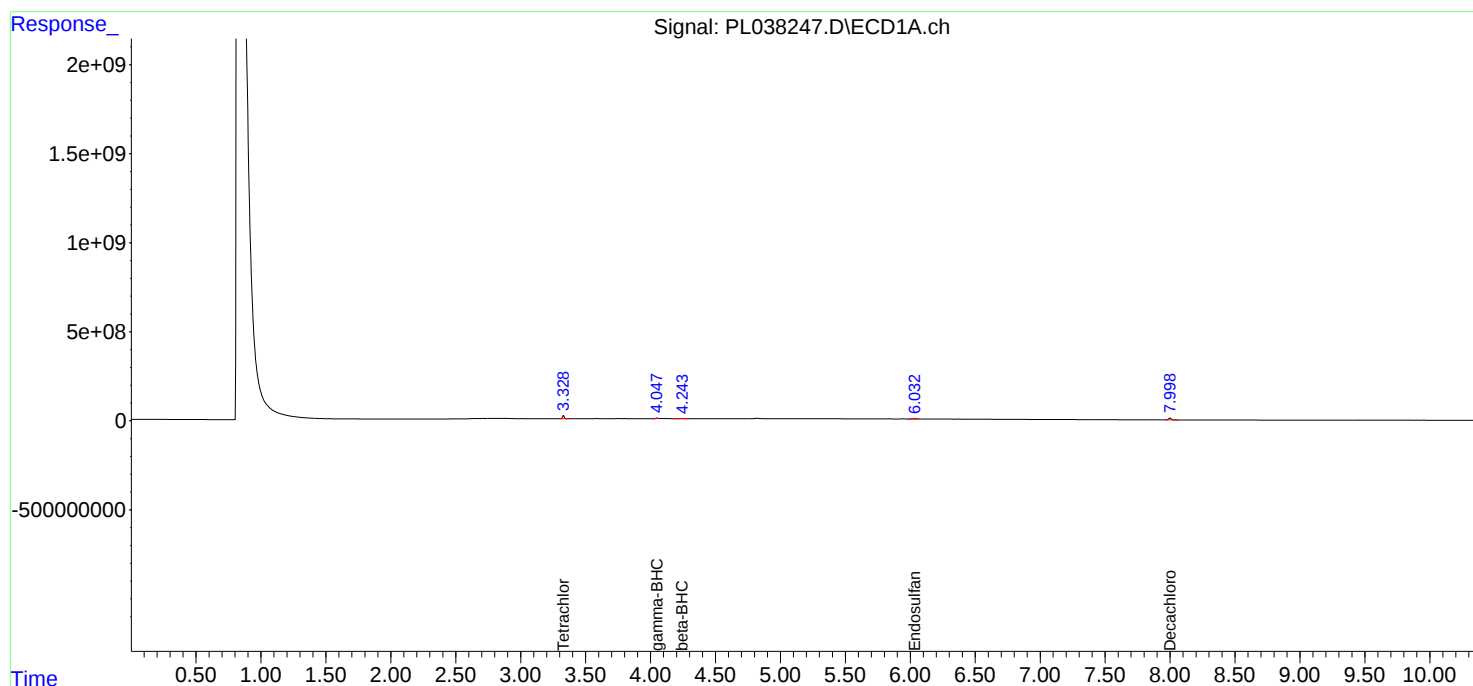


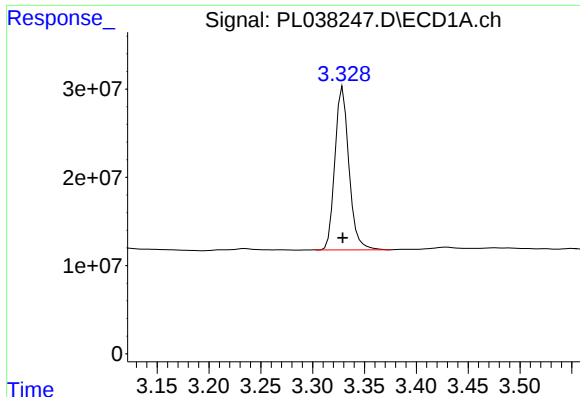

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 174157646
Conc: 23.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

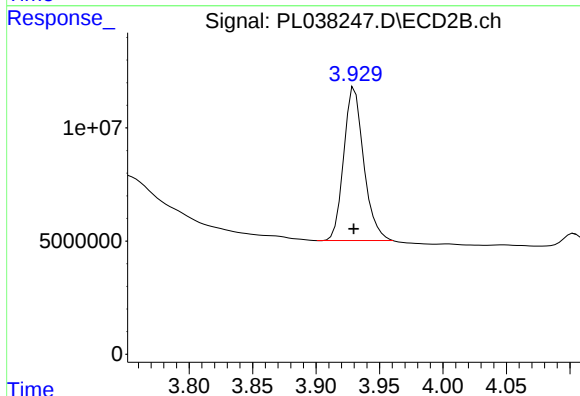


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 74206459
Conc: 28.27 ng/ml

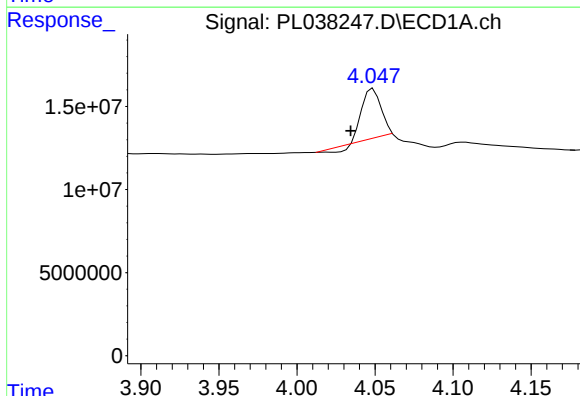


#3 gamma-BHC (Lindane)

R.T.: 4.049 min
Delta R.T.: 0.014 min
Response: 24534310
Conc: 2.34 ng/ml

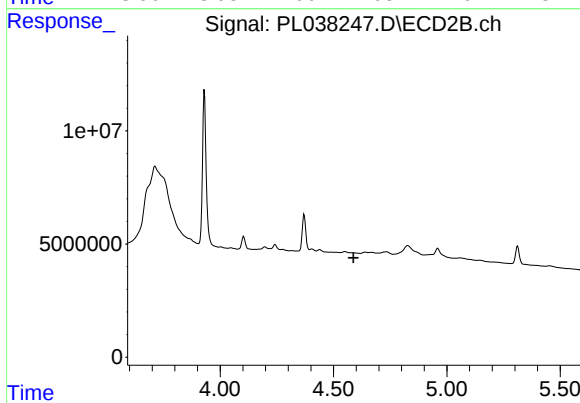

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.588 min
Response: 0
Conc: N.D.

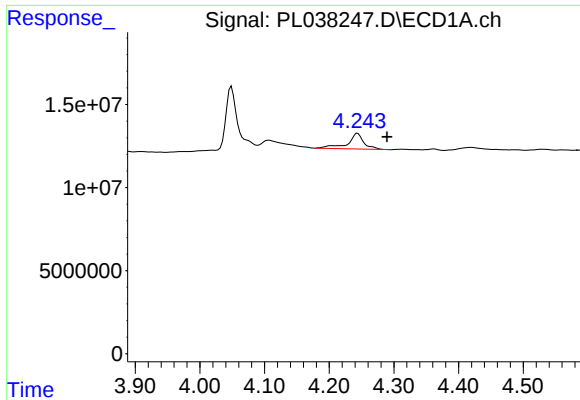

#6 beta-BHC


R.T.: 4.244 min
Delta R.T.: -0.045 min
Response: 16492218
Conc: 3.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

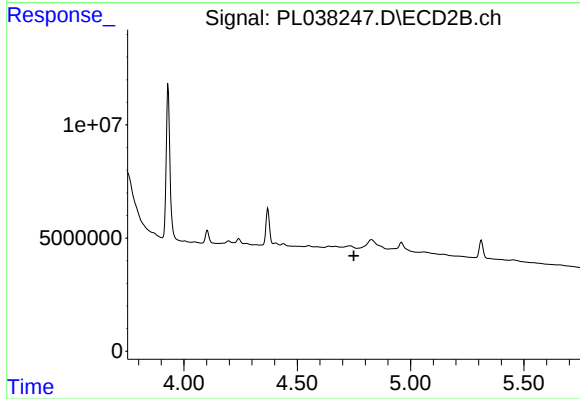


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

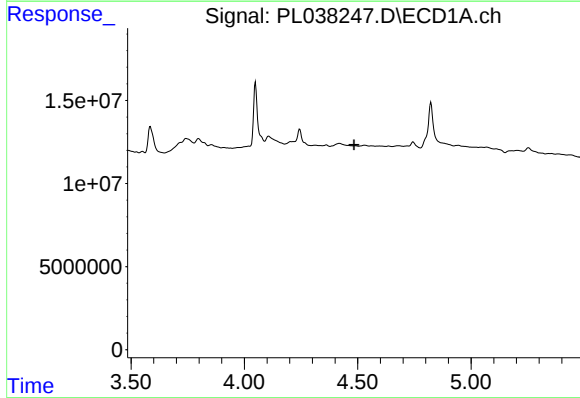


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

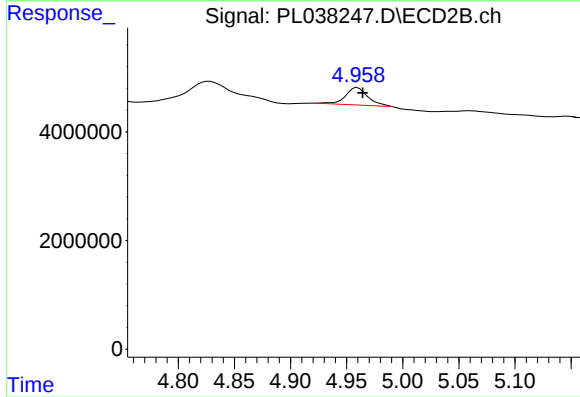

#7 delta-BHC


R.T.: 4.960 min
Delta R.T.: -0.005 min
Response: 4367110
Conc: 1.32 ng/ml

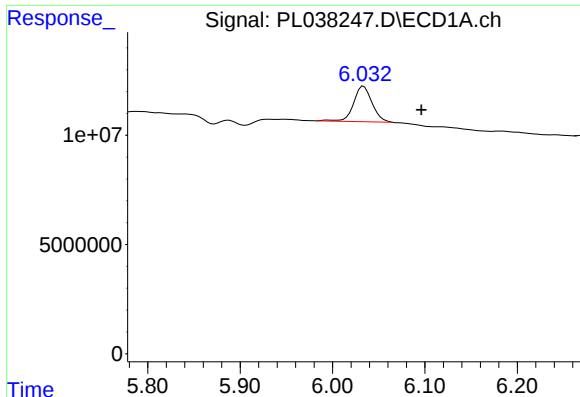

#15 Endosulfan II


R.T.: 6.034 min
Delta R.T.: -0.062 min
Response: 22502204
Conc: 2.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

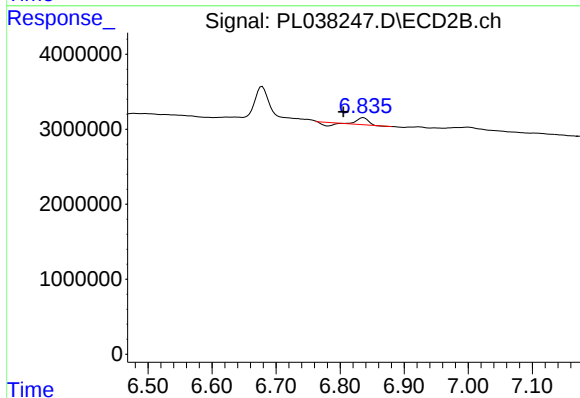


#15 Endosulfan II

R.T.: 6.837 min
Delta R.T.: 0.031 min
Response: 659767
Conc: 0.27 ng/ml

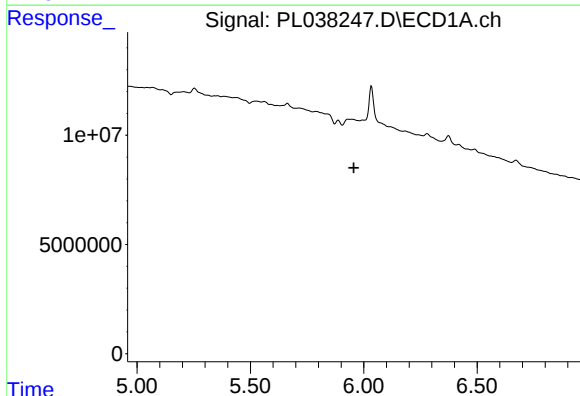


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.956 min
Response: 0
Conc: N.D.

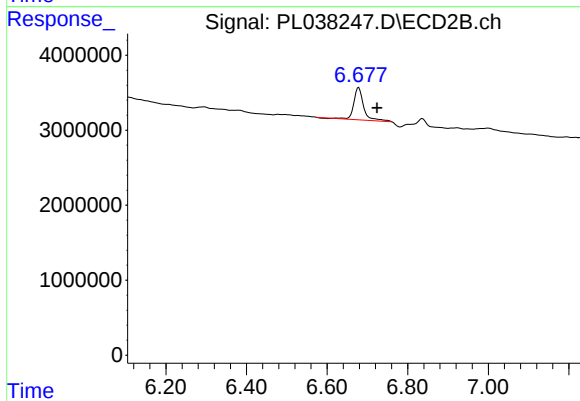

#16 4,4'-DDD


R.T.: 6.678 min
Delta R.T.: -0.046 min
Response: 7266431
Conc: 3.39 ng/ml

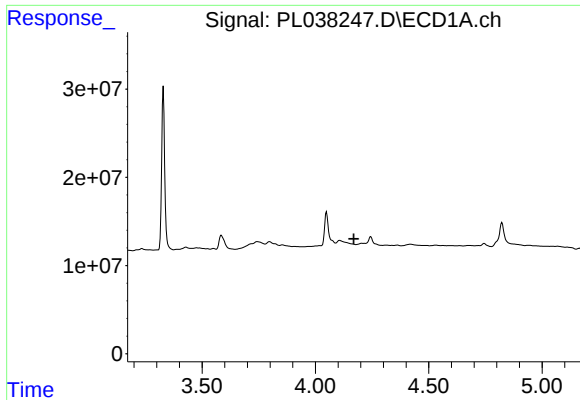

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

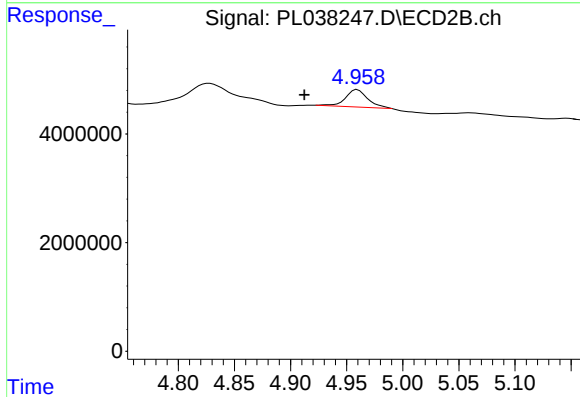


#23 Chlordane-1

R.T.: 4.960 min
Delta R.T.: 0.047 min
Response: 4367110
Conc: 37.68 ng/ml

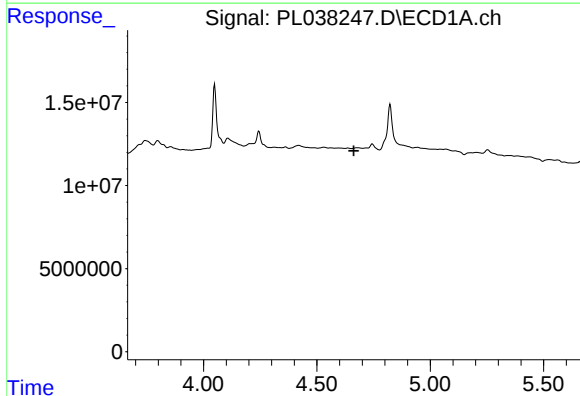


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.663 min
Response: 0
Conc: N.D.

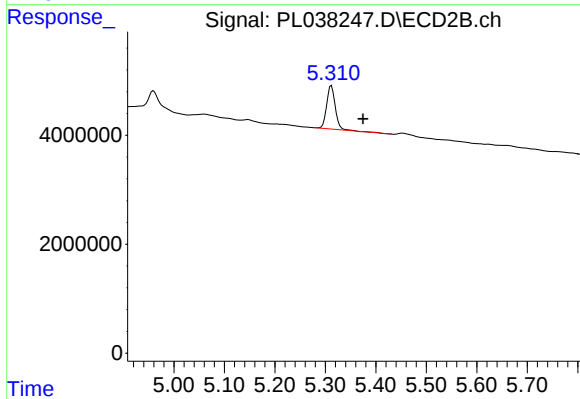

#24 Chlordane-2


R.T.: 5.312 min
Delta R.T.: -0.063 min
Response: 9216272
Conc: 76.96 ng/ml

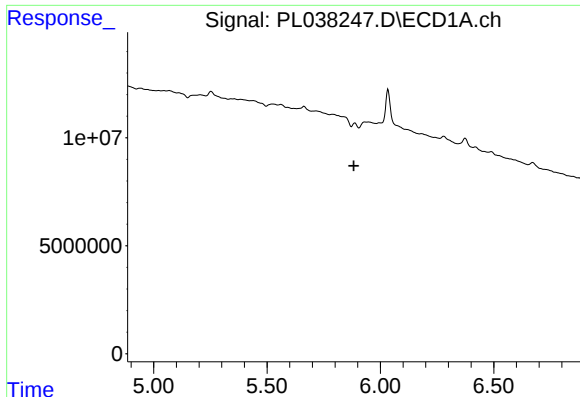

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

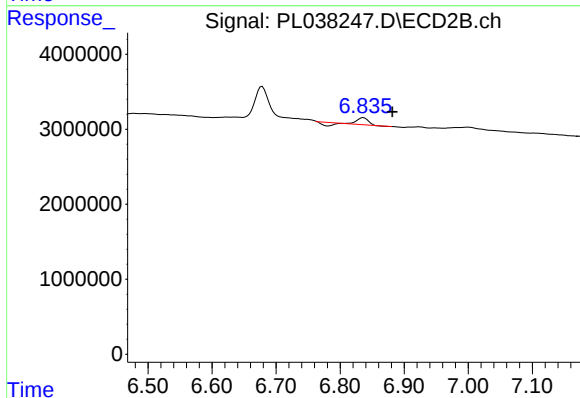


#27 Chlordane-5

R.T.: 6.837 min
Delta R.T.: -0.045 min
Response: 659767
Conc: 7.37 ng/ml

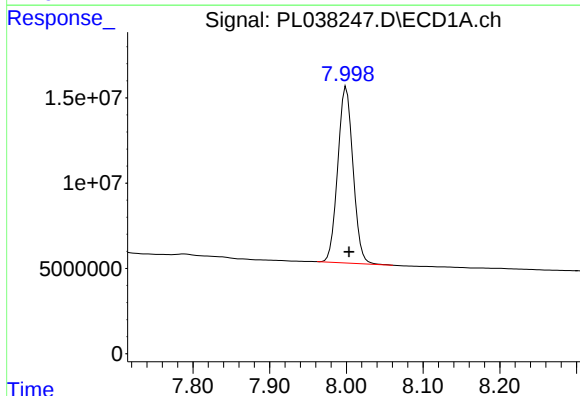

#28 Decachlorobiphenyl

R.T.: 8.000 min
Delta R.T.: -0.004 min
Response: 142813924
Conc: 18.83 ng/ml

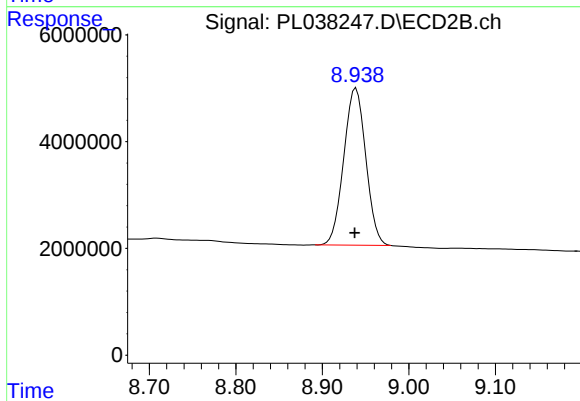

#28 Decachlorobiphenyl

R.T.: 8.939 min
Delta R.T.: 0.002 min
Response: 51987787
Conc: 21.27 ng/ml