

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
 Data File : PL038256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2018 03:31
 Operator : AJ\SJ
 Sample : J4026-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:58:23 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.931	160.1E6	64041973	21.505	24.398
28)	SA Decachlor...	8.000	8.938	137.4E6	49576321	18.106	20.281
Target Compounds							
3)	MA gamma-BHC...	4.050	0.000	9161247	0	0.874	N.D. #
6)	B beta-BHC	4.245f	0.000	13612567	0	2.884	N.D. #
7)	B delta-BHC	0.000	4.959	0	4333415	N.D.	1.307 #
15)	B Endosulfa...	6.034f	0.000	28207912	0	3.557	N.D. #
16)	A 4,4'-DDD	5.955	6.678f	12849835	7587680	1.752	3.545 #
23)	Chlordane-1	0.000	4.959	0	4333415	N.D.	37.394 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
Data File : PL038256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2018 03:31
Operator : AJ\SJ
Sample : J4026-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:58:23 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

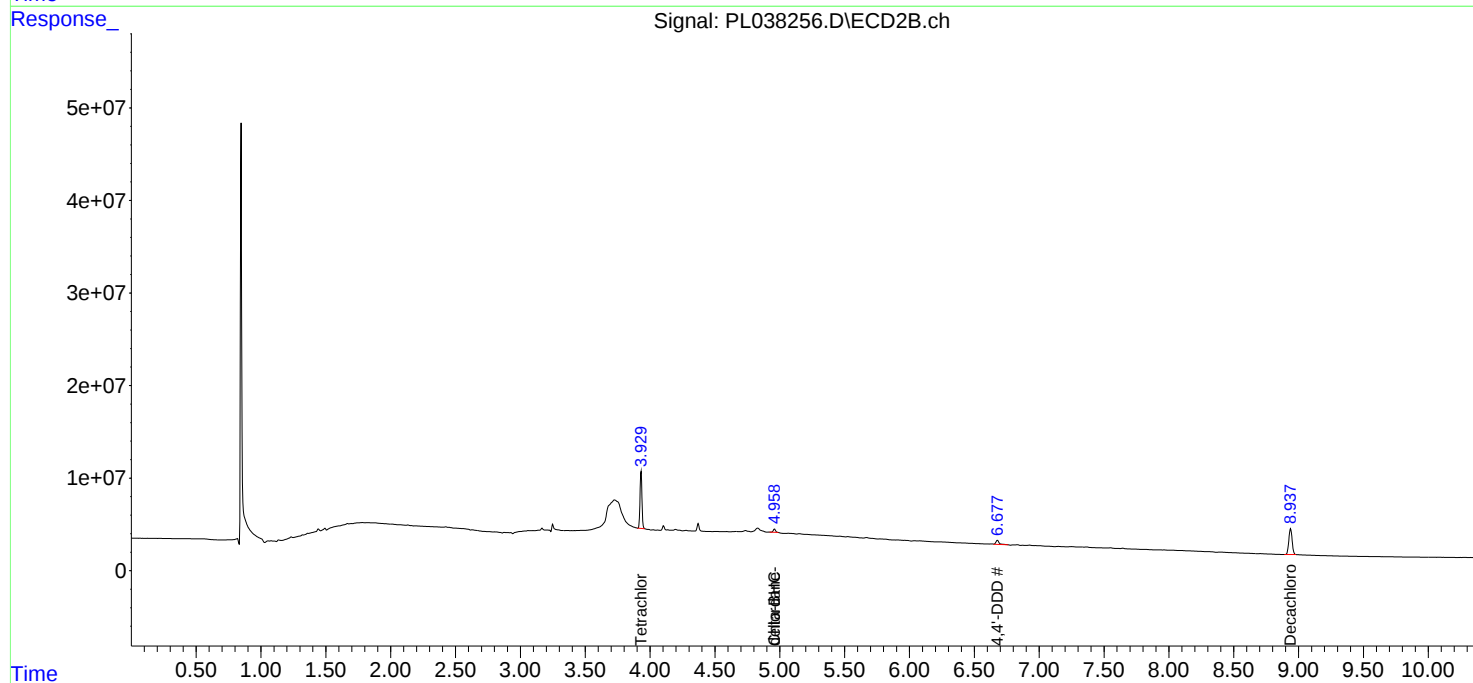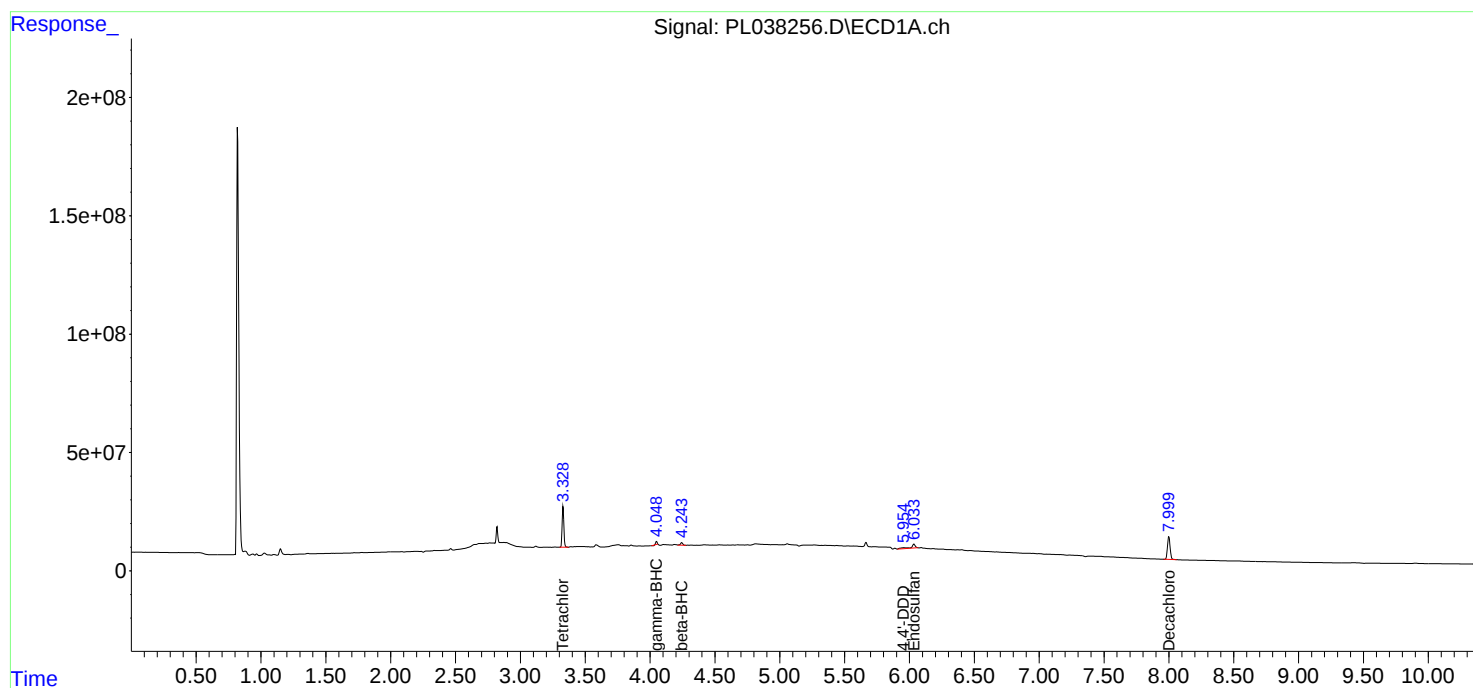


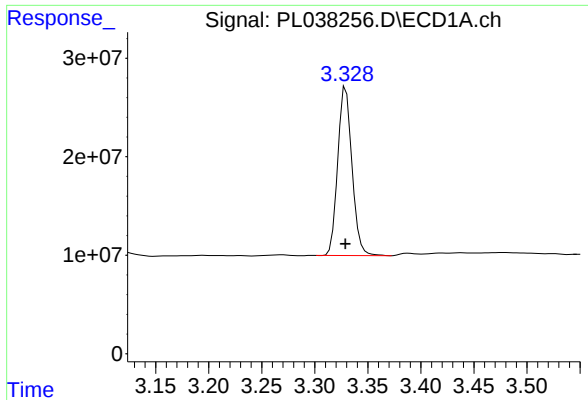

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 160134018
Conc: 21.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

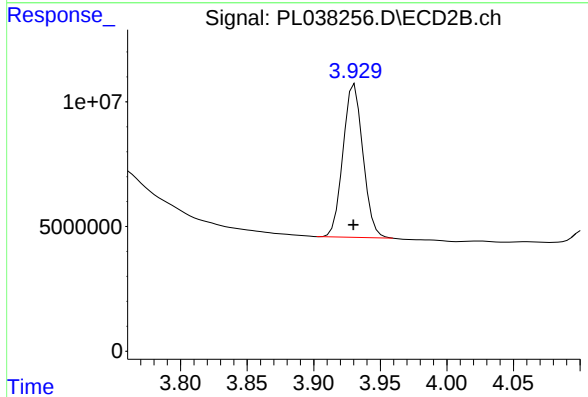


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 64041973
Conc: 24.40 ng/ml

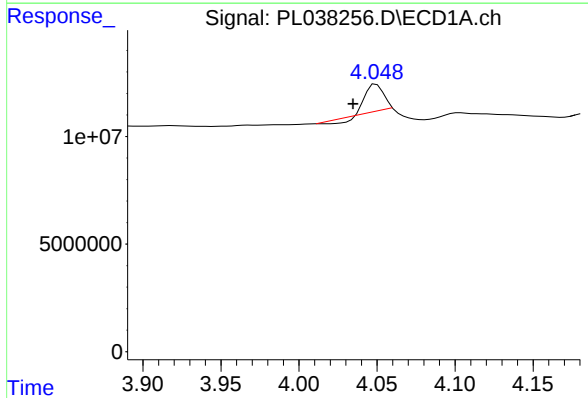


#3 gamma-BHC (Lindane)

R.T.: 4.050 min
Delta R.T.: 0.015 min
Response: 9161247
Conc: 0.87 ng/ml

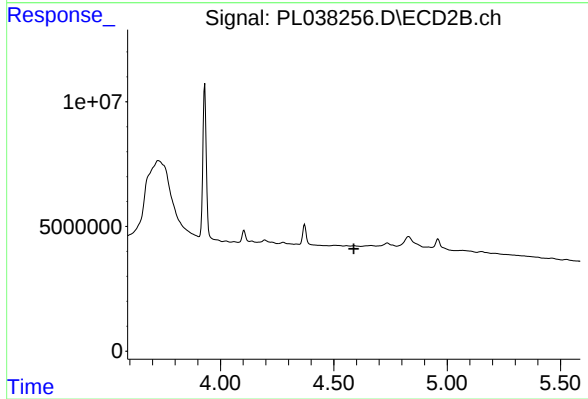

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.588 min
Response: 0
Conc: N.D.

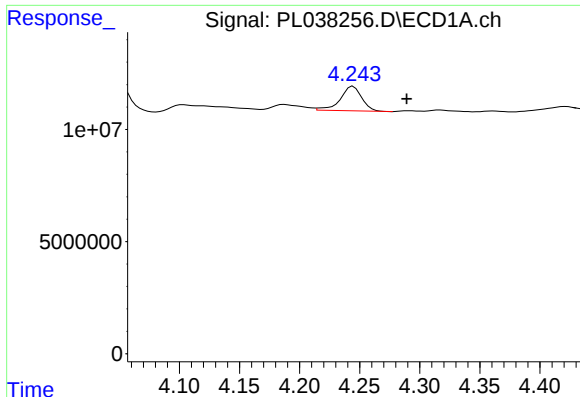

#6 beta-BHC


R.T.: 4.245 min
Delta R.T.: -0.045 min
Response: 13612567
Conc: 2.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

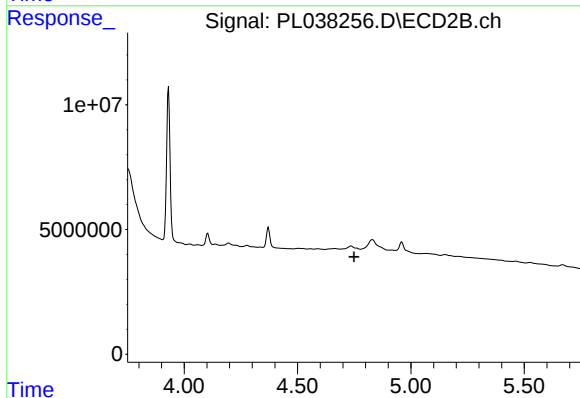


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

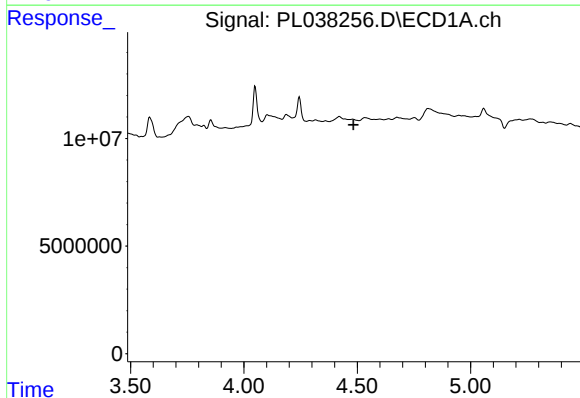


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

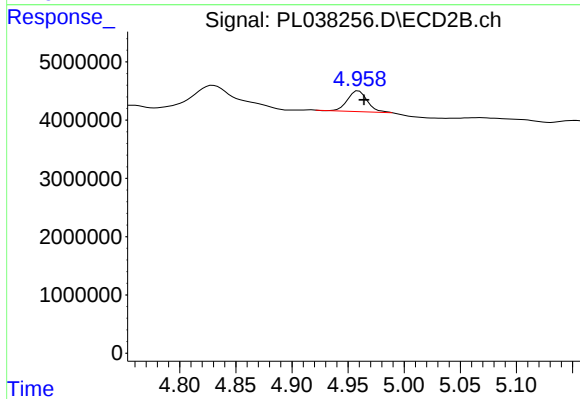

#7 delta-BHC


R.T.: 4.959 min
Delta R.T.: -0.005 min
Response: 4333415
Conc: 1.31 ng/ml

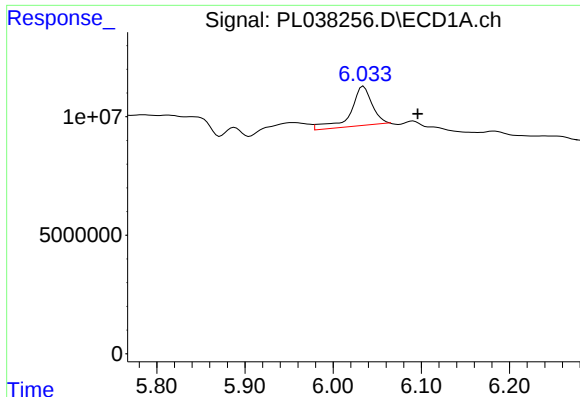

#15 Endosulfan II


R.T.: 6.034 min
Delta R.T.: -0.062 min
Response: 28207912
Conc: 3.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

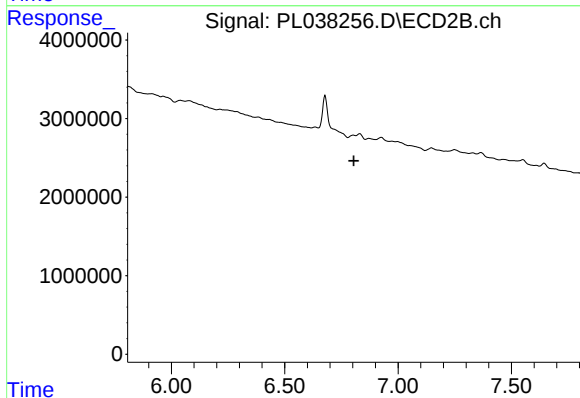


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.805 min
Response: 0
Conc: N.D.

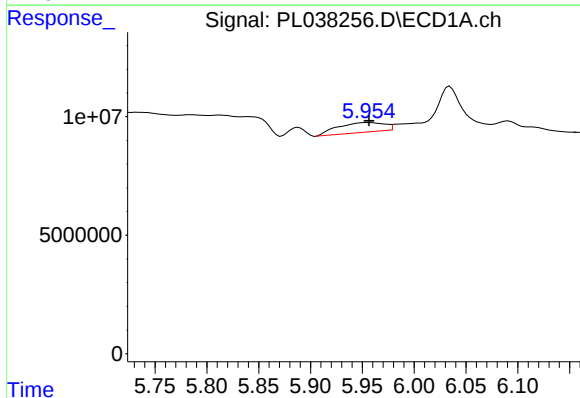


#16 4,4'-DDD

R.T.: 5.955 min
Delta R.T.: -0.001 min
Response: 12849835
Conc: 1.75 ng/ml

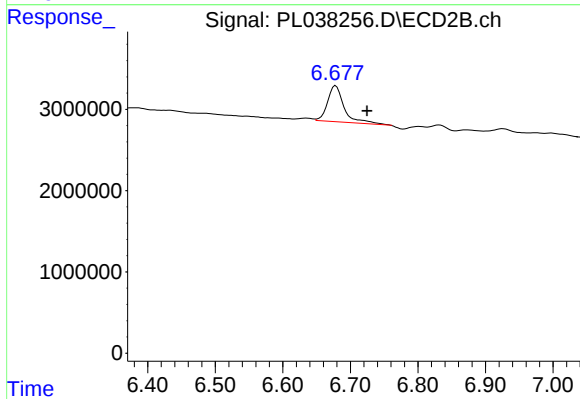

#16 4,4'-DDD


R.T.: 6.678 min
Delta R.T.: -0.046 min
Response: 7587680
Conc: 3.54 ng/ml

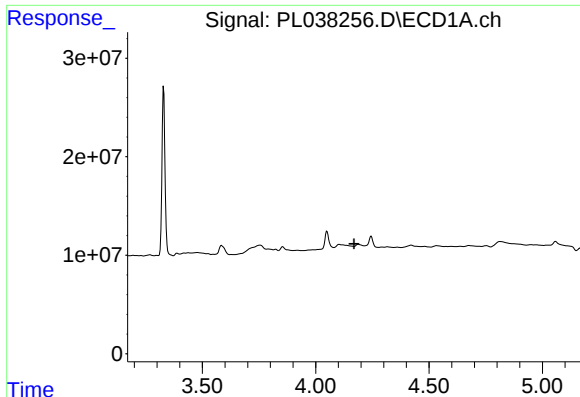

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

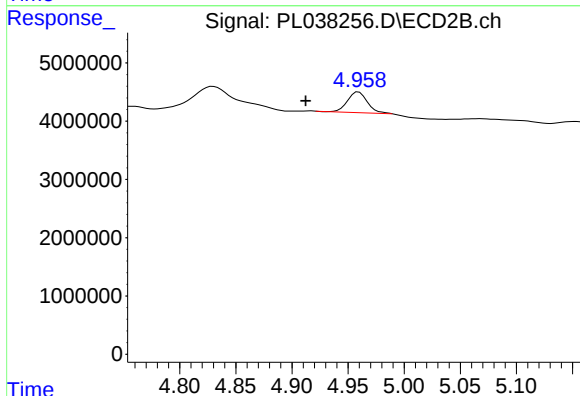


#23 Chlordane-1

R.T.: 4.959 min
Delta R.T.: 0.047 min
Response: 4333415
Conc: 37.39 ng/ml

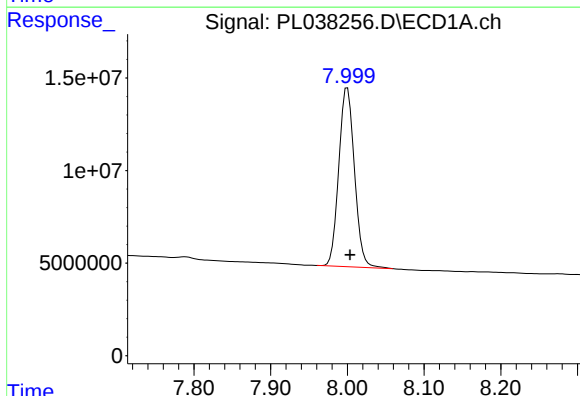

#28 Decachlorobiphenyl

R.T.: 8.000 min
Delta R.T.: -0.004 min
Response: 137350856
Conc: 18.11 ng/ml

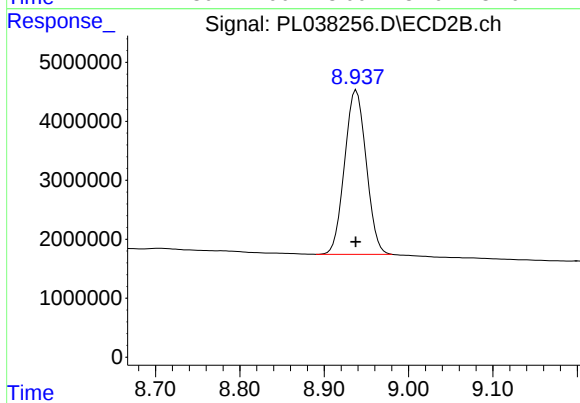

#28 Decachlorobiphenyl

R.T.: 8.938 min
Delta R.T.: 0.000 min
Response: 49576321
Conc: 20.28 ng/ml