

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
 Data File : PL038273.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2018 07:31
 Operator : AJ\SJ
 Sample : J4035-13
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 5-B

Manual Integrations
 APPROVED

Sohil
 7/19/2018 2:04:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 08:02:32 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.328	3.930	74283113	30998610	9.976	11.809
28) SA Decachlor...	7.998	8.937	71686765	30026924	9.450m	12.284 #
Target Compounds						
12) B 4,4'-DDE	5.441	6.242	85883551	24493458	8.958	9.160
17) MA 4,4'-DDT	6.187	7.022	12711326	4732083	1.711	2.220 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071818\
Data File : PL038273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2018 07:31
Operator : AJ\SJ
Sample : J4035-13
Misc :
ALS Vial : 64 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
5-B


Manual Integrations
APPROVED

Sohil
7/19/2018 2:04:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 08:02:32 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

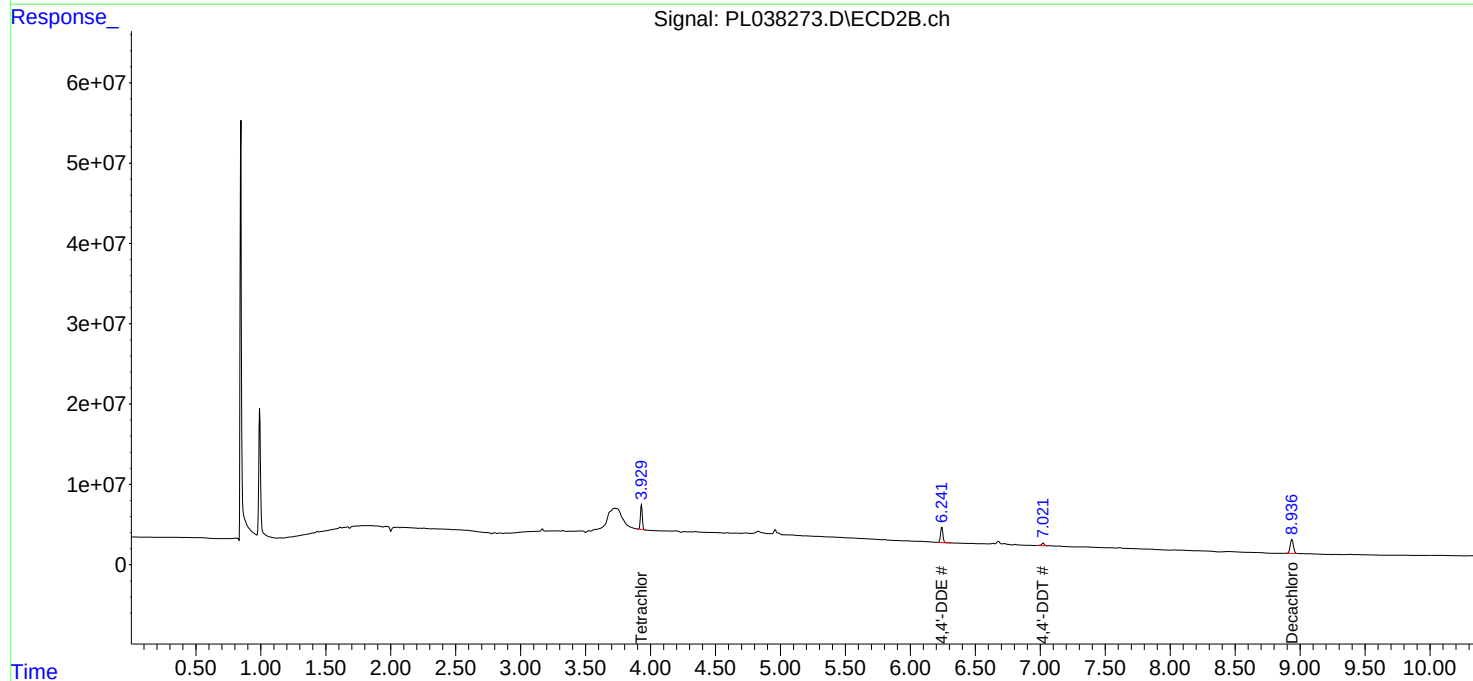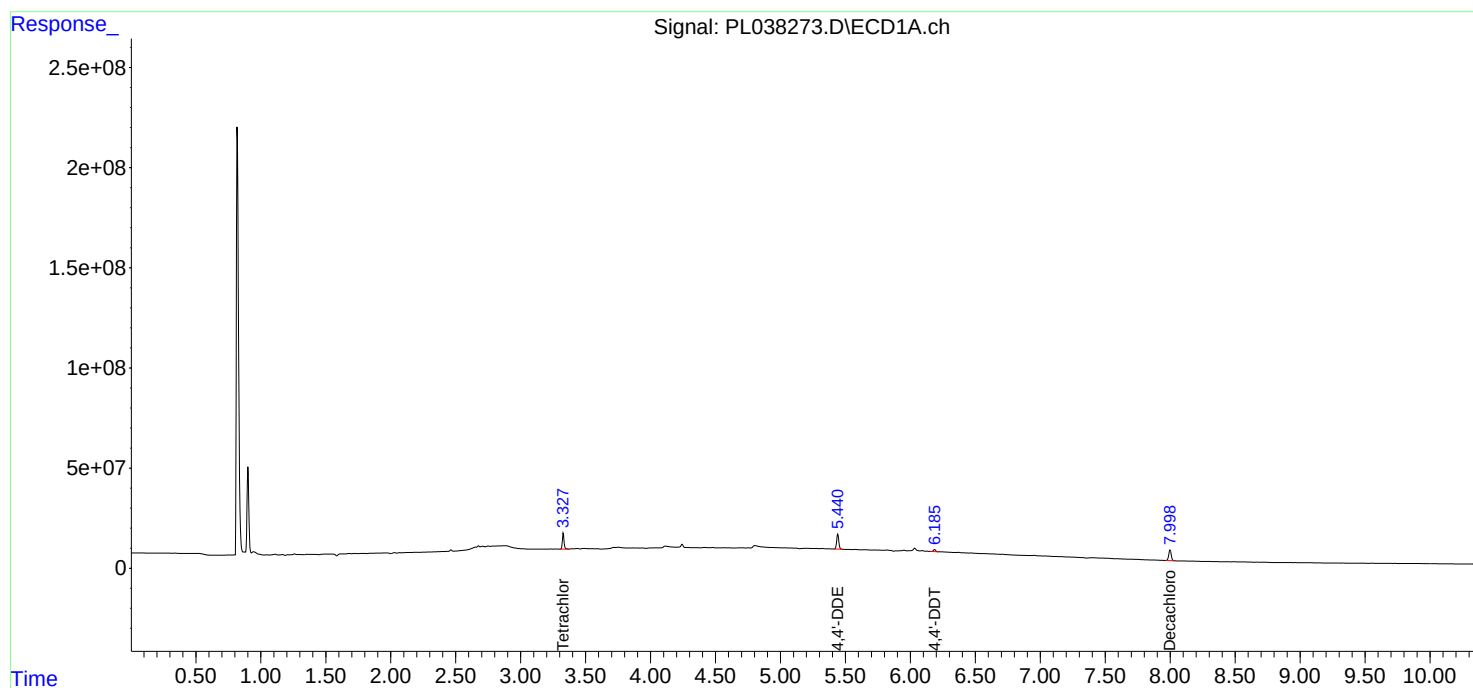

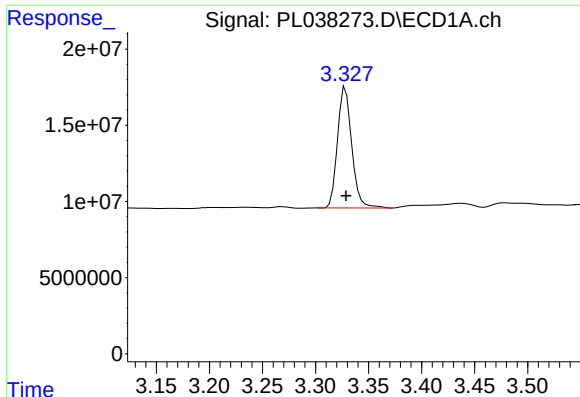


#1 Tetrachloro-m-xylene

R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 74283113
Conc: 9.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
5-B


Manual Integrations
APPROVED

Sohil
7/19/2018 2:04:23 PM

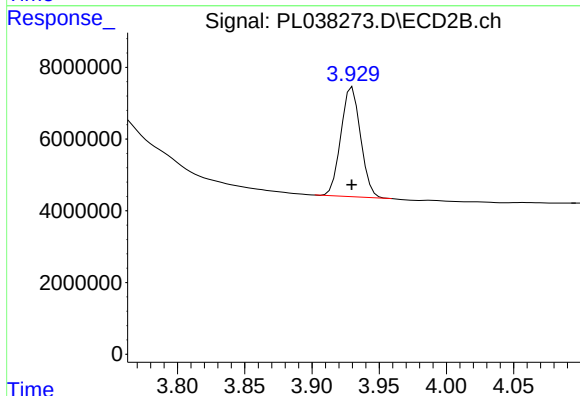


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 30998610
Conc: 11.81 ng/ml

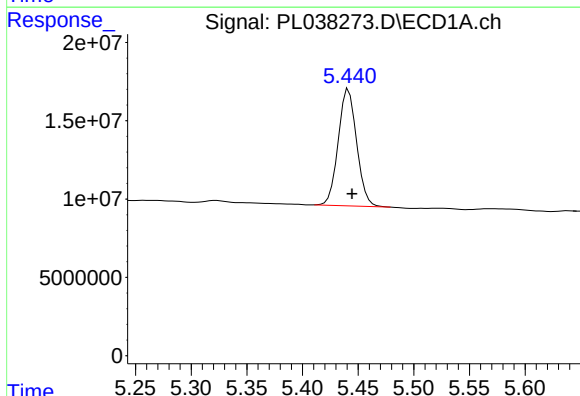


#12 4,4'-DDE

R.T.: 5.441 min
Delta R.T.: -0.003 min
Response: 85883551
Conc: 8.96 ng/ml

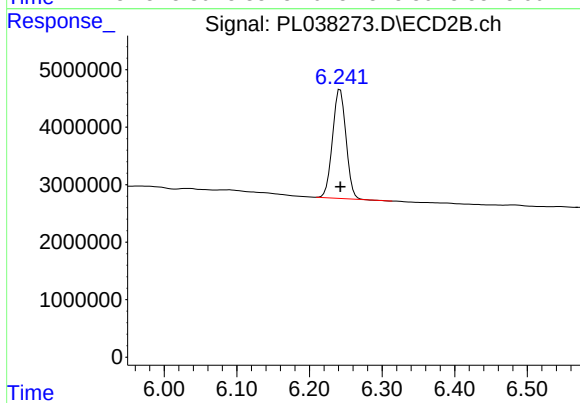

#12 4,4'-DDE

R.T.: 6.242 min
Delta R.T.: 0.000 min
Response: 24493458
Conc: 9.16 ng/ml

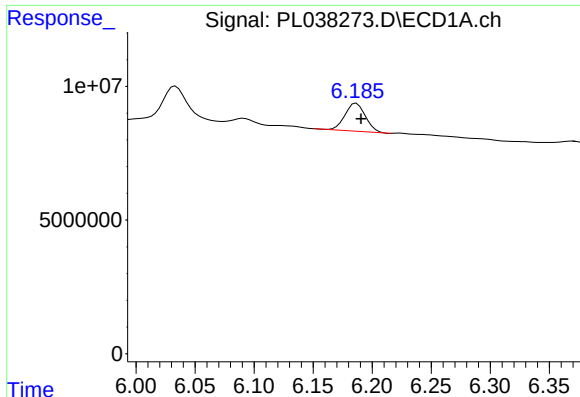


#17 4,4'-DDT

R.T.: 6.187 min
Delta R.T.: -0.004 min
Response: 12711326
Conc: 1.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
5-B


Manual Integrations
APPROVED

Sohil
7/19/2018 2:04:23 PM

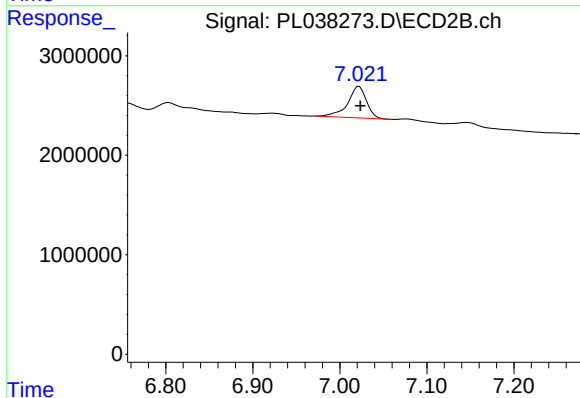


#17 4,4'-DDT

R.T.: 7.022 min
Delta R.T.: -0.001 min
Response: 4732083
Conc: 2.22 ng/ml

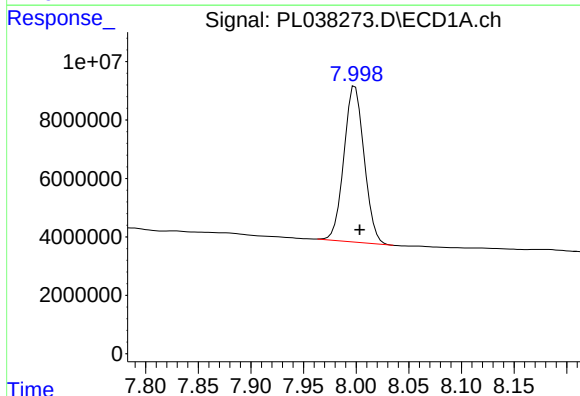

#28 Decachlorobiphenyl

R.T.: 7.998 min
Delta R.T.: -0.006 min
Response: 71686765
Conc: 9.45 ng/ml m

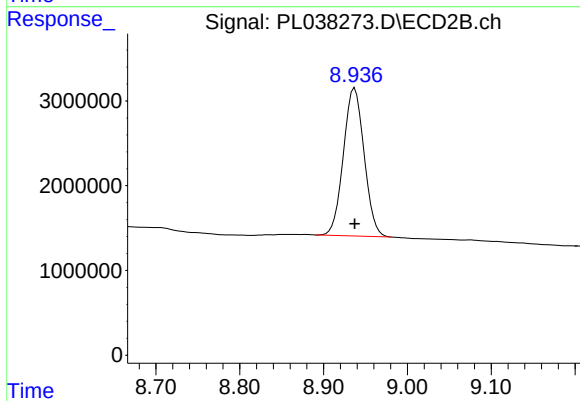

#28 Decachlorobiphenyl

R.T.: 8.937 min
Delta R.T.: 0.000 min
Response: 30026924
Conc: 12.28 ng/ml