

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
 Data File : PL050566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 18:27
 Operator : SM\AJ
 Sample : K3835-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-3(6-8)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 00:57:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 18 09:14:47 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.930	180.0E6	49747612	17.918	17.436
28)	SA Decachlor...	7.979	8.960	162.1E6	47006652	16.005	16.622
Target Compounds							
8)	B Heptachlo...	0.000	5.808f	0	5630655	N.D.	1.472 #
9)	A Endosulfan I	5.331f	0.000	6396203	0	0.440	N.D. #
10)	B gamma-Chl...	5.231f	0.000	61578490	0	3.902	N.D. #
11)	B alpha-Chl...	5.268	0.000	20478738	0	1.342	N.D. #
15)	B Endosulfa...	0.000	6.842	0	655311	N.D.	0.206 #
22)	Mirex	7.110	0.000	1650403	0	0.168	N.D. #
25)	Chlordane-3	5.231f	0.000	61578490	0	43.991	N.D. #
26)	Chlordane-4	5.268	0.000	20478738	0	15.526	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
Data File : PL050566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 18:27
Operator : SM\AJ
Sample : K3835-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
SB-3(6-8)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 00:57:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Thu Jul 18 09:14:47 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

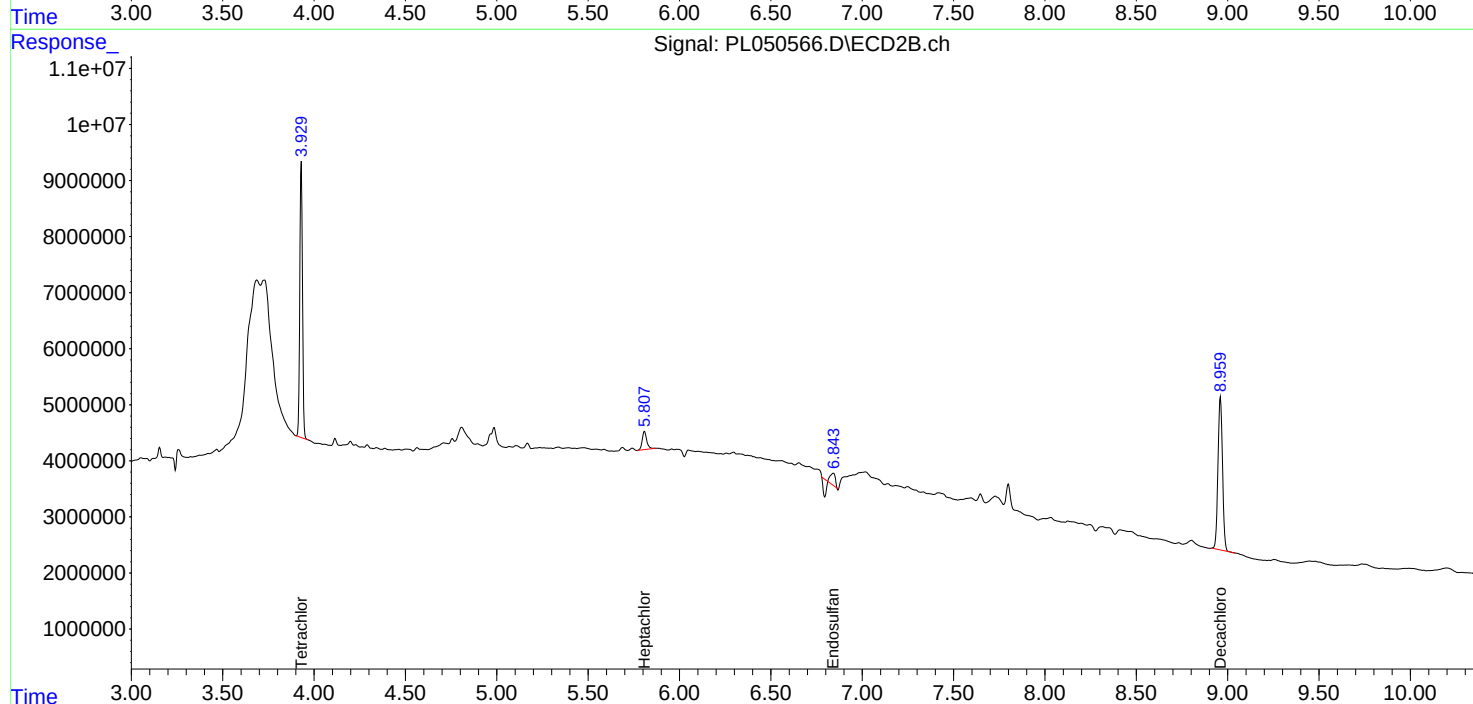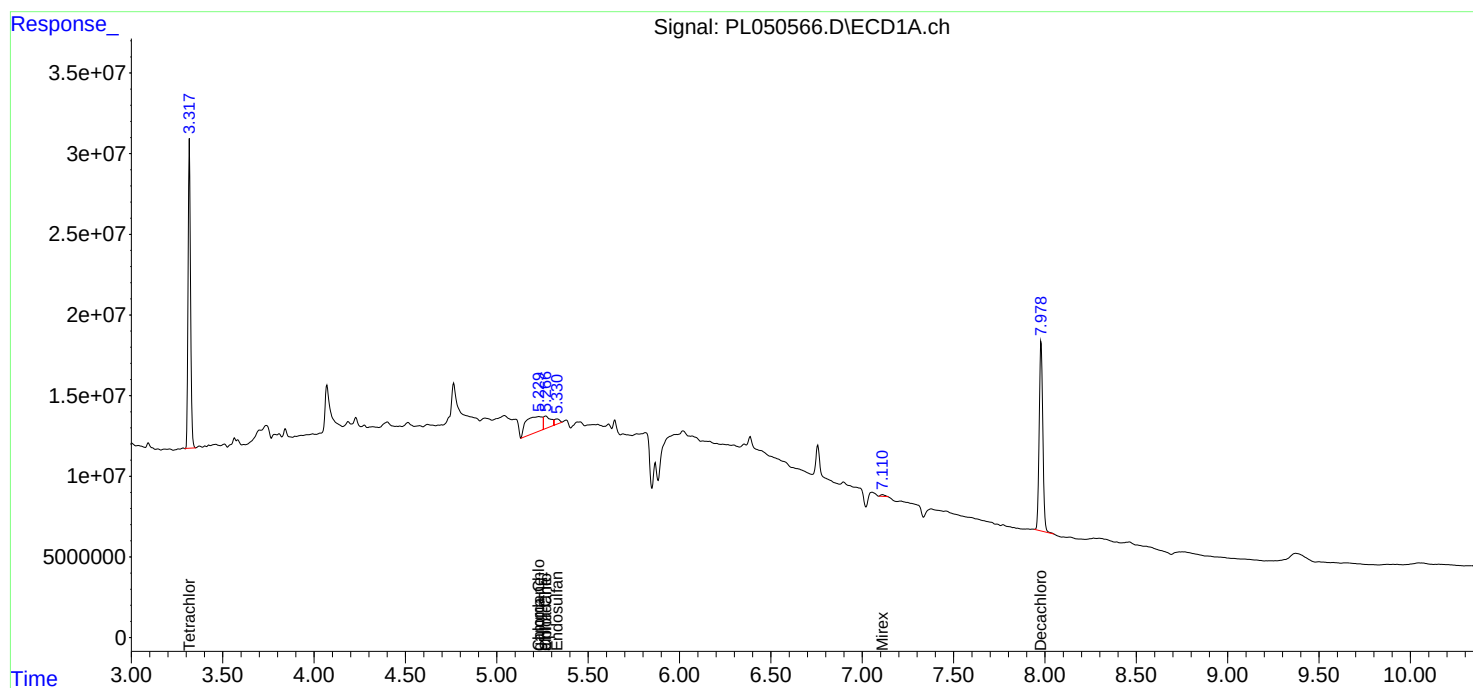


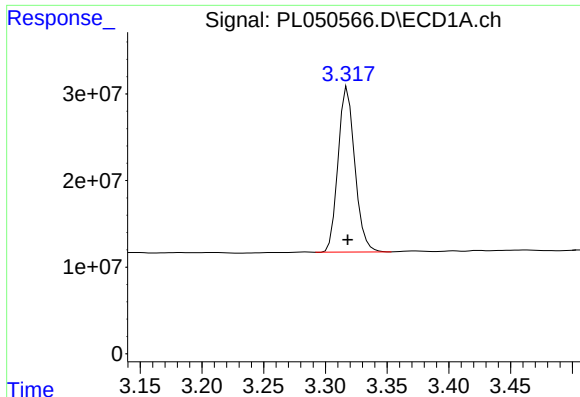

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 180040889
Conc: 17.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-3(6-8)

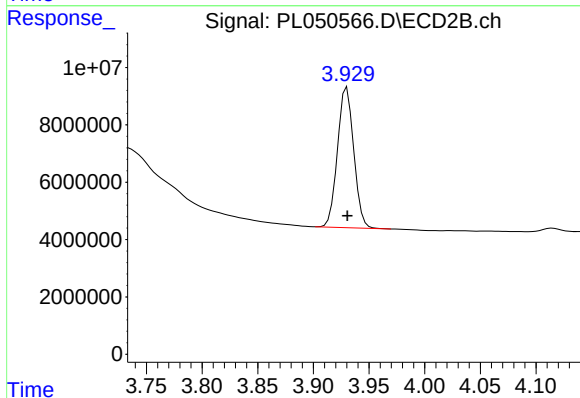


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 49747612
Conc: 17.44 ng/ml

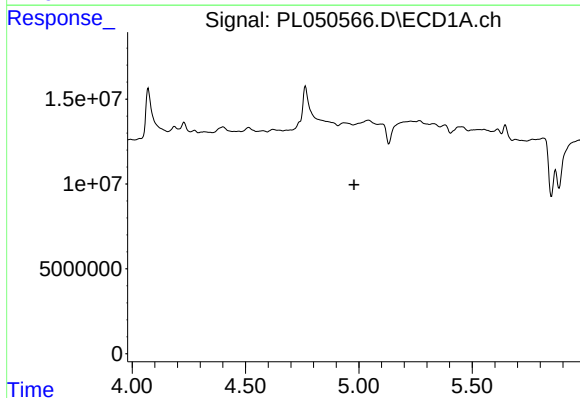


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

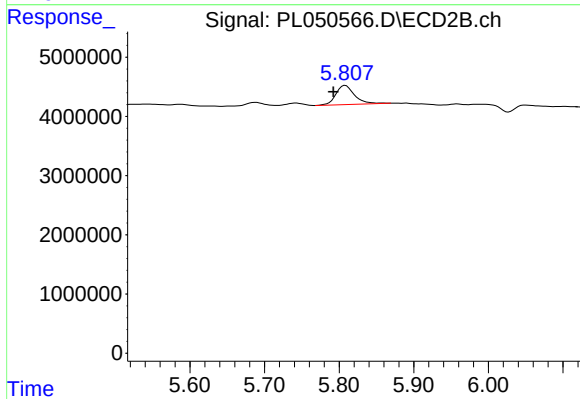

#8 Heptachlor epoxide


R.T.: 5.808 min
Delta R.T.: 0.016 min
Response: 5630655
Conc: 1.47 ng/ml

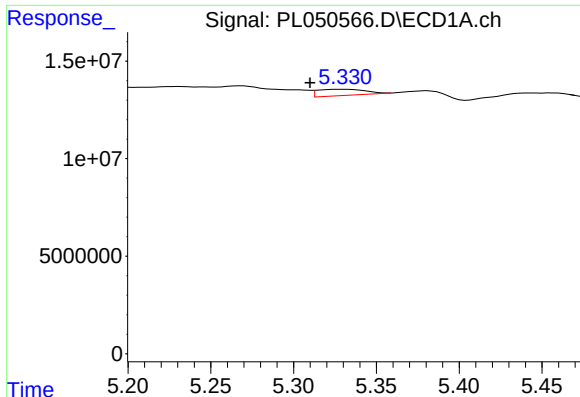

#9 Endosulfan I


R.T.: 5.331 min
Delta R.T.: 0.021 min
Response: 6396203
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-3(6-8)

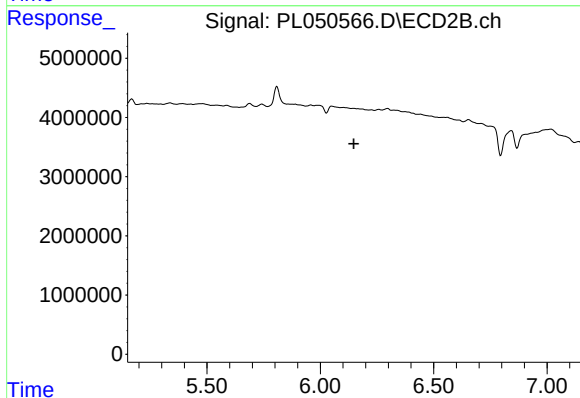


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

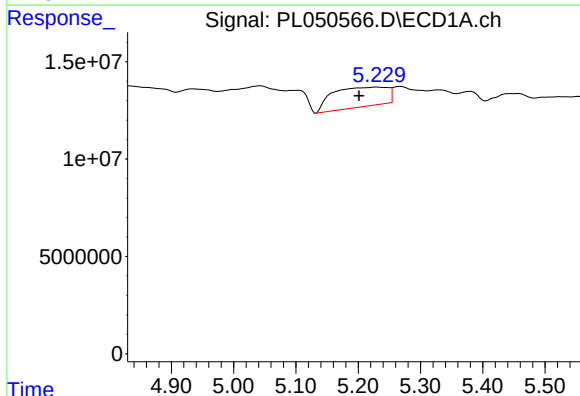


#10 gamma-Chlordane

R.T.: 5.231 min
Delta R.T.: 0.029 min
Response: 61578490
Conc: 3.90 ng/ml

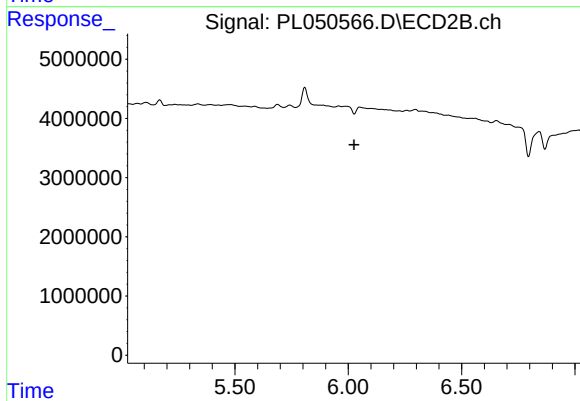

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

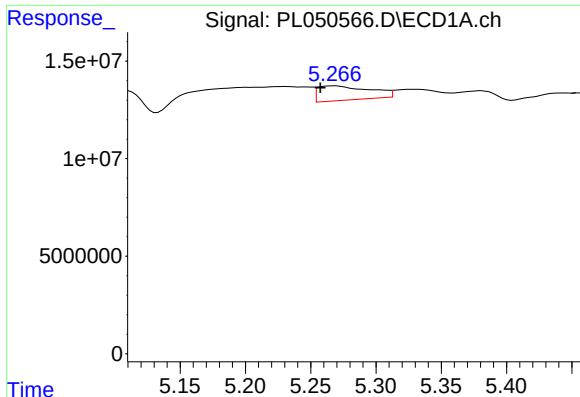

#11 alpha-Chlordane


R.T.: 5.268 min
Delta R.T.: 0.011 min
Response: 20478738
Conc: 1.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-3(6-8)

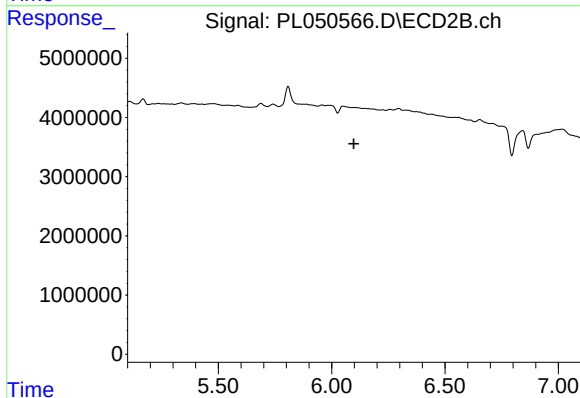


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

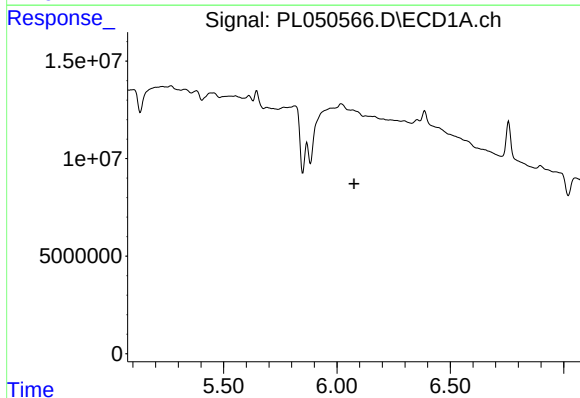


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

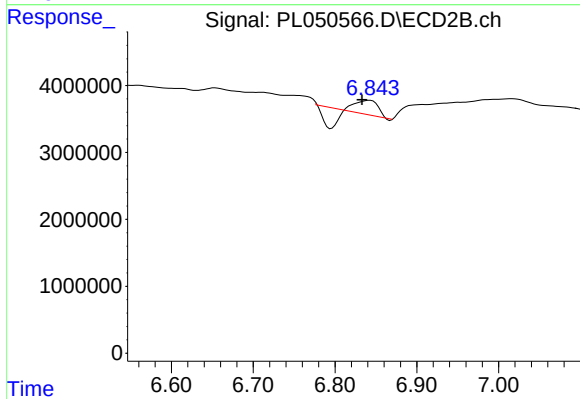

#15 Endosulfan II

R.T.: 6.842 min
Delta R.T.: 0.009 min
Response: 655311
Conc: 0.21 ng/ml

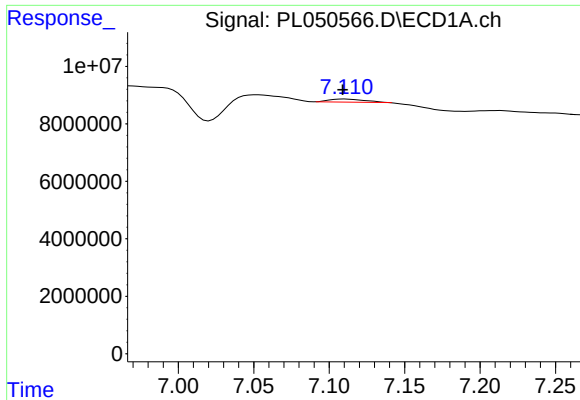

#22 Mirex


R.T.: 7.110 min

Delta R.T.: 0.001 min

Response: 1650403

Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-3(6-8)

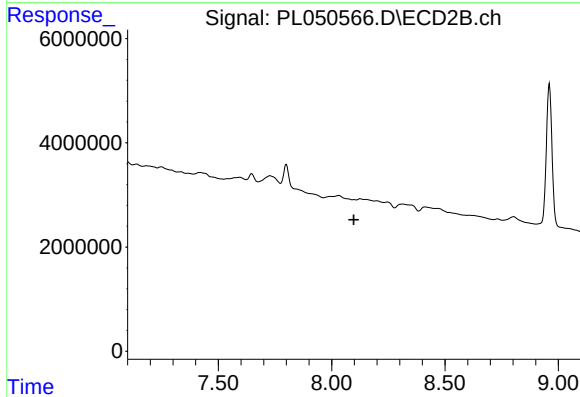


#22 Mirex

R.T.: 0.000 min

Exp R.T. : 8.097 min

Response: 0

Conc: N.D.

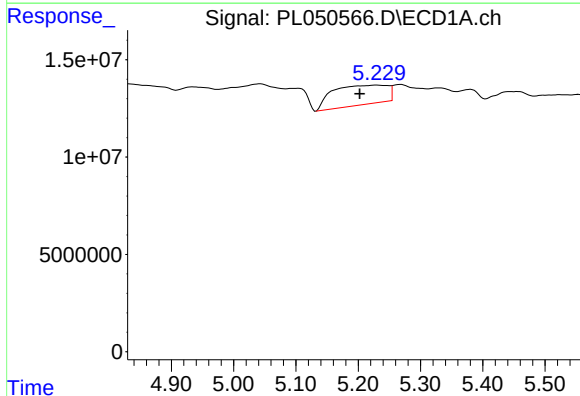


#25 Chlordane-3

R.T.: 5.231 min

Delta R.T.: 0.028 min

Response: 61578490

Conc: 43.99 ng/ml

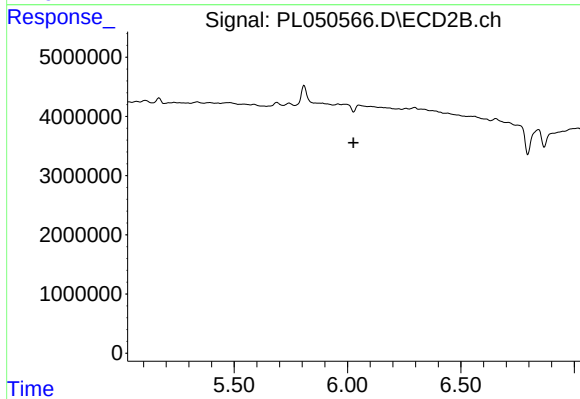


#25 Chlordane-3

R.T.: 0.000 min

Exp R.T. : 6.027 min

Response: 0


Conc: N.D.

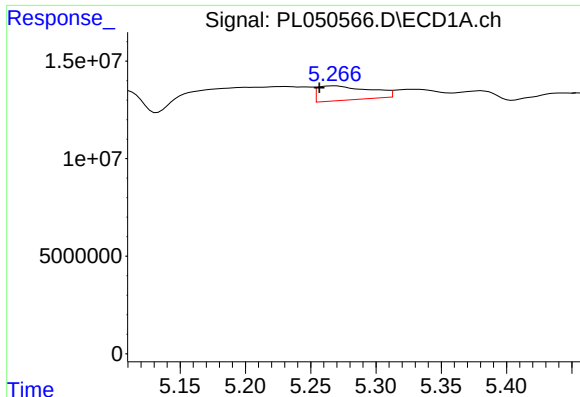

#26 Chlordane-4


R.T.: 5.268 min
Delta R.T.: 0.011 min
Response: 20478738
Conc: 15.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-3(6-8)

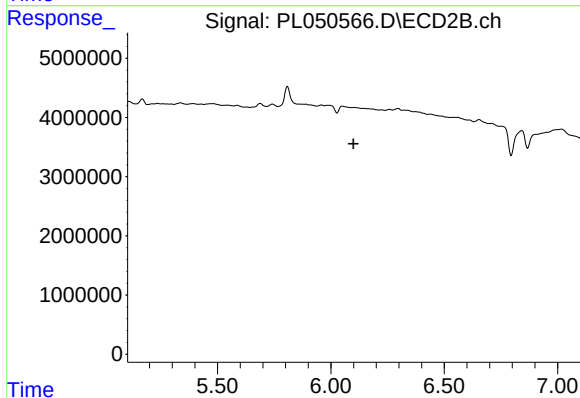


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

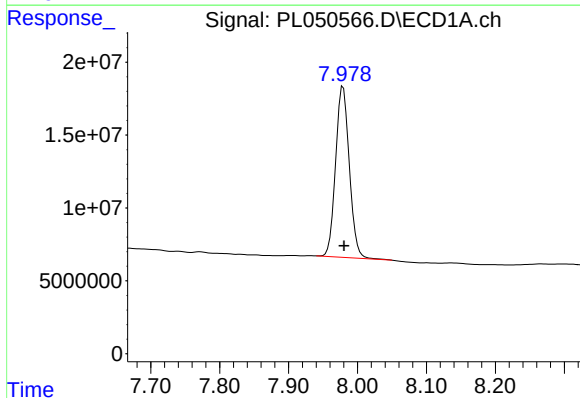

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.001 min
Response: 162060054
Conc: 16.01 ng/ml

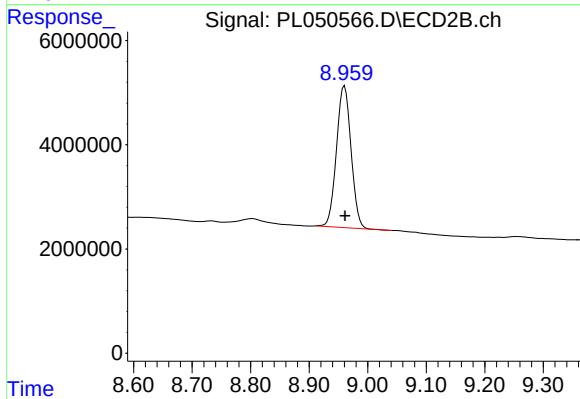

#28 Decachlorobiphenyl

R.T.: 8.960 min
Delta R.T.: -0.001 min
Response: 47006652
Conc: 16.62 ng/ml