

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
 Data File : PL050570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 19:24
 Operator : SM\AJ
 Sample : K3835-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-5(7-9)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 00:58:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 18 09:14:47 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.930	172.4E6	48463368	17.158	16.986
28)	SA Decachlor...	7.980	8.960	165.0E6	46997285	16.293	16.619
Target Compounds							
8)	B Heptachlo...	0.000	5.807	0	6876967	N.D.	1.798 #
9)	A Endosulfan I	5.334f	0.000	6384693	0	0.439	N.D. #
10)	B gamma-Chl...	5.196	0.000	30565836	0	1.937	N.D. #
11)	B alpha-Chl...	5.268	0.000	33656462	0	2.206	N.D. #
16)	A 4,4'-DDD	5.935	0.000	4705541	0	0.393	N.D. #
22)	Mirex	7.110	0.000	1843184	0	0.188	N.D. #
25)	Chlordane-3	5.196	0.000	30565836	0	21.836	N.D. #
26)	Chlordane-4	5.268	0.000	33656462	0	25.517	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
Data File : PL050570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 19:24
Operator : SM\AJ
Sample : K3835-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB-5(7-9)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 00:58:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Thu Jul 18 09:14:47 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

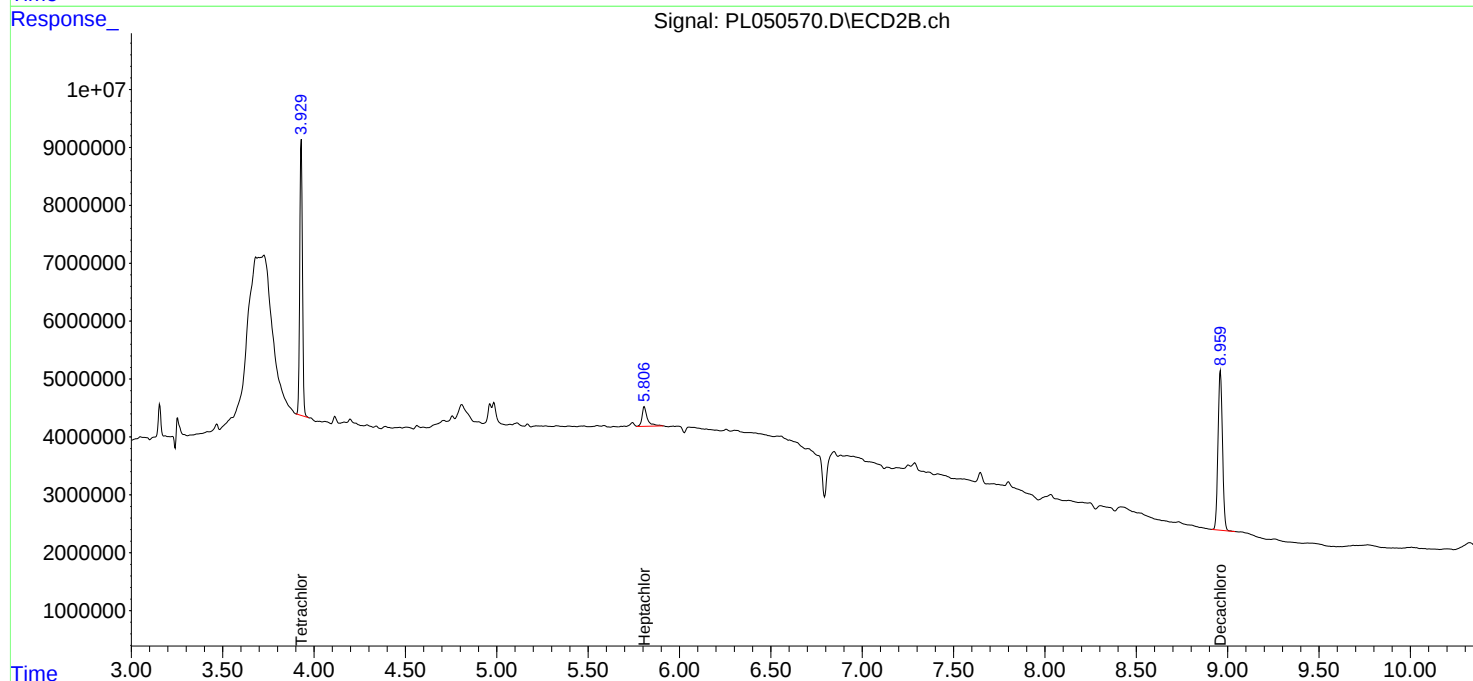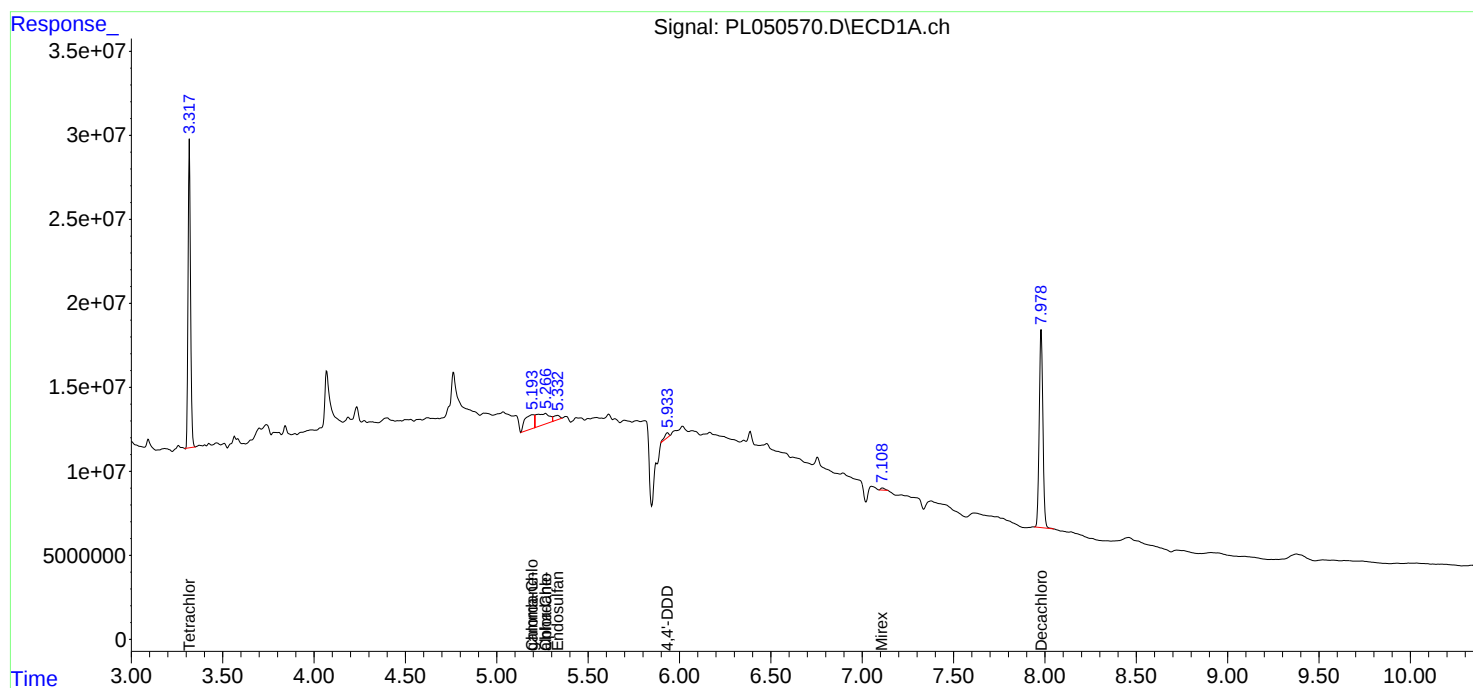


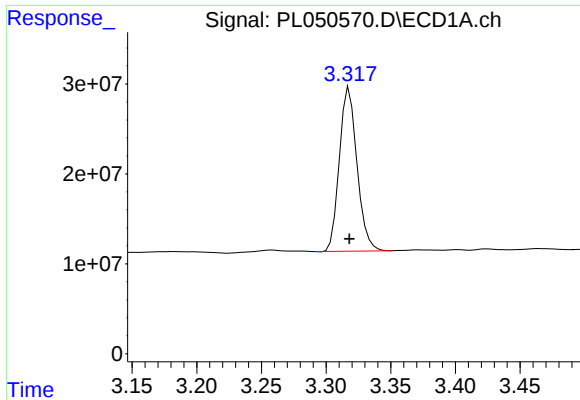

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 172400463
Conc: 17.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-5(7-9)

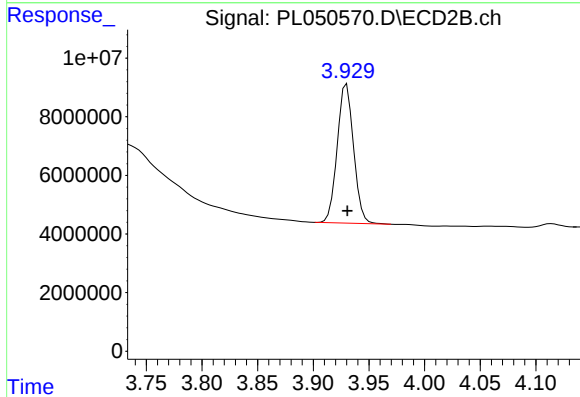


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 48463368
Conc: 16.99 ng/ml

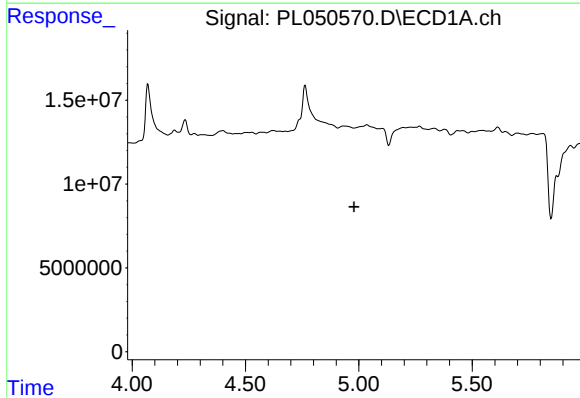


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

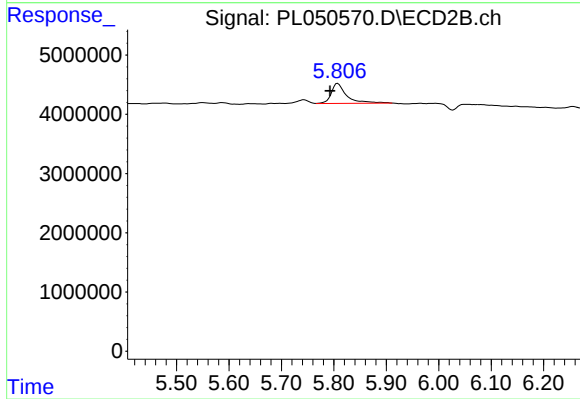

#8 Heptachlor epoxide


R.T.: 5.807 min
Delta R.T.: 0.015 min
Response: 6876967
Conc: 1.80 ng/ml

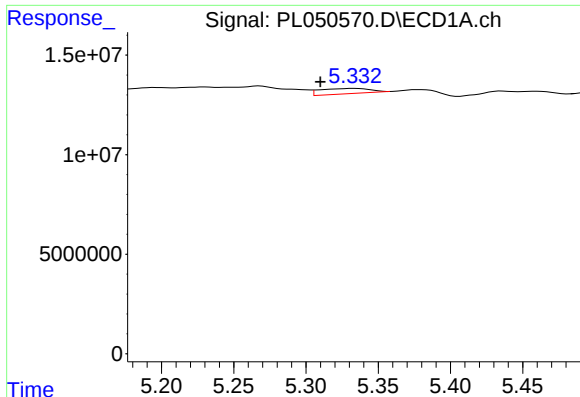

#9 Endosulfan I


R.T.: 5.334 min
Delta R.T.: 0.024 min
Response: 6384693
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-5(7-9)

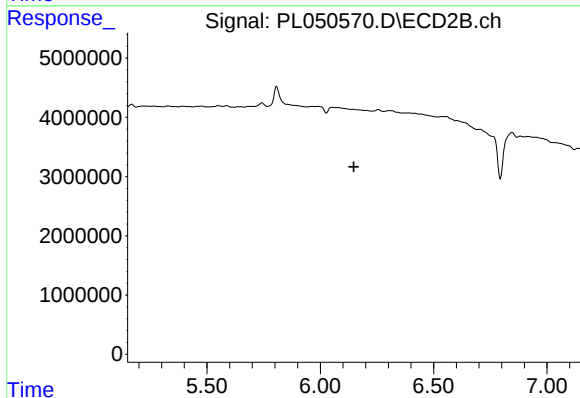


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

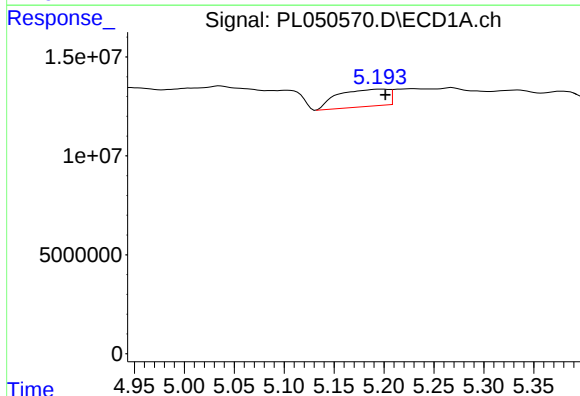


#10 gamma-Chlordane

R.T.: 5.196 min
Delta R.T.: -0.005 min
Response: 30565836
Conc: 1.94 ng/ml

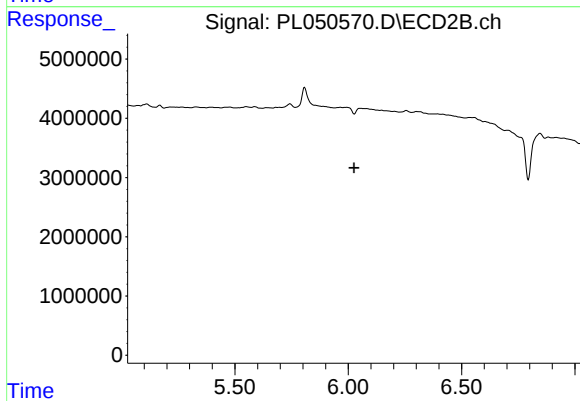

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

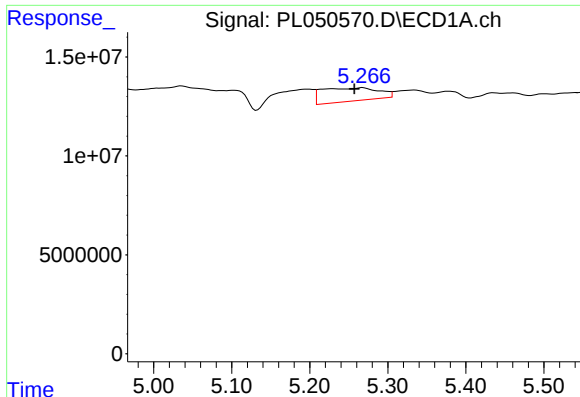

#11 alpha-Chlordane


R.T.: 5.268 min
Delta R.T.: 0.011 min
Response: 33656462
Conc: 2.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-5(7-9)

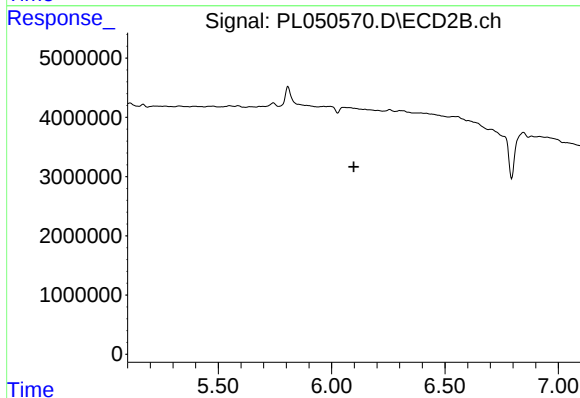


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

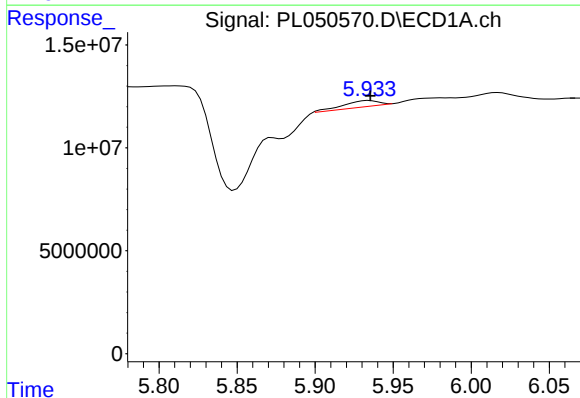


#16 4,4'-DDD

R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 4705541
Conc: 0.39 ng/ml

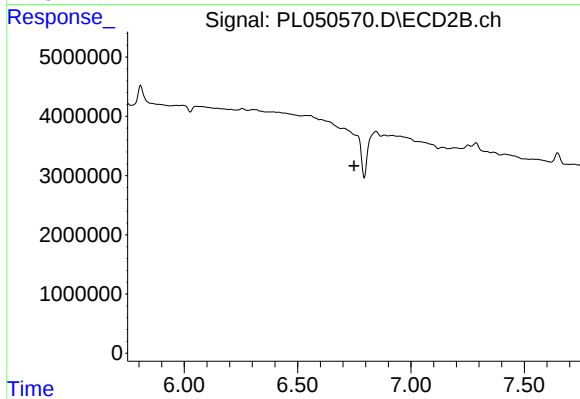

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

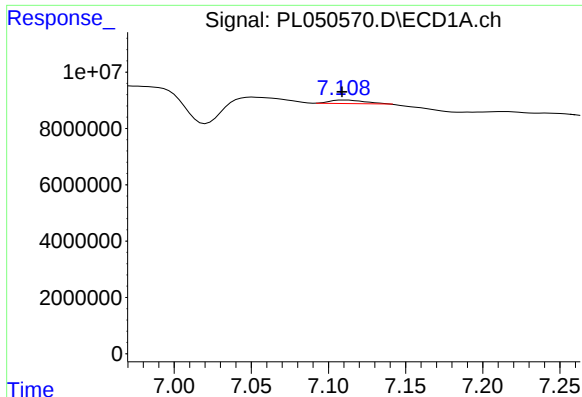

#22 Mirex


R.T.: 7.110 min
Delta R.T.: 0.001 min
Response: 1843184
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-5(7-9)

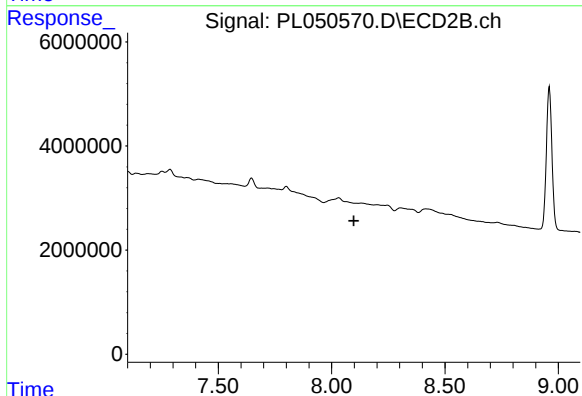


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.097 min
Response: 0
Conc: N.D.

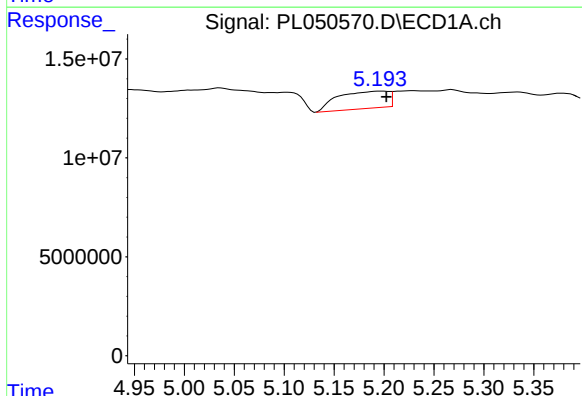


#25 Chlordane-3

R.T.: 5.196 min
Delta R.T.: -0.006 min
Response: 30565836
Conc: 21.84 ng/ml

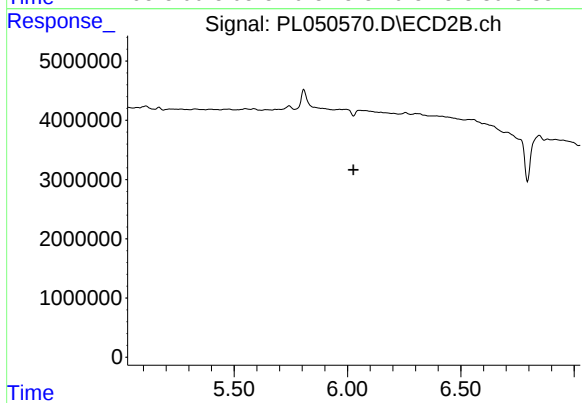

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

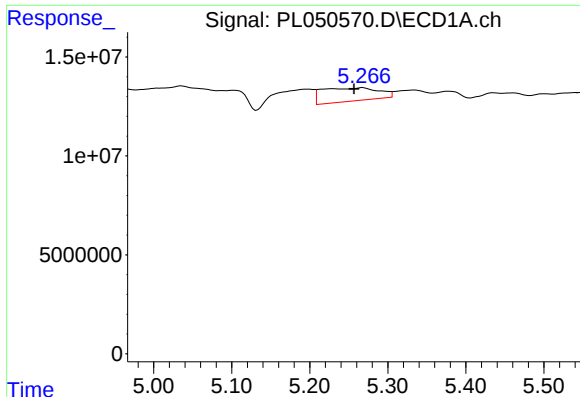

#26 Chlordane-4


R.T.: 5.268 min
Delta R.T.: 0.011 min
Response: 33656462
Conc: 25.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-5(7-9)

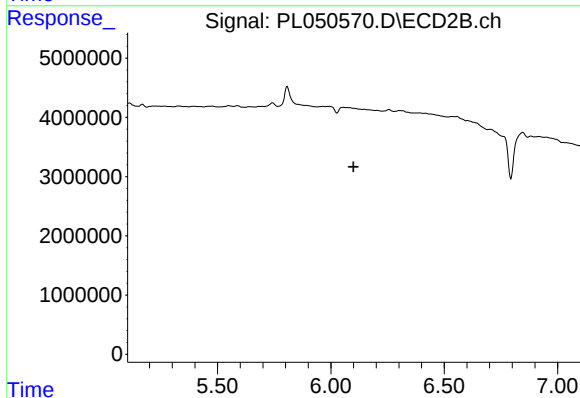


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

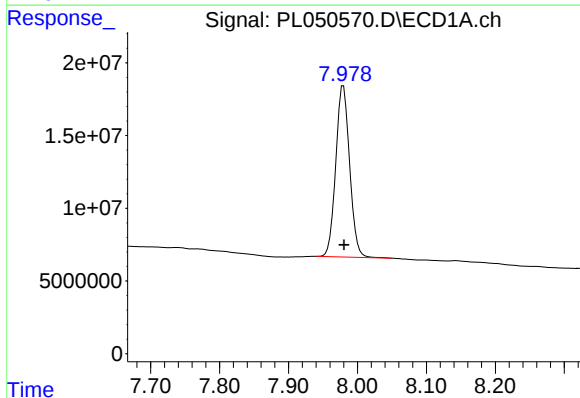

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 164974191
Conc: 16.29 ng/ml

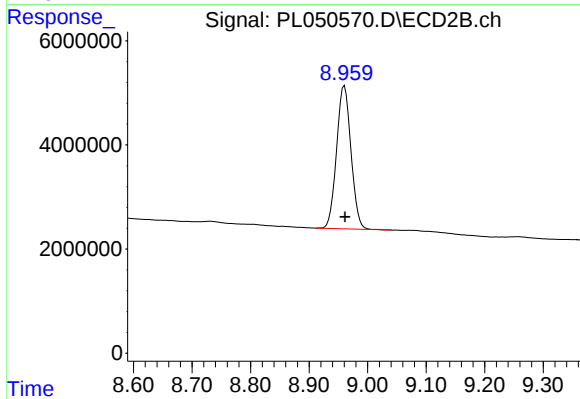

#28 Decachlorobiphenyl

R.T.: 8.960 min
Delta R.T.: -0.001 min
Response: 46997285
Conc: 16.62 ng/ml