

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
 Data File : PL050580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 22:02
 Operator : SM\AJ
 Sample : K3835-28
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-10(8-10)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:44:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.930	209.0E6	57789932	20.800	20.254
28)	SA Decachlor...	7.981	8.962	200.0E6	56023759	19.756	19.811
Target Compounds							
7)	B delta-BHC	0.000	4.985	0	8003691	N.D.	2.069 #
8)	B Heptachlo...	0.000	5.807	0	13609841	N.D.	3.558 #
9)	A Endosulfan I	5.332f	0.000	7104566	0	0.488	N.D. #
10)	B gamma-Chl...	5.226f	0.000	63972487	0	4.053	N.D. #
11)	B alpha-Chl...	5.267	0.000	22971640	0	1.506	N.D. #
15)	B Endosulfa...	0.000	6.846	0	323670	N.D.	0.102 #
22)	Mirex	7.113	0.000	2647929	0	0.270	N.D. #
25)	Chlordane-3	5.226f	0.000	63972487	0	45.702	N.D. #
26)	Chlordane-4	5.267	0.000	22971640	0	17.416	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
Data File : PL050580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 22:02
Operator : SM\AJ
Sample : K3835-28
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB-10(8-10)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:44:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

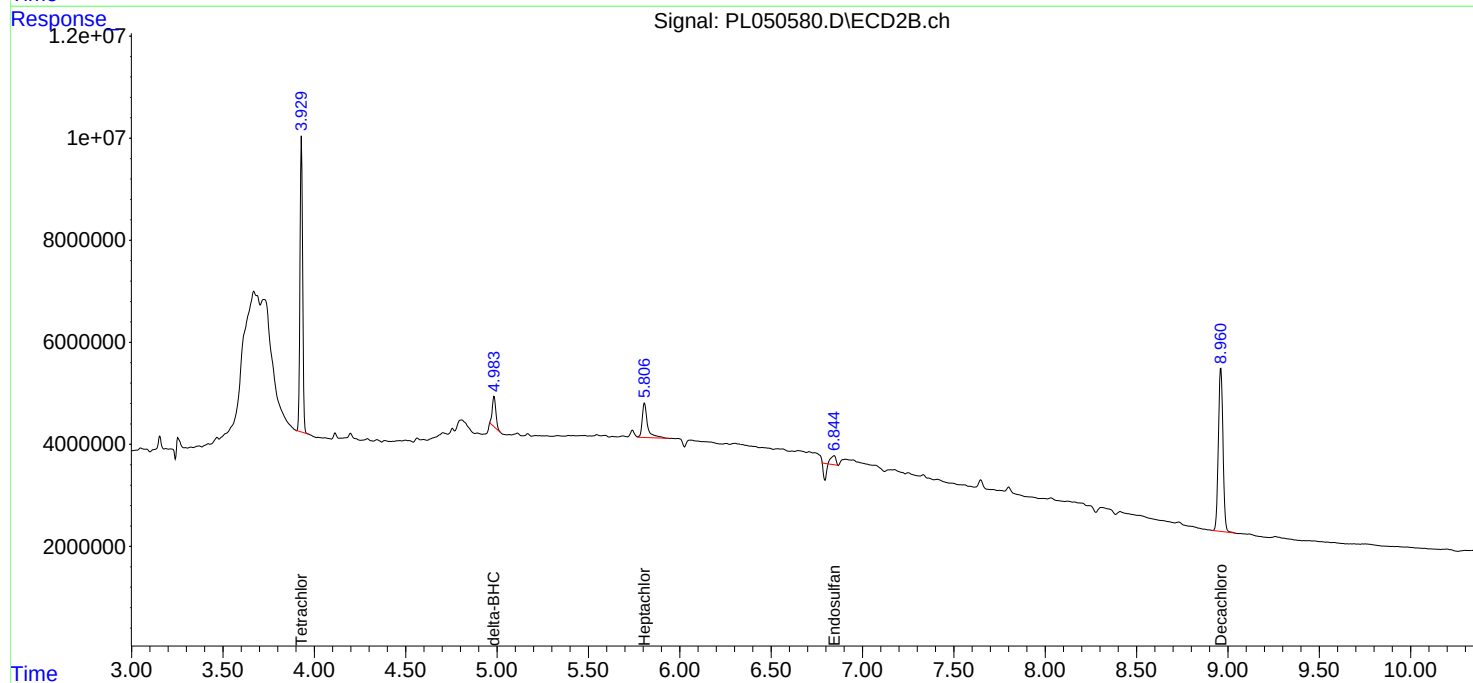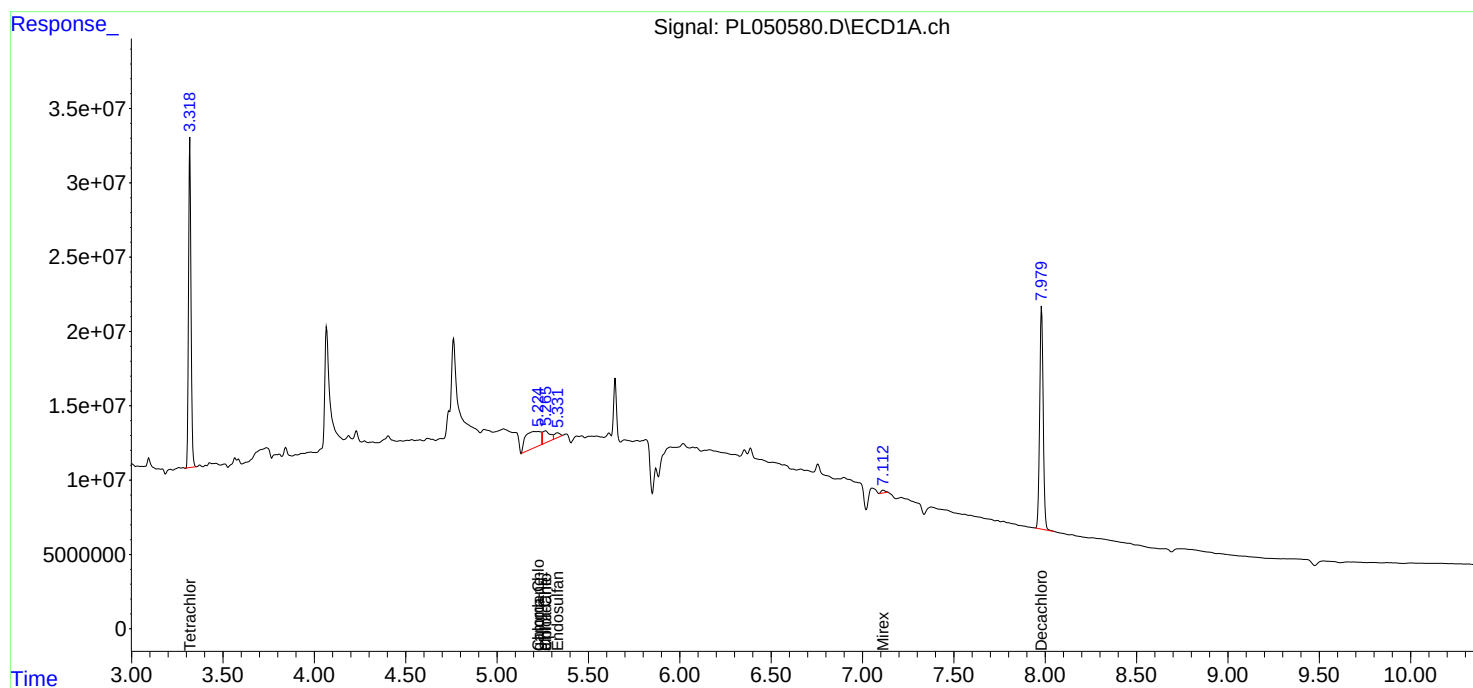


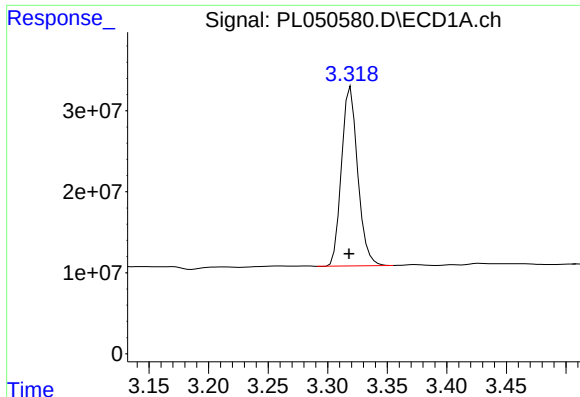

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.001 min
Response: 208995659
Conc: 20.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-10(8-10)

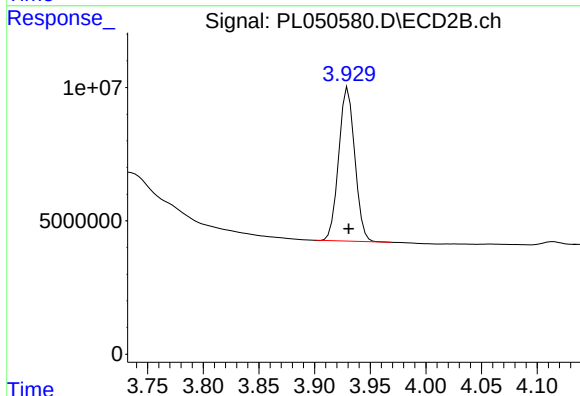


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 57789932
Conc: 20.25 ng/ml

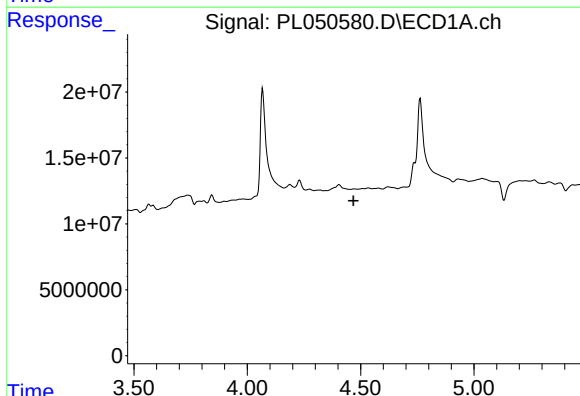


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

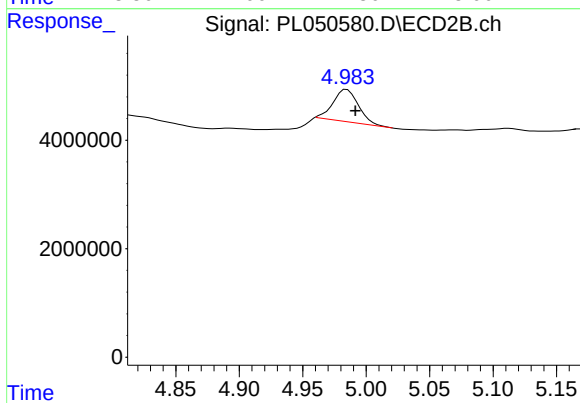

#7 delta-BHC


R.T.: 4.985 min
Delta R.T.: -0.007 min
Response: 8003691
Conc: 2.07 ng/ml

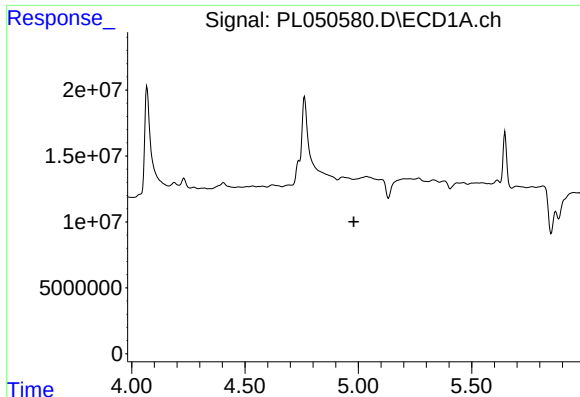

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-10(8-10)

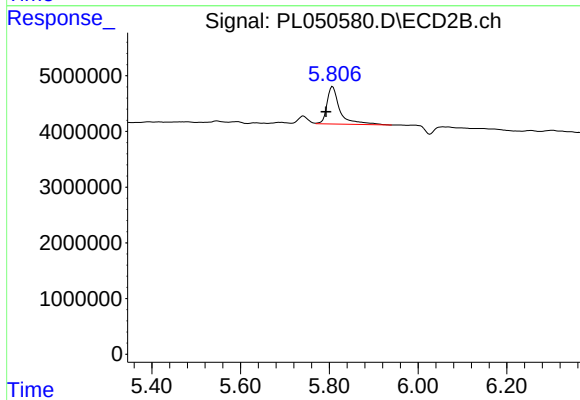


#8 Heptachlor epoxide

R.T.: 5.807 min
Delta R.T.: 0.015 min
Response: 13609841
Conc: 3.56 ng/ml

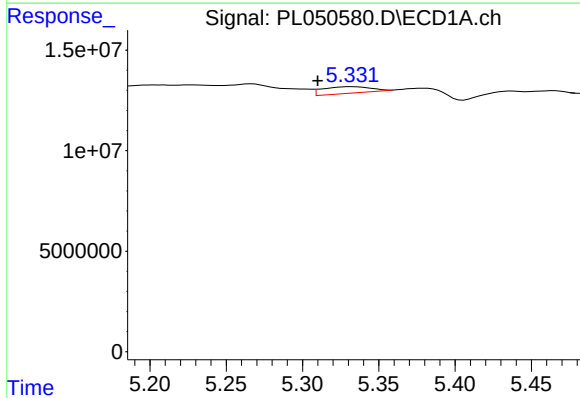


#9 Endosulfan I

R.T.: 5.332 min
Delta R.T.: 0.023 min
Response: 7104566
Conc: 0.49 ng/ml

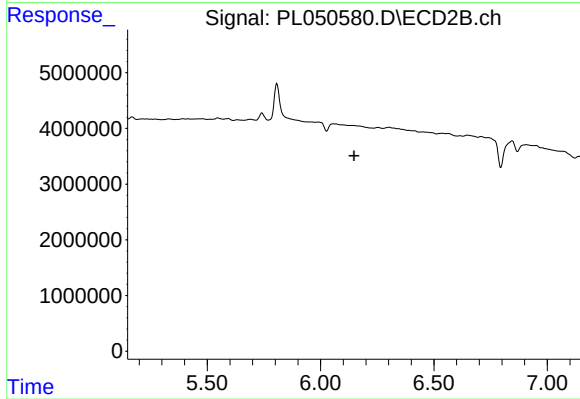

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

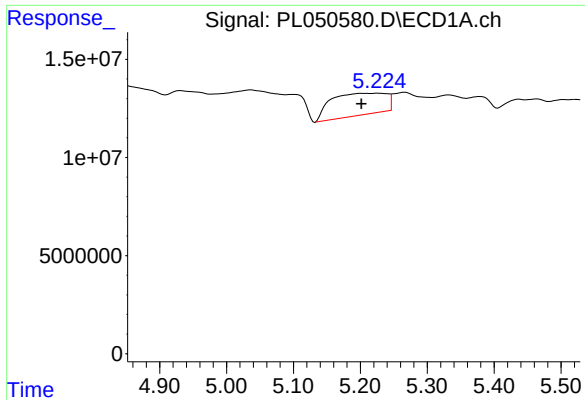

#10 gamma-Chlordane


R.T.: 5.226 min
Delta R.T.: 0.024 min
Response: 63972487
Conc: 4.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-10(8-10)

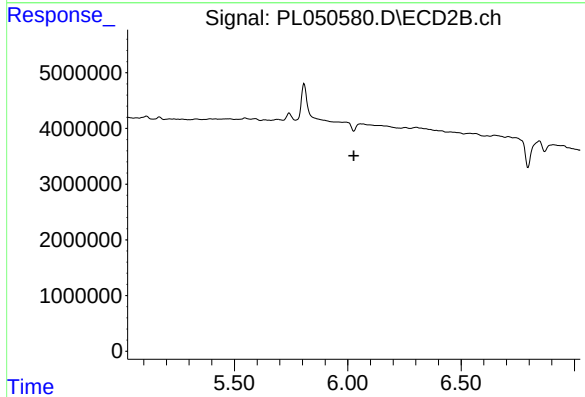


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

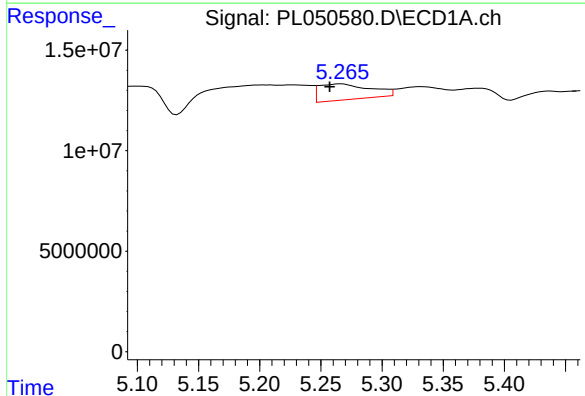


#11 alpha-Chlordane

R.T.: 5.267 min
Delta R.T.: 0.009 min
Response: 22971640
Conc: 1.51 ng/ml

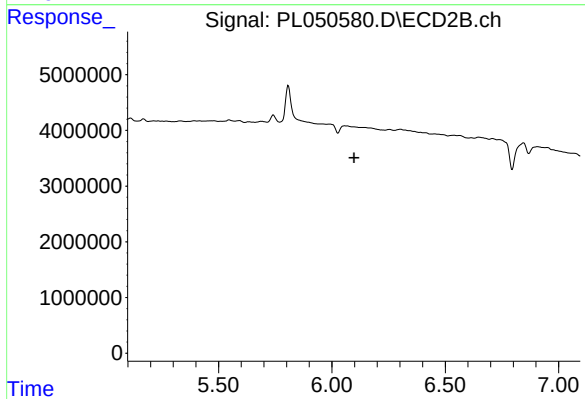

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.098 min
Response: 0
Conc: N.D.

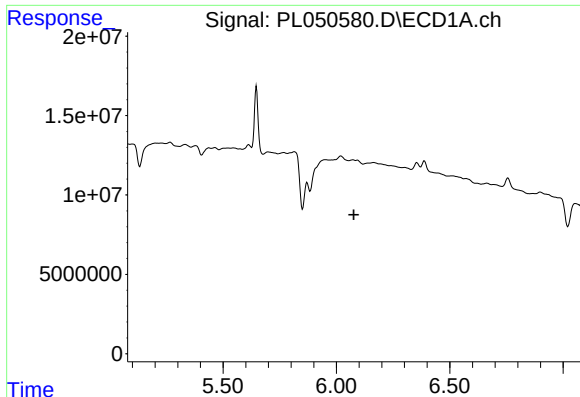

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-10(8-10)

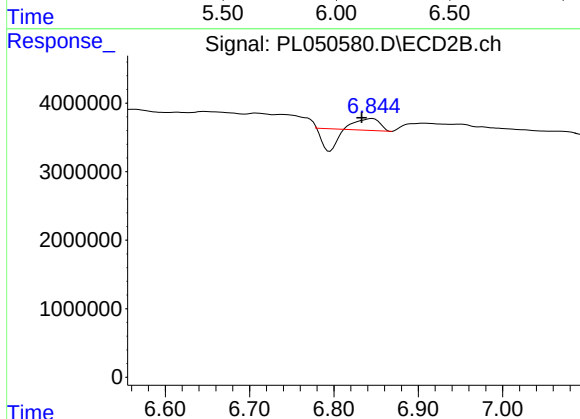


#15 Endosulfan II

R.T.: 6.846 min
Delta R.T.: 0.012 min
Response: 323670
Conc: 0.10 ng/ml

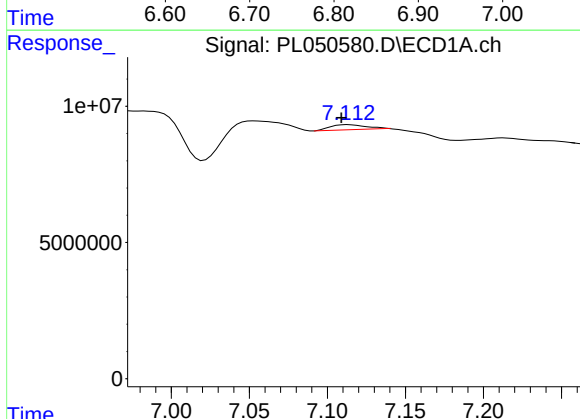


#22 Mirex

R.T.: 7.113 min
Delta R.T.: 0.004 min
Response: 2647929
Conc: 0.27 ng/ml

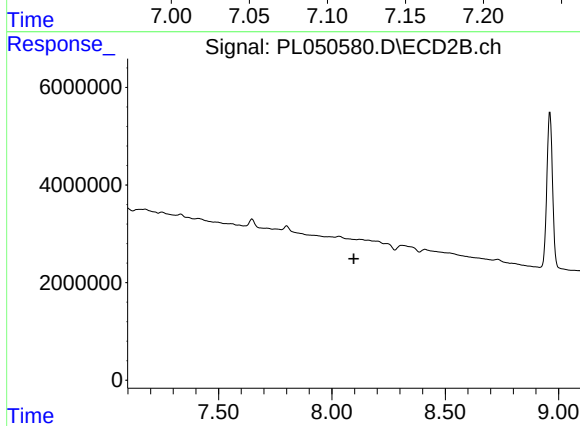

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.097 min
Response: 0
Conc: N.D.

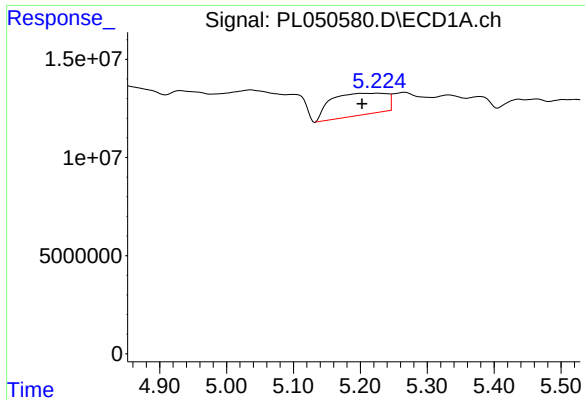

#25 Chlordane-3


R.T.: 5.226 min
Delta R.T.: 0.024 min
Response: 63972487
Conc: 45.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-10(8-10)

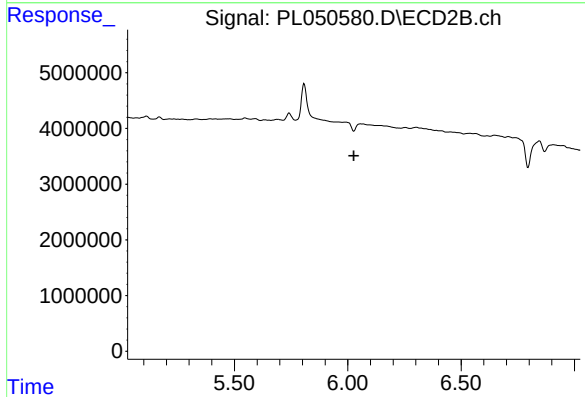


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

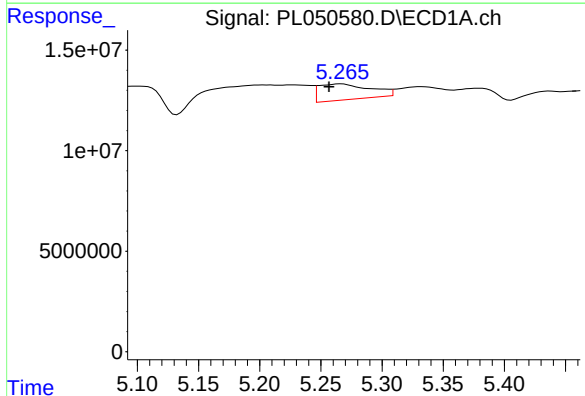


#26 Chlordane-4

R.T.: 5.267 min
Delta R.T.: 0.010 min
Response: 22971640
Conc: 17.42 ng/ml

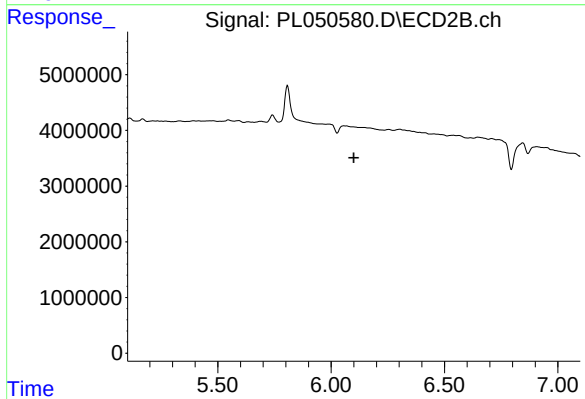

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

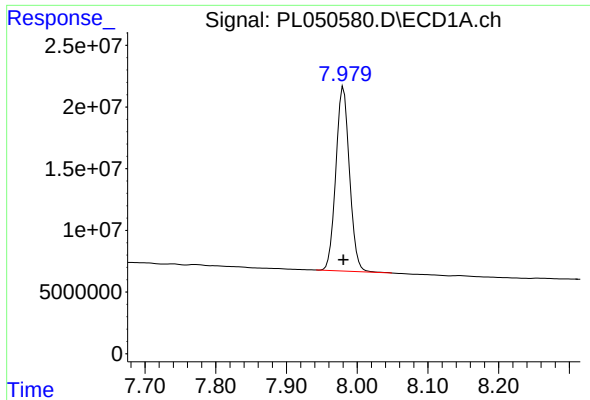

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 200032962
Conc: 19.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-10(8-10)

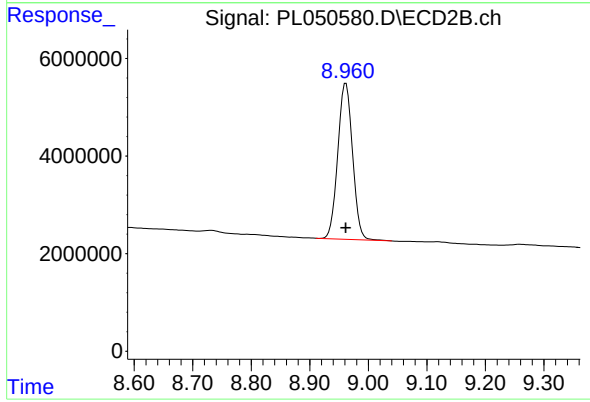

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: 0.000 min
Response: 56023759
Conc: 19.81 ng/ml