

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
 Data File : PL050586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 23:48
 Operator : SM\AJ
 Sample : K3835-32
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-7(13-15)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:46:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.930	154.8E6	43424494	15.407	15.220
28)	SA Decachlor...	7.981	8.962	153.3E6	42128762	15.142	14.897
Target Compounds							
6)	B beta-BHC	0.000	4.757f	0	180606	N.D.	0.104 #
8)	B Heptachlo...	0.000	5.809f	0	7719581	N.D.	2.018 #
9)	A Endosulfan I	5.333f	0.000	11438840	0	0.787	N.D. #
10)	B gamma-Chl...	5.202	0.000	42978423	0	2.723	N.D. #
11)	B alpha-Chl...	5.269	0.000	24284273	0	1.592	N.D. #
25)	Chlordane-3	5.202	0.000	42978423	0	30.704	N.D. #
26)	Chlordane-4	5.269	0.000	24284273	0	18.411	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
Data File : PL050586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 23:48
Operator : SM\AJ
Sample : K3835-32
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
SB-7(13-15)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:46:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

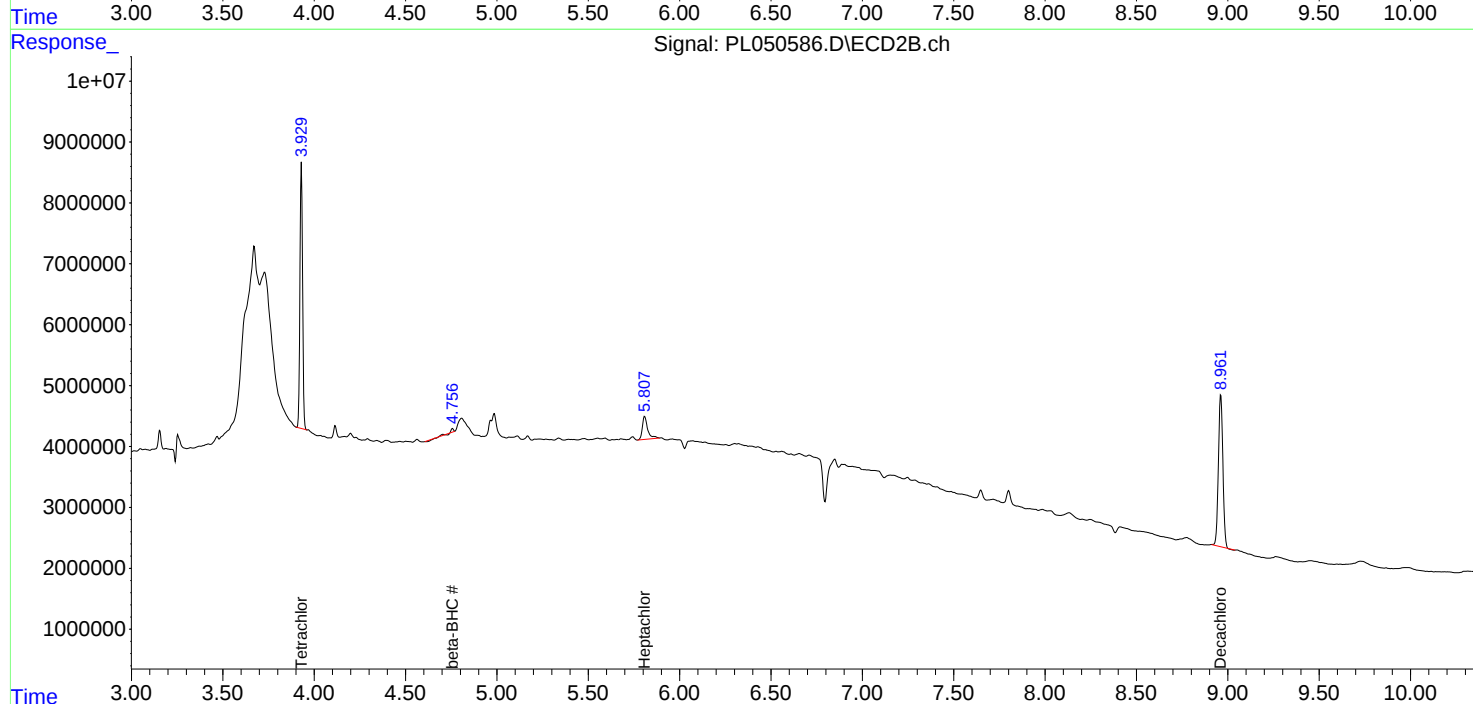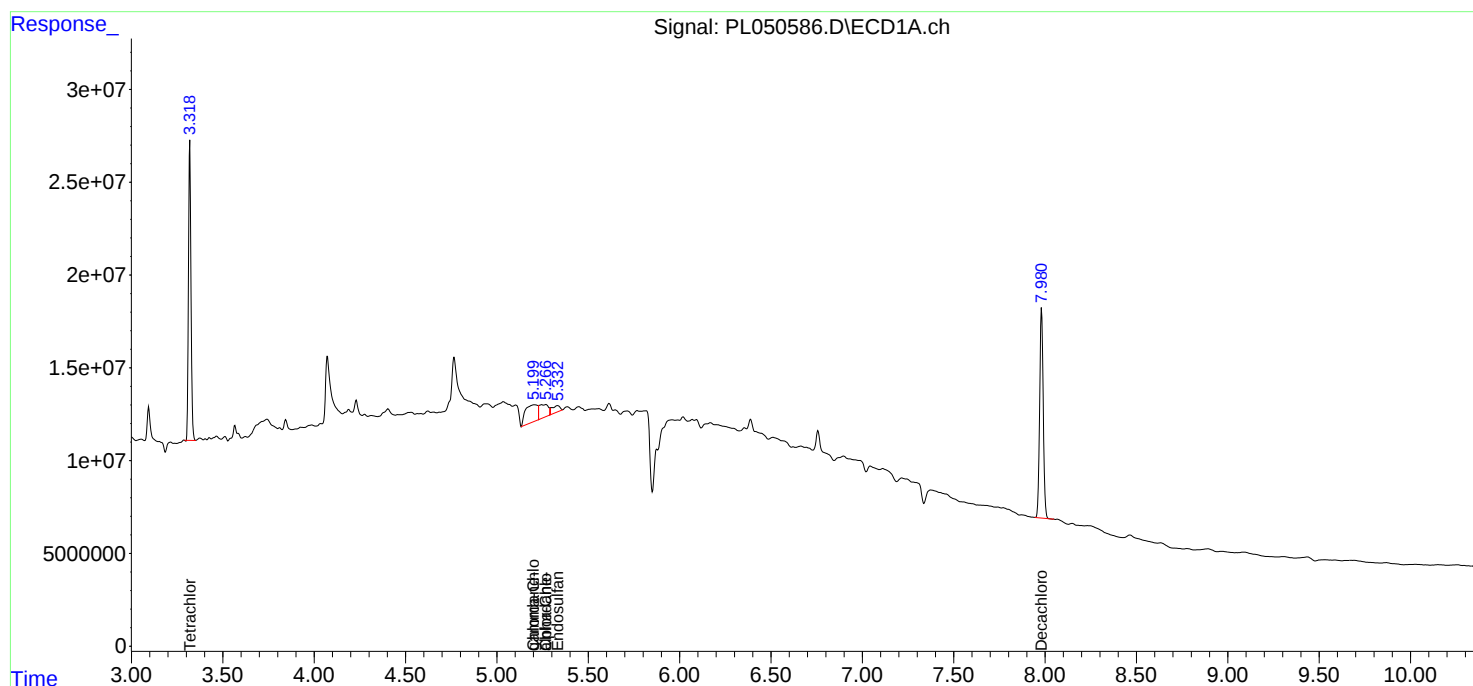


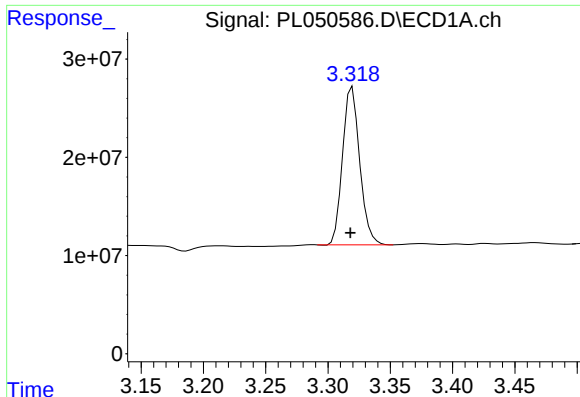

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.001 min
Response: 154803362
Conc: 15.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7(13-15)

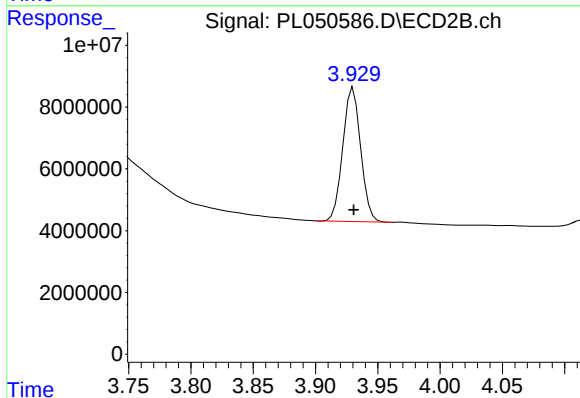


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 43424494
Conc: 15.22 ng/ml

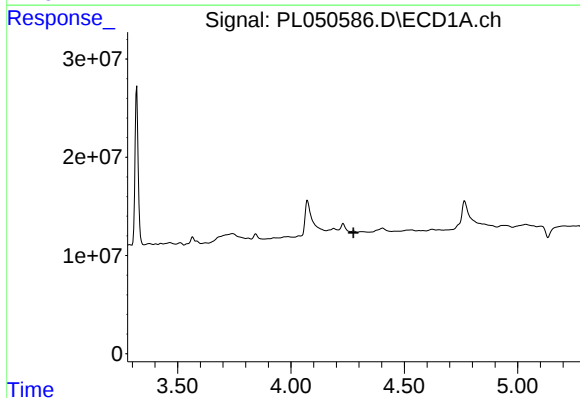


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

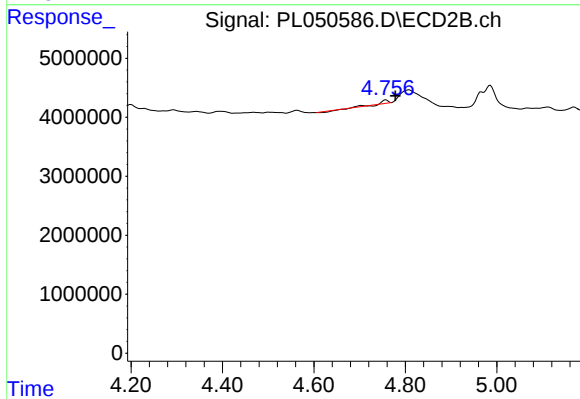

#6 beta-BHC


R.T.: 4.757 min
Delta R.T.: -0.021 min
Response: 180606
Conc: 0.10 ng/ml

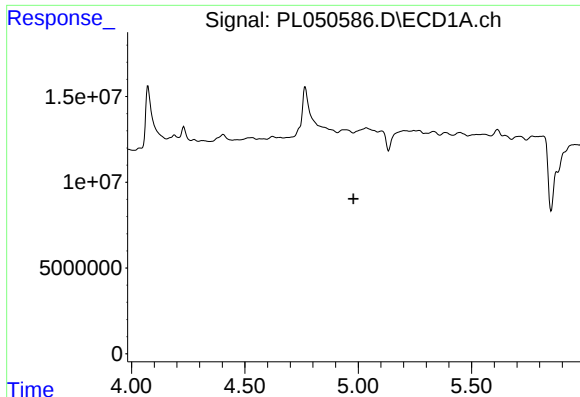

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-7(13-15)

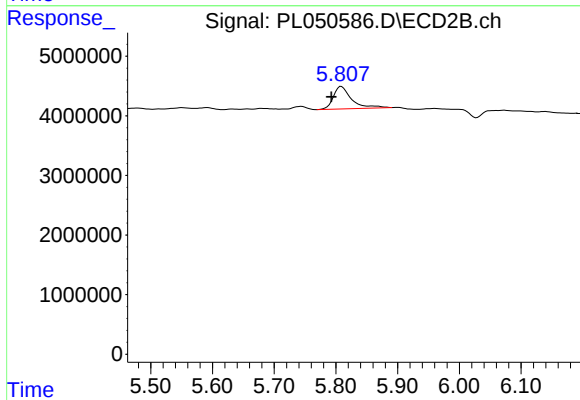


#8 Heptachlor epoxide

R.T.: 5.809 min
Delta R.T.: 0.016 min
Response: 7719581
Conc: 2.02 ng/ml

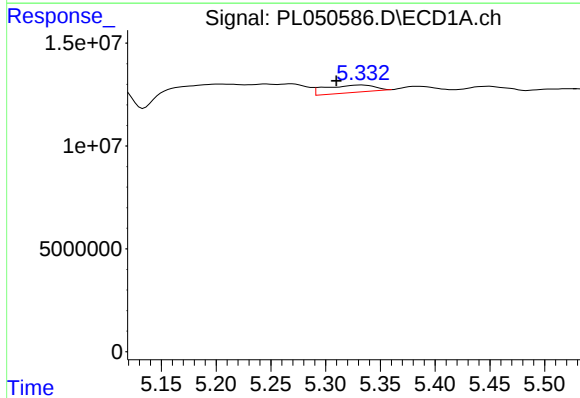


#9 Endosulfan I

R.T.: 5.333 min
Delta R.T.: 0.023 min
Response: 11438840
Conc: 0.79 ng/ml

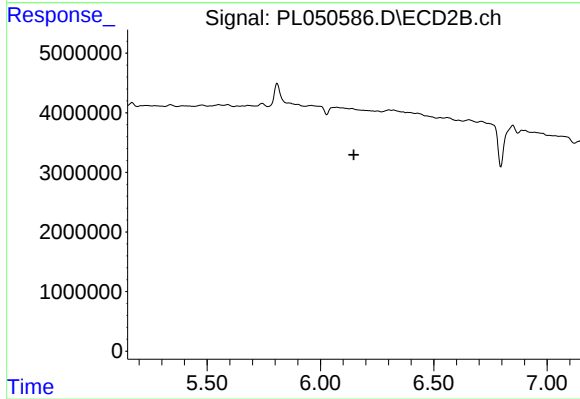

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

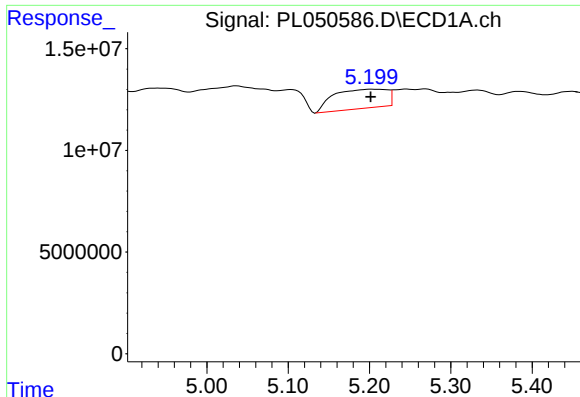

#10 gamma-Chlordane


R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 42978423
Conc: 2.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7(13-15)

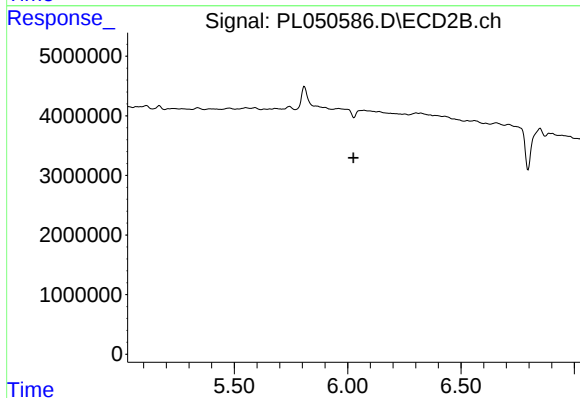


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

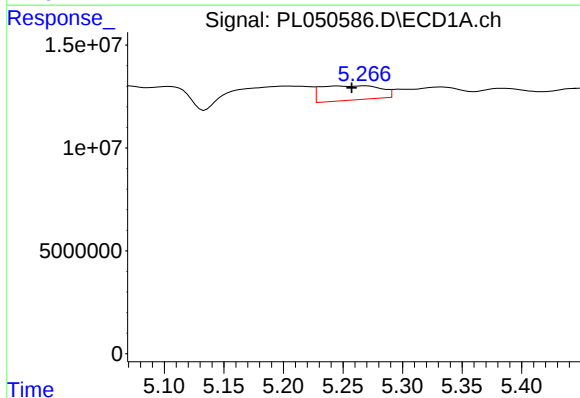


#11 alpha-Chlordane

R.T.: 5.269 min
Delta R.T.: 0.011 min
Response: 24284273
Conc: 1.59 ng/ml

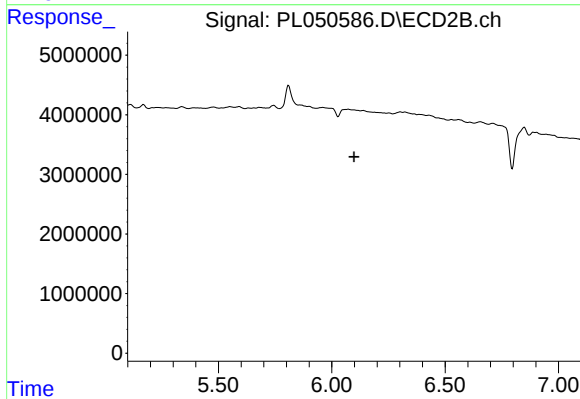

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

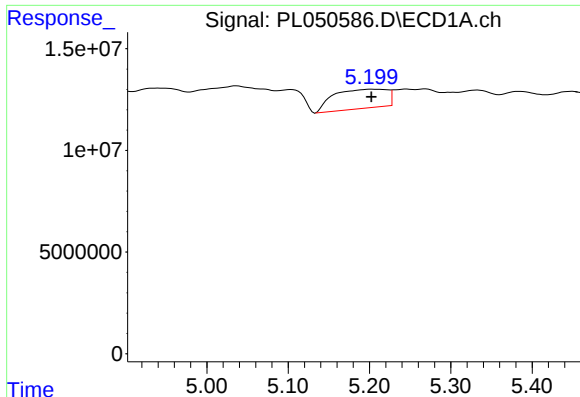

#25 Chlordane-3


R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 42978423
Conc: 30.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7(13-15)

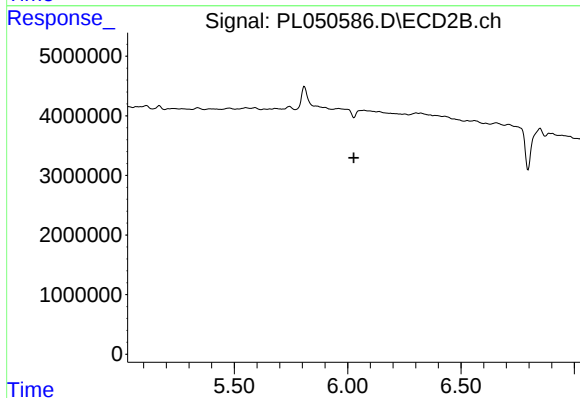


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

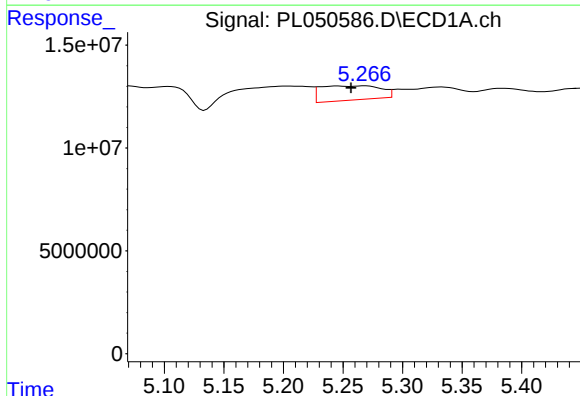


#26 Chlordane-4

R.T.: 5.269 min
Delta R.T.: 0.012 min
Response: 24284273
Conc: 18.41 ng/ml

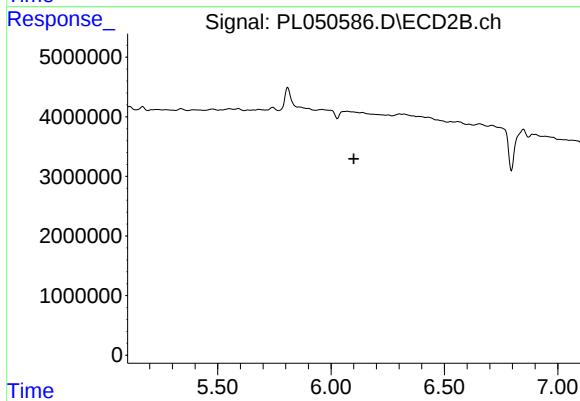

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

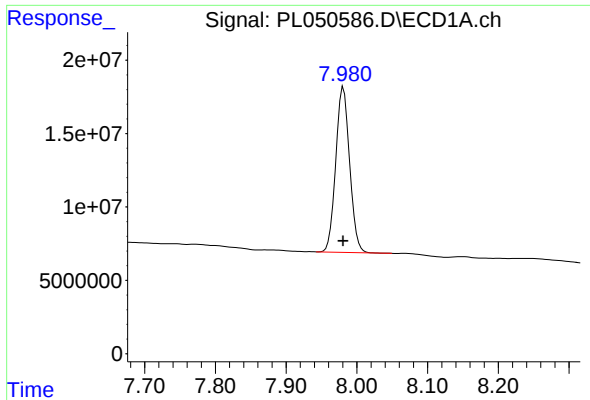

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 153320363
Conc: 15.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7(13-15)

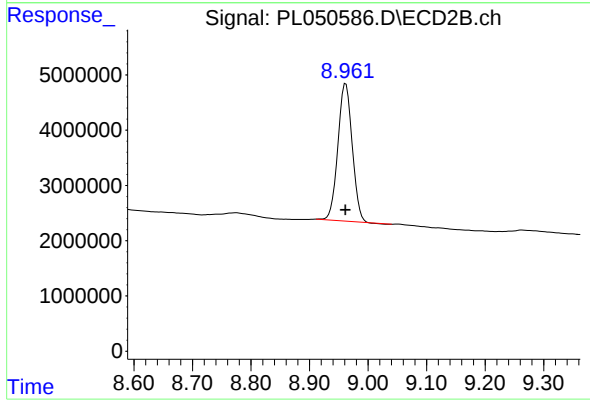

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: 0.000 min
Response: 42128762
Conc: 14.90 ng/ml