

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
 Data File : PL050587.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2019 00:03
 Operator : SM\AJ
 Sample : K3615-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-06-071719-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:46:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.930	99756419	27392257	9.928	9.601
28)	SA Decachlor...	7.981	8.961	113.0E6	35589169	11.164	12.585
Target Compounds							
6)	B beta-BHC	0.000	4.801f	0	4812756	N.D.	2.784 #
8)	B Heptachlo...	0.000	5.808f	0	6784592	N.D.	1.774 #
10)	B gamma-Chl...	5.223f	0.000	20939950	0	1.327	N.D. #
11)	B alpha-Chl...	0.000	6.100	0	4314782	N.D.	1.177 #
12)	B 4,4'-DDE	5.425	6.257	28863996	7624809	1.926	2.116
17)	MA 4,4'-DDT	6.168	0.000	6000699	0	0.484	N.D. #
25)	Chlordane-3	5.223f	0.000	20939950	0	14.959	N.D. #
26)	Chlordane-4	0.000	6.100	0	4314782	N.D.	7.428 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
Data File : PL050587.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2019 00:03
Operator : SM\AJ
Sample : K3615-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HR-06-071719-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:46:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

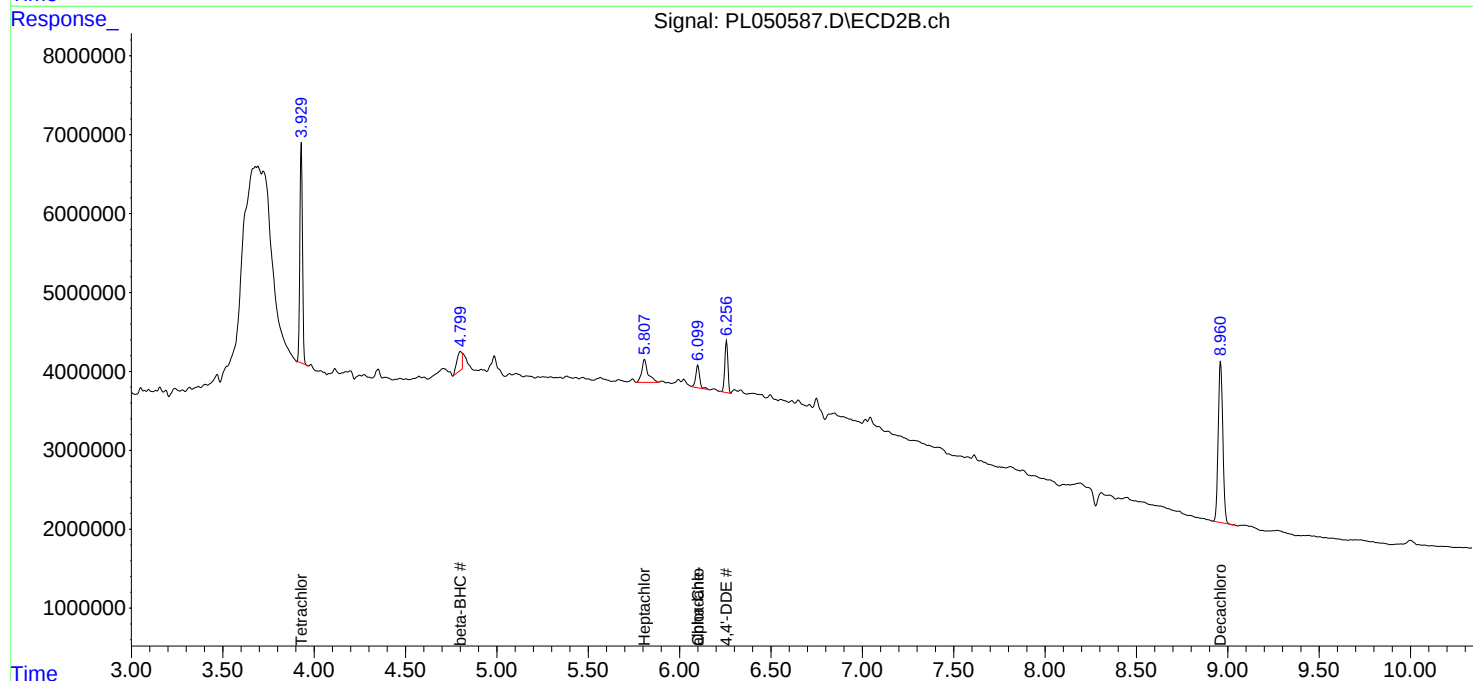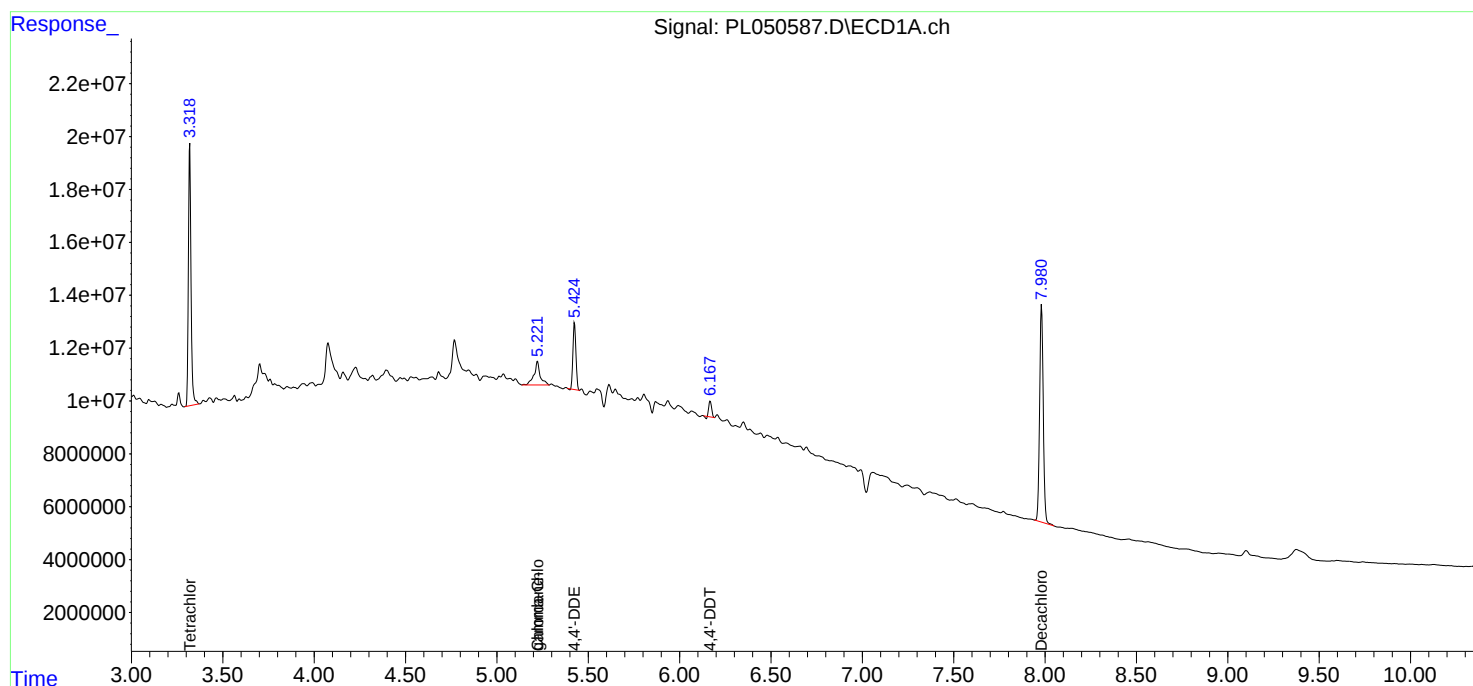


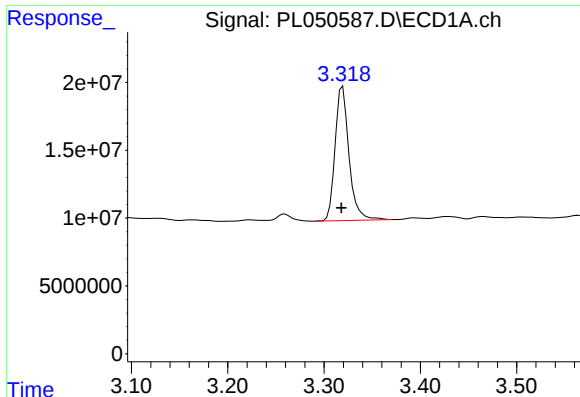

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.001 min
Response: 99756419
Conc: 9.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-06-071719-A

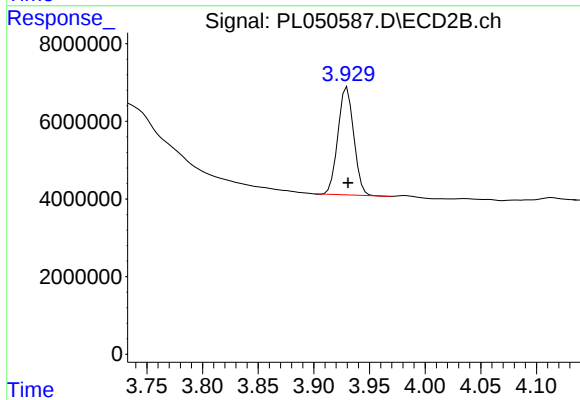


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 27392257
Conc: 9.60 ng/ml

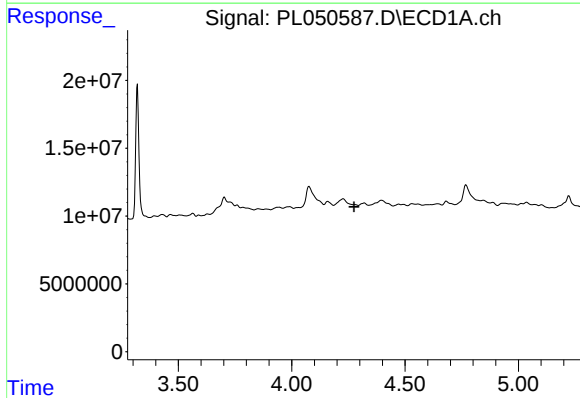


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

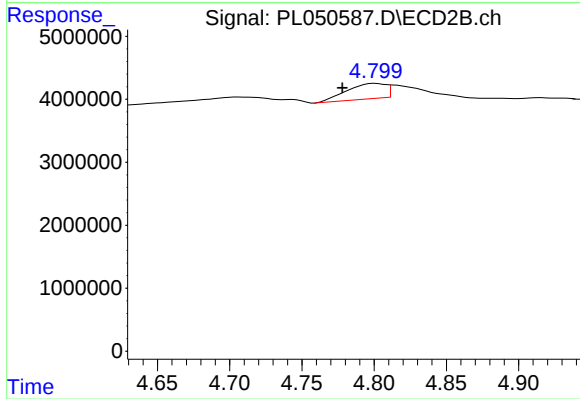

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.023 min
Response: 4812756
Conc: 2.78 ng/ml

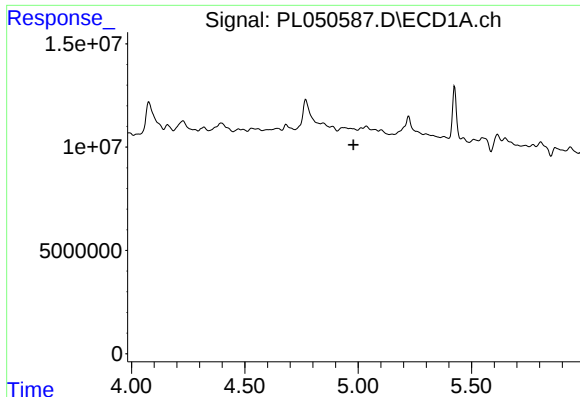

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HR-06-071719-A

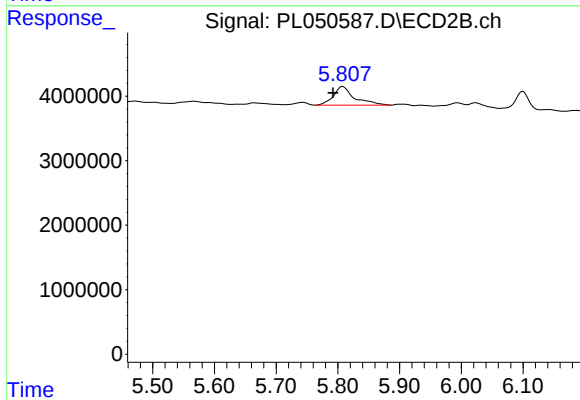


#8 Heptachlor epoxide

R.T.: 5.808 min
Delta R.T.: 0.016 min
Response: 6784592
Conc: 1.77 ng/ml

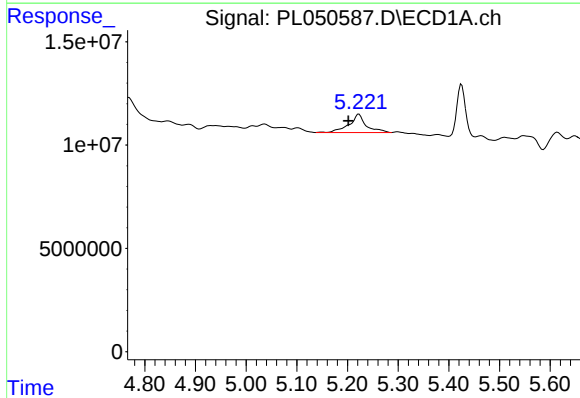


#10 gamma-Chlordane

R.T.: 5.223 min
Delta R.T.: 0.021 min
Response: 20939950
Conc: 1.33 ng/ml

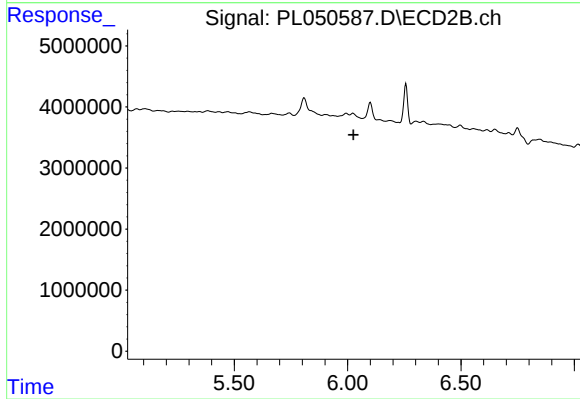

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

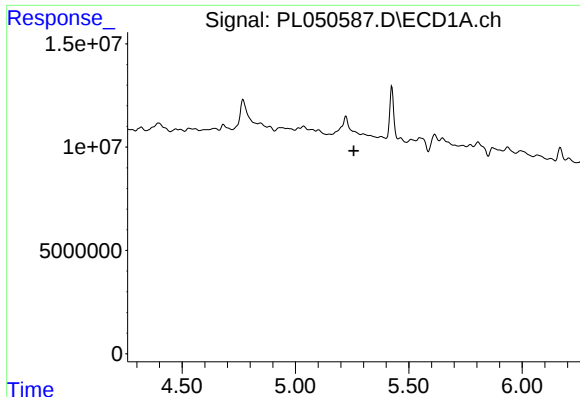

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HR-06-071719-A

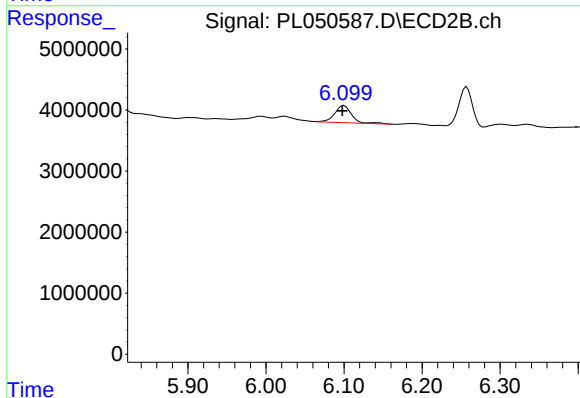


#11 alpha-Chlordane

R.T.: 6.100 min
Delta R.T.: 0.002 min
Response: 4314782
Conc: 1.18 ng/ml

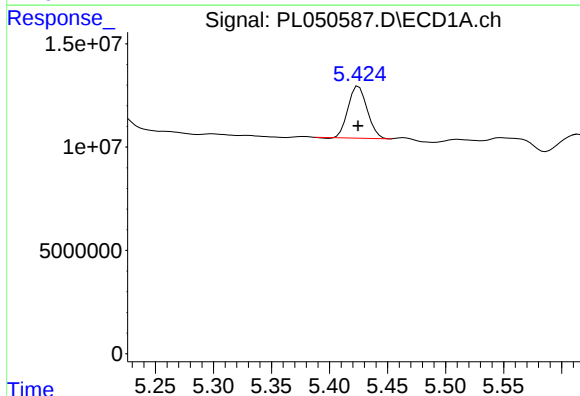


#12 4,4'-DDE

R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 28863996
Conc: 1.93 ng/ml

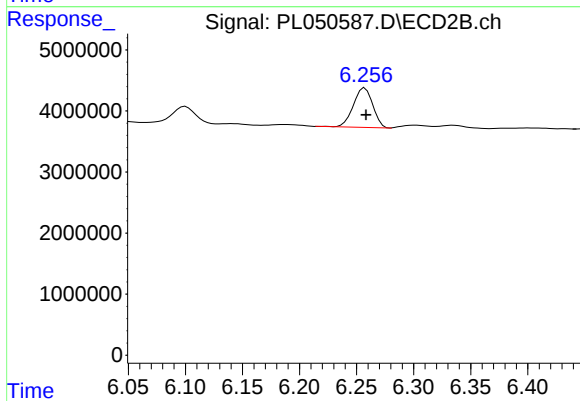

#12 4,4'-DDE


R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 7624809
Conc: 2.12 ng/ml

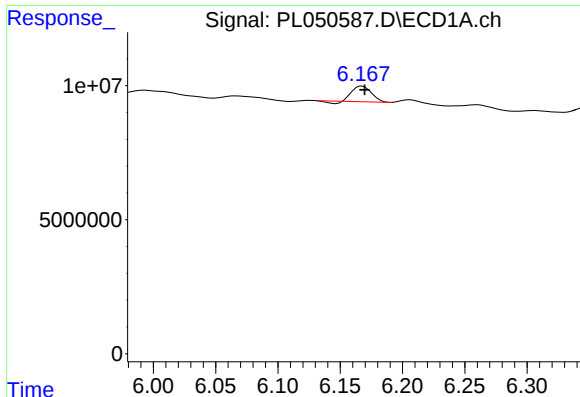

#17 4,4'-DDT


R.T.: 6.168 min
Delta R.T.: -0.002 min
Response: 6000699
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-06-071719-A

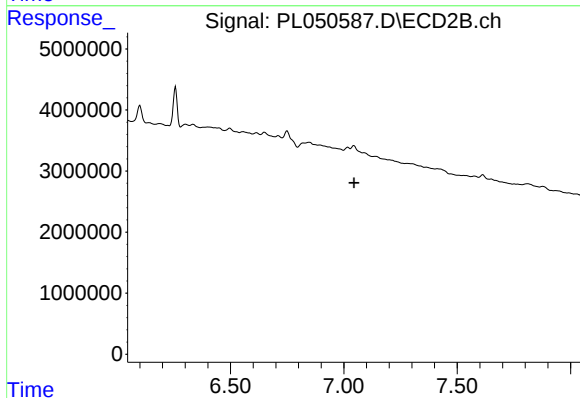


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

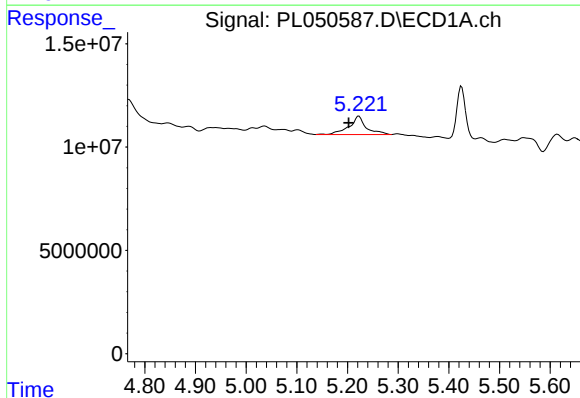


#25 Chlordane-3

R.T.: 5.223 min
Delta R.T.: 0.020 min
Response: 20939950
Conc: 14.96 ng/ml

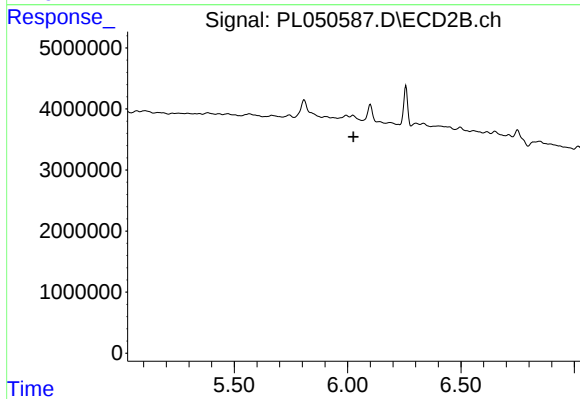

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

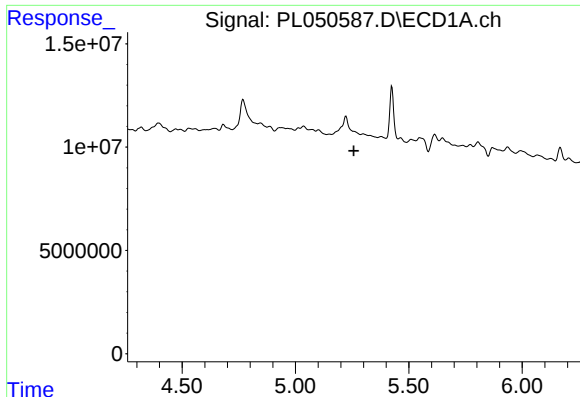

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HR-06-071719-A

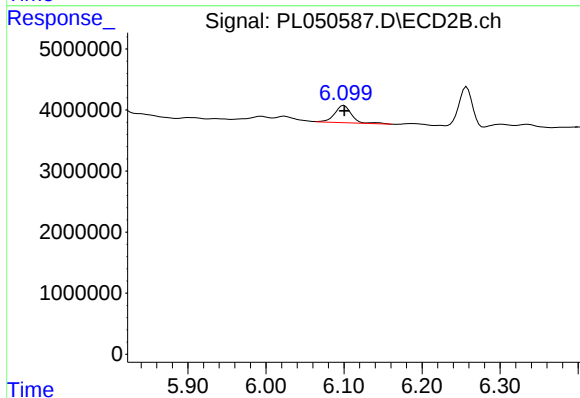


#26 Chlordane-4

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 4314782
Conc: 7.43 ng/ml

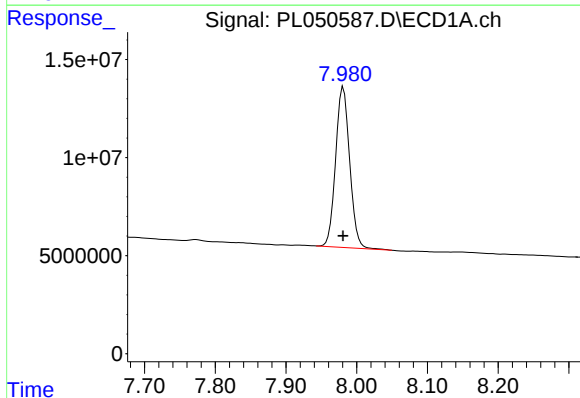

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 113038274
Conc: 11.16 ng/ml

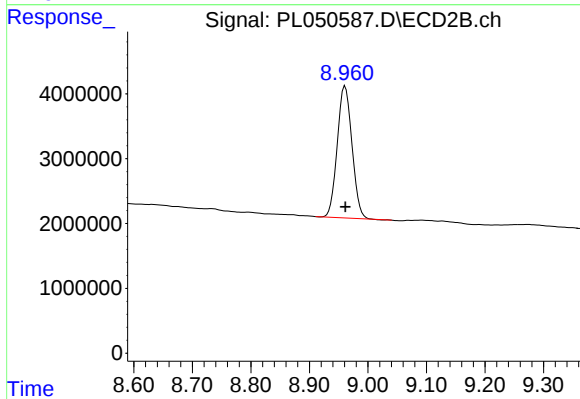

#28 Decachlorobiphenyl

R.T.: 8.961 min
Delta R.T.: 0.000 min
Response: 35589169
Conc: 12.58 ng/ml