

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
 Data File : PL050592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2019 01:19
 Operator : SM\AJ
 Sample : K3835-44
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-6(8-10)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:47:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.930	189.9E6	53063643	18.902	18.598
28)	SA Decachlor...	7.981	8.962	173.1E6	51615043	17.099	18.252
Target Compounds							
6)	B beta-BHC	0.000	4.755f	0	693872	N.D.	0.401 #
7)	B delta-BHC	0.000	4.985	0	5098270	N.D.	1.318 #
8)	B Heptachlo...	0.000	5.808f	0	7829234	N.D.	2.047 #
10)	B gamma-Chl...	5.200	0.000	25419706	0	1.611	N.D. #
11)	B alpha-Chl...	5.268	0.000	7875584	0	0.516	N.D. #
19)	B Endosulfa...	6.483f	0.000	16312656	0	1.280	N.D. #
21)	B Endrin ke...	0.000	7.648	0	4434212	N.D.	1.534 #
25)	Chlordane-3	5.200	0.000	25419706	0	18.160	N.D. #
26)	Chlordane-4	5.268	0.000	7875584	0	5.971	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
Data File : PL050592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2019 01:19
Operator : SM\AJ
Sample : K3835-44
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB-6(8-10)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:47:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

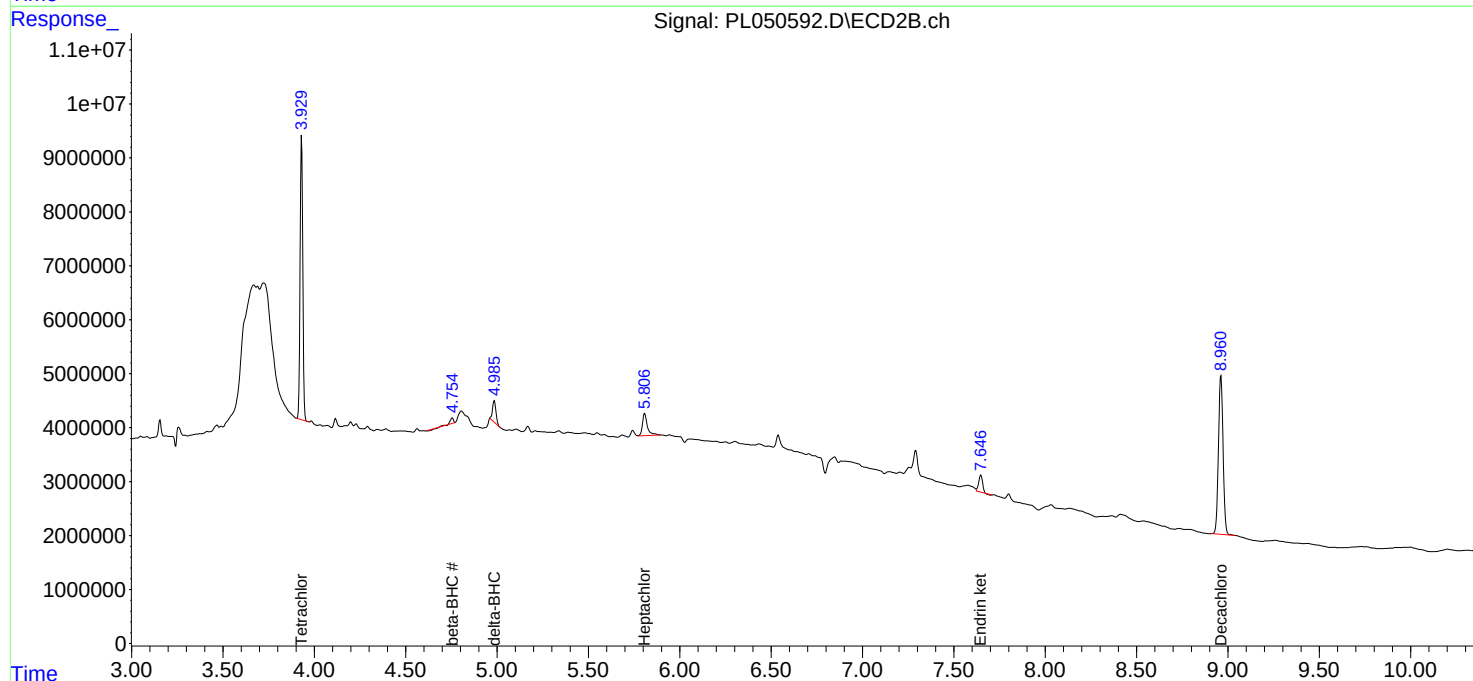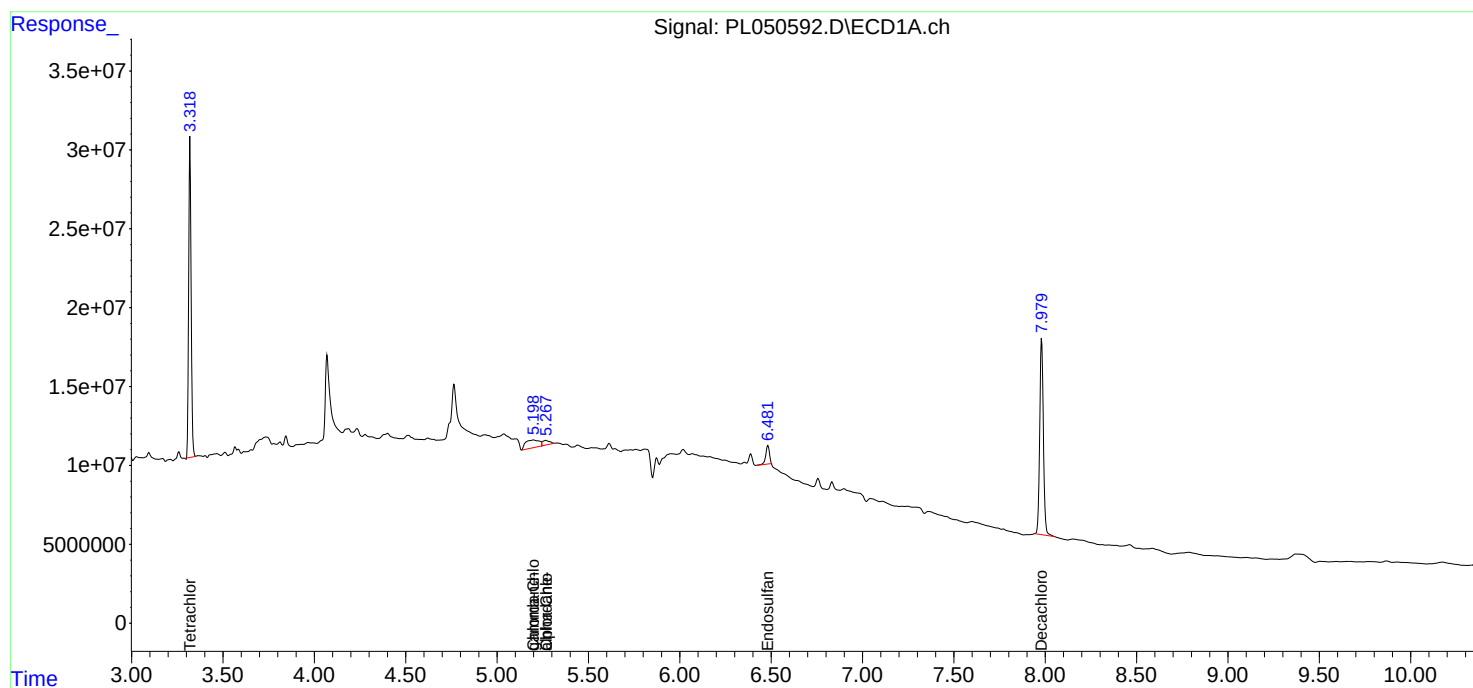


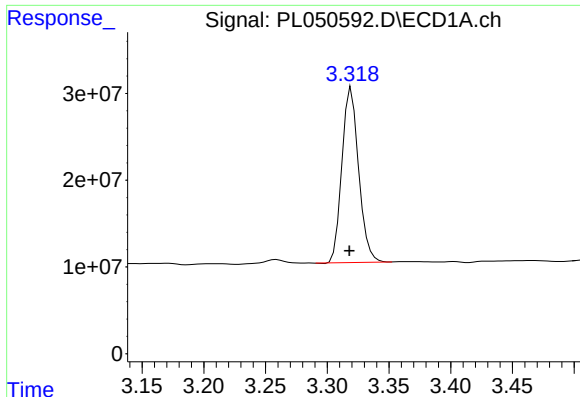

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: 0.002 min
Response: 189927732
Conc: 18.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6(8-10)

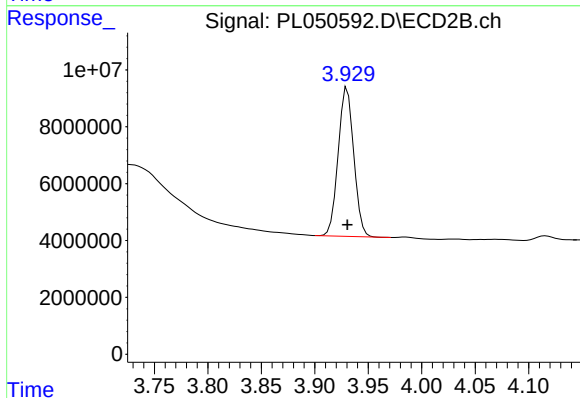


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 53063643
Conc: 18.60 ng/ml

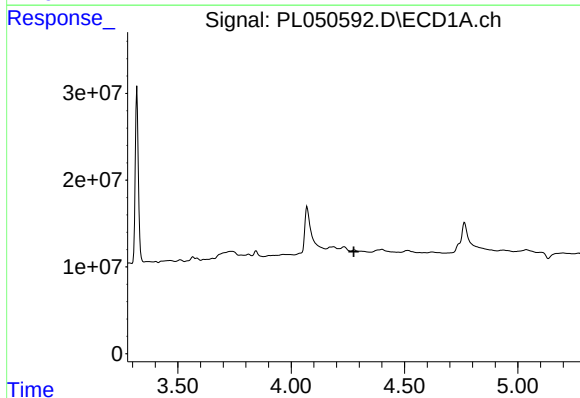


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

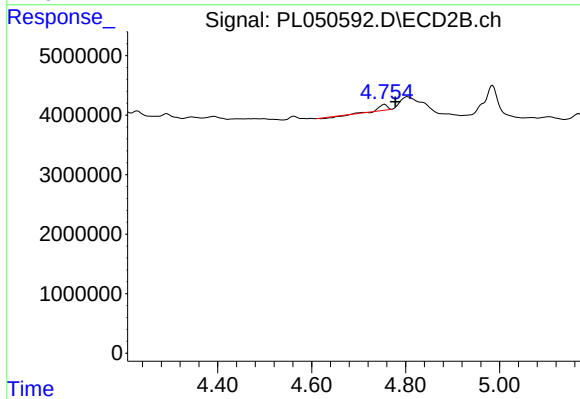

#6 beta-BHC


R.T.: 4.755 min
Delta R.T.: -0.023 min
Response: 693872
Conc: 0.40 ng/ml

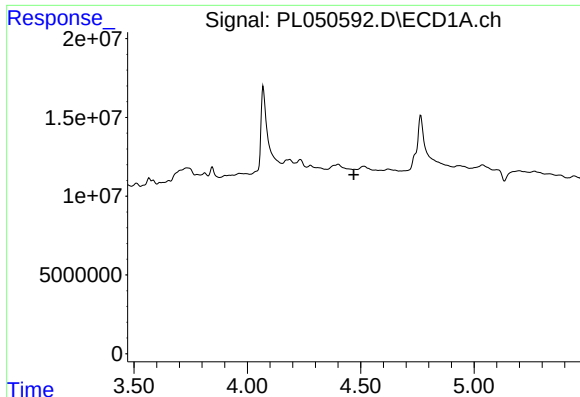

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-6(8-10)

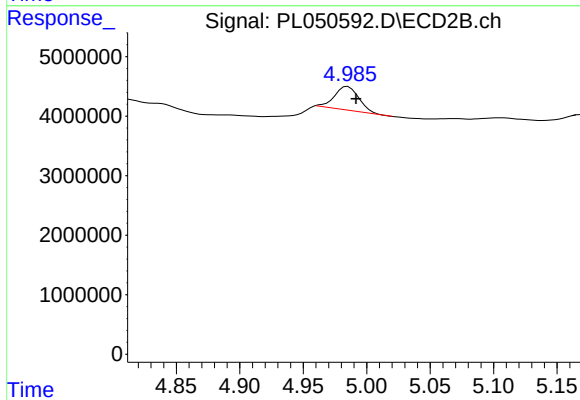


#7 delta-BHC

R.T.: 4.985 min
Delta R.T.: -0.006 min
Response: 5098270
Conc: 1.32 ng/ml

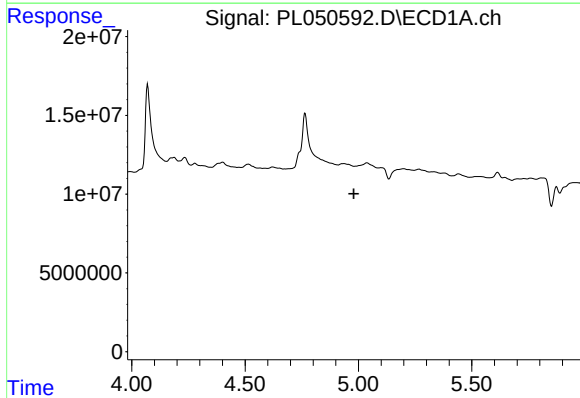


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

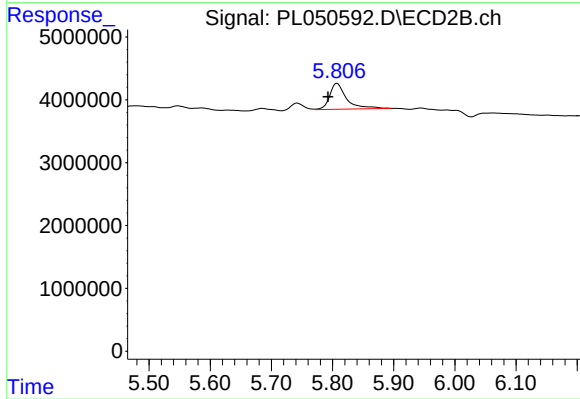

#8 Heptachlor epoxide


R.T.: 5.808 min
Delta R.T.: 0.015 min
Response: 7829234
Conc: 2.05 ng/ml

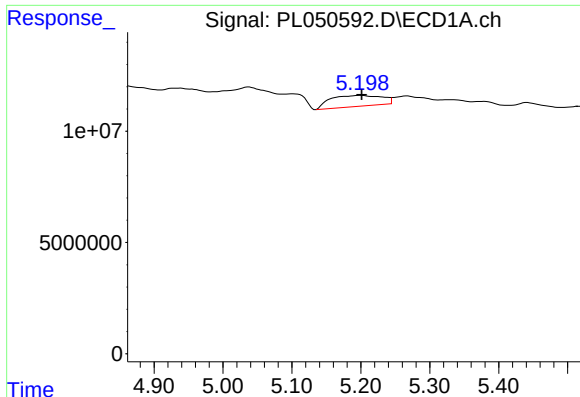

#10 gamma-Chlordane


R.T.: 5.200 min
Delta R.T.: -0.002 min
Response: 25419706
Conc: 1.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6(8-10)

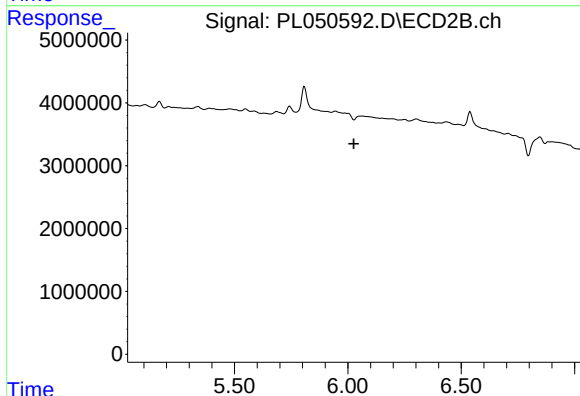


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

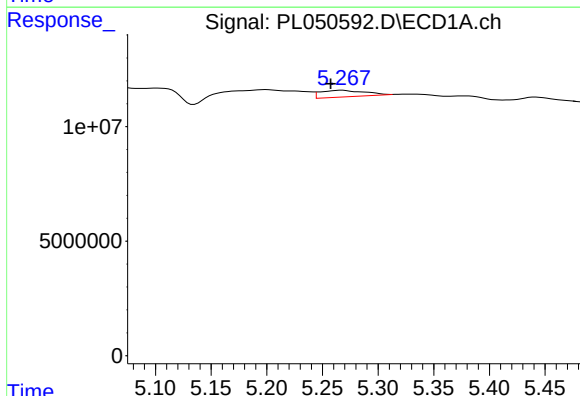


#11 alpha-Chlordane

R.T.: 5.268 min
Delta R.T.: 0.011 min
Response: 7875584
Conc: 0.52 ng/ml

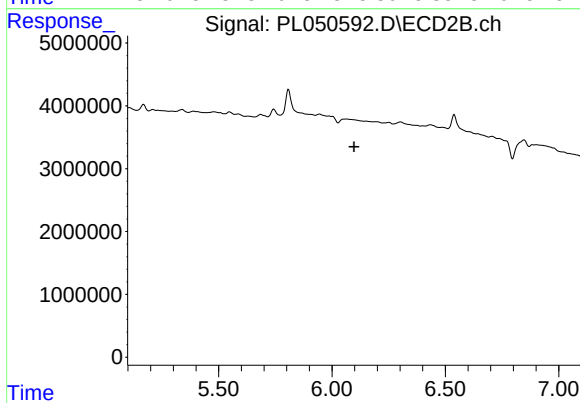

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.098 min
Response: 0
Conc: N.D.

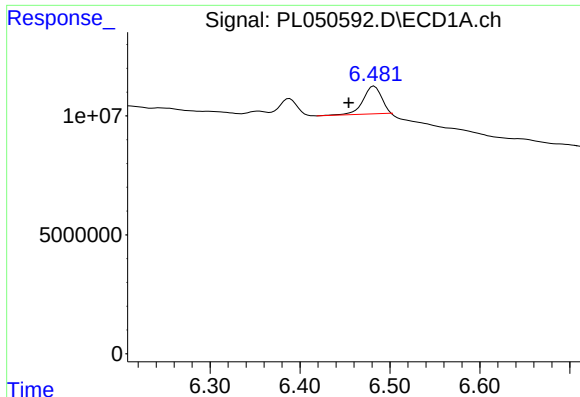

#19 Endosulfan Sulfate


R.T.: 6.483 min
Delta R.T.: 0.028 min
Response: 16312656
Conc: 1.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6(8-10)

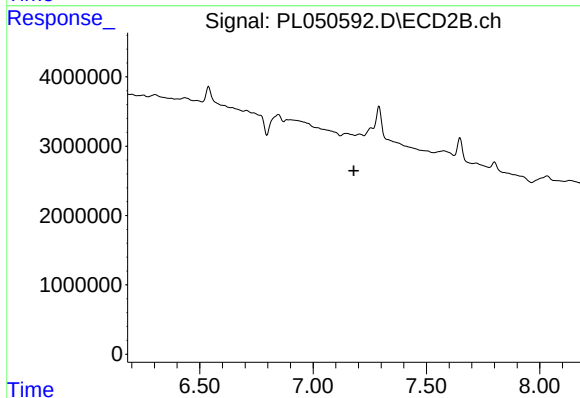


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.180 min
Response: 0
Conc: N.D.

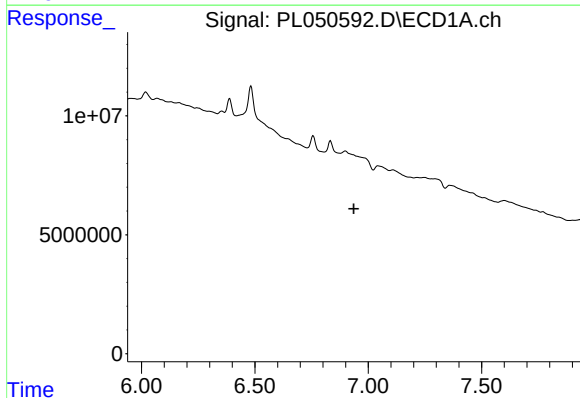


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.936 min
Response: 0
Conc: N.D.

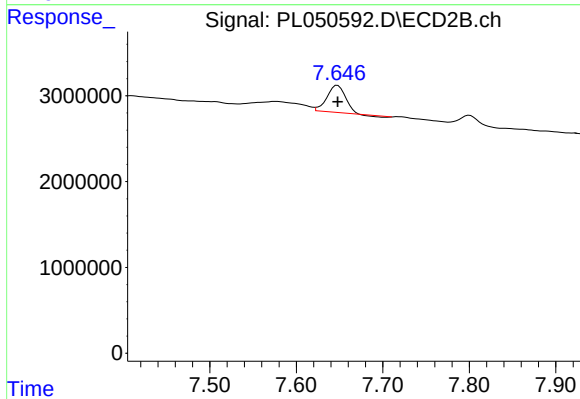

#21 Endrin ketone


R.T.: 7.648 min
Delta R.T.: 0.000 min
Response: 4434212
Conc: 1.53 ng/ml

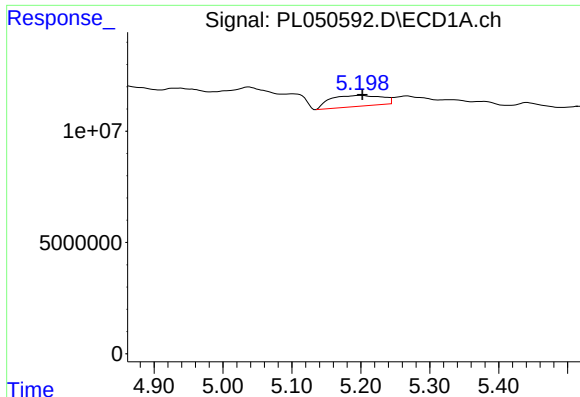

#25 Chlordane-3


R.T.: 5.200 min
Delta R.T.: -0.002 min
Response: 25419706
Conc: 18.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6(8-10)

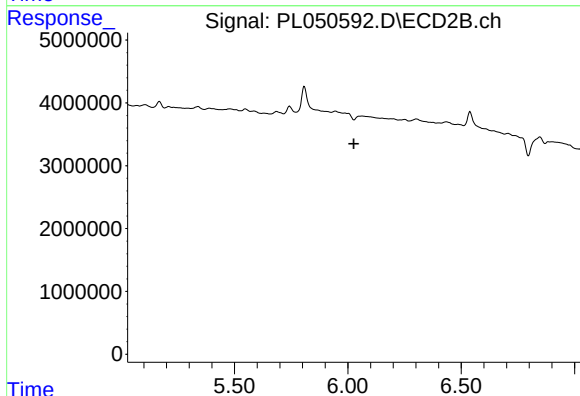


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

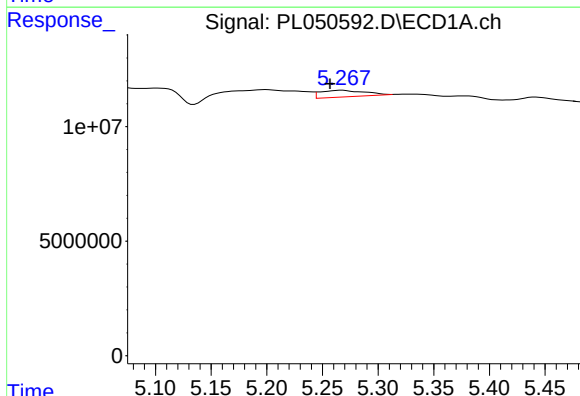


#26 Chlordane-4

R.T.: 5.268 min
Delta R.T.: 0.011 min
Response: 7875584
Conc: 5.97 ng/ml

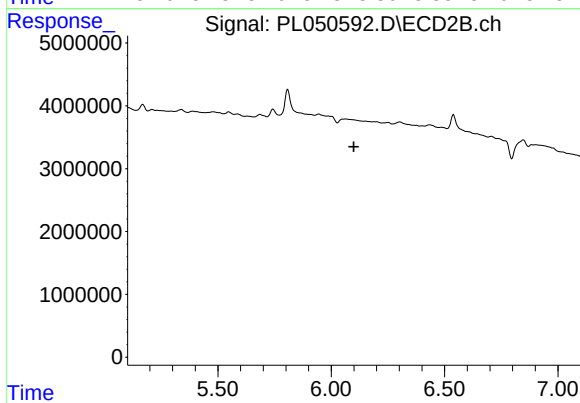

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

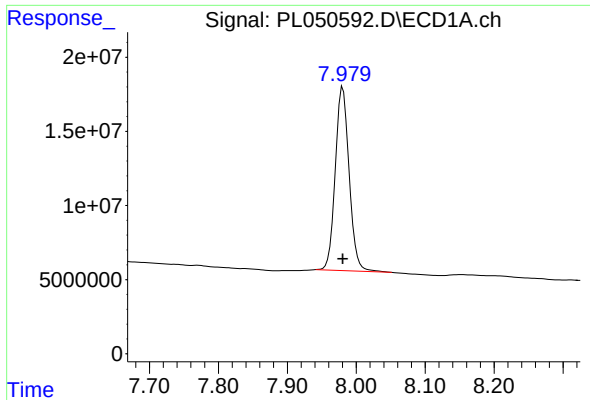

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 173129898
Conc: 17.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6(8-10)

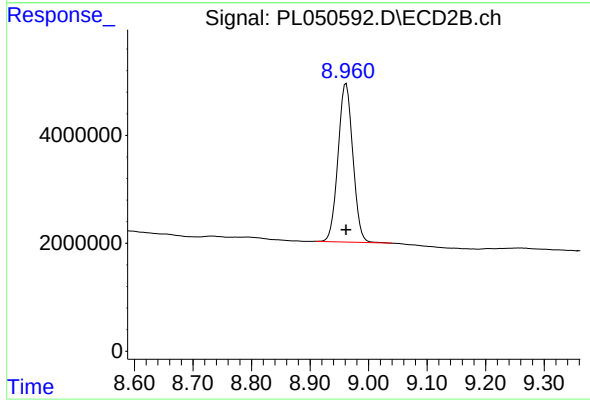

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: 0.000 min
Response: 51615043
Conc: 18.25 ng/ml