

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
 Data File : PL050571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 19:39
 Operator : SM\AJ
 Sample : K3835-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-12(0-2)

Manual Integrations
 APPROVED

Ankita
 7/19/2019 12:01:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 00:59:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 18 09:14:47 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.318	3.930	100.4E6	28095508	9.988	9.847
28) SA Decachlor...	7.980	8.962	118.2E6	33472688	11.677	11.837
Target Compounds						
12) B 4,4'-DDE	5.422	6.256	67220624	16852953	4.486m	4.677m
17) MA 4,4'-DDT	6.168	7.044	59439540	7846756	4.799	2.907m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
Data File : PL050571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 19:39
Operator : SM\AJ
Sample : K3835-23
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-12(0-2)


Manual Integrations
APPROVED

Ankita
7/19/2019 12:01:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 00:59:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Thu Jul 18 09:14:47 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

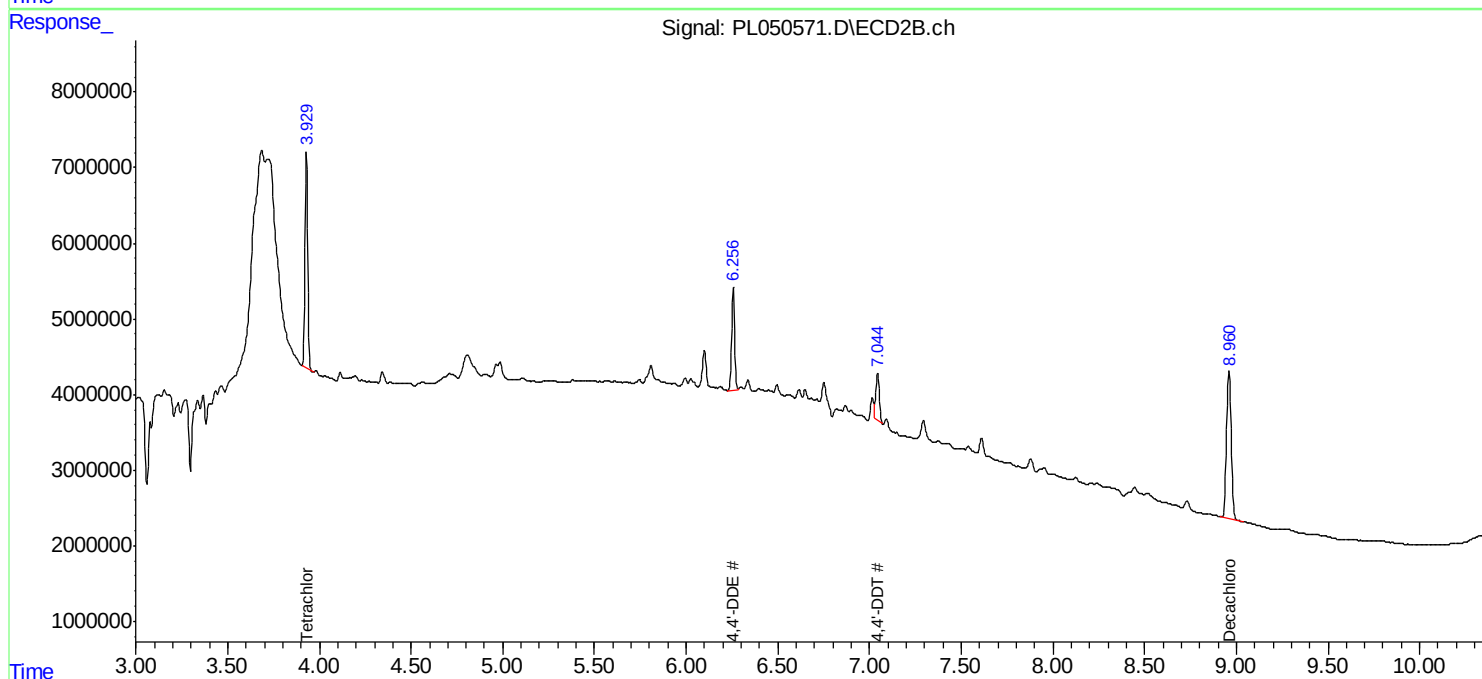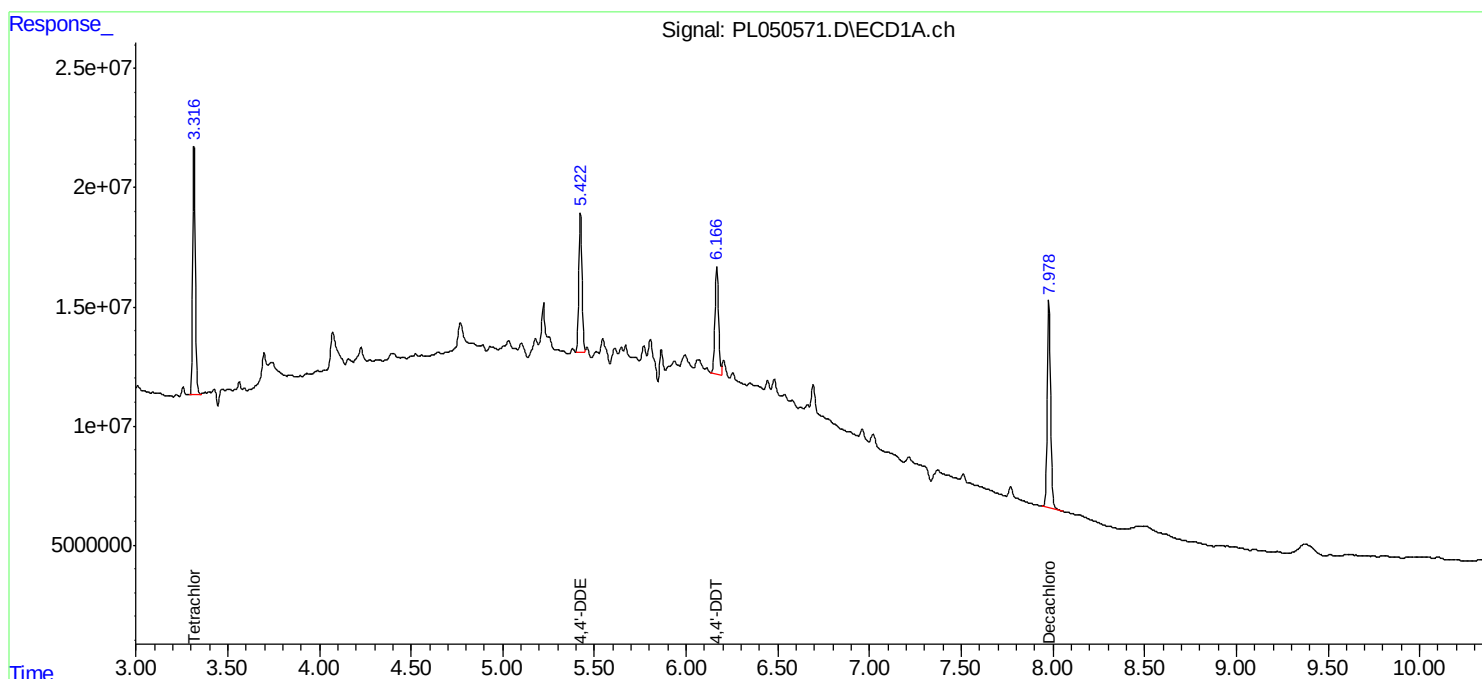

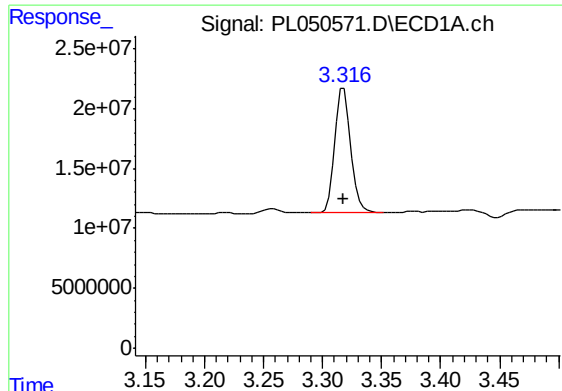


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 100355390
Conc: 9.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-12(0-2)


Manual Integrations
APPROVED

Ankita
7/19/2019 12:01:35 PM

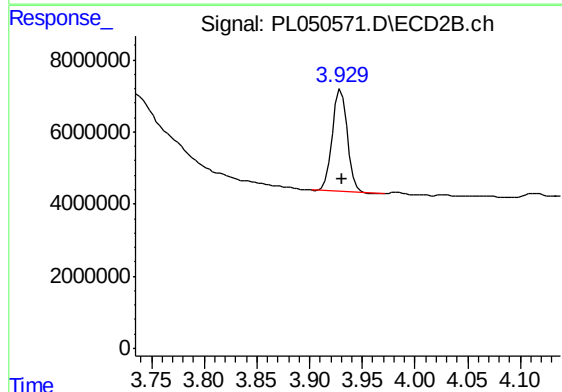


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 28095508
Conc: 9.85 ng/ml

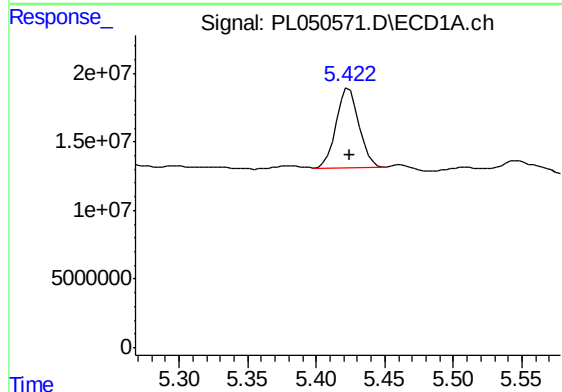


#12 4,4'-DDE

R.T.: 5.422 min
Delta R.T.: -0.002 min
Response: 67220624
Conc: 4.49 ng/ml m

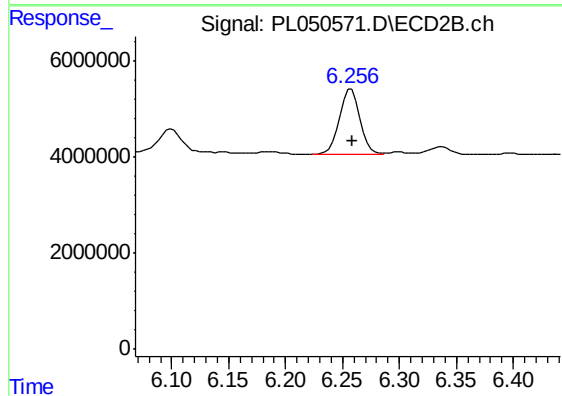

#12 4,4'-DDE

R.T.: 6.256 min
Delta R.T.: -0.002 min
Response: 16852953
Conc: 4.68 ng/ml m

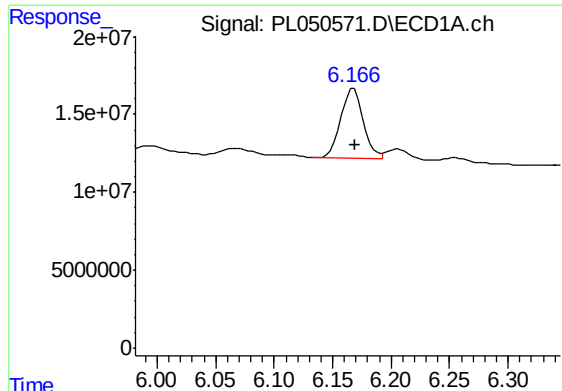


#17 4,4'-DDT

R.T.: 6.168 min
Delta R.T.: -0.002 min
Response: 59439540
Conc: 4.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-12(0-2)


Manual Integrations
APPROVED

Ankita
7/19/2019 12:01:35 PM

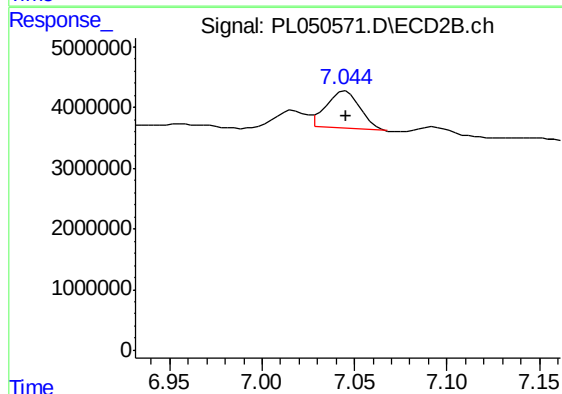


#17 4,4'-DDT

R.T.: 7.044 min
Delta R.T.: -0.002 min
Response: 7846756
Conc: 2.91 ng/ml m

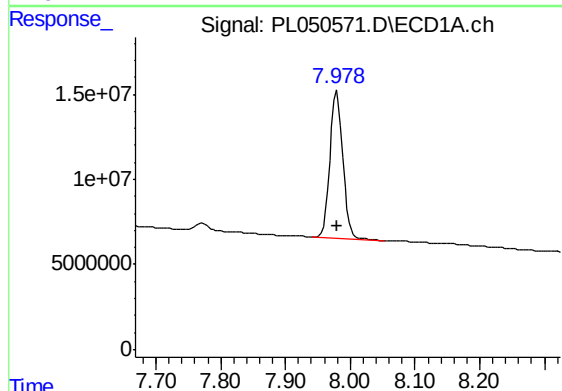

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.001 min
Response: 118228956
Conc: 11.68 ng/ml

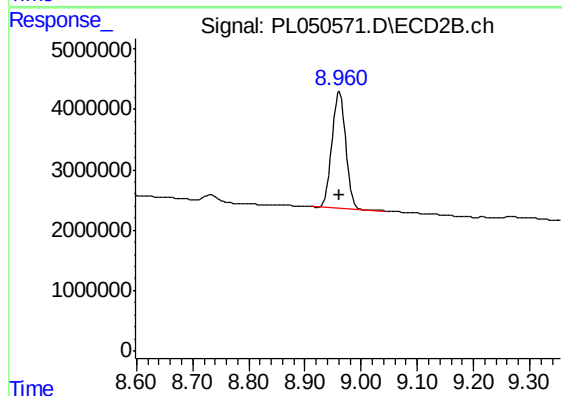

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: 0.000 min
Response: 33472688
Conc: 11.84 ng/ml