

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
 Data File : PL050603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2019 04:49
 Operator : SM\AJ
 Sample : K3868-05
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 7/19/2019 12:02:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 05:31:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.318	3.930	121.0E6	36338246	12.038	12.736
28) SA Decachlor...	7.980	8.961	150.3E6	41986192	14.841	14.847
Target Compounds						
12) B 4,4'-DDE	5.422	6.253	31174326	12153085	2.080m	3.373 #
14) MA Endrin	5.802	6.616	22759067	5977567	1.546m	1.927

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071819\
Data File : PL050603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2019 04:49
Operator : SM\AJ
Sample : K3868-05
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-1


Manual Integrations
APPROVED

Ankita
7/19/2019 12:02:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 05:31:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

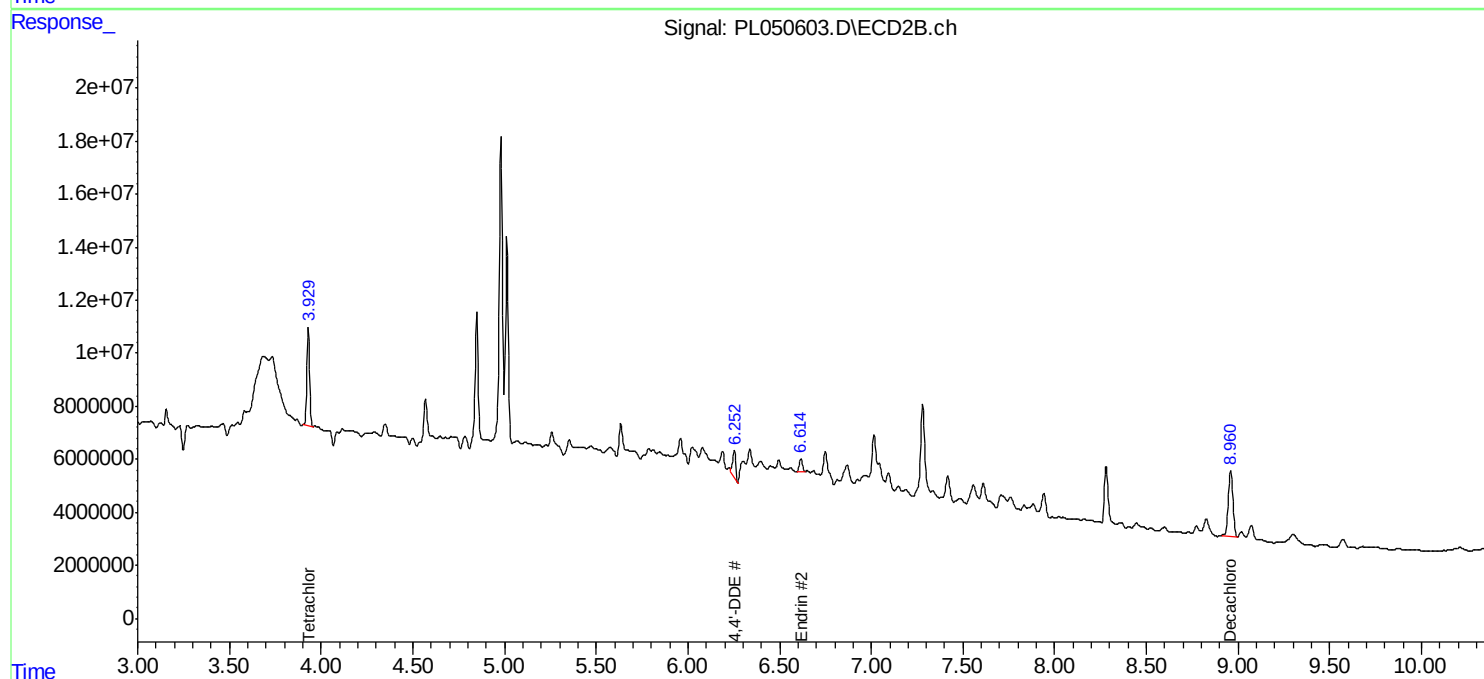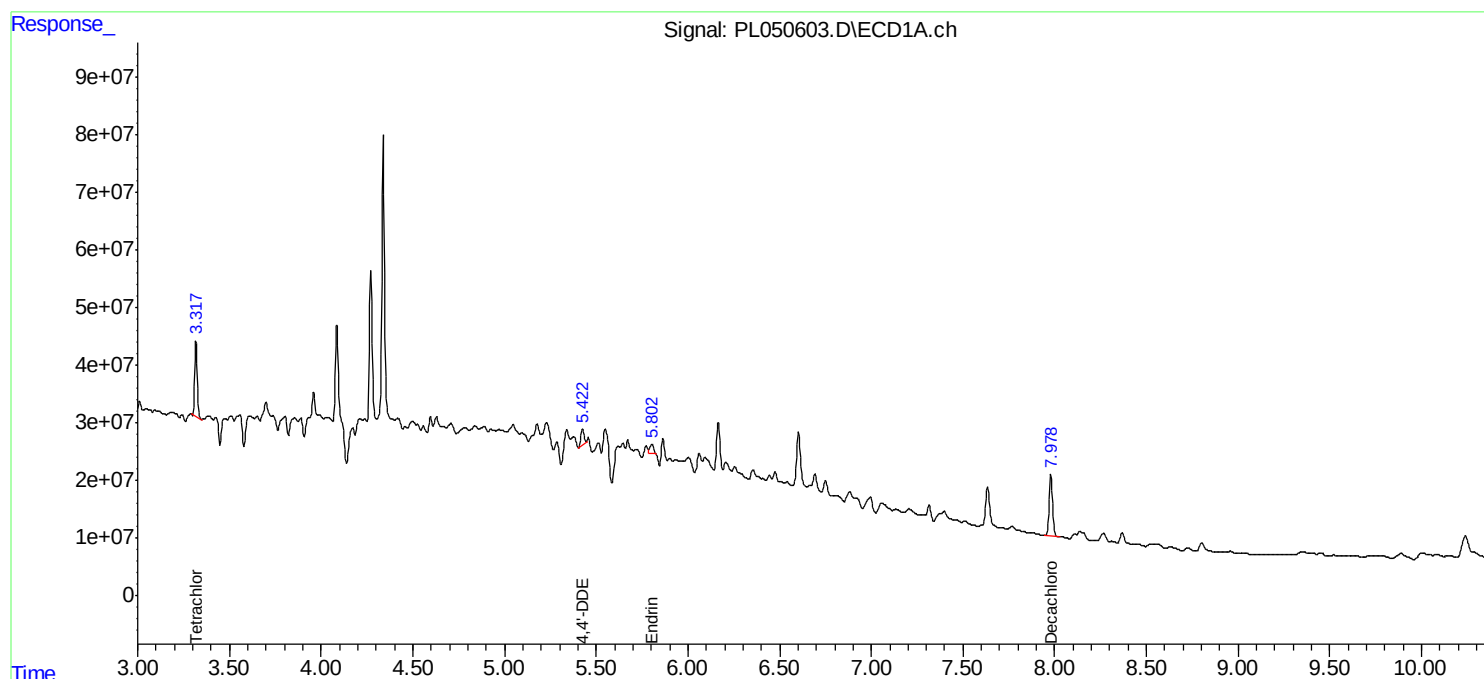

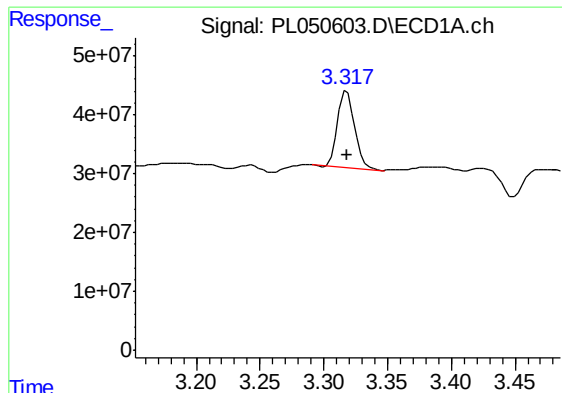


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 120954772
Conc: 12.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
7/19/2019 12:02:19 PM

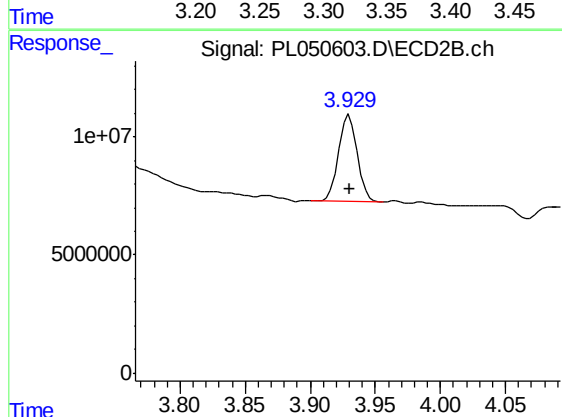


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 36338246
Conc: 12.74 ng/ml

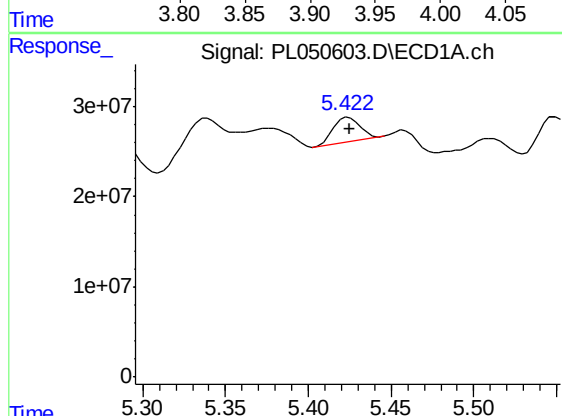


#12 4,4'-DDE

R.T.: 5.422 min
Delta R.T.: -0.002 min
Response: 31174326
Conc: 2.08 ng/ml m

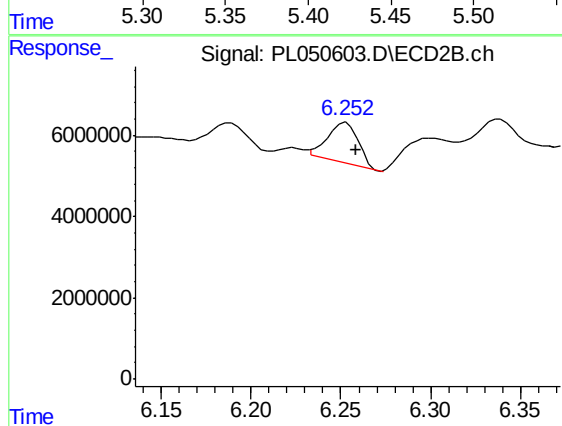

#12 4,4'-DDE

R.T.: 6.253 min
Delta R.T.: -0.005 min
Response: 12153085
Conc: 3.37 ng/ml

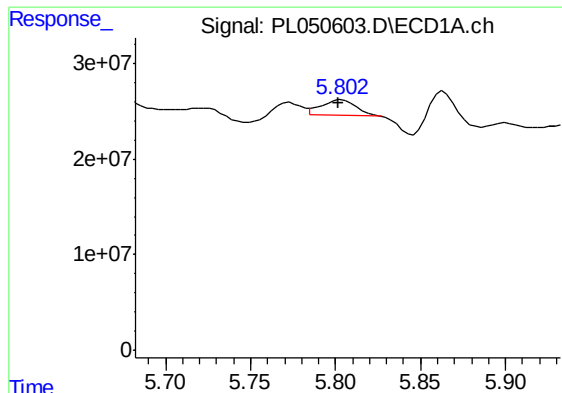


#14 Endrin

R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 22759067
Conc: 1.55 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
7/19/2019 12:02:19 PM

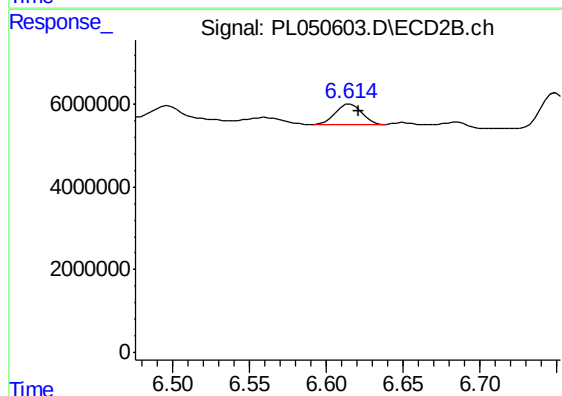


#14 Endrin

R.T.: 6.616 min
Delta R.T.: -0.006 min
Response: 5977567
Conc: 1.93 ng/ml

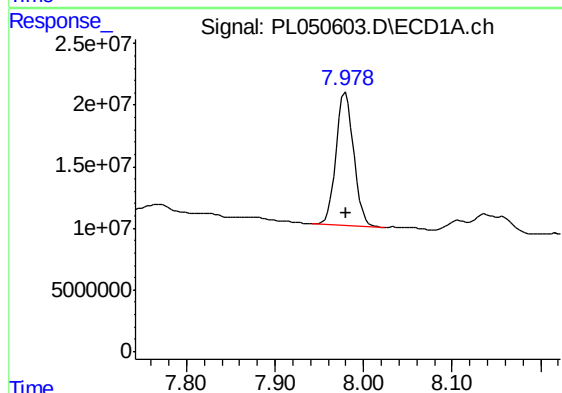

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 150270765
Conc: 14.84 ng/ml

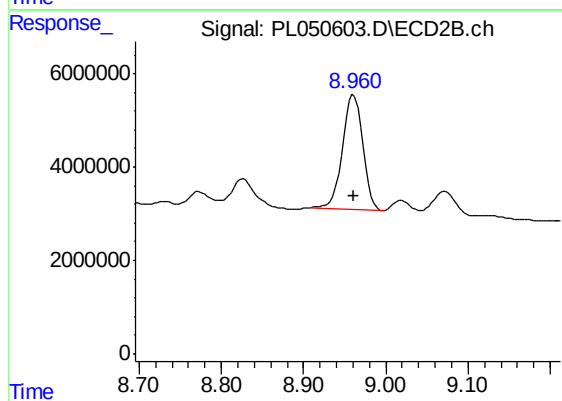

#28 Decachlorobiphenyl

R.T.: 8.961 min
Delta R.T.: 0.000 min
Response: 41986192
Conc: 14.85 ng/ml