

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071822\
 Data File : PL076493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2022 19:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 00:14:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.637	4.620	14658584	39675580	20.348	19.623
28)	SA Decachlor...	11.622	10.354	12327791	31361343	20.896	18.691
Target Compounds							
2)	A alpha-BHC	0.000	5.340	0	6652880	N.D.	2.426 #
7)	B delta-BHC	0.000	6.385	0	469539	N.D.	0.196 #
10)	B gamma-Chl...	0.000	7.314f	0	542090	N.D.	0.272 #
13)	MA Dieldrin	0.000	7.725f	0	722377	N.D.	0.382 #
14)	MA Endrin	0.000	8.043	0	1500486	N.D.	1.038 #
17)	MA 4,4'-DDT	0.000	8.441	0	364314	N.D.	0.233 #
21)	B Endrin ke...	0.000	9.256f	0	229166	N.D.	0.136 #
22)	Mirex	0.000	9.490f	0	289708	N.D.	0.219 #
25)	Chlordane-3	0.000	7.314f	0	542090	N.D.	3.201 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071822\
Data File : PL076493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2022 19:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 00:14:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

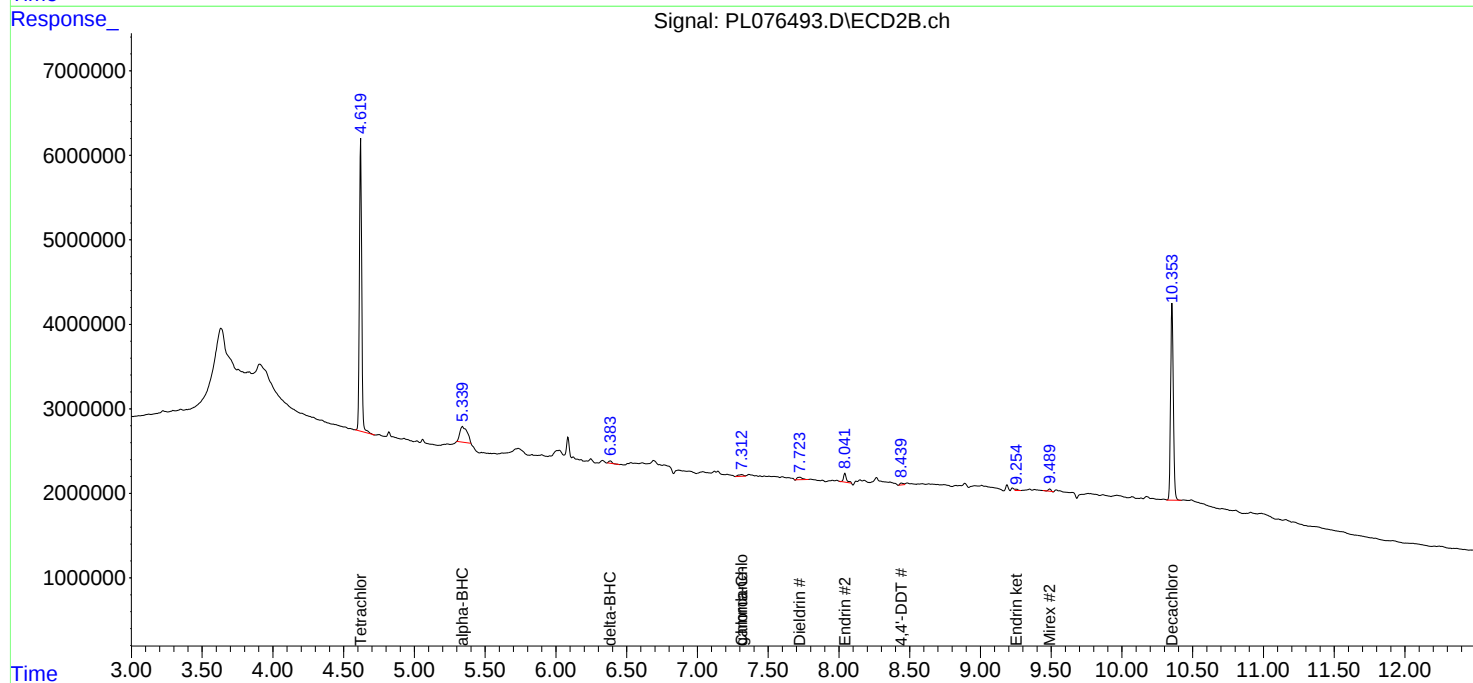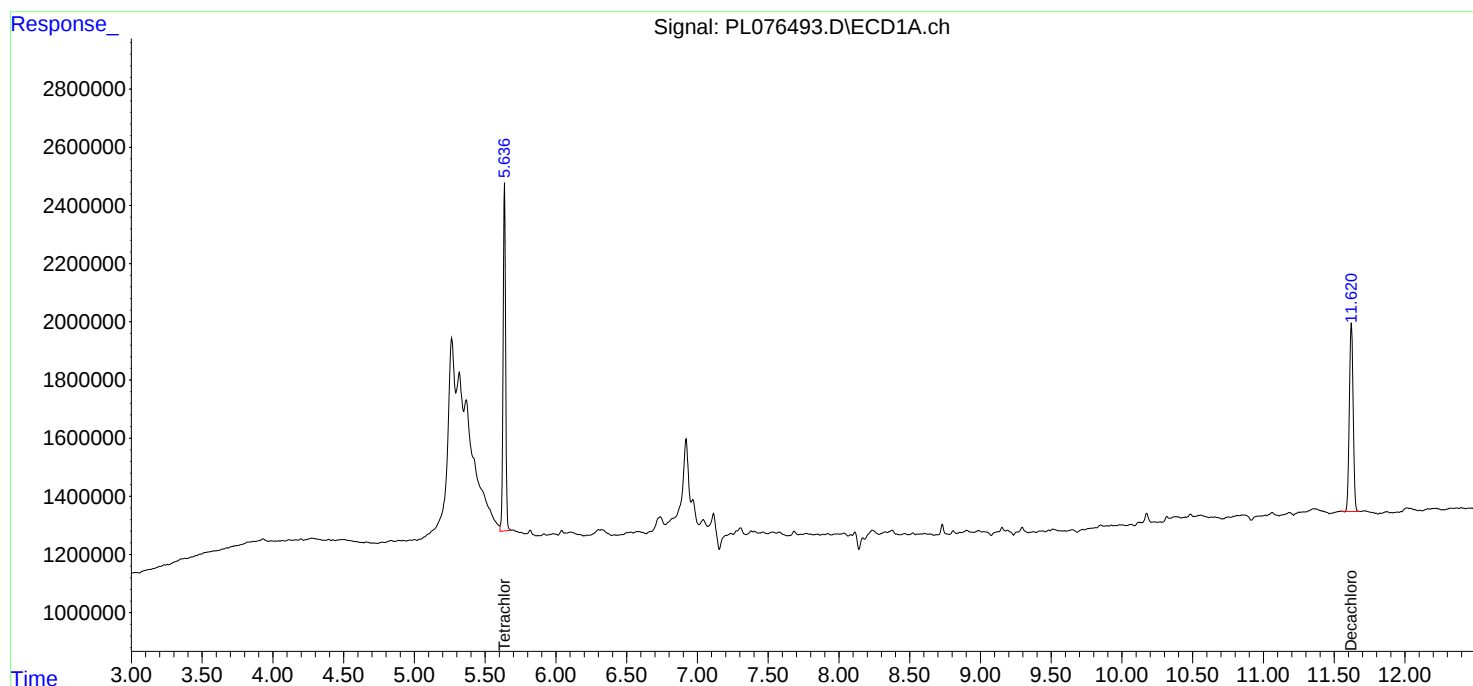


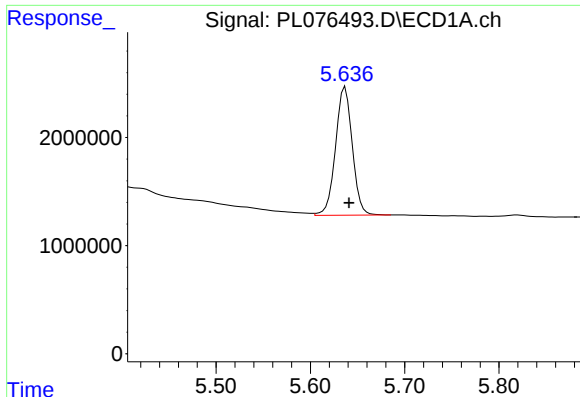

#1 Tetrachloro-m-xylene


R.T.: 5.637 min
Delta R.T.: -0.004 min
Response: 14658584
Conc: 20.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

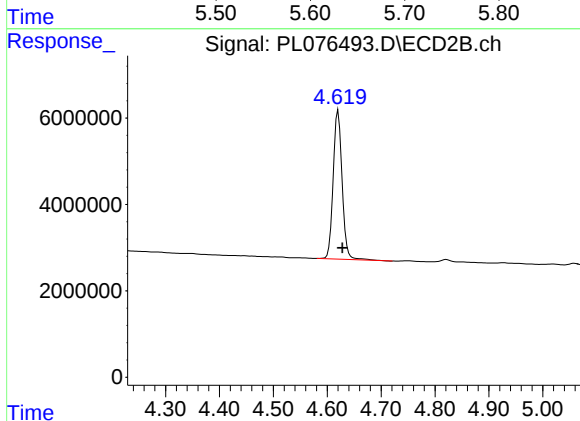


#1 Tetrachloro-m-xylene

R.T.: 4.620 min
Delta R.T.: -0.008 min
Response: 39675580
Conc: 19.62 ng/ml

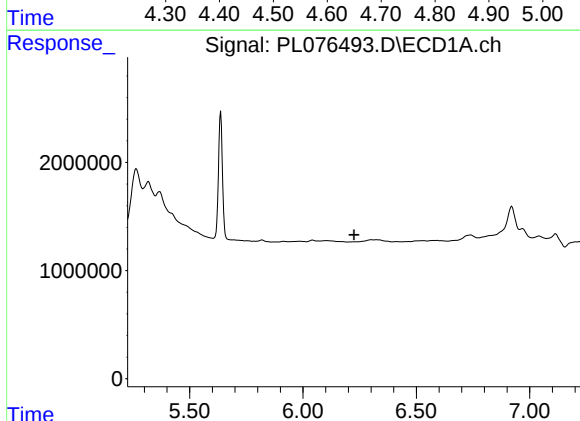


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 6.225 min
Response: 0
Conc: N.D.

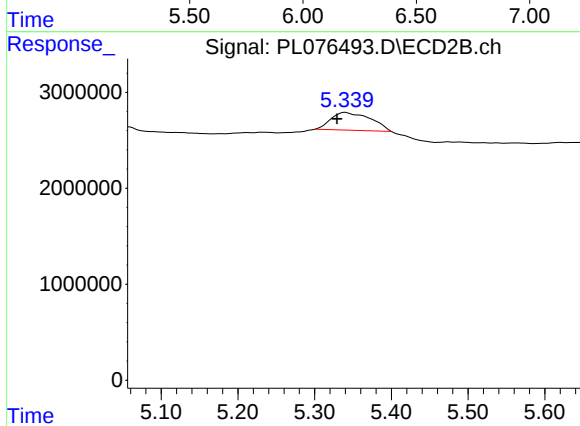

#2 alpha-BHC


R.T.: 5.340 min
Delta R.T.: 0.010 min
Response: 6652880
Conc: 2.43 ng/ml

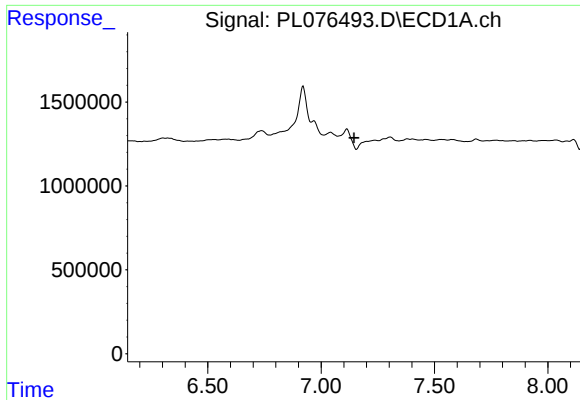

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

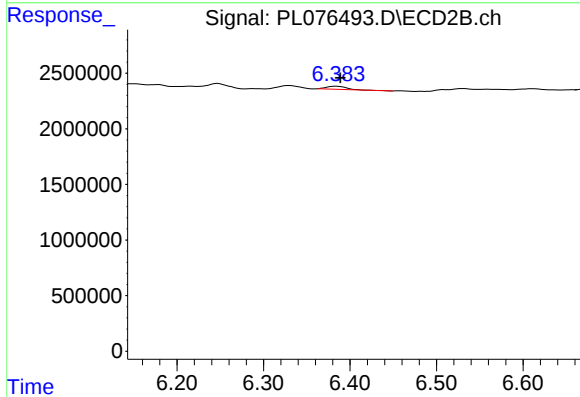


#7 delta-BHC

R.T.: 6.385 min
Delta R.T.: -0.004 min
Response: 469539
Conc: 0.20 ng/ml

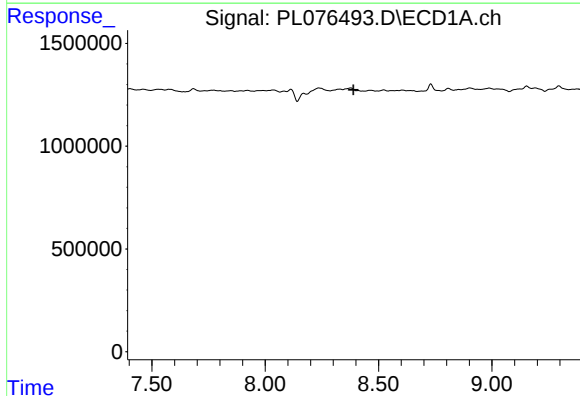


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.389 min
Response: 0
Conc: N.D.

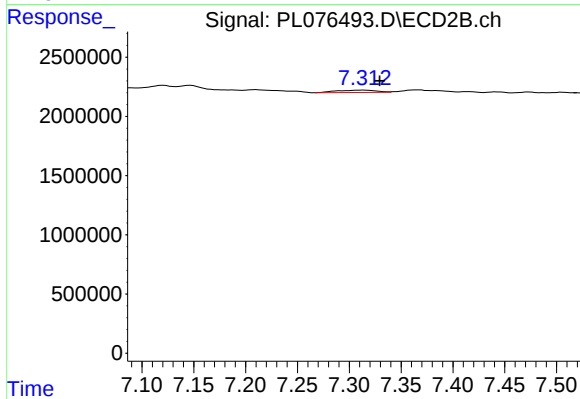

#10 gamma-Chlordane


R.T.: 7.314 min
Delta R.T.: -0.016 min
Response: 542090
Conc: 0.27 ng/ml

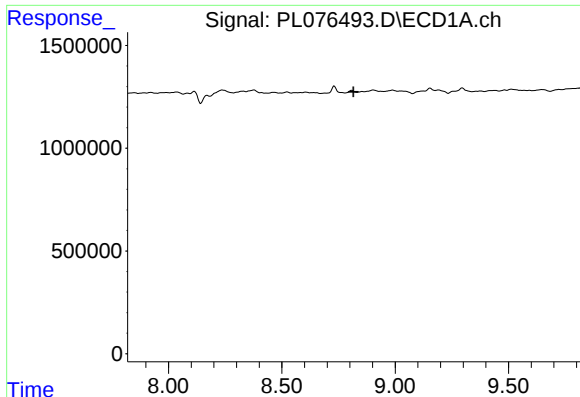

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

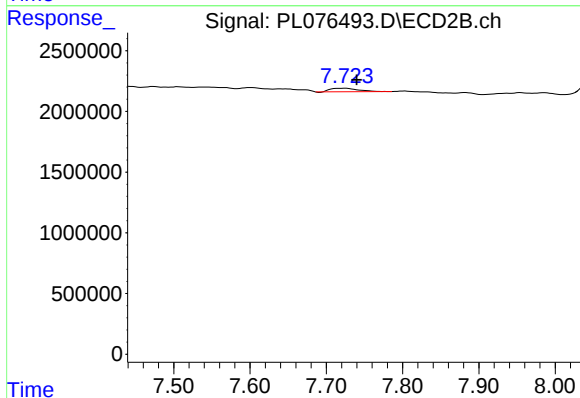


#13 Dieldrin

R.T.: 7.725 min
Delta R.T.: -0.015 min
Response: 722377
Conc: 0.38 ng/ml

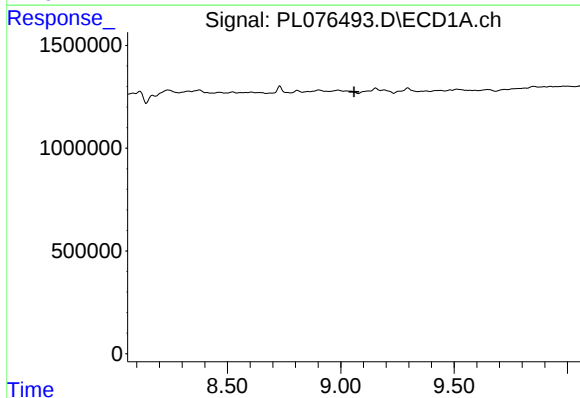


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

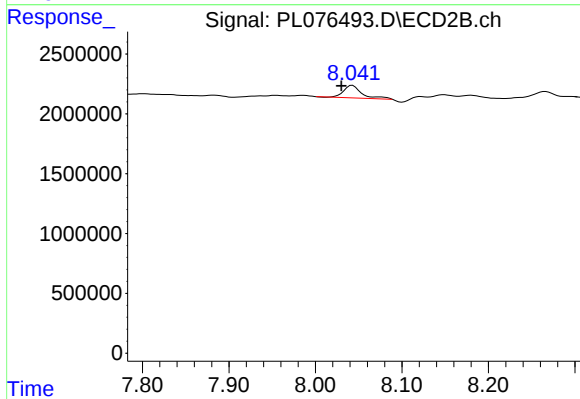

#14 Endrin


R.T.: 8.043 min
Delta R.T.: 0.013 min
Response: 1500486
Conc: 1.04 ng/ml

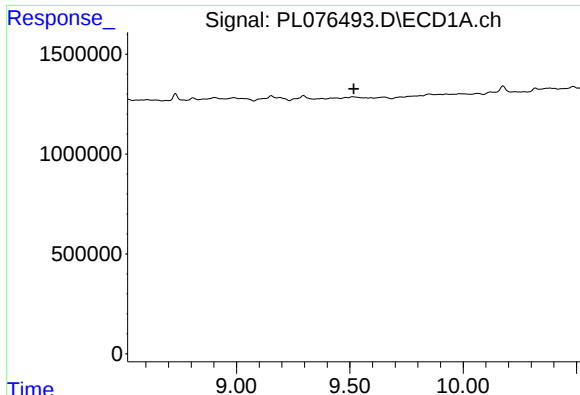

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.517 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

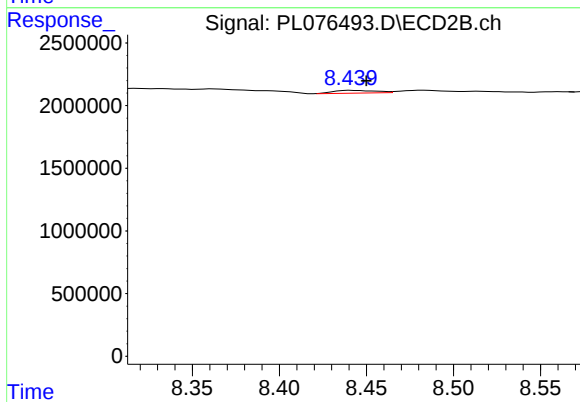


#17 4,4'-DDT

R.T.: 8.441 min
Delta R.T.: -0.009 min
Response: 364314
Conc: 0.23 ng/ml

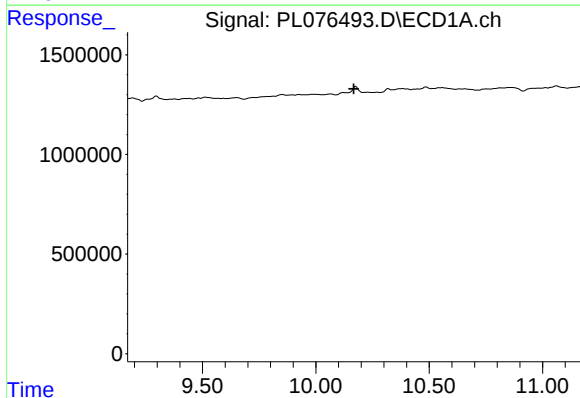


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 10.167 min
Response: 0
Conc: N.D.

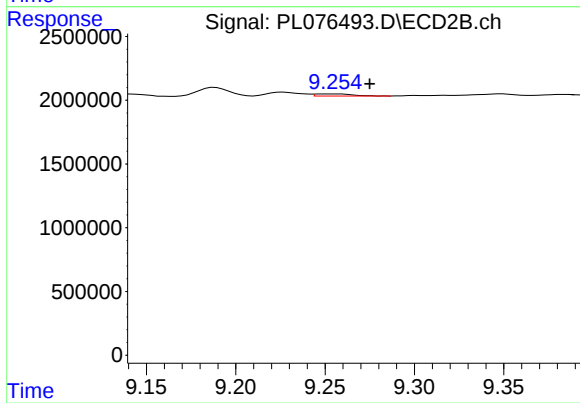

#21 Endrin ketone


R.T.: 9.256 min
Delta R.T.: -0.019 min
Response: 229166
Conc: 0.14 ng/ml

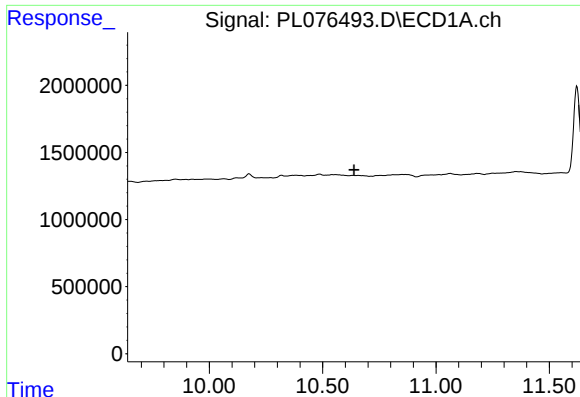

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 10.638 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

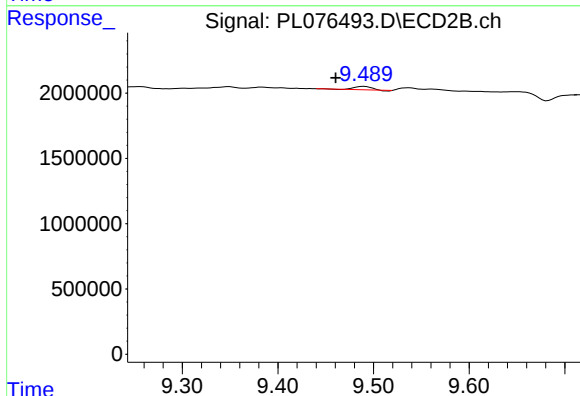


#22 Mirex

R.T.: 9.490 min
Delta R.T.: 0.030 min
Response: 289708
Conc: 0.22 ng/ml

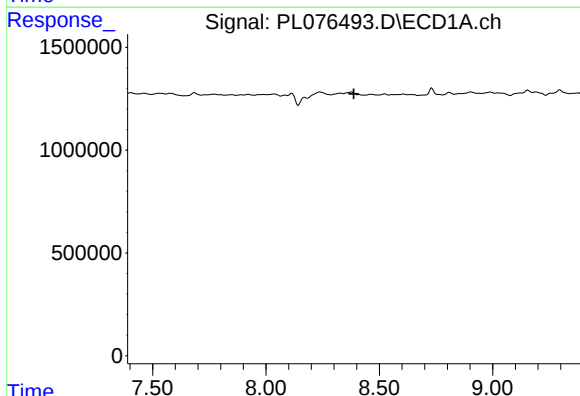


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 8.388 min
Response: 0
Conc: N.D.

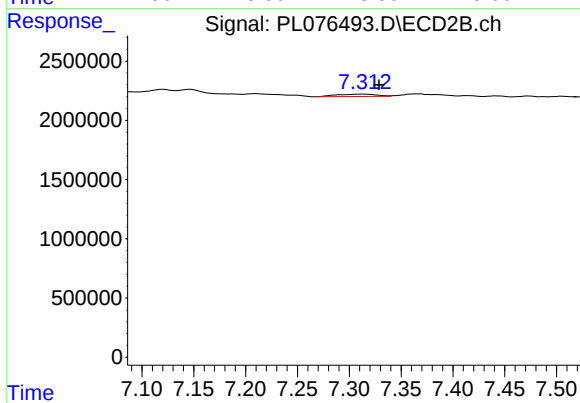

#25 Chlordane-3


R.T.: 7.314 min
Delta R.T.: -0.015 min
Response: 542090
Conc: 3.20 ng/ml

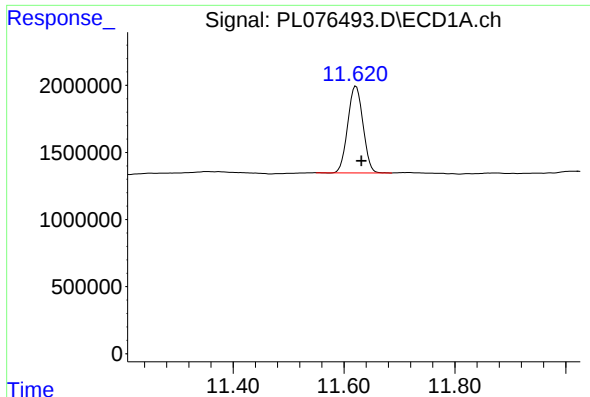

#28 Decachlorobiphenyl

R.T.: 11.622 min
Delta R.T.: -0.010 min
Response: 12327791
Conc: 20.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

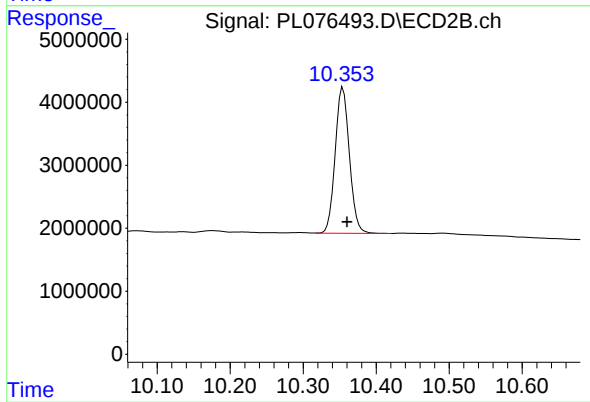

#28 Decachlorobiphenyl

R.T.: 10.354 min
Delta R.T.: -0.006 min
Response: 31361343
Conc: 18.69 ng/ml