

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071822\
 Data File : PL076480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2022 14:23
 Operator : AR\AJ
 Sample : N3697-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PIPELINE-PIGGING-TK2045L

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 15:58:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.645	4.627	8139342	35770075	11.298m	17.692 #
28)	SA Decachlor...	11.632	10.363	4477301	7074319	7.589	4.216 #
Target Compounds							
6)	B beta-BHC	6.879	6.131	1732770	6203300	3.942	5.672m#
16)	A 4,4'-DDD	9.197	8.186	1771098	3629912	3.390	2.503m#
18)	B Endrin al...	9.438	8.518	1837808	6070815	3.808	4.845m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071822\
Data File : PL076480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2022 14:23
Operator : AR\AJ
Sample : N3697-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PIPELINE-PIGGING-TK2045L

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 15:58:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

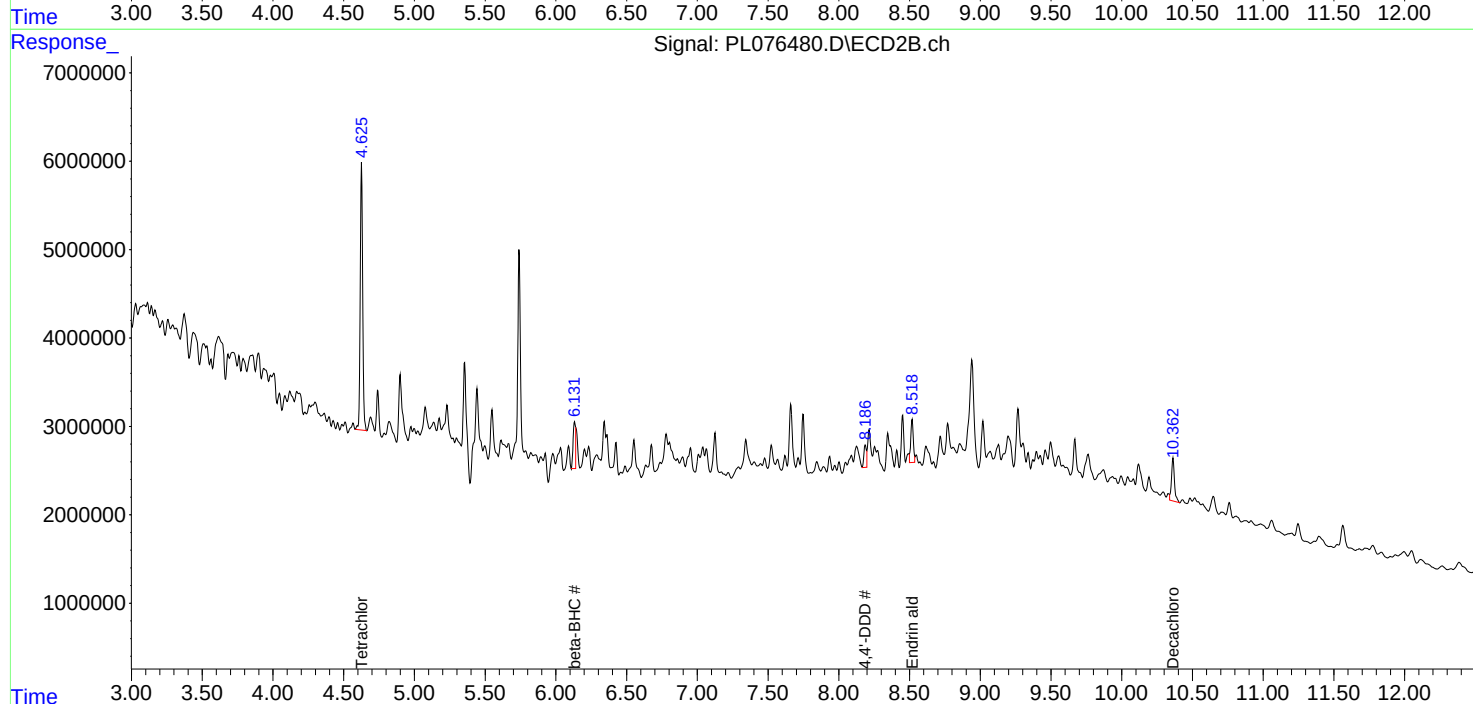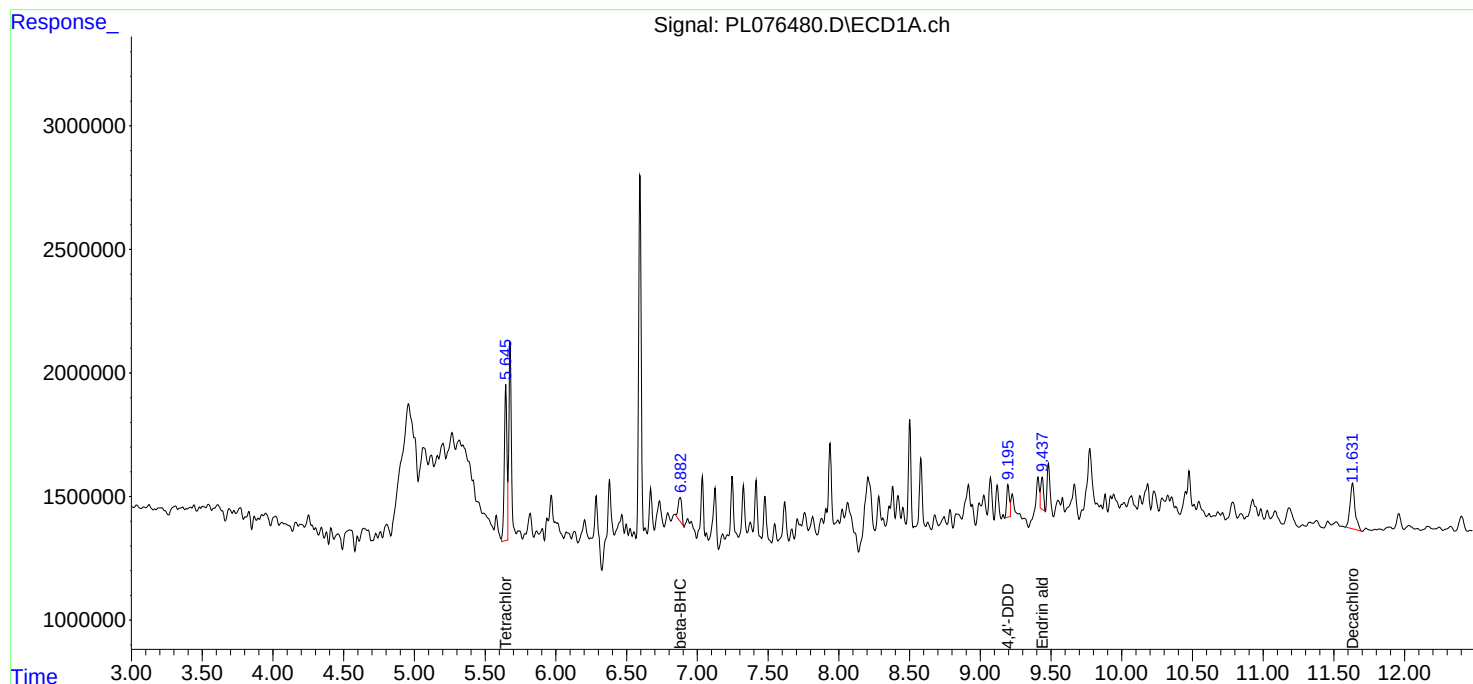


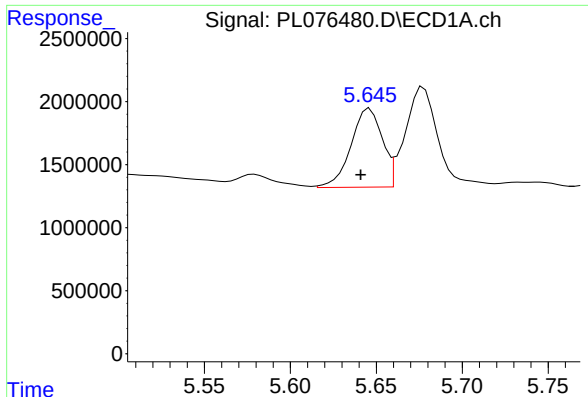

#1 Tetrachloro-m-xylene


R.T.: 5.645 min
Delta R.T.: 0.004 min
Response: 8139342
Conc: 11.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PIPELINE-PIGGING-TK2045L

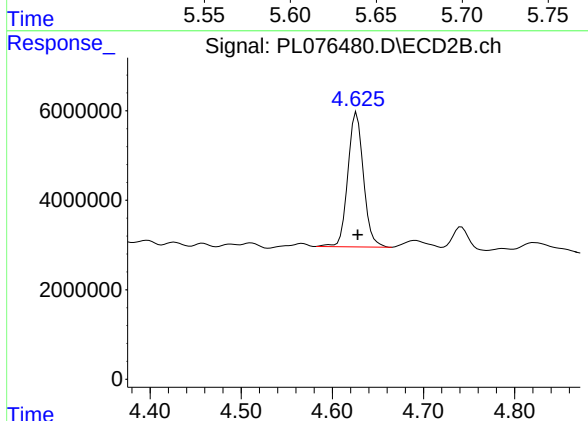


#1 Tetrachloro-m-xylene

R.T.: 4.627 min
Delta R.T.: -0.001 min
Response: 35770075
Conc: 17.69 ng/ml

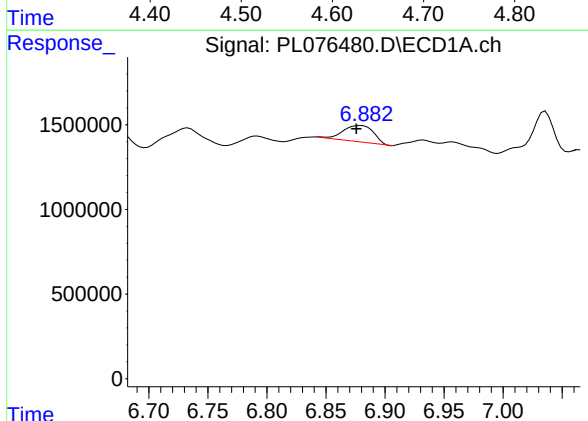


#6 beta-BHC

R.T.: 6.879 min
Delta R.T.: 0.004 min
Response: 1732770
Conc: 3.94 ng/ml

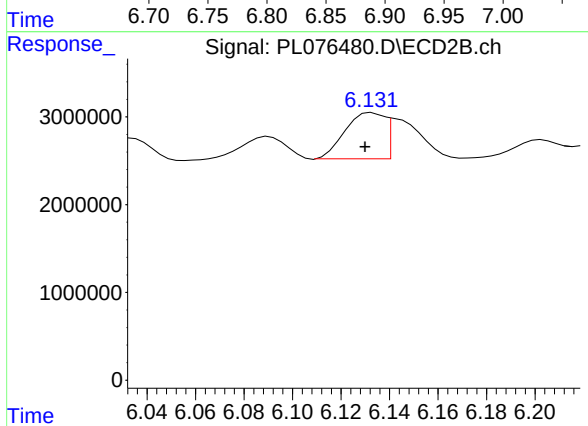

#6 beta-BHC


R.T.: 6.131 min
Delta R.T.: 0.002 min
Response: 6203300
Conc: 5.67 ng/ml m

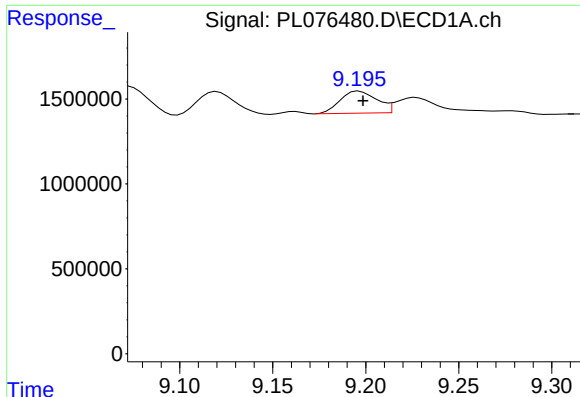

#16 4,4'-DDD


R.T.: 9.197 min
Delta R.T.: -0.002 min
Response: 1771098
Conc: 3.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PIPELINE-PIGGING-TK2045L

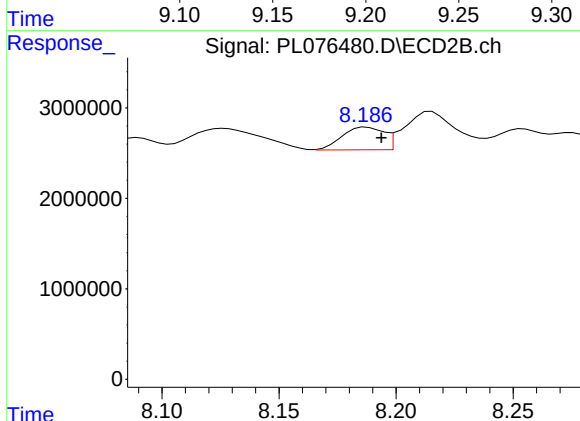


#16 4,4'-DDD

R.T.: 8.186 min
Delta R.T.: -0.008 min
Response: 3629912
Conc: 2.50 ng/ml m

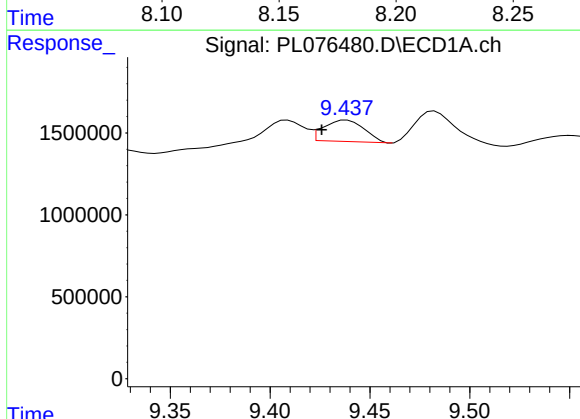


#18 Endrin aldehyde

R.T.: 9.438 min
Delta R.T.: 0.012 min
Response: 1837808
Conc: 3.81 ng/ml

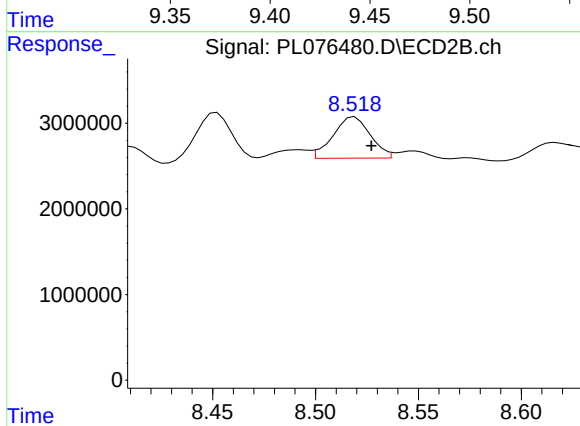

#18 Endrin aldehyde


R.T.: 8.518 min
Delta R.T.: -0.009 min
Response: 6070815
Conc: 4.84 ng/ml m

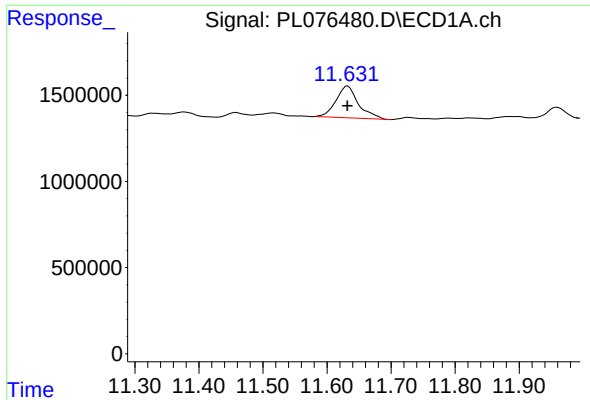

#28 Decachlorobiphenyl

R.T.: 11.632 min
Delta R.T.: 0.000 min
Response: 4477301
Conc: 7.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PIPELINE-PIGGING-TK2045L

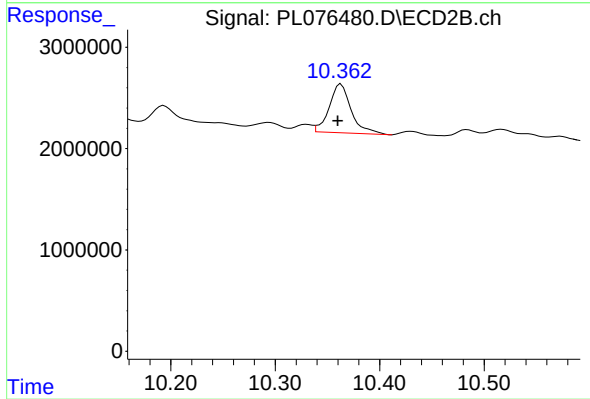

#28 Decachlorobiphenyl

R.T.: 10.363 min
Delta R.T.: 0.003 min
Response: 7074319
Conc: 4.22 ng/ml