

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071822\
 Data File : PL076487.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2022 17:49
 Operator : AR\AJ
 Sample : N3697-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CASING-NUMBER-5D-WATERING

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 18:21:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.637	4.619	12572131	32510847	17.452	16.080m
28)	SA Decachlor...	11.620	10.354	8586868	21509277	14.555	12.819

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071822\
Data File : PL076487.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2022 17:49
Operator : AR\AJ
Sample : N3697-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CASING-NUMBER-5D-WATERING

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 18:21:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

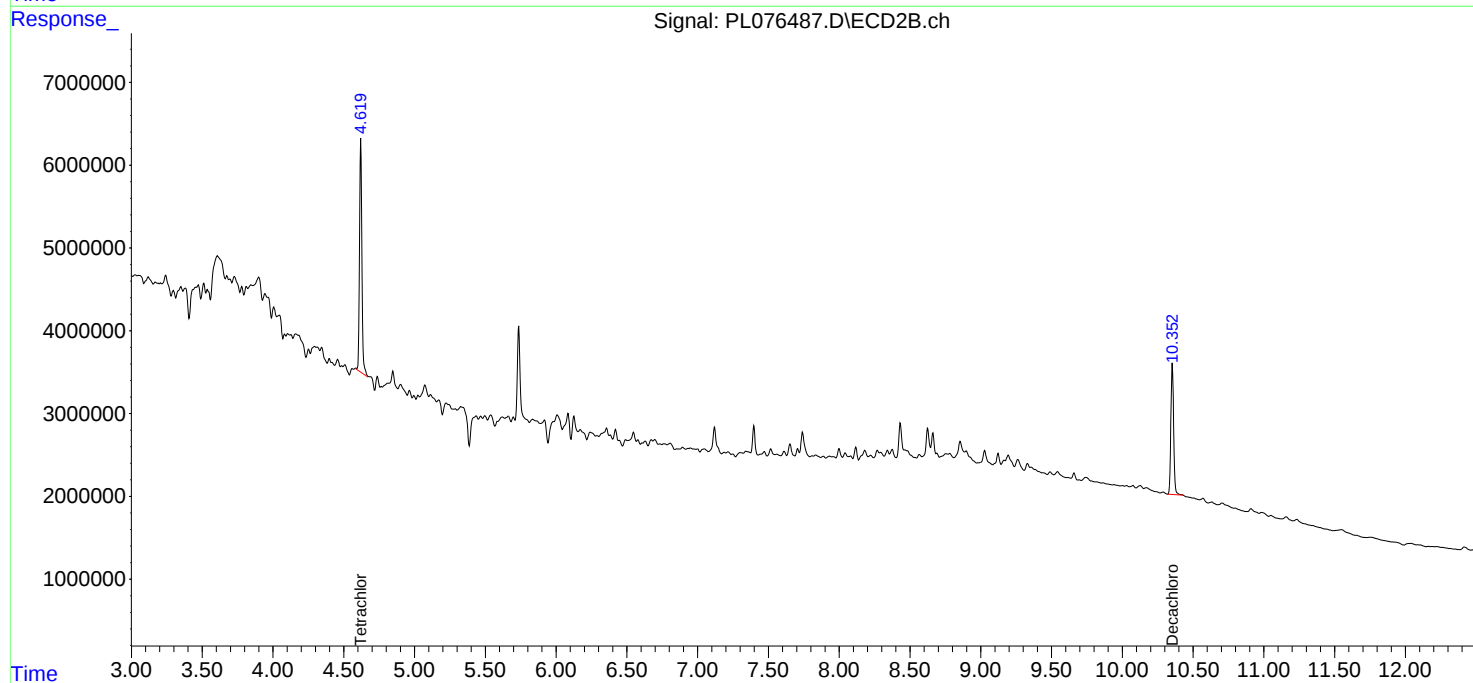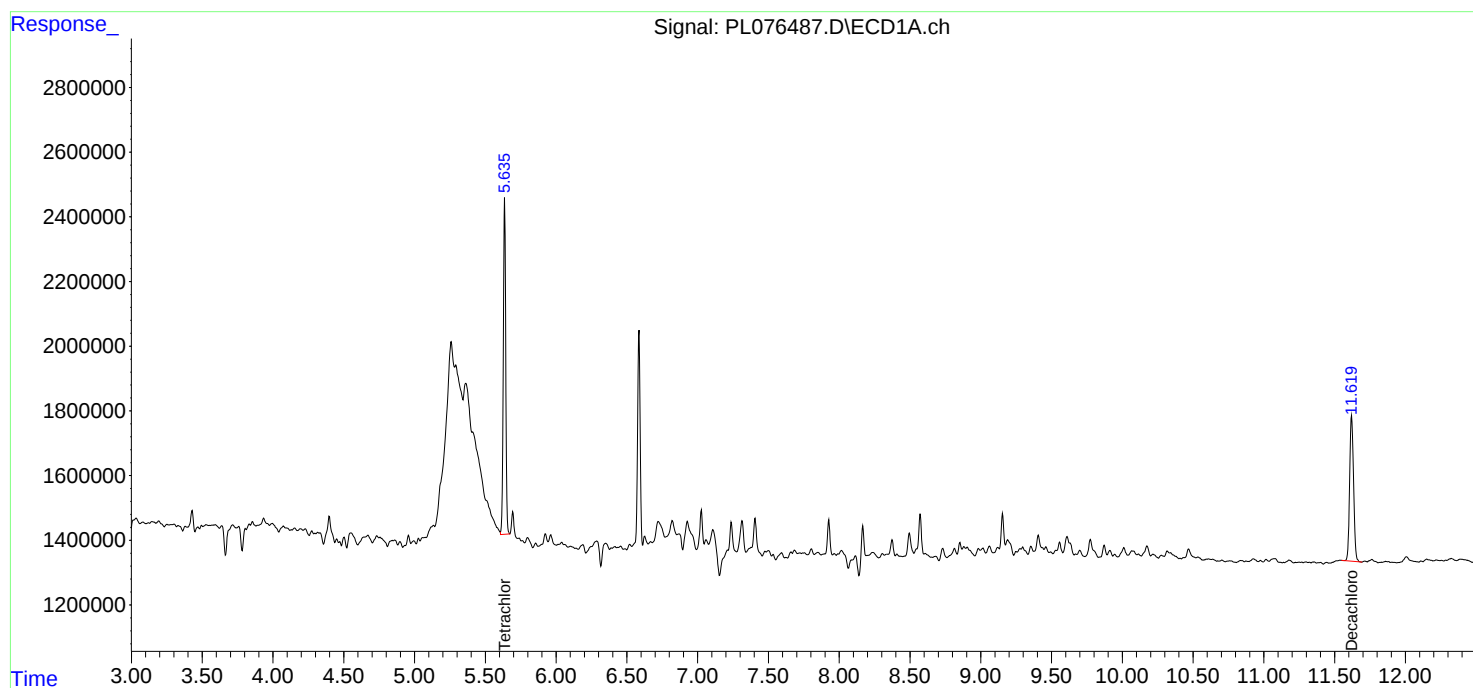


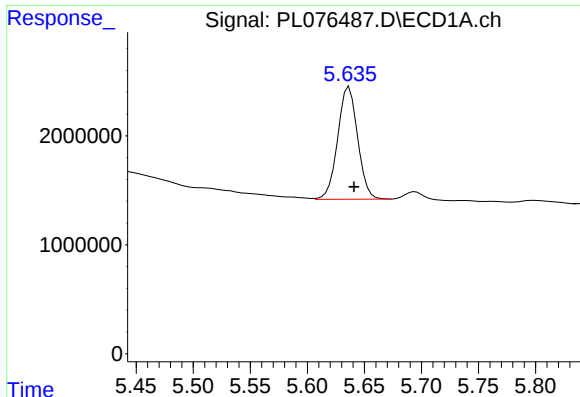

#1 Tetrachloro-m-xylene


R.T.: 5.637 min
Delta R.T.: -0.004 min
Response: 12572131
Conc: 17.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
CASING-NUMBER-5D-WATERING

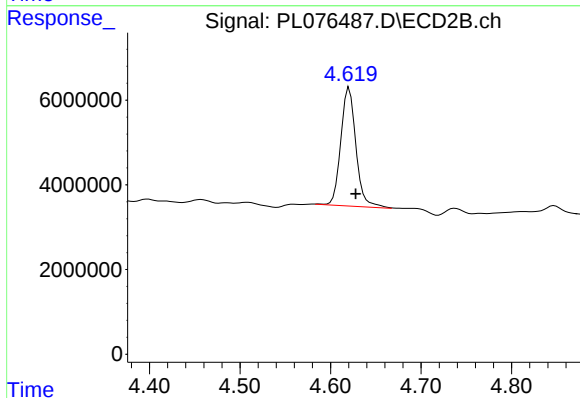


#1 Tetrachloro-m-xylene

R.T.: 4.619 min
Delta R.T.: -0.009 min
Response: 32510847
Conc: 16.08 ng/ml m

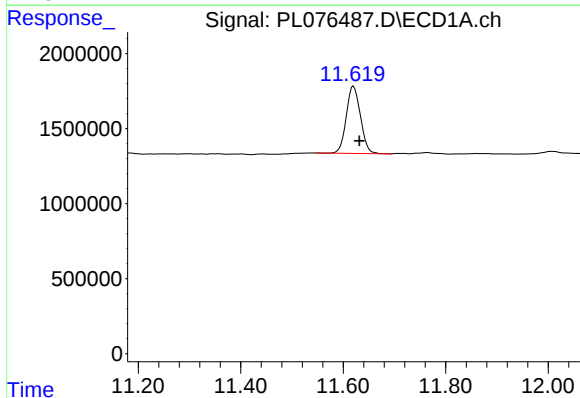

#28 Decachlorobiphenyl

R.T.: 11.620 min
Delta R.T.: -0.012 min
Response: 8586868
Conc: 14.55 ng/ml

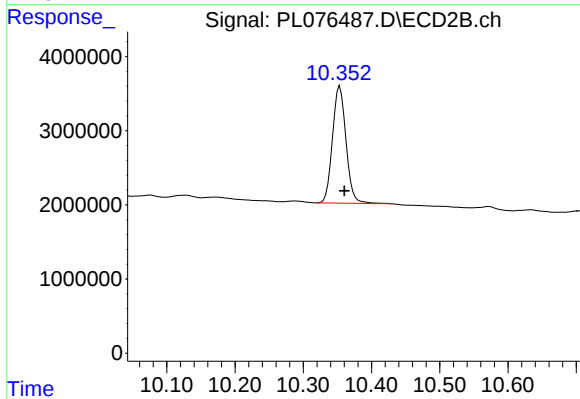

#28 Decachlorobiphenyl

R.T.: 10.354 min
Delta R.T.: -0.006 min
Response: 21509277
Conc: 12.82 ng/ml