

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071822\
 Data File : PL076488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2022 18:06
 Operator : AR\AJ
 Sample : N3697-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PIPELINE-PIGGING-TK2045L

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 18:22:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.636	4.623	9291339	39672600	12.898m	19.622 #
2)	SA Decachlor...	11.618	10.354	5274291	8185562	8.940m	4.878 #
Target Compounds							
6)	B beta-BHC	6.872	6.125	1474529	5357330	3.355m	4.899m#
16)	A 4,4'-DDD	9.186	8.179f	1976405	3467532	3.783m	2.391m#
18)	B Endrin al...	9.429	8.540	2115819	1505535	4.384m	1.201m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071822\
Data File : PL076488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2022 18:06
Operator : AR\AJ
Sample : N3697-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PIPELINE-PIGGING-TK2045L

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 18:22:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

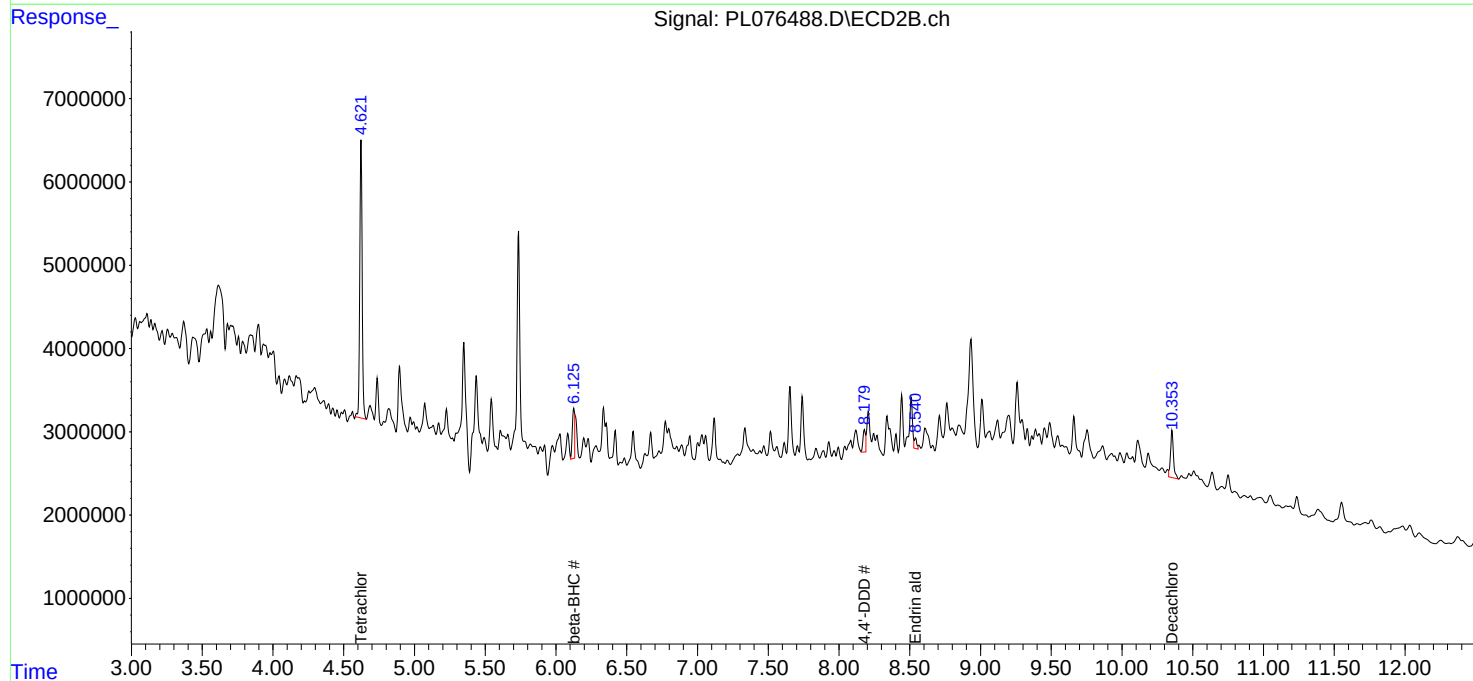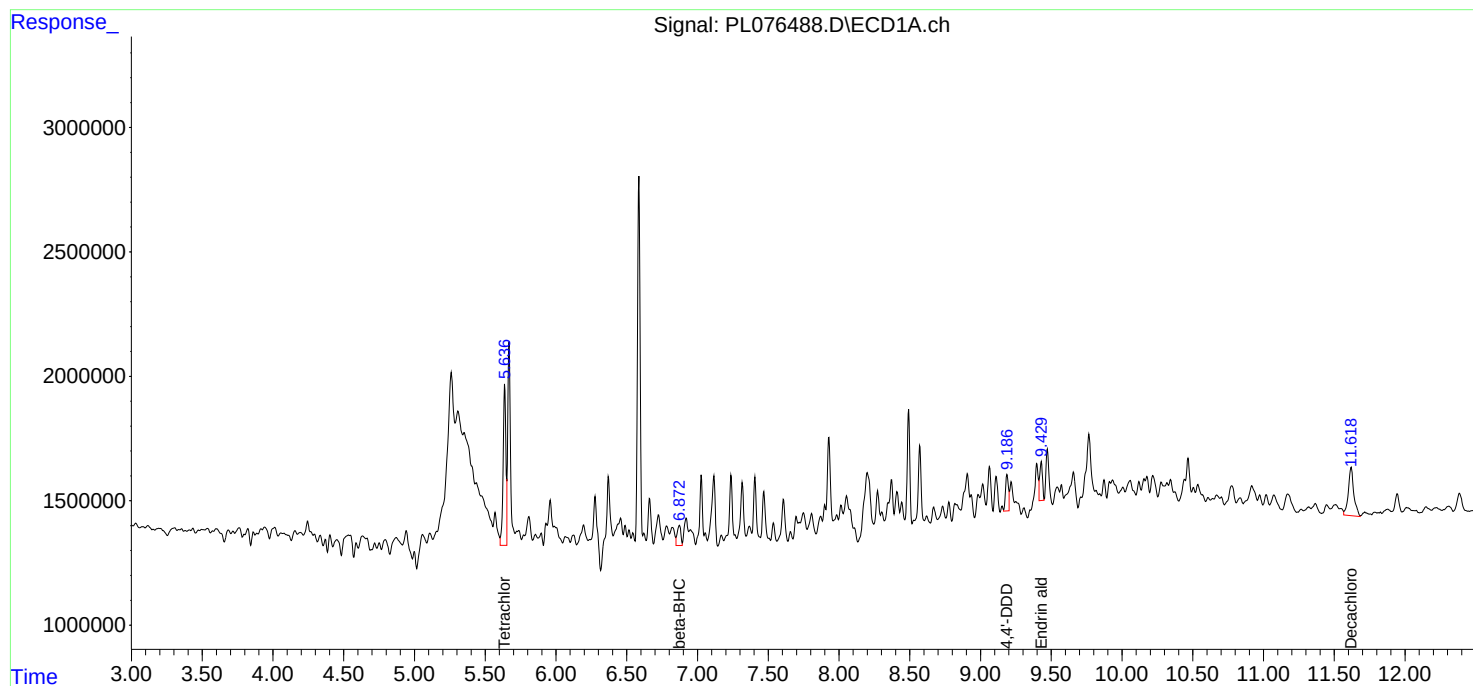


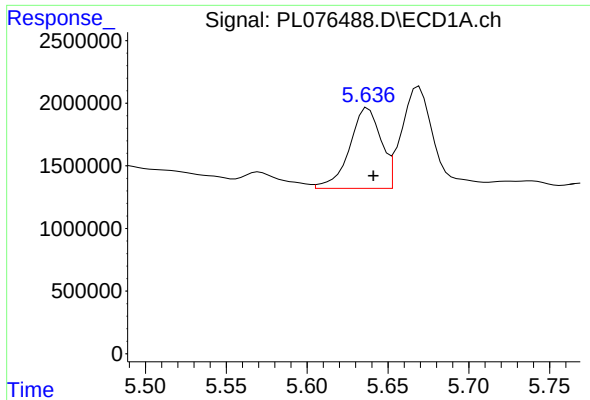

#1 Tetrachloro-m-xylene


R.T.: 5.636 min
Delta R.T.: -0.005 min
Response: 9291339
Conc: 12.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PIPELINE-PIGGING-TK2045L

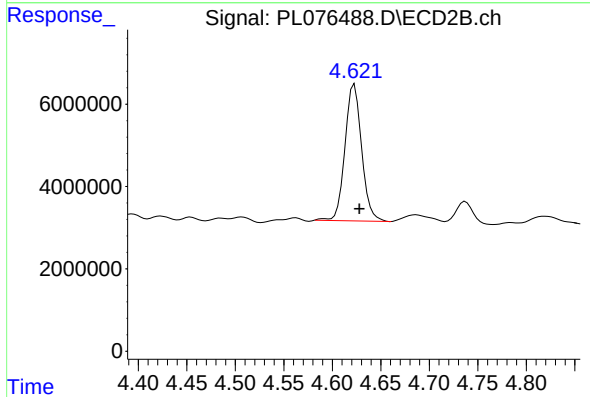


#1 Tetrachloro-m-xylene

R.T.: 4.623 min
Delta R.T.: -0.005 min
Response: 39672600
Conc: 19.62 ng/ml

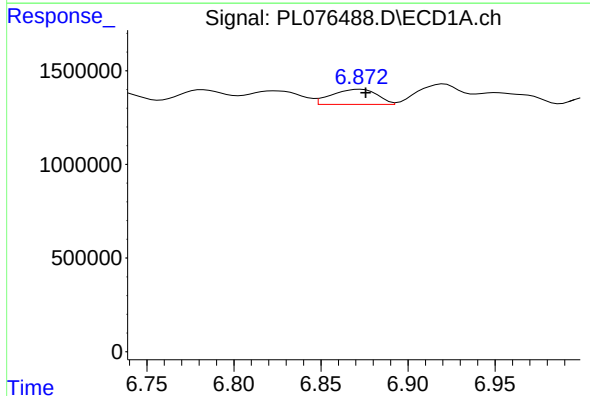


#6 beta-BHC

R.T.: 6.872 min
Delta R.T.: -0.004 min
Response: 1474529
Conc: 3.35 ng/ml m

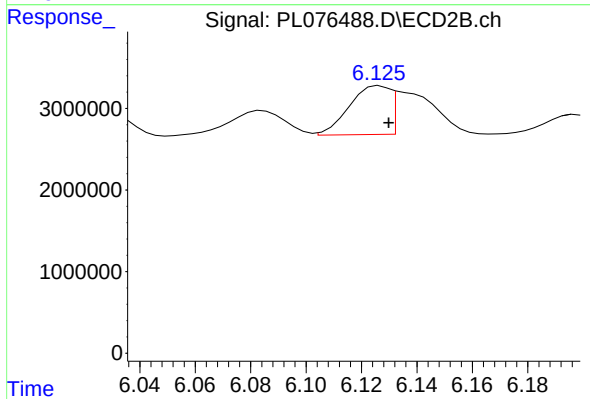

#6 beta-BHC


R.T.: 6.125 min
Delta R.T.: -0.005 min
Response: 5357330
Conc: 4.90 ng/ml m

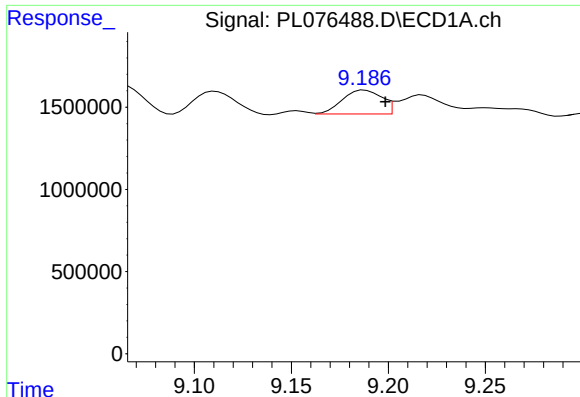

#16 4,4'-DDD


R.T.: 9.186 min
Delta R.T.: -0.012 min
Response: 1976405
Conc: 3.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PIPELINE-PIGGING-TK2045L

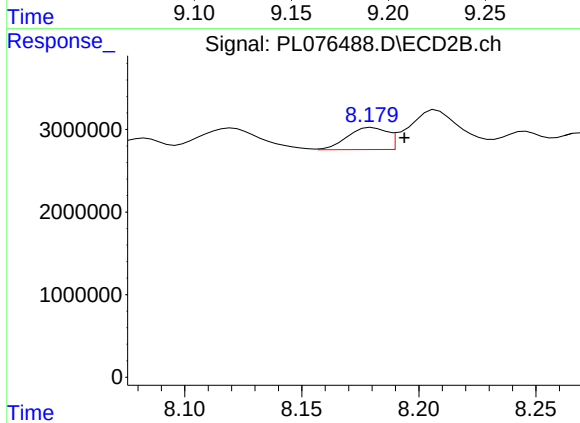


#16 4,4'-DDD

R.T.: 8.179 min
Delta R.T.: -0.015 min
Response: 3467532
Conc: 2.39 ng/ml m

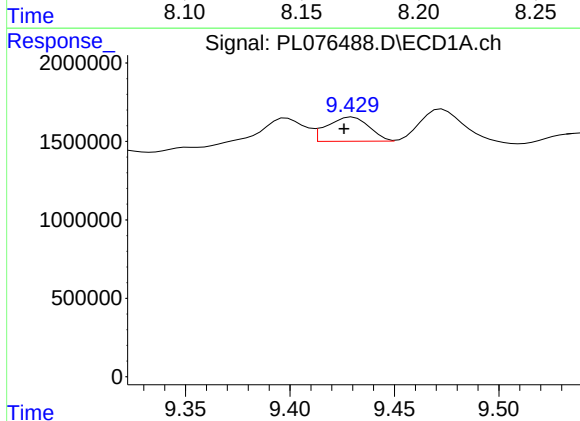


#18 Endrin aldehyde

R.T.: 9.429 min
Delta R.T.: 0.003 min
Response: 2115819
Conc: 4.38 ng/ml m

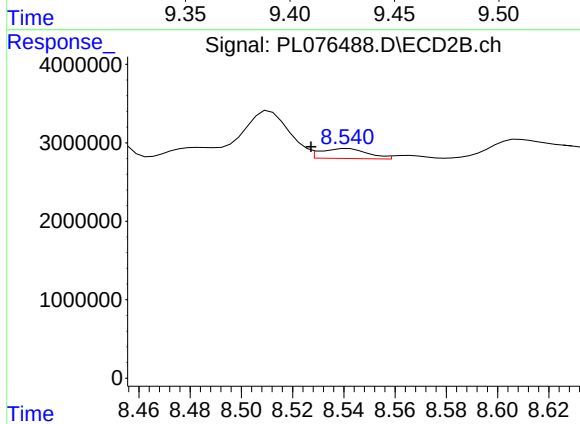

#18 Endrin aldehyde


R.T.: 8.540 min
Delta R.T.: 0.013 min
Response: 1505535
Conc: 1.20 ng/ml m

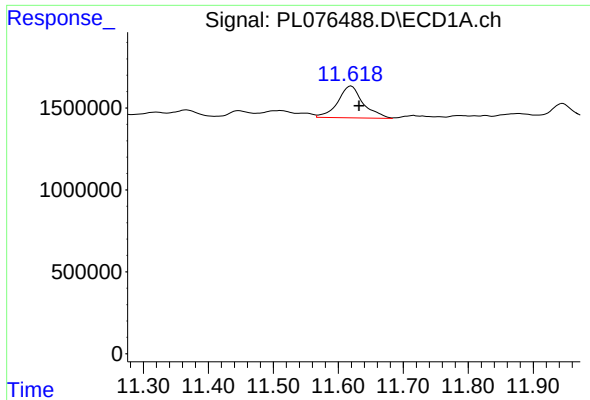

#28 Decachlorobiphenyl

R.T.: 11.618 min
Delta R.T.: -0.013 min
Response: 5274291
Conc: 8.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PIPELINE-PIGGING-TK2045L

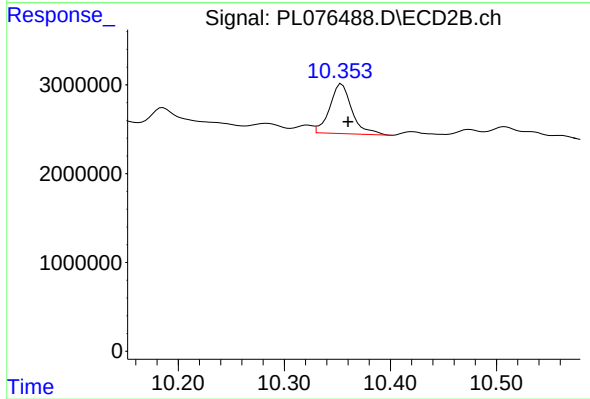

#28 Decachlorobiphenyl

R.T.: 10.354 min
Delta R.T.: -0.006 min
Response: 8185562
Conc: 4.88 ng/ml