

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071822\
 Data File : PL076498.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2022 22:18
 Operator : AR\AJ
 Sample : N3746-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-071522

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 00:17:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.636	4.621	9064358	24583568	12.582	12.159
28)	SA Decachlor...	11.621	10.355	7797298	19702374	13.217	11.742
Target Compounds							
10)	B gamma-Chl...	8.380	7.318	892177	1818542	1.228m	0.912m#
11)	B alpha-Chl...	8.464	7.385	1618709	2636542	2.237m	1.311m#
17)	MA 4,4'-DDT	9.508	8.437	322096	1329947	0.542m	0.851m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071822\
Data File : PL076498.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2022 22:18
Operator : AR\AJ
Sample : N3746-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-02-071522

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 00:17:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

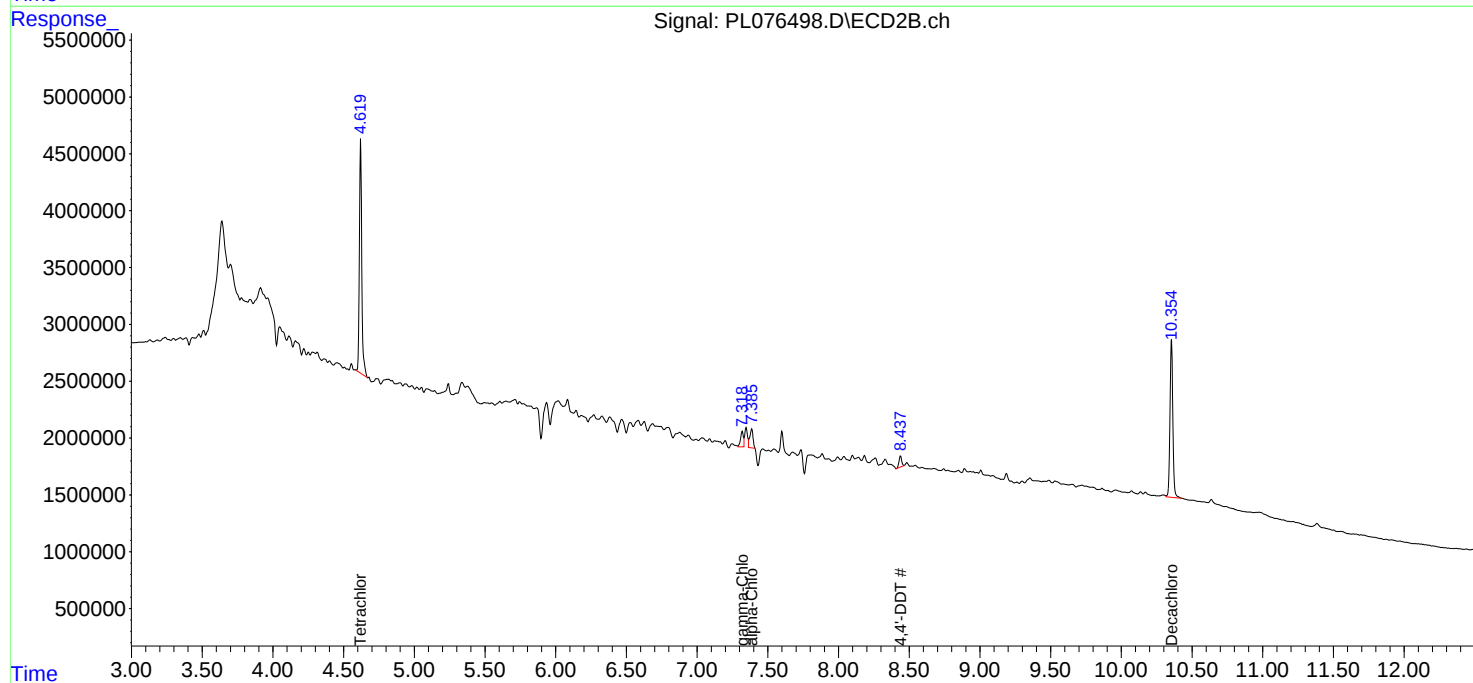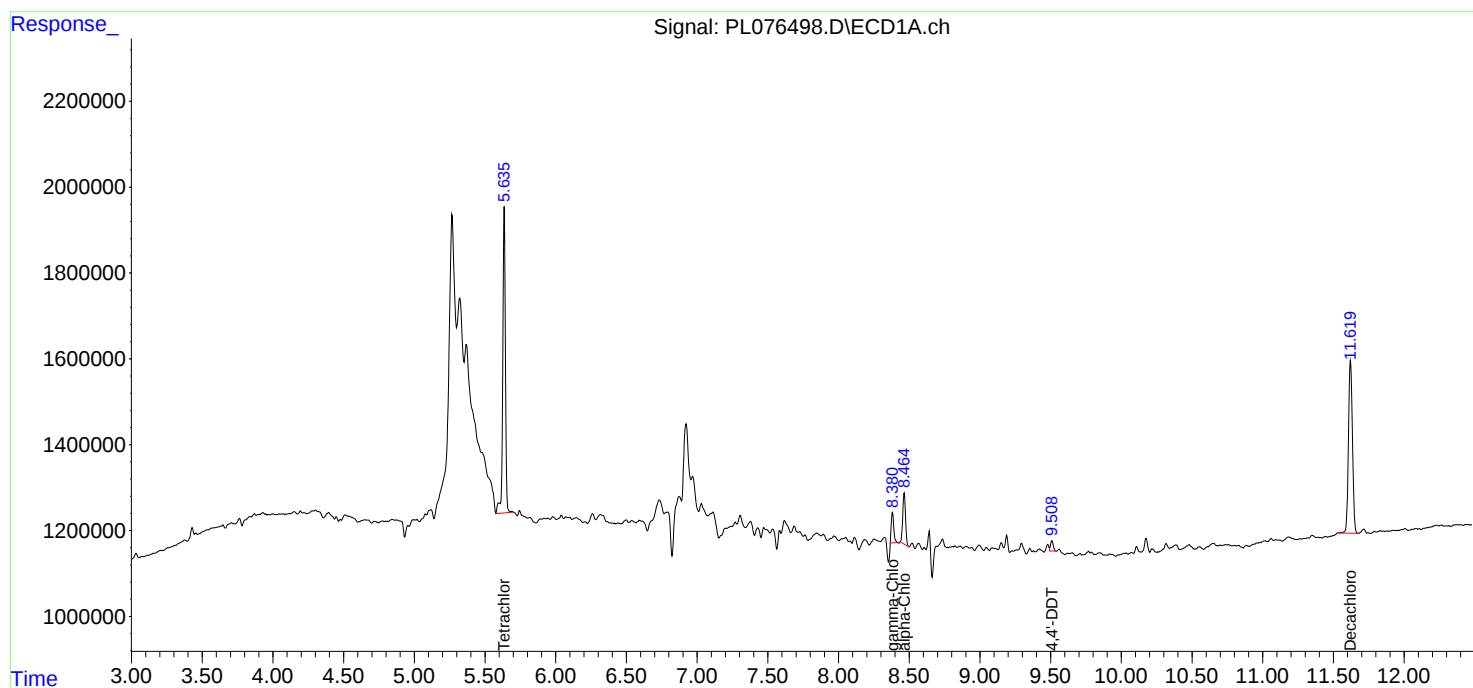


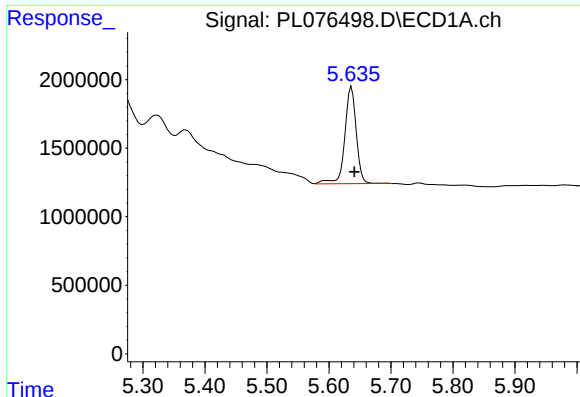

#1 Tetrachloro-m-xylene


R.T.: 5.636 min
Delta R.T.: -0.005 min
Response: 9064358
Conc: 12.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-071522

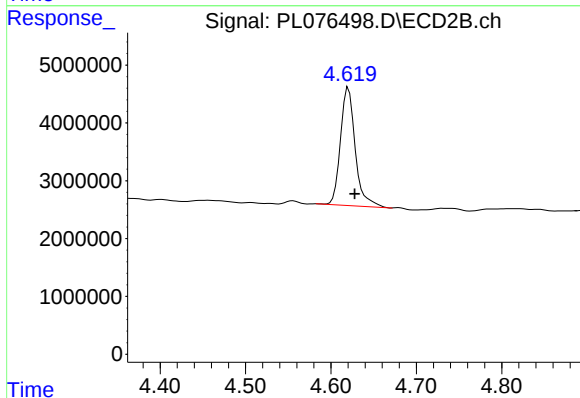


#1 Tetrachloro-m-xylene

R.T.: 4.621 min
Delta R.T.: -0.007 min
Response: 24583568
Conc: 12.16 ng/ml

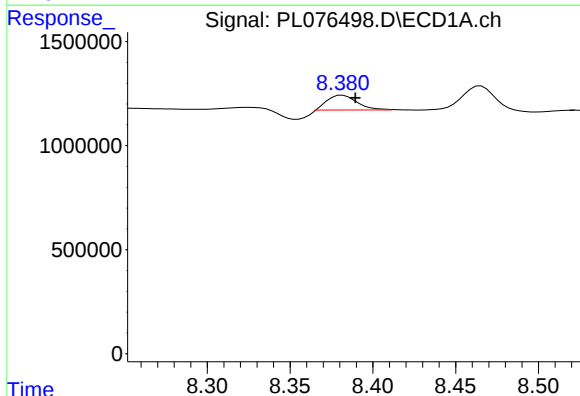


#10 gamma-Chlordane

R.T.: 8.380 min
Delta R.T.: -0.009 min
Response: 892177
Conc: 1.23 ng/ml m

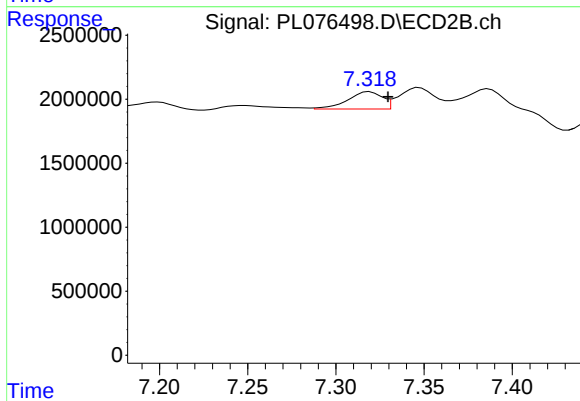

#10 gamma-Chlordane


R.T.: 7.318 min
Delta R.T.: -0.012 min
Response: 1818542
Conc: 0.91 ng/ml m

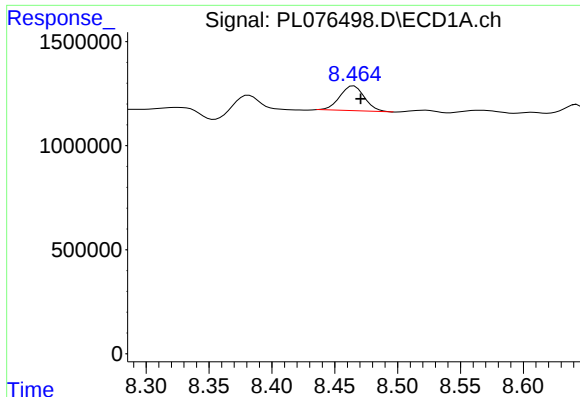

#11 alpha-Chlordane


R.T.: 8.464 min
Delta R.T.: -0.007 min
Response: 1618709
Conc: 2.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-071522

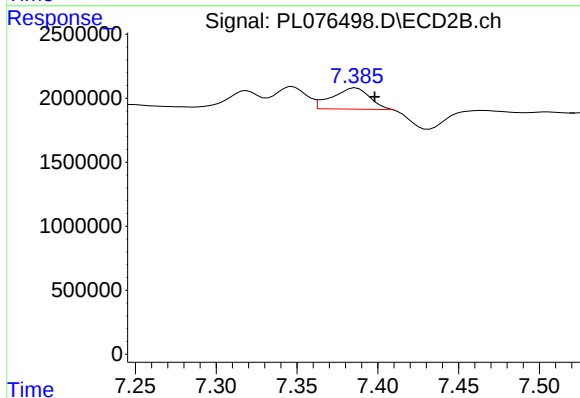


#11 alpha-Chlordane

R.T.: 7.385 min
Delta R.T.: -0.013 min
Response: 2636542
Conc: 1.31 ng/ml m

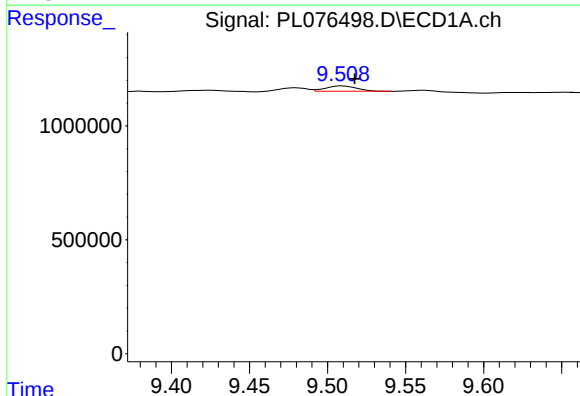


#17 4,4'-DDT

R.T.: 9.508 min
Delta R.T.: -0.009 min
Response: 322096
Conc: 0.54 ng/ml m

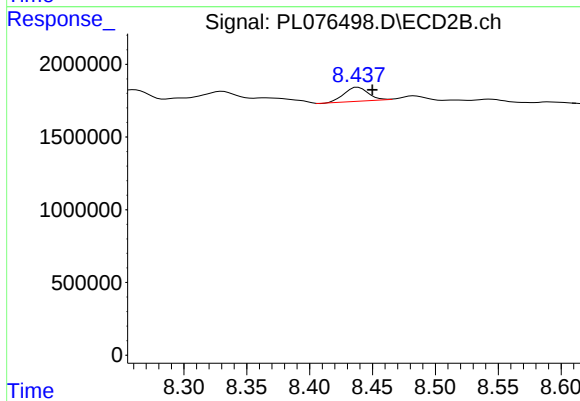

#17 4,4'-DDT


R.T.: 8.437 min
Delta R.T.: -0.013 min
Response: 1329947
Conc: 0.85 ng/ml m

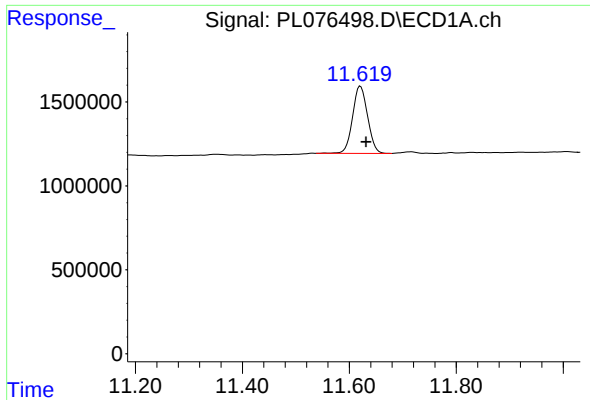

#28 Decachlorobiphenyl

R.T.: 11.621 min
Delta R.T.: -0.011 min
Response: 7797298
Conc: 13.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-071522

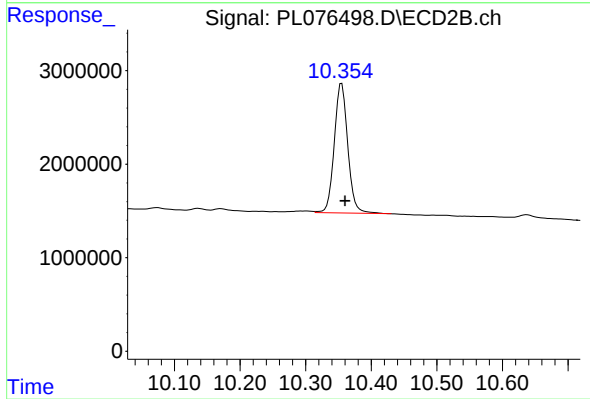

#28 Decachlorobiphenyl

R.T.: 10.355 min
Delta R.T.: -0.005 min
Response: 19702374
Conc: 11.74 ng/ml