

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071823\
 Data File : PL084001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 20:52
 Operator : AR\AJ
 Sample : 03639-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:44:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.688	22218409	11169261	11.110	10.057
28)	SA Decachlor...	9.020	7.870	11948284	10404655	9.179m	9.364
Target Compounds							
17)	MA 4,4'-DDT	6.979	5.975	1899068	1846557	1.191m	2.027 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071823\
Data File : PL084001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 20:52
Operator : AR\AJ
Sample : 03639-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:44:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

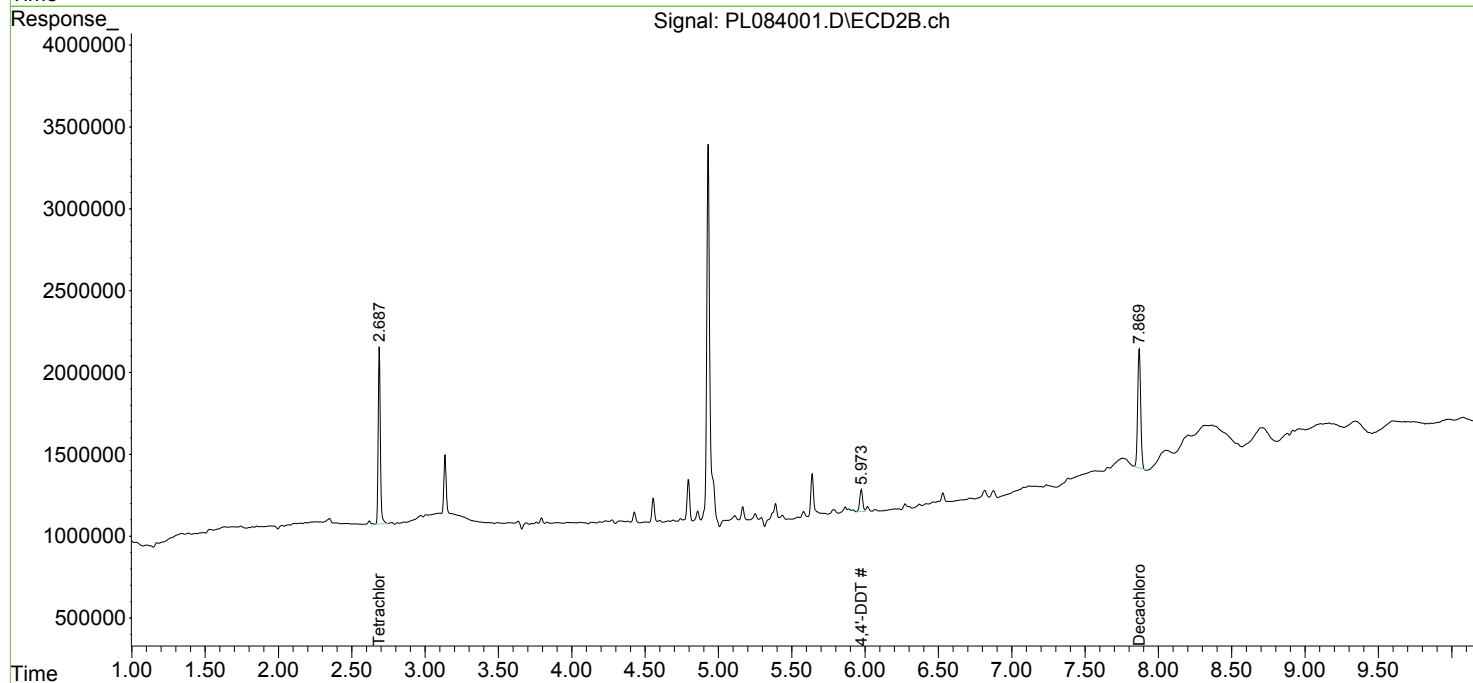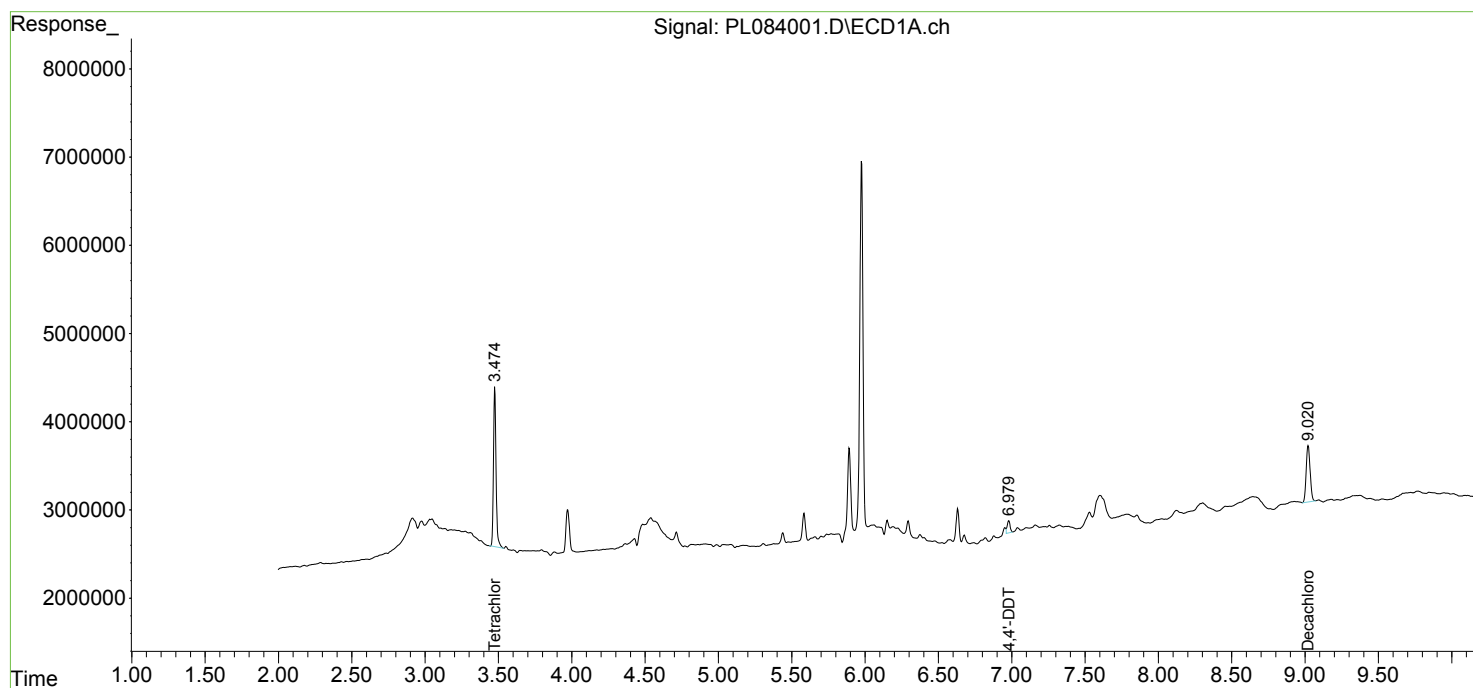


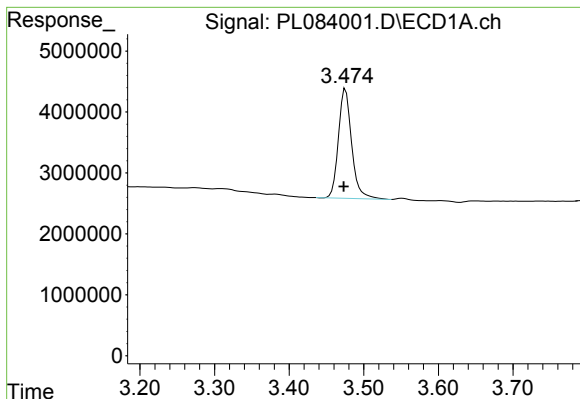

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 22218409
Conc: 11.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP3

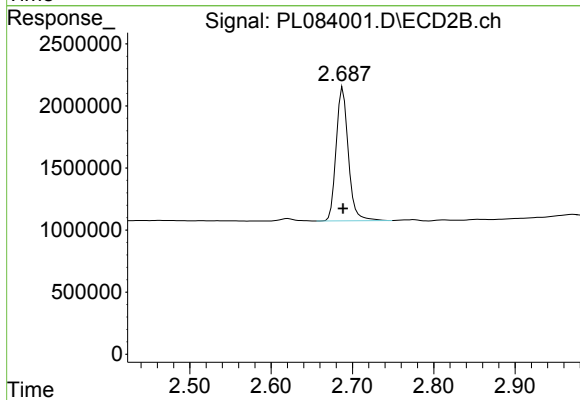


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: 0.000 min
Response: 11169261
Conc: 10.06 ng/ml

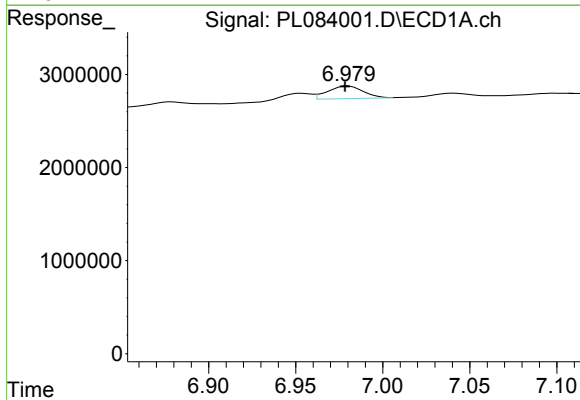


#17 4,4'-DDT

R.T.: 6.979 min
Delta R.T.: 0.000 min
Response: 1899068
Conc: 1.19 ng/ml m

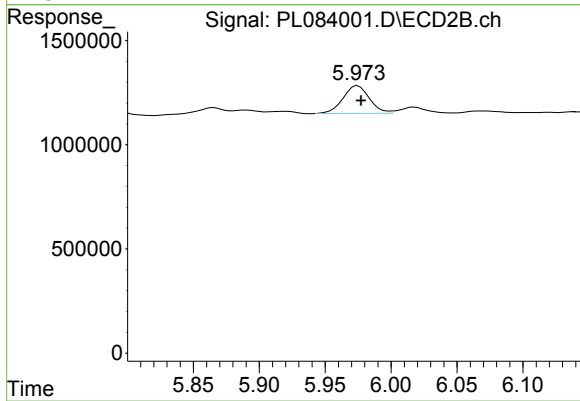

#17 4,4'-DDT


R.T.: 5.975 min
Delta R.T.: -0.002 min
Response: 1846557
Conc: 2.03 ng/ml

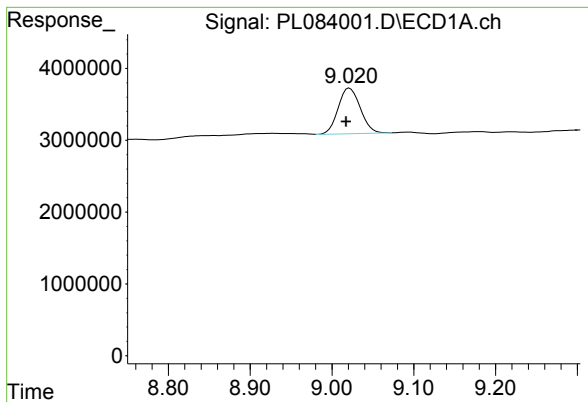

#28 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.003 min
Response: 11948284
Conc: 9.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP3

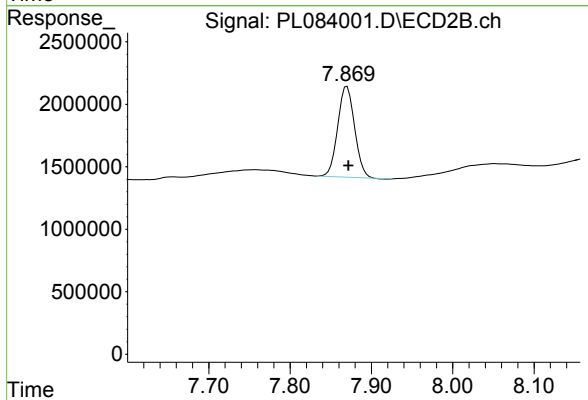

#28 Decachlorobiphenyl

R.T.: 7.870 min
Delta R.T.: -0.002 min
Response: 10404655
Conc: 9.36 ng/ml