

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071823\
 Data File : PL084003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 21:20
 Operator : AR\AJ
 Sample : 03639-21
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:44:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.688	37817444	19487052	18.910	17.547
28)	SA Decachlor...	9.022	7.871	21788271	19009465	16.739	17.108
Target Compounds							
13)	MA Dieldrin	6.293	5.290	1430057	956766	0.598m	0.735m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071823\
Data File : PL084003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 21:20
Operator : AR\AJ
Sample : 03639-21
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:44:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

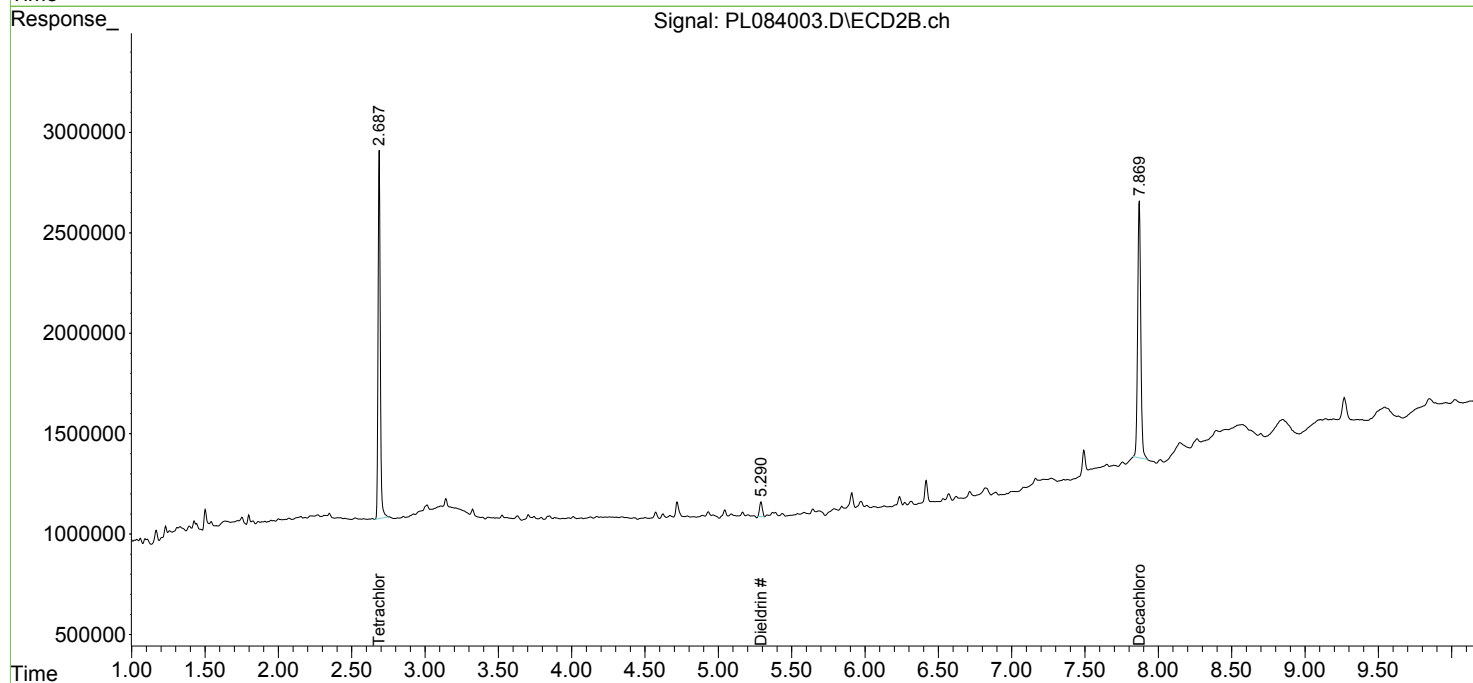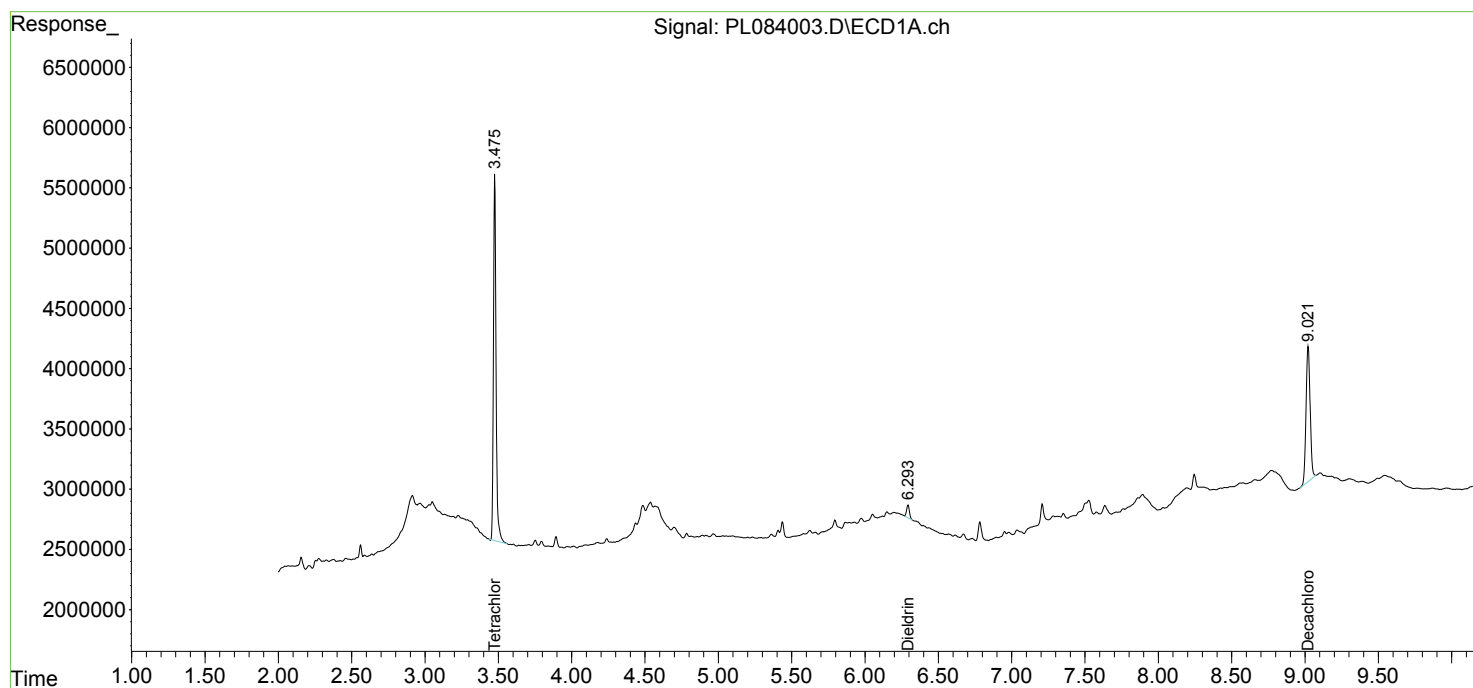


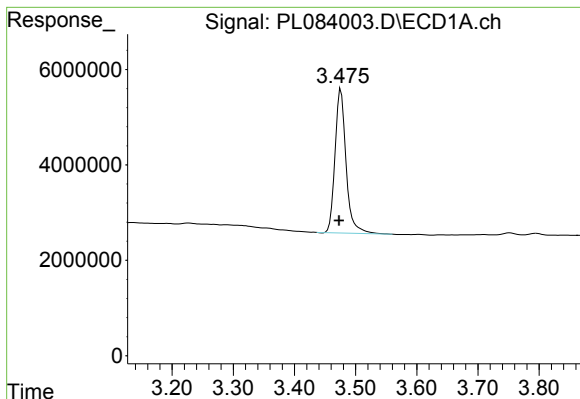

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 37817444
Conc: 18.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP5

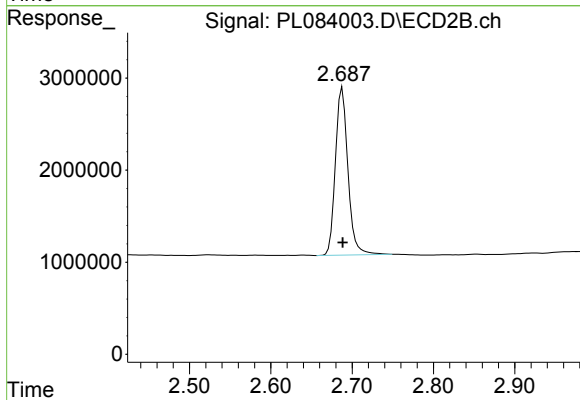


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: 0.000 min
Response: 19487052
Conc: 17.55 ng/ml

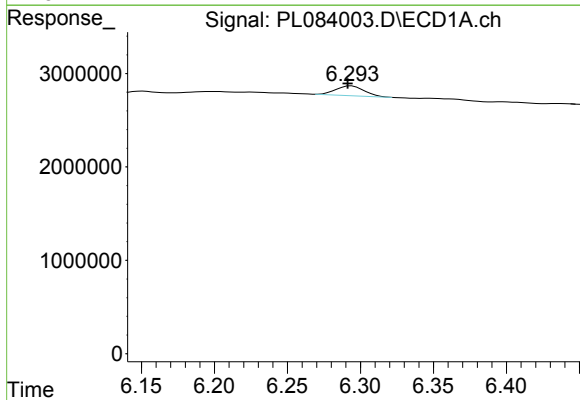


#13 Dieldrin

R.T.: 6.293 min
Delta R.T.: 0.001 min
Response: 1430057
Conc: 0.60 ng/ml m

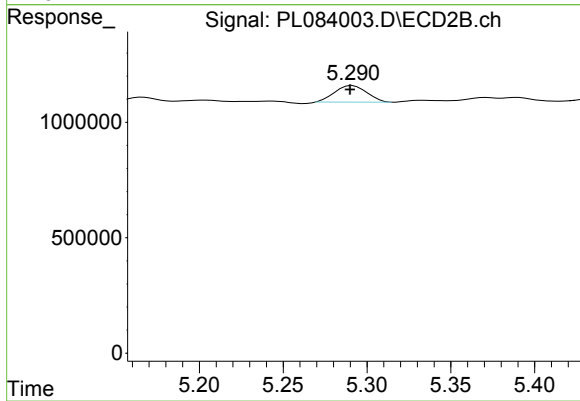

#13 Dieldrin

R.T.: 5.290 min
Delta R.T.: 0.000 min
Response: 956766
Conc: 0.73 ng/ml m

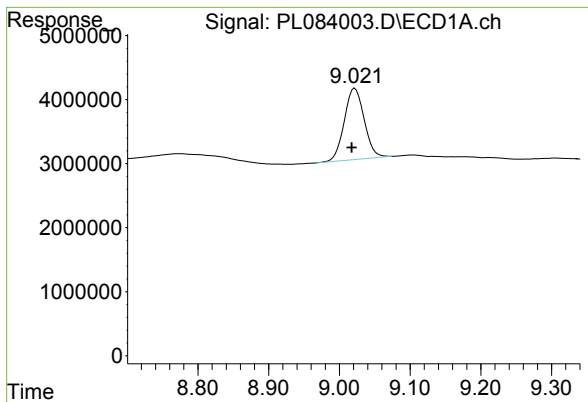

#28 Decachlorobiphenyl


R.T.: 9.022 min

Delta R.T.: 0.005 min

Response: 21788271

Conc: 16.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP5

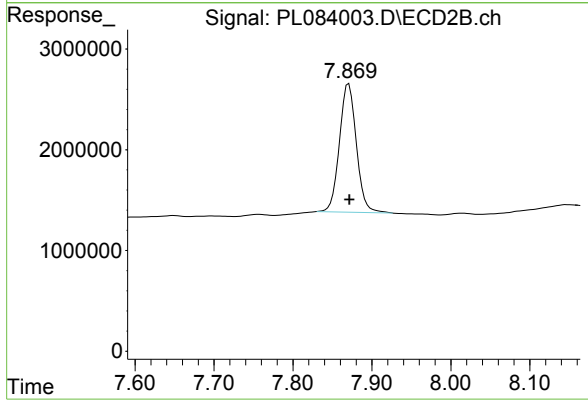

#28 Decachlorobiphenyl

R.T.: 7.871 min

Delta R.T.: 0.000 min

Response: 19009465

Conc: 17.11 ng/ml