

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071825\
 Data File : PL096446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2025 10:08
 Operator : AR\AJ
 Sample : Q2600-02RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 23:22:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.828	73563084	123.4E6	20.160	21.383
28)	SA Decachlor...	9.018	7.992	38602574	68329223	13.723	13.703
Target Compounds							
4)	MA Heptachlor	4.927f	0.000	40847139	0	8.916	N.D. #
7)	B delta-BHC	4.756	0.000	15371586	0	3.430	N.D. #
8)	B Heptachlo...	5.682f	0.000	13298919	0	3.205	N.D. #
9)	A Endosulfan I	6.044	0.000	3649194	0	0.904	N.D. #
11)	B alpha-Chl...	6.013	0.000	9733519	0	2.223	N.D. #
14)	MA Endrin	0.000	5.718	0	6851811	N.D.	1.124 #
15)	B Endosulfa...	6.746	0.000	5465911	0	1.575	N.D. #
18)	B Endrin al...	0.000	6.176	0	3983363	N.D.	0.894 #
26)	Chlordane-4	6.013	0.000	9733519	0	10.848	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071825\
Data File : PL096446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2025 10:08
Operator : AR\AJ
Sample : Q2600-02RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 23:22:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

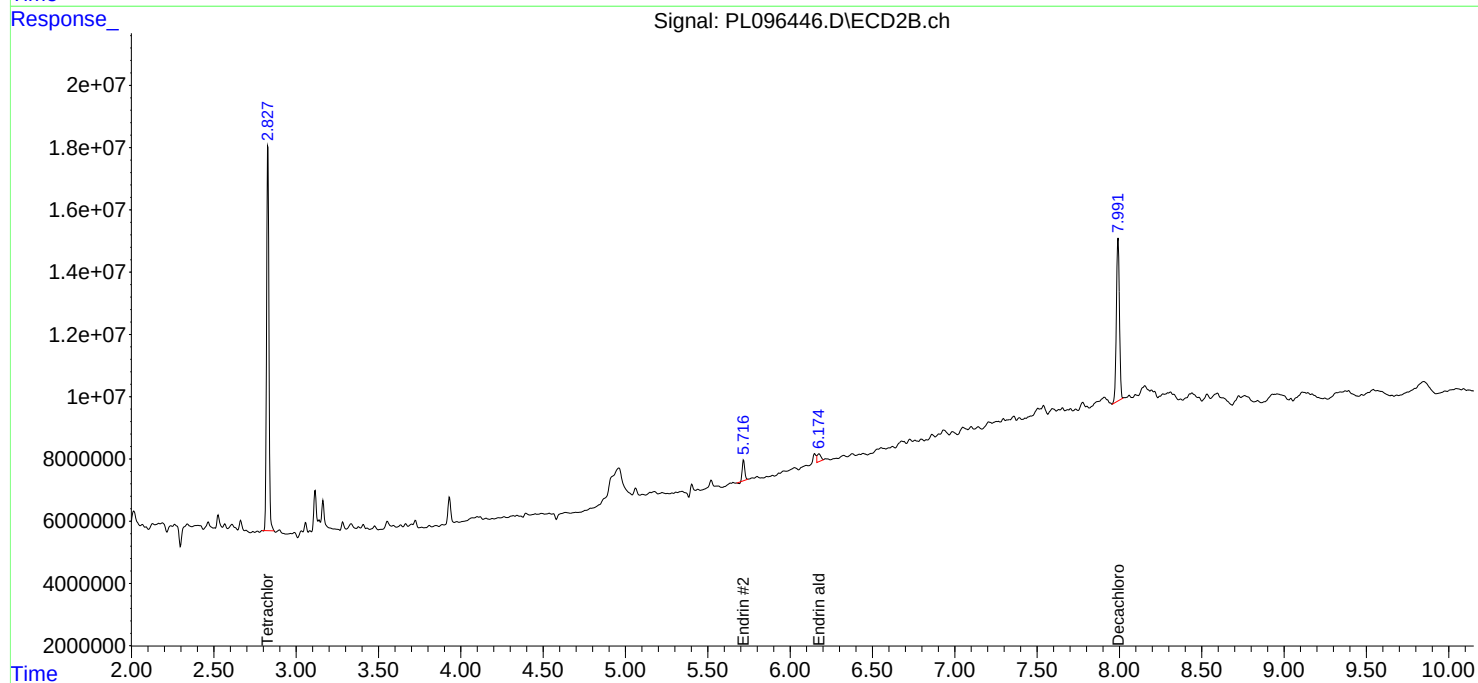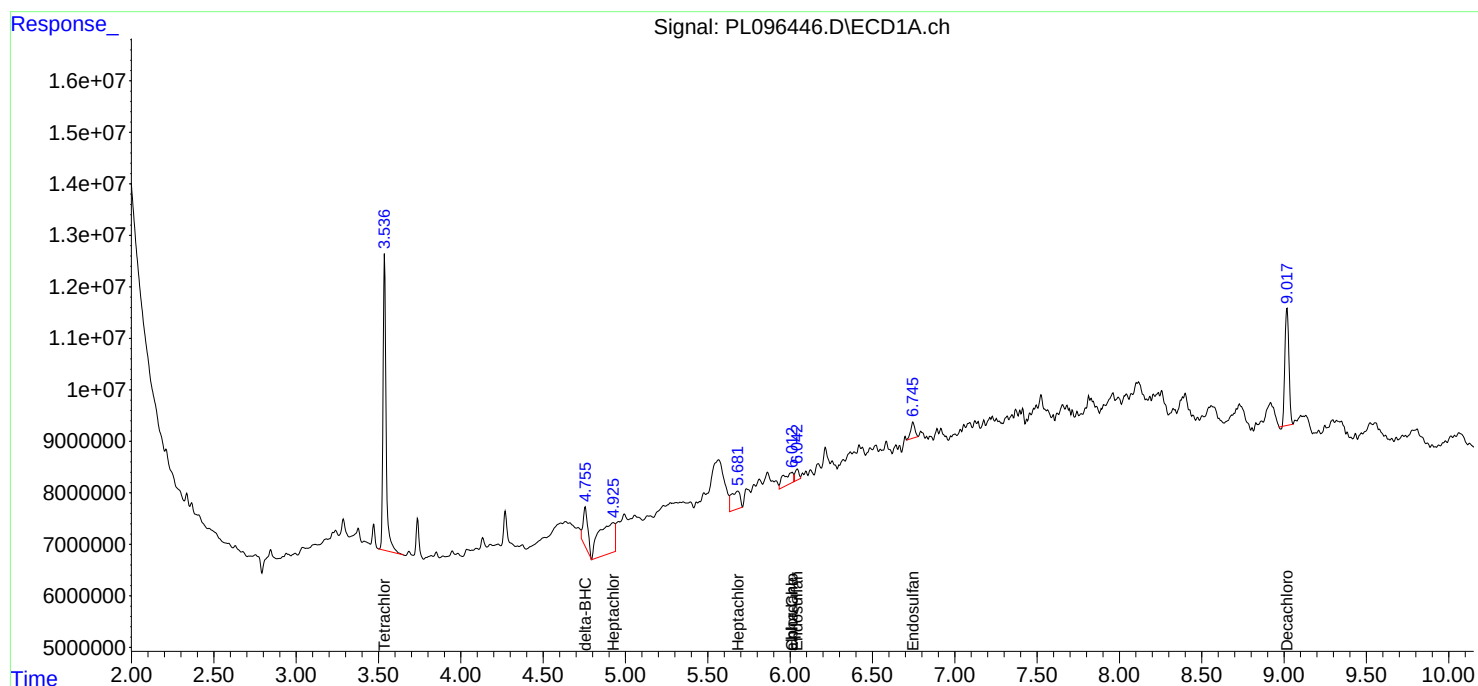


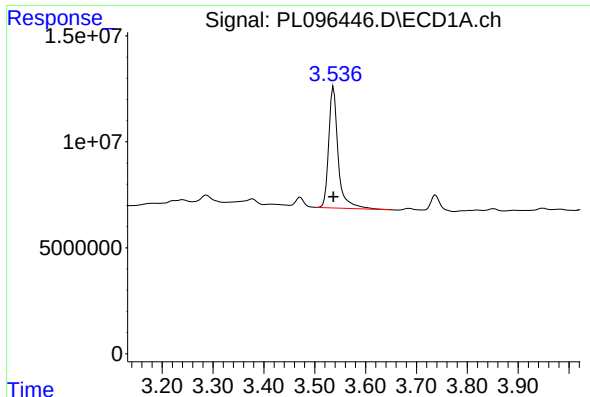

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 73563084
Conc: 20.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

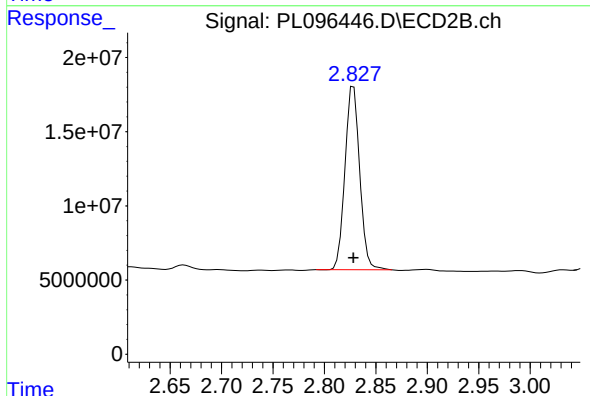


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 123403819
Conc: 21.38 ng/ml

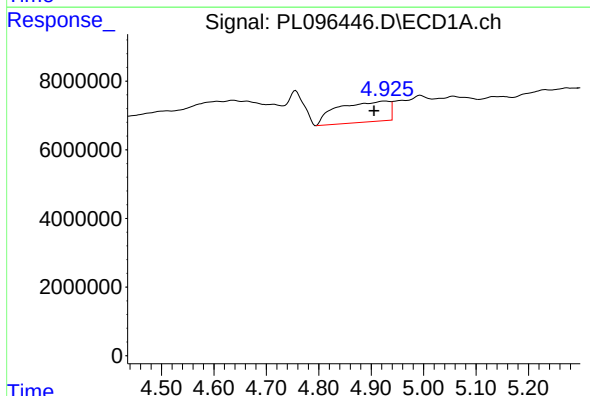


#4 Heptachlor

R.T.: 4.927 min
Delta R.T.: 0.022 min
Response: 40847139
Conc: 8.92 ng/ml

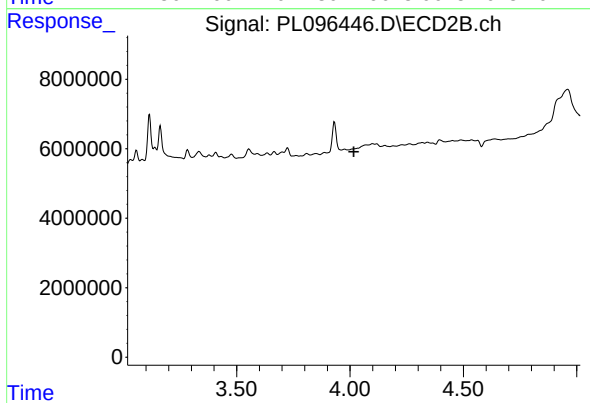

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.016 min
Response: 0
Conc: N.D.

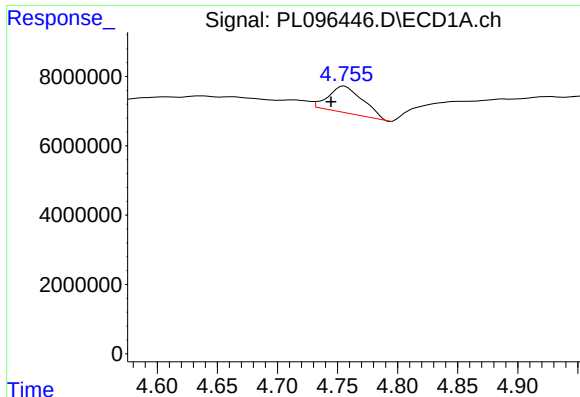

#7 delta-BHC


R.T.: 4.756 min
Delta R.T.: 0.011 min
Response: 15371586
Conc: 3.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

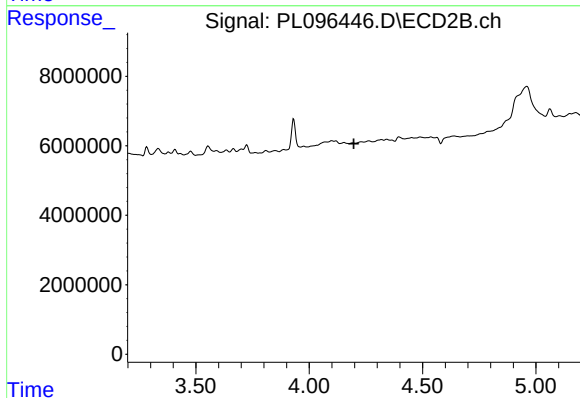


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.196 min
Response: 0
Conc: N.D.

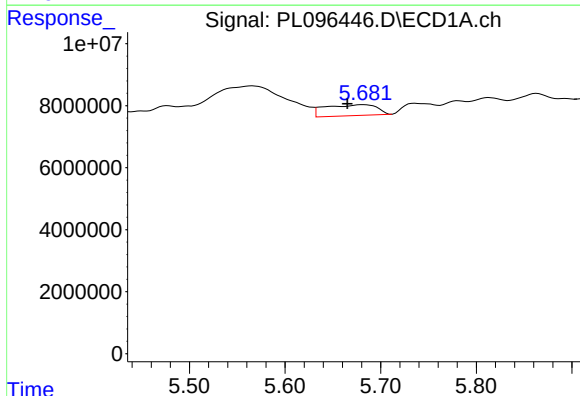


#8 Heptachlor epoxide

R.T.: 5.682 min
Delta R.T.: 0.017 min
Response: 13298919
Conc: 3.21 ng/ml

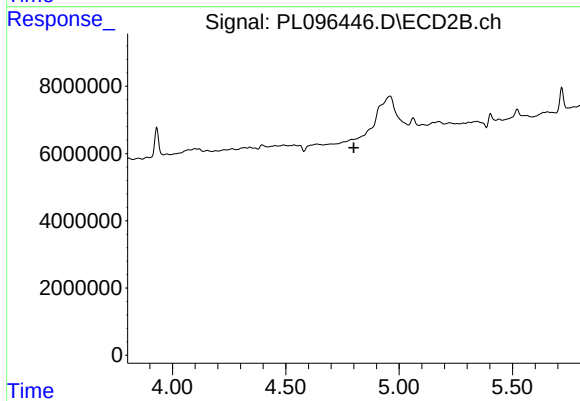

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

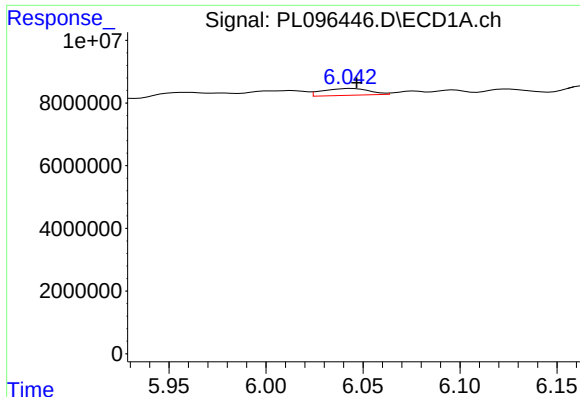

#9 Endosulfan I


R.T.: 6.044 min
Delta R.T.: -0.003 min
Response: 3649194
Conc: 0.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

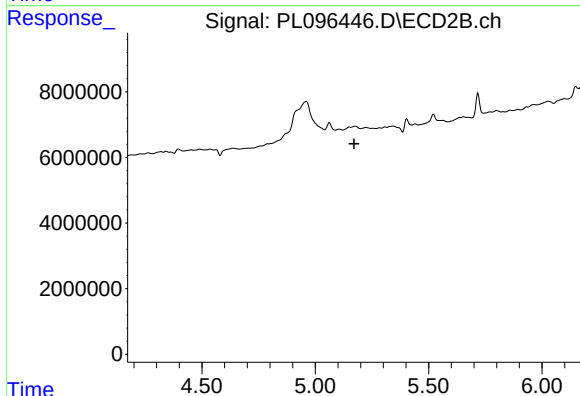


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.172 min
Response: 0
Conc: N.D.

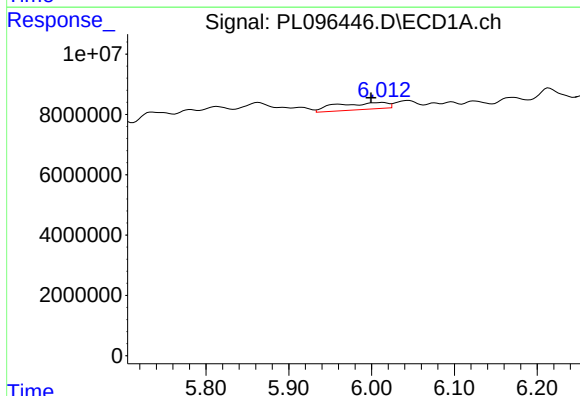


#11 alpha-Chlordane

R.T.: 6.013 min
Delta R.T.: 0.013 min
Response: 9733519
Conc: 2.22 ng/ml

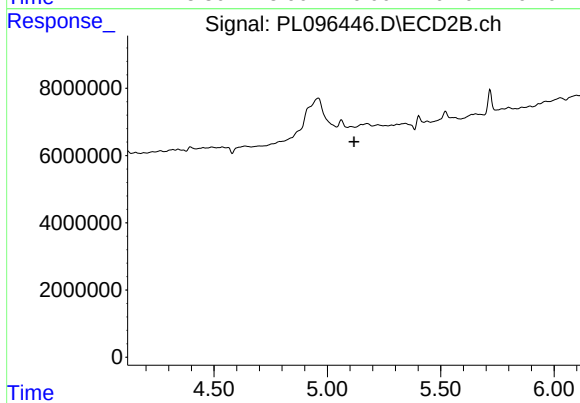

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

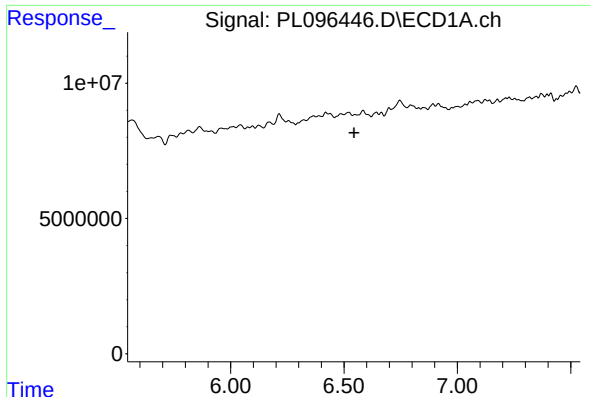

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

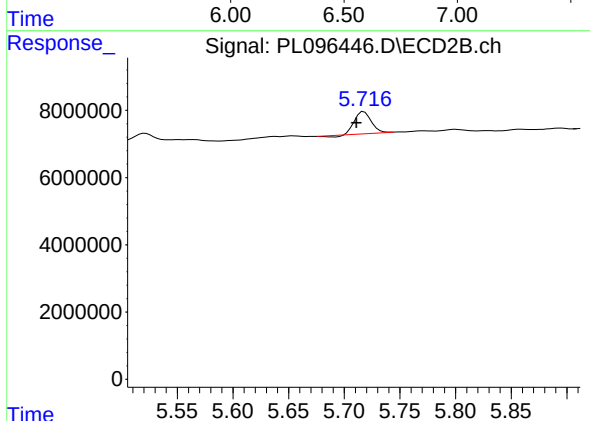


#14 Endrin

R.T.: 5.718 min
Delta R.T.: 0.007 min
Response: 6851811
Conc: 1.12 ng/ml

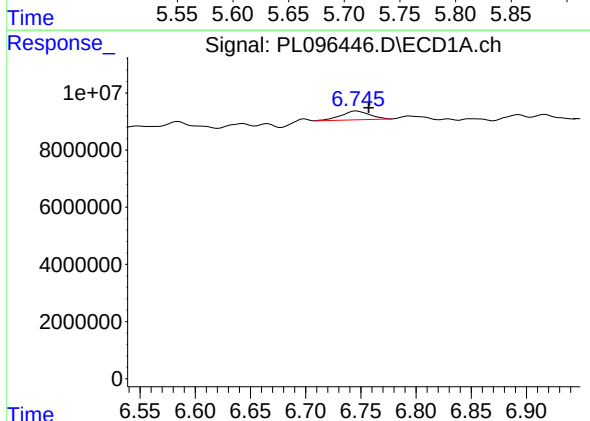


#15 Endosulfan II

R.T.: 6.746 min
Delta R.T.: -0.010 min
Response: 5465911
Conc: 1.58 ng/ml

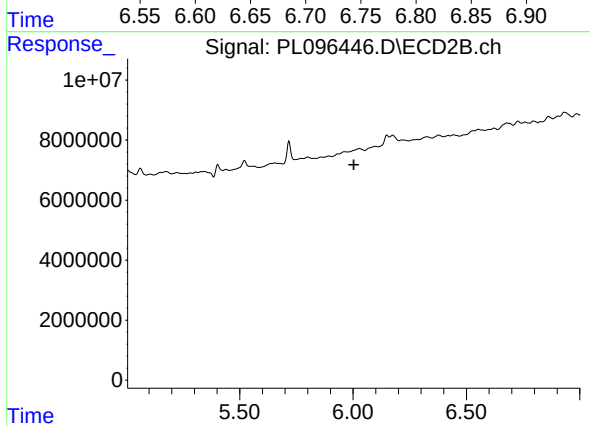

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.003 min
Response: 0
Conc: N.D.

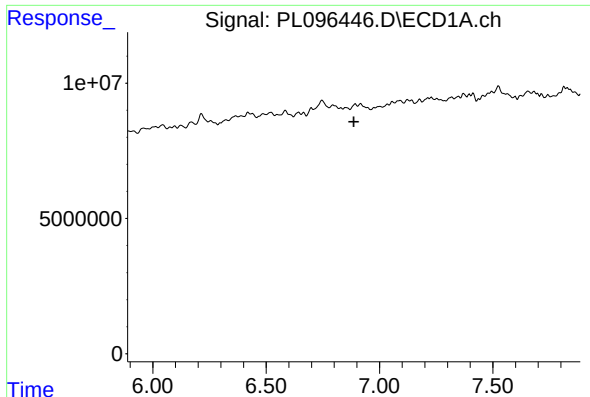

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.886 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

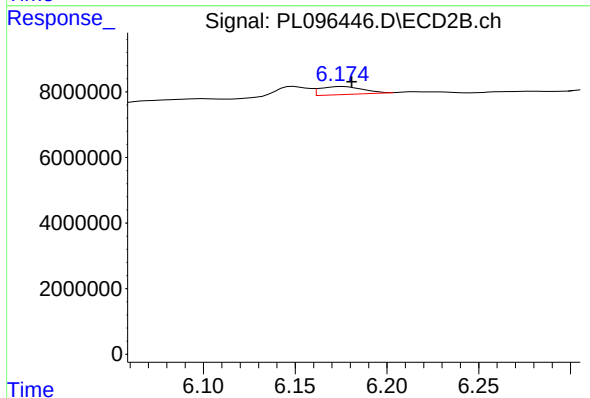


#18 Endrin aldehyde

R.T.: 6.176 min
Delta R.T.: -0.005 min
Response: 3983363
Conc: 0.89 ng/ml

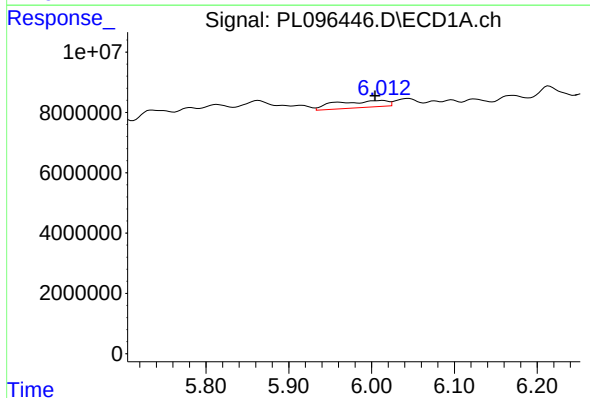


#26 Chlordane-4

R.T.: 6.013 min
Delta R.T.: 0.009 min
Response: 9733519
Conc: 10.85 ng/ml

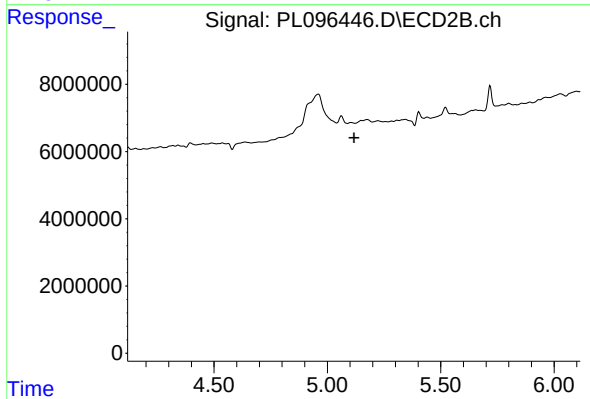

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.118 min
Response: 0
Conc: N.D.

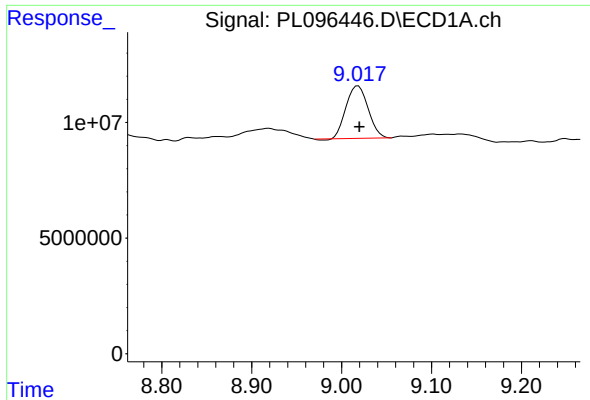

#28 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: -0.002 min
Response: 38602574
Conc: 13.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

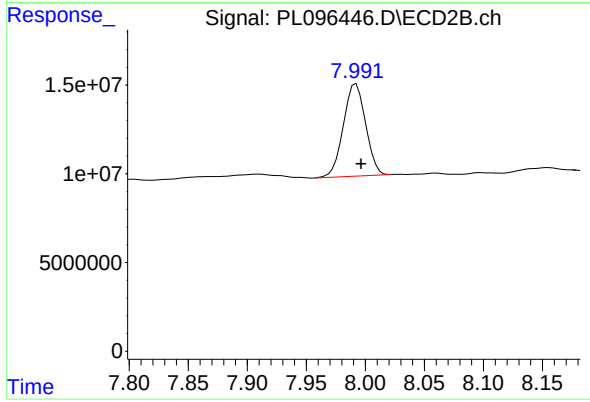

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.004 min
Response: 68329223
Conc: 13.70 ng/ml