

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071825\
 Data File : PL096449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2025 10:49
 Operator : AR\AJ
 Sample : Q2622-01 10X RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2819RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 23:23:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.828	0	12065539	N.D.	2.091 #
28)	SA Decachlor...	0.000	7.992	0	9381660	N.D.	1.881 #
Target Compounds							
8)	B Heptachlo...	5.654	0.000	20242942	0	4.879	N.D. #
9)	A Endosulfan I	0.000	5.189f	0	14596241	N.D.	2.035 #
13)	MA Dieldrin	0.000	5.434	0	5405016	N.D.	0.793 #
14)	MA Endrin	0.000	5.718	0	13060386	N.D.	2.142 #
15)	B Endosulfa...	6.750	0.000	15651975	0	4.511	N.D. #
16)	A 4,4'-DDD	6.660f	0.000	13195148	0	4.532	N.D. #
18)	B Endrin al...	0.000	6.177	0	7095579	N.D.	1.593 #
20)	A Methoxychlor	0.000	6.706f	0	4973176	N.D.	1.637 #
27)	Chlordane-5	0.000	6.044f	0	5375407	N.D.	18.964 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071825\
Data File : PL096449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2025 10:49
Operator : AR\AJ
Sample : Q2622-01 10X RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
2819RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 23:23:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

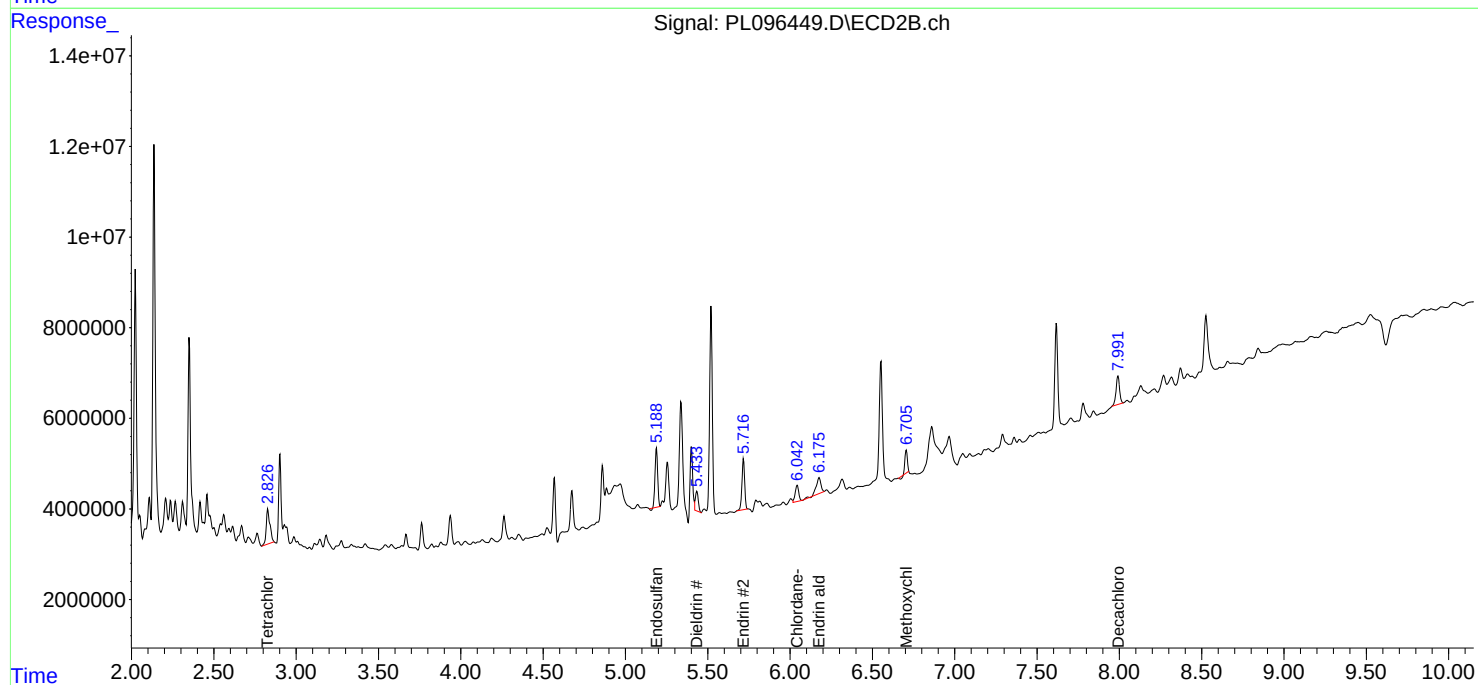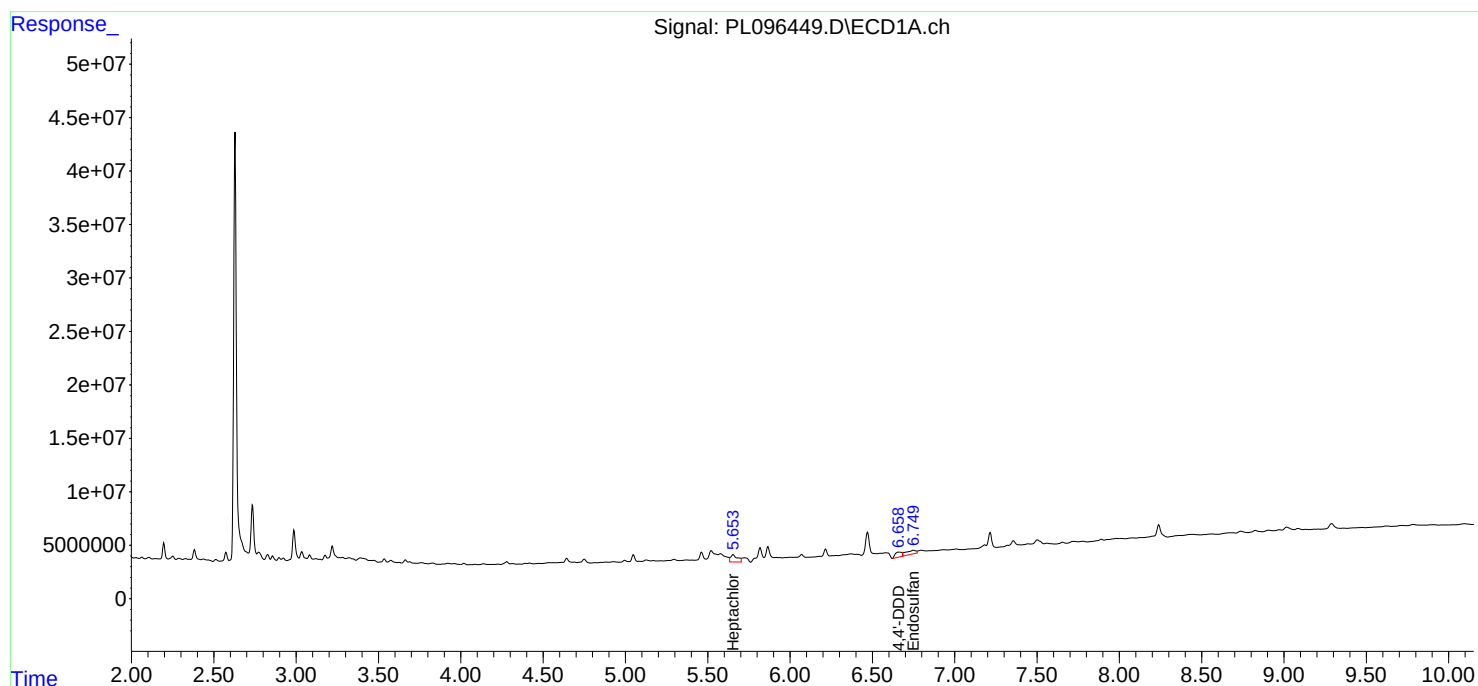


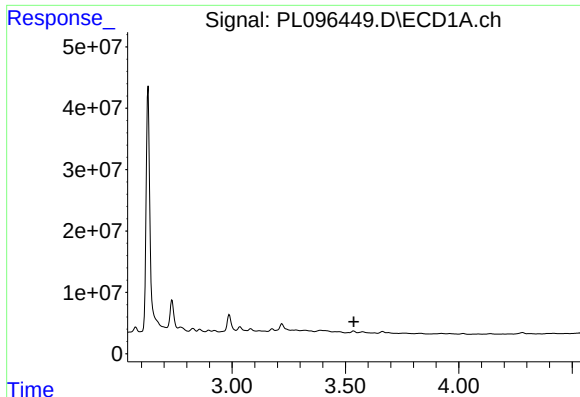

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2819RE

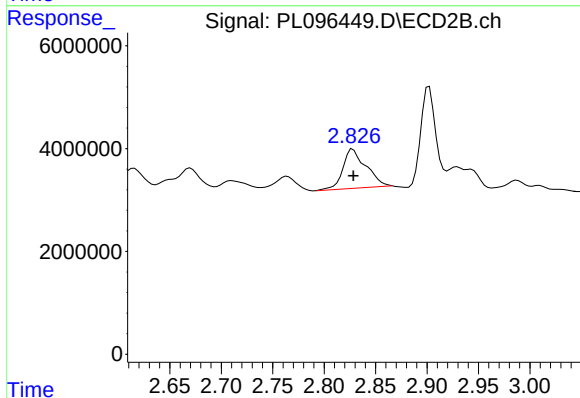


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 12065539
Conc: 2.09 ng/ml

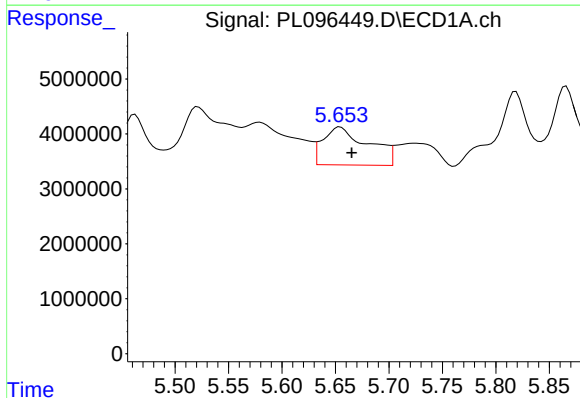


#8 Heptachlor epoxide

R.T.: 5.654 min
Delta R.T.: -0.011 min
Response: 20242942
Conc: 4.88 ng/ml

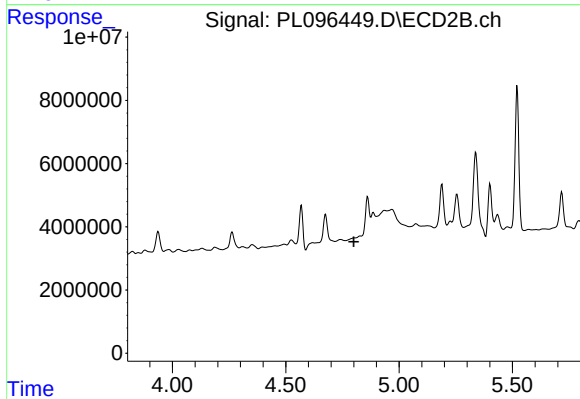

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

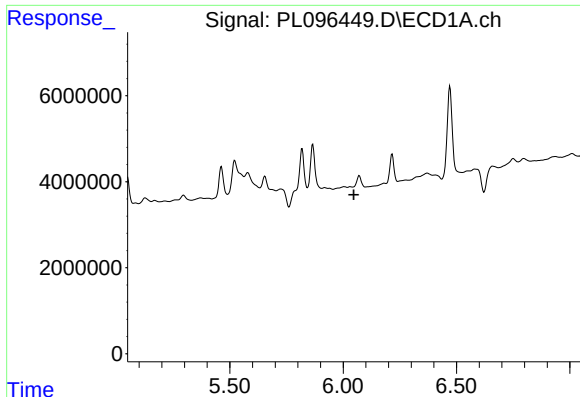

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2819RE

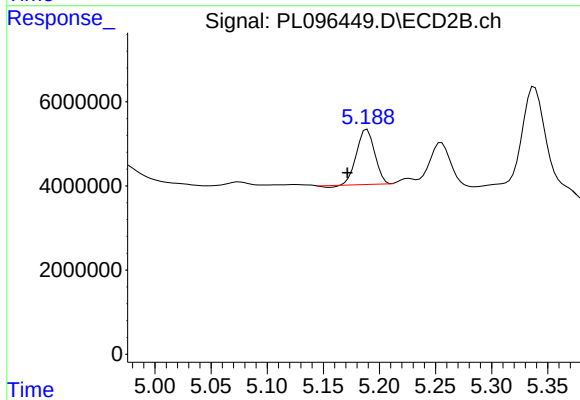


#9 Endosulfan I

R.T.: 5.189 min
Delta R.T.: 0.017 min
Response: 14596241
Conc: 2.03 ng/ml

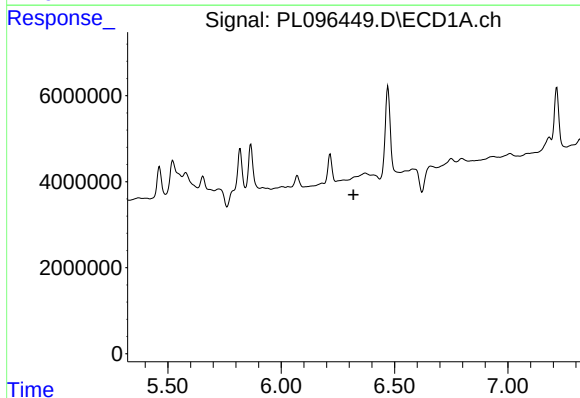


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.319 min
Response: 0
Conc: N.D.

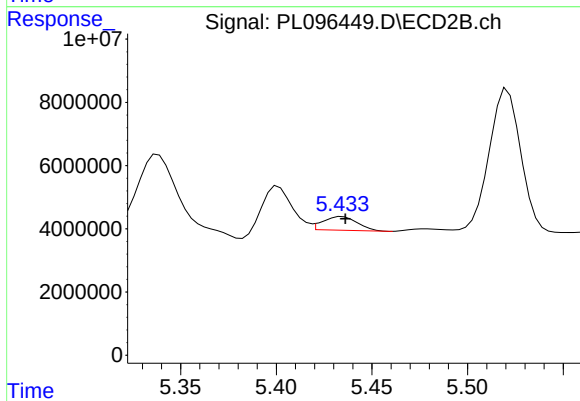

#13 Dieldrin


R.T.: 5.434 min
Delta R.T.: -0.002 min
Response: 5405016
Conc: 0.79 ng/ml

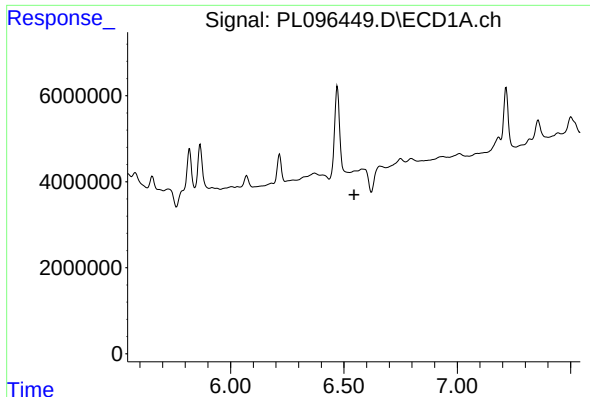

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2819RE

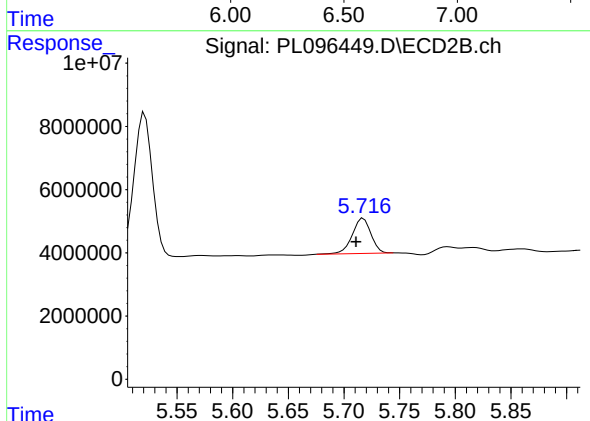


#14 Endrin

R.T.: 5.718 min
Delta R.T.: 0.007 min
Response: 13060386
Conc: 2.14 ng/ml

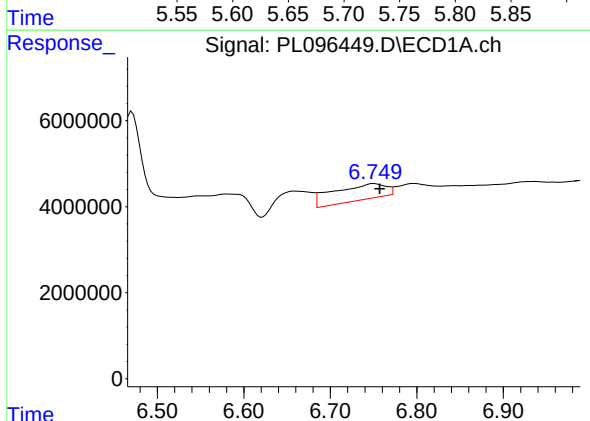


#15 Endosulfan II

R.T.: 6.750 min
Delta R.T.: -0.006 min
Response: 15651975
Conc: 4.51 ng/ml

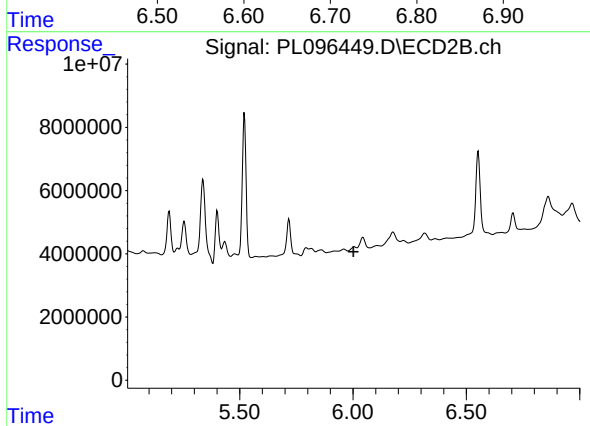

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.003 min
Response: 0
Conc: N.D.

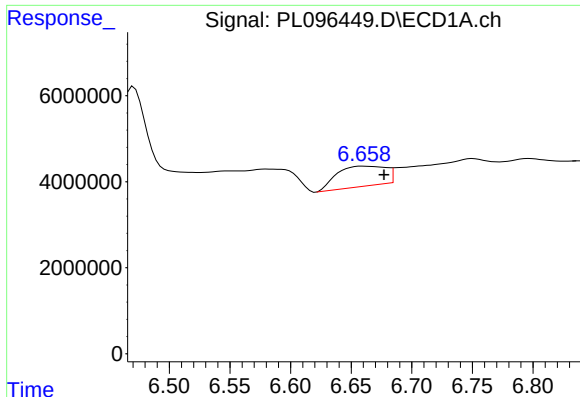

#16 4,4'-DDD


R.T.: 6.660 min
Delta R.T.: -0.017 min
Response: 13195148
Conc: 4.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
2819RE

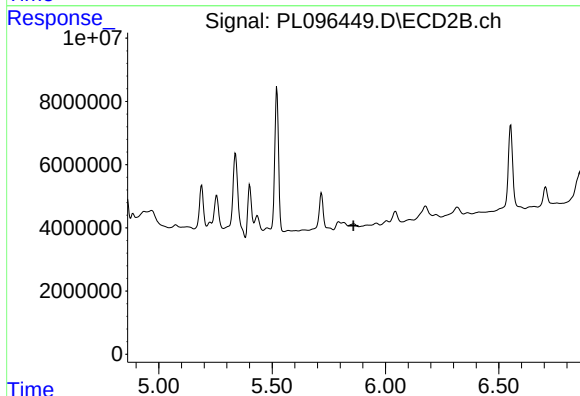


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.859 min
Response: 0
Conc: N.D.

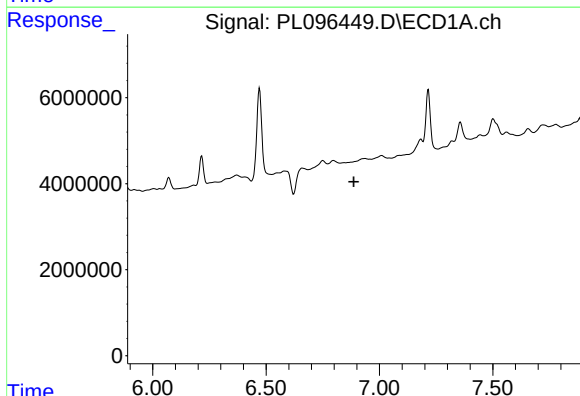


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

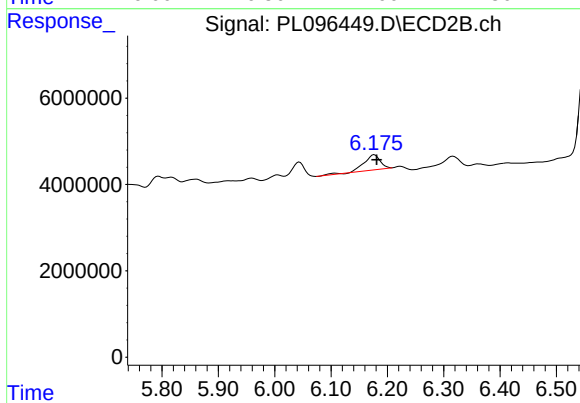

#18 Endrin aldehyde


R.T.: 6.177 min
Delta R.T.: -0.004 min
Response: 7095579
Conc: 1.59 ng/ml

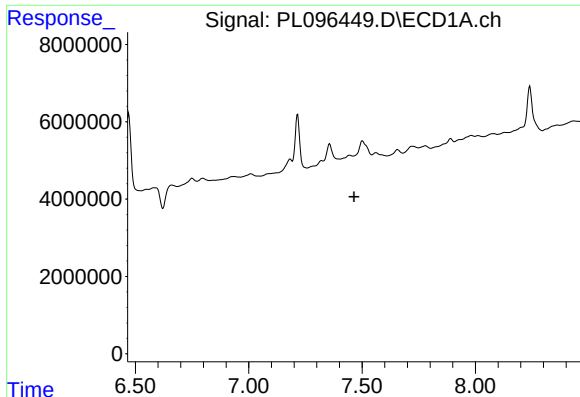

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2819RE

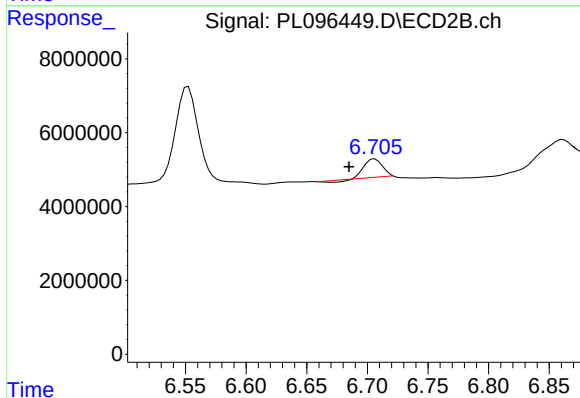


#20 Methoxychlor

R.T.: 6.706 min
Delta R.T.: 0.021 min
Response: 4973176
Conc: 1.64 ng/ml

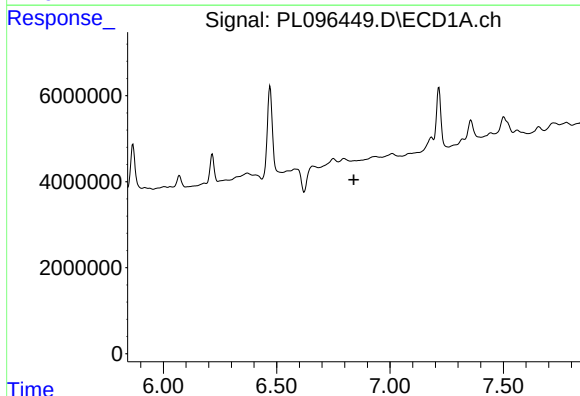


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.841 min
Response: 0
Conc: N.D.

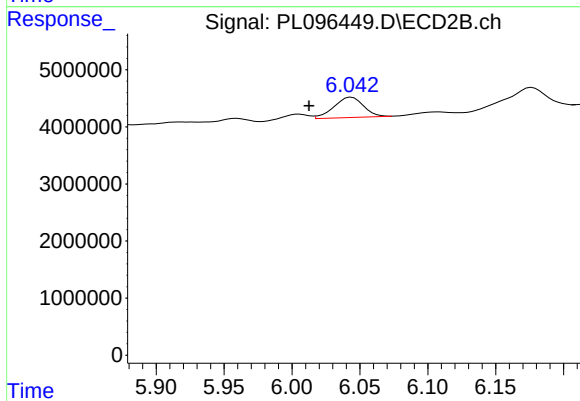

#27 Chlordane-5


R.T.: 6.044 min
Delta R.T.: 0.031 min
Response: 5375407
Conc: 18.96 ng/ml

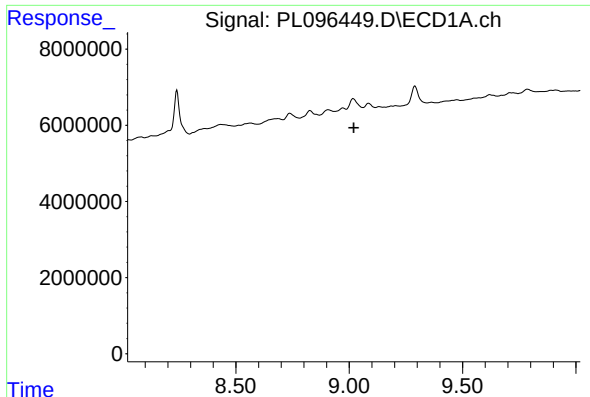

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.020 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2819RE

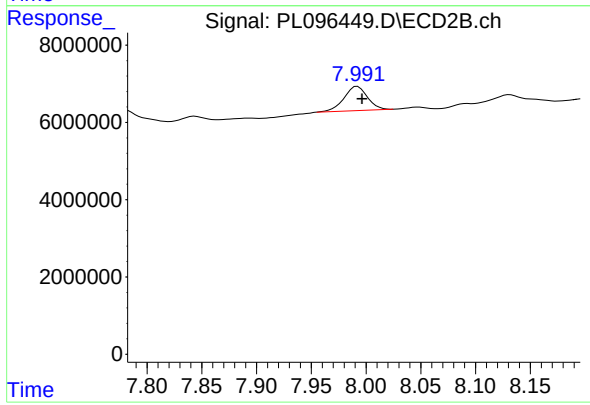

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.004 min
Response: 9381660
Conc: 1.88 ng/ml