

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071825\
 Data File : PL096464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2025 14:40
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 23:25:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.825	76334212	132.2E6	20.919	22.907
28)	SA Decachlor...	9.023	7.994	59436309	105.1E6	21.129	21.073
Target Compounds							
15)	B Endosulfa...	0.000	6.023f	0 13425098	N.D.	2.289	#
27)	Chlordane-5	0.000	6.023	0 13425098	N.D.	47.363	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071825\
Data File : PL096464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2025 14:40
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 23:25:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

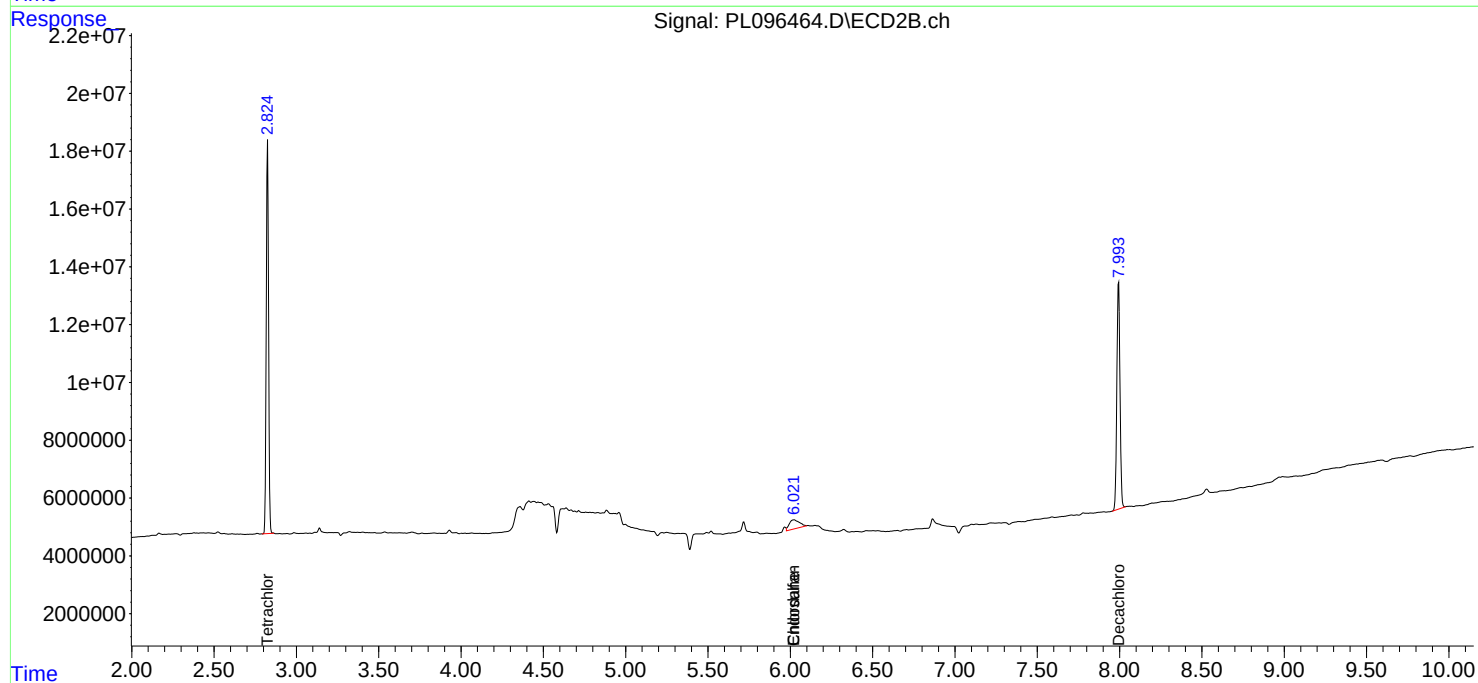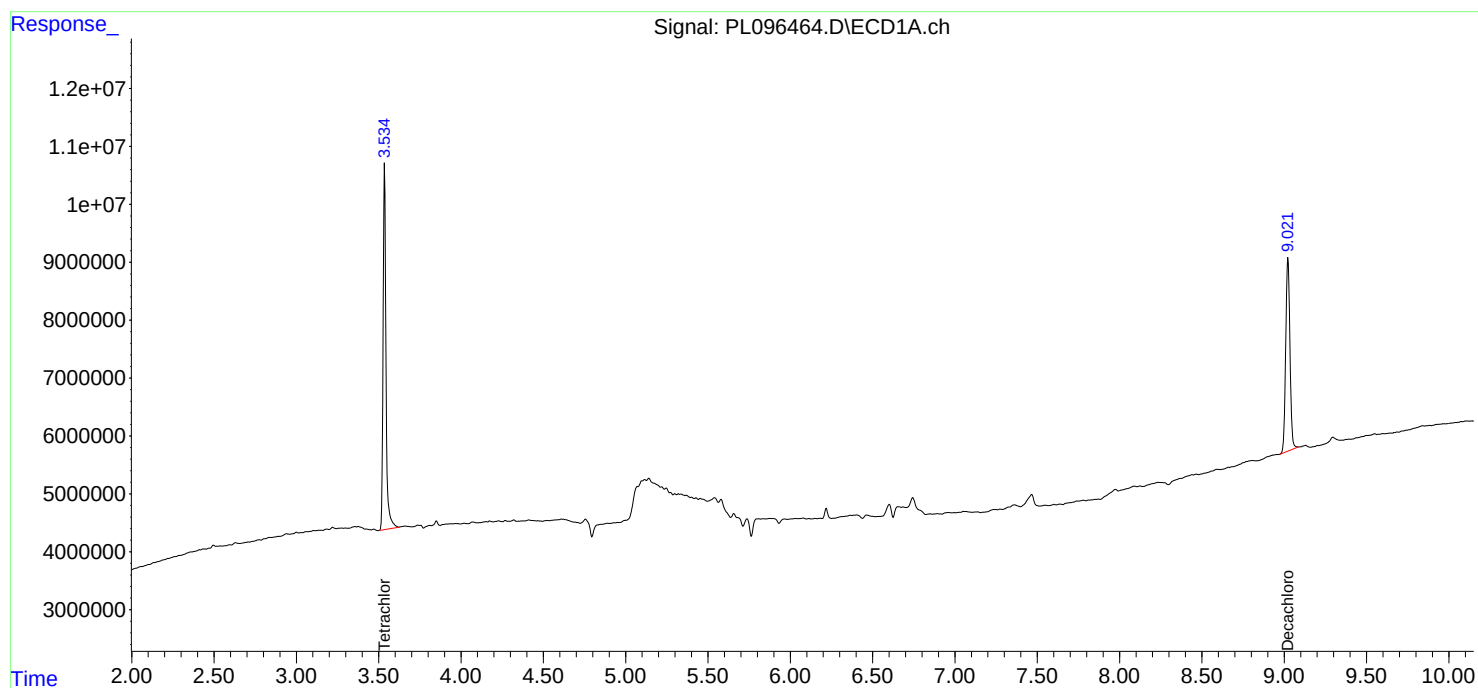


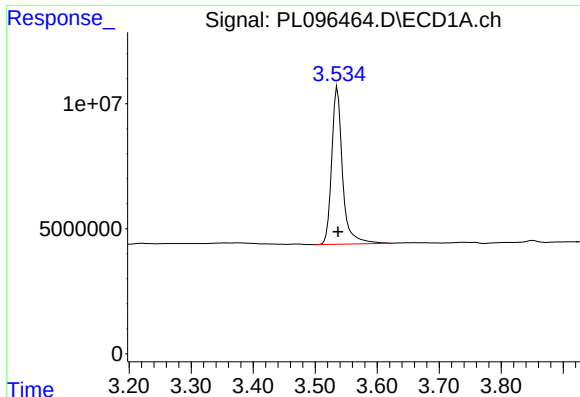

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: -0.001 min
Response: 76334212
Conc: 20.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

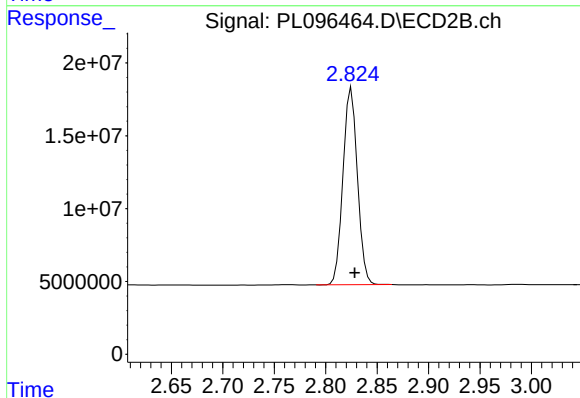


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: -0.003 min
Response: 132204013
Conc: 22.91 ng/ml

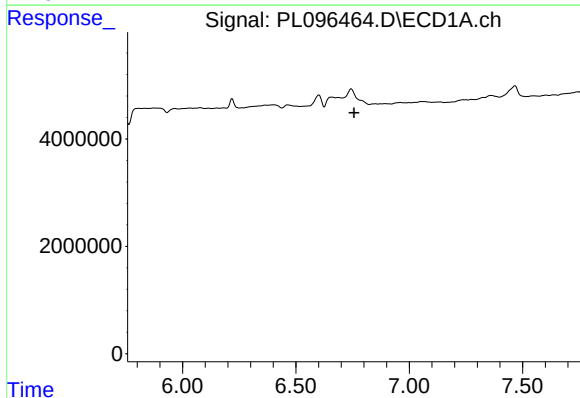


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.757 min
Response: 0
Conc: N.D.

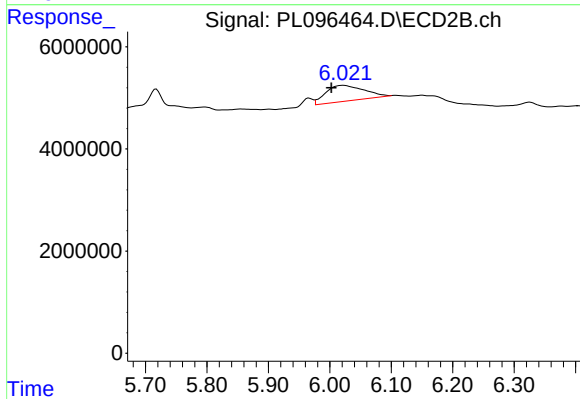

#15 Endosulfan II


R.T.: 6.023 min
Delta R.T.: 0.020 min
Response: 13425098
Conc: 2.29 ng/ml

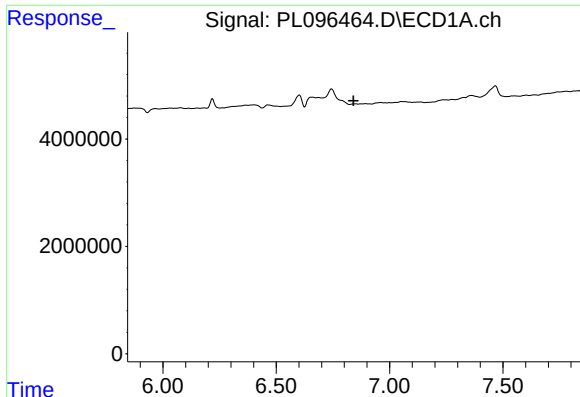

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.841 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

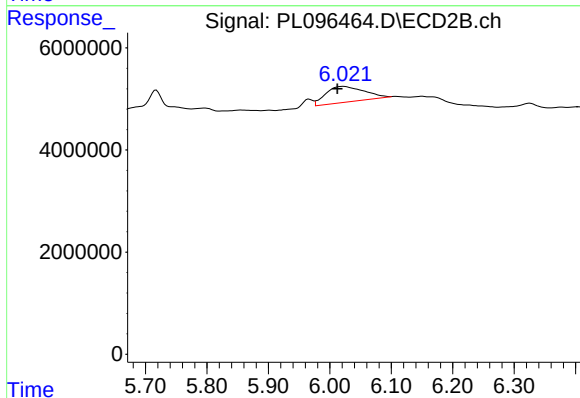


#27 Chlordane-5

R.T.: 6.023 min
Delta R.T.: 0.010 min
Response: 13425098
Conc: 47.36 ng/ml

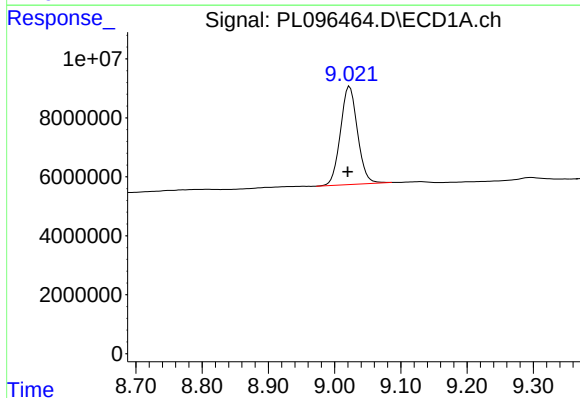

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.003 min
Response: 59436309
Conc: 21.13 ng/ml

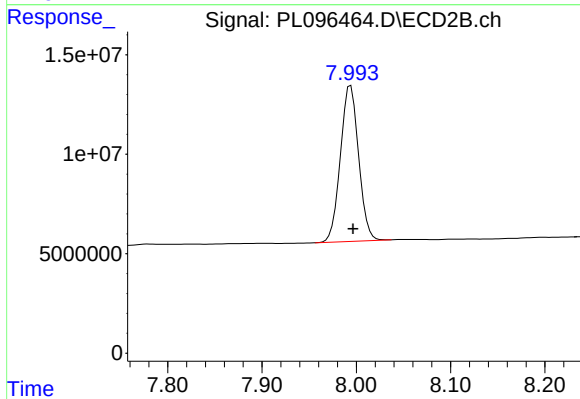

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: -0.002 min
Response: 105081095
Conc: 21.07 ng/ml