

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071919\
 Data File : PL050663.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2019 23:50
 Operator : SM\AJ
 Sample : K3903-07
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 180107-NYCT-AVE-Z-COMP-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 02:09:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.930	193.3E6	58803050	19.241	20.609
28)	SA Decachlor...	7.979	8.960	214.8E6	58994525	21.218	20.862
Target Compounds							
8)	B Heptachlo...	0.000	5.808f	0	4226279	N.D.	1.105 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071919\
Data File : PL050663.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2019 23:50
Operator : SM\AJ
Sample : K3903-07
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
180107-NYCT-AVE-Z-COMP-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 02:09:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

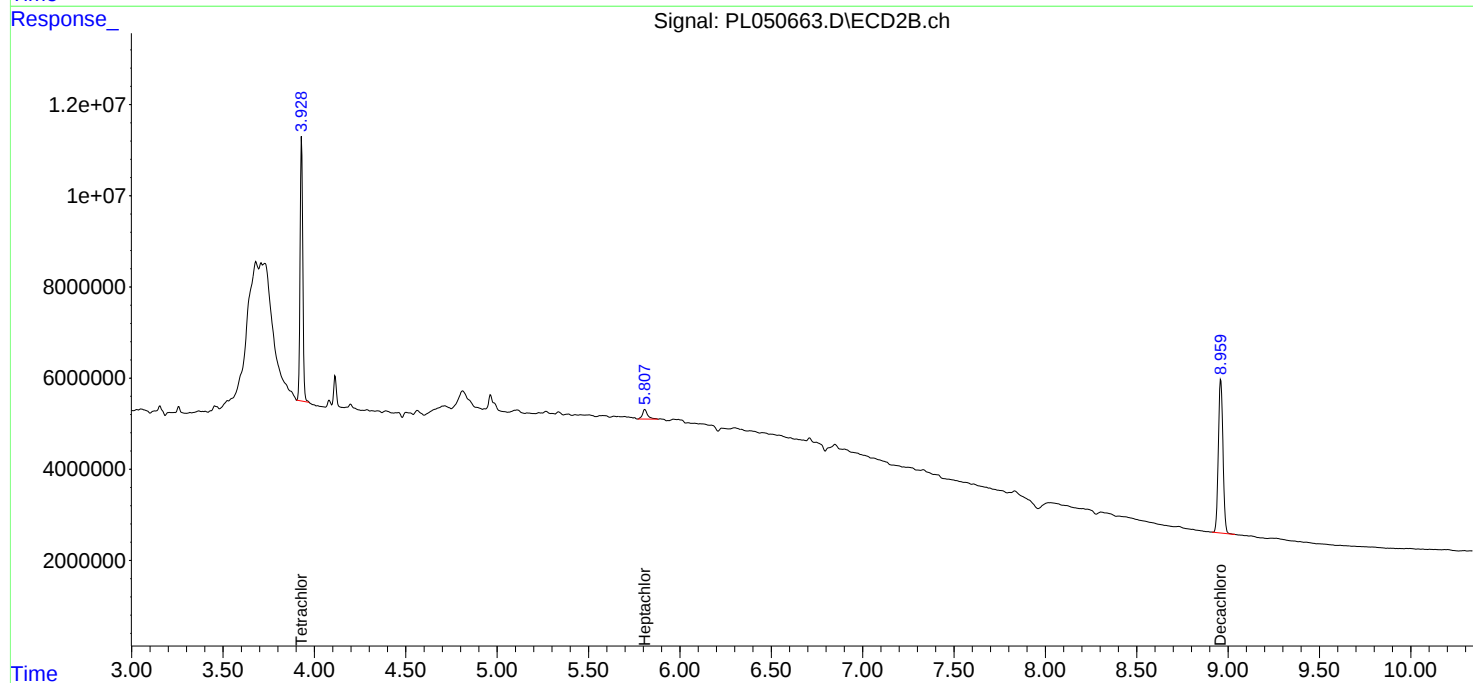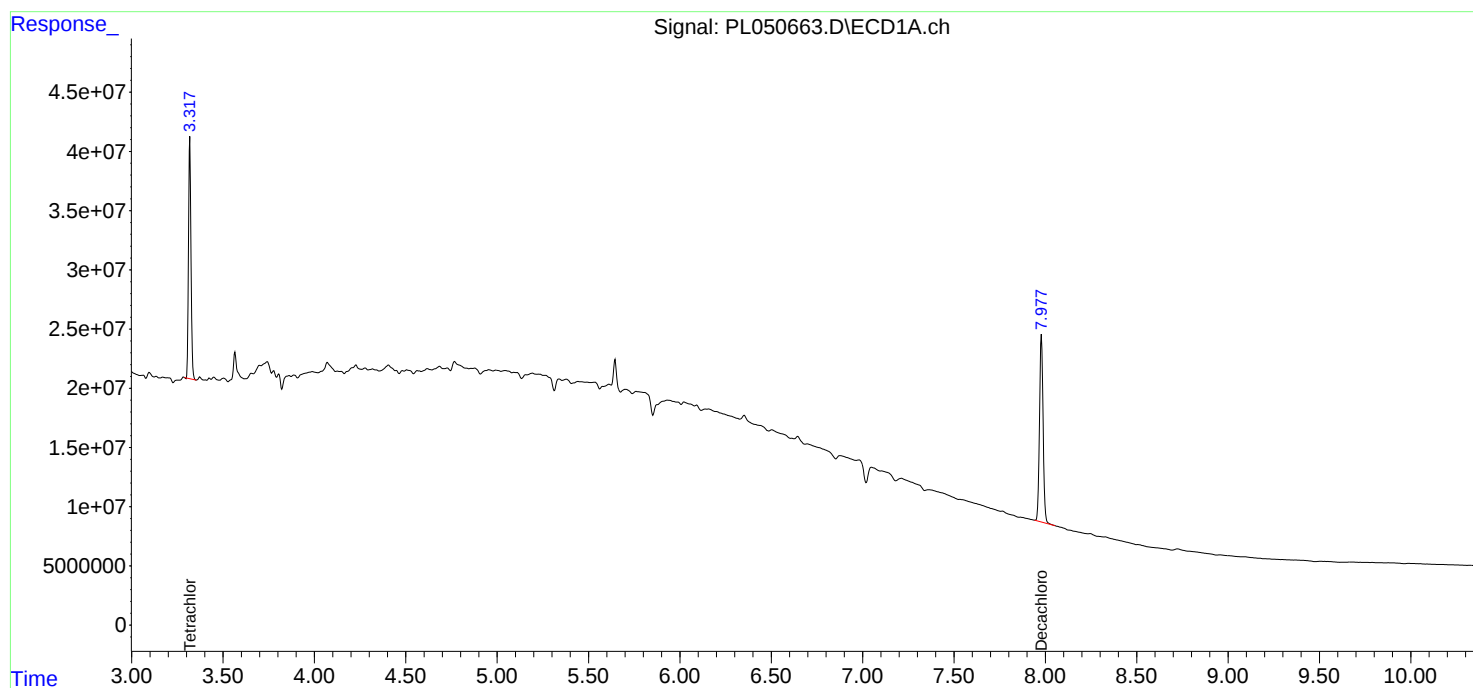


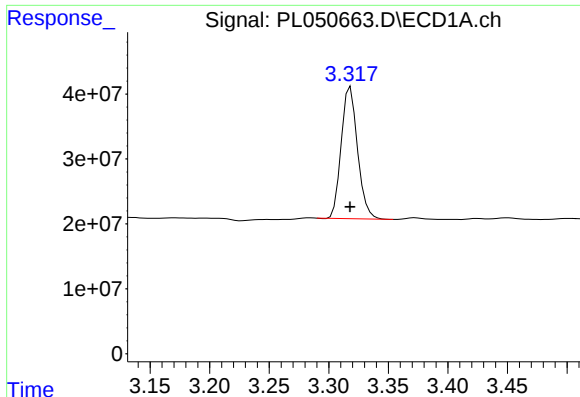

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 193330646
Conc: 19.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
180107-NYCT-AVE-Z-COMP-1-2

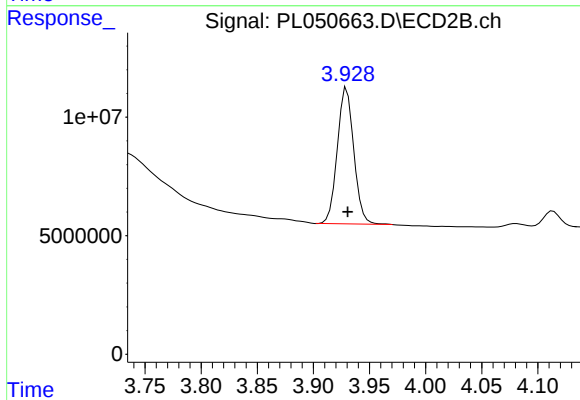


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 58803050
Conc: 20.61 ng/ml

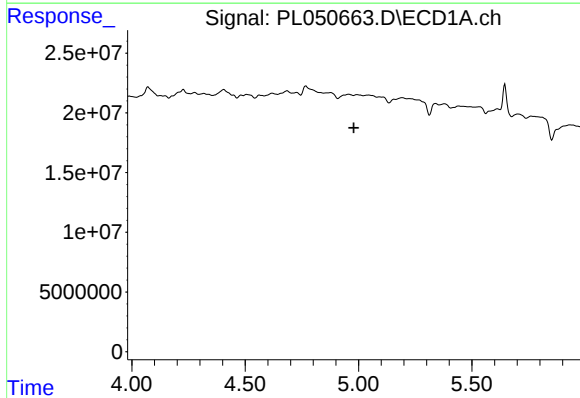


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

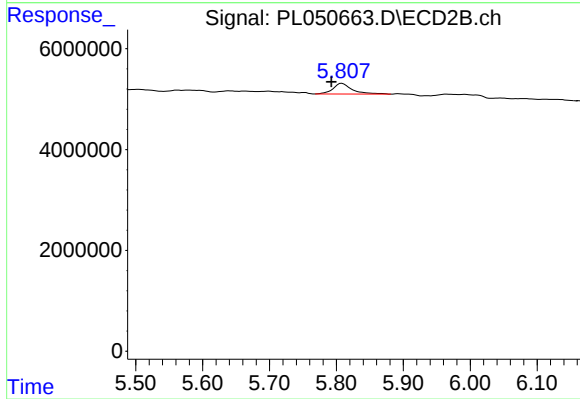

#8 Heptachlor epoxide

R.T.: 5.808 min
Delta R.T.: 0.016 min
Response: 4226279
Conc: 1.10 ng/ml

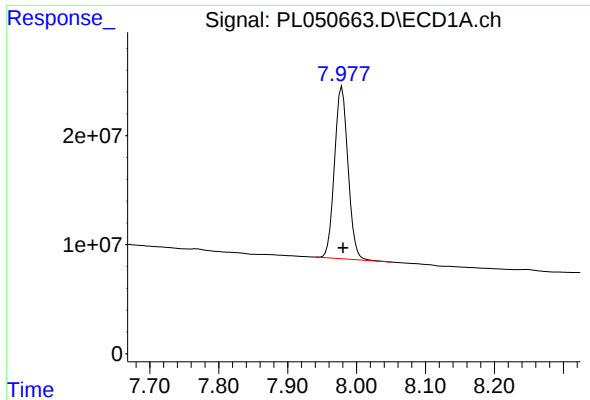

#28 Decachlorobiphenyl


R.T.: 7.979 min

Delta R.T.: -0.002 min

Response: 214841294

Conc: 21.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
180107-NYCT-AVE-Z-COMP-1-2

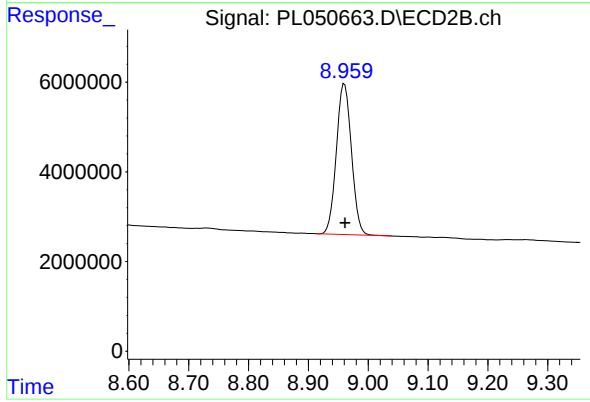

#28 Decachlorobiphenyl

R.T.: 8.960 min

Delta R.T.: -0.001 min

Response: 58994525

Conc: 20.86 ng/ml