

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
 Data File : PL068212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2021 18:49
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PEM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 03:57:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 03:26:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.646	5.571	8221940	19725024	19.157	19.330
28)	SA Decachlor...	10.425	11.493	11567132	18270640	20.567	20.483
Target Compounds							
2)	A alpha-BHC	5.353	6.151	5518100	12195493	9.426	8.970
3)	MA gamma-BHC...	5.776	6.547	5363603	11843374	9.436	9.179
6)	B beta-BHC	6.155	6.799	3198336	8188287	10.930	11.591
8)	B Heptachlo...	0.000	8.040	0	379912	N.D.	0.336 #
14)	MA Endrin	8.073	8.968	25448392	45622740	50.887	51.023
17)	MA 4,4'-DDT	8.501	9.428	51176274	93680097	102.028	99.254
20)	A Methoxychlor	9.096	9.912	71713350	121.6E6	229.257	239.425
21)	B Endrin ke...	0.000	10.072	0	444743	N.D.	0.446 #
23)	Chlordane-1	0.000	6.979f	0	534723	N.D.	13.896 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
Data File : PL068212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2021 18:49
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PEM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 03:57:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 03:26:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

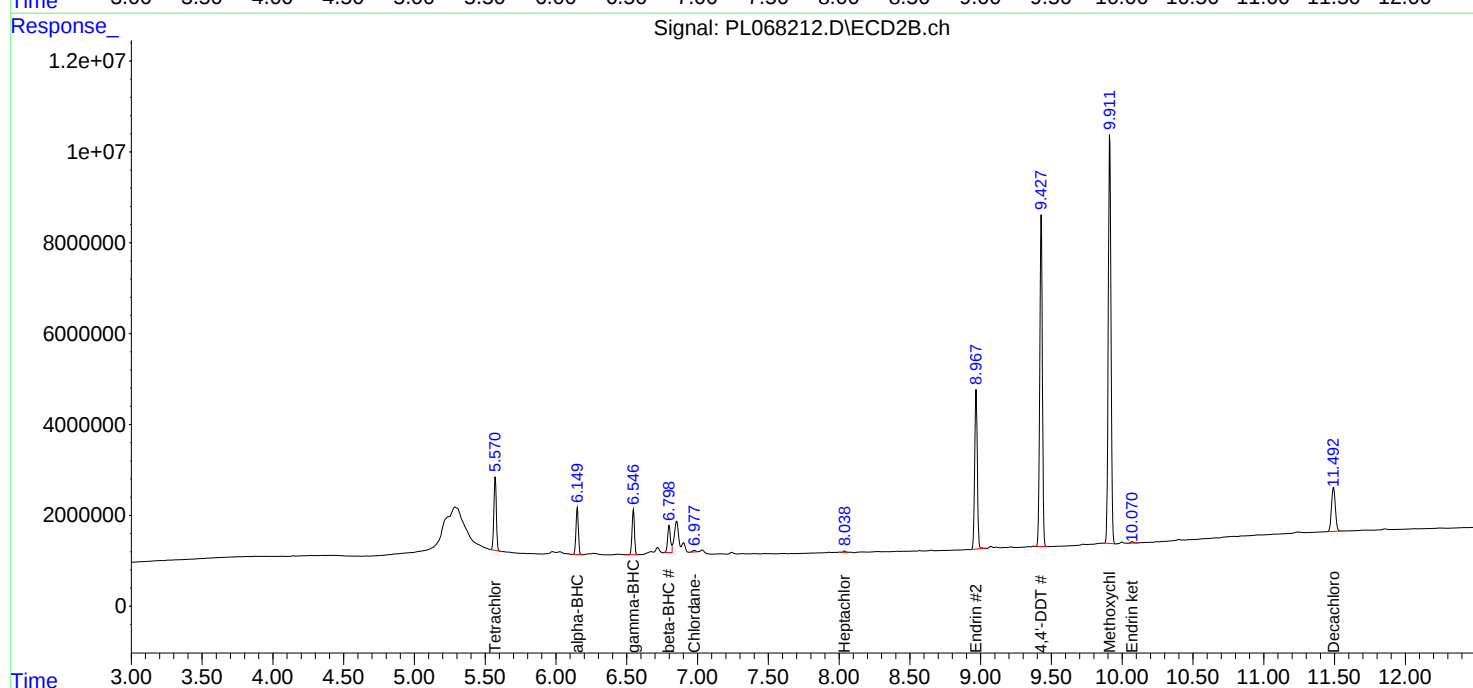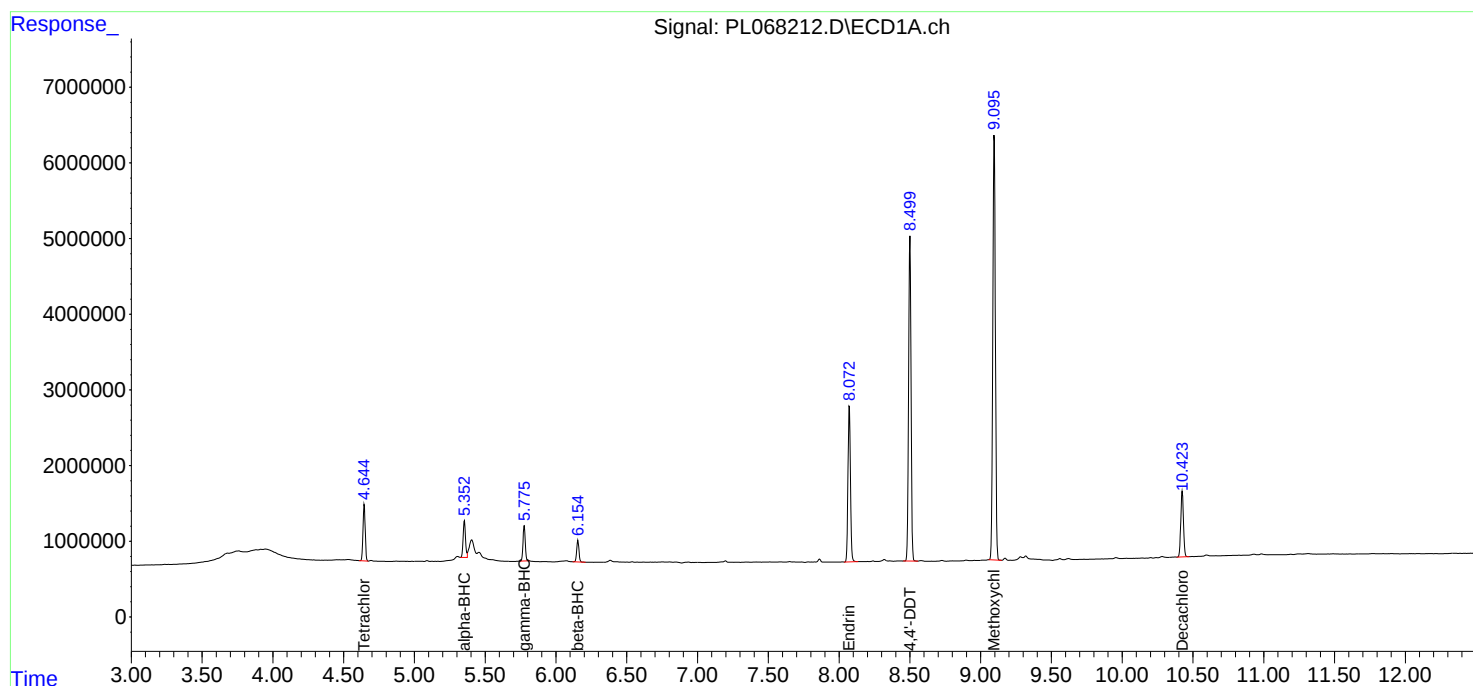


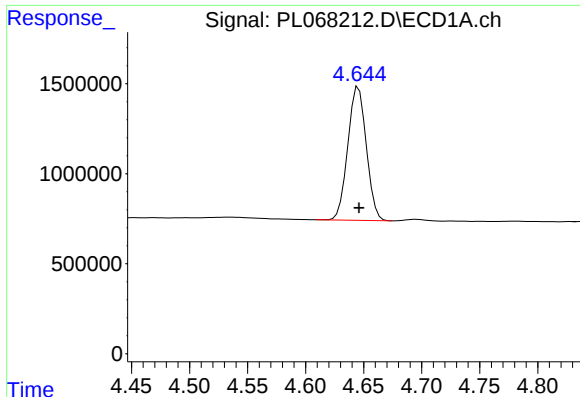

#1 Tetrachloro-m-xylene


R.T.: 4.646 min
Delta R.T.: 0.000 min
Response: 8221940
Conc: 19.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

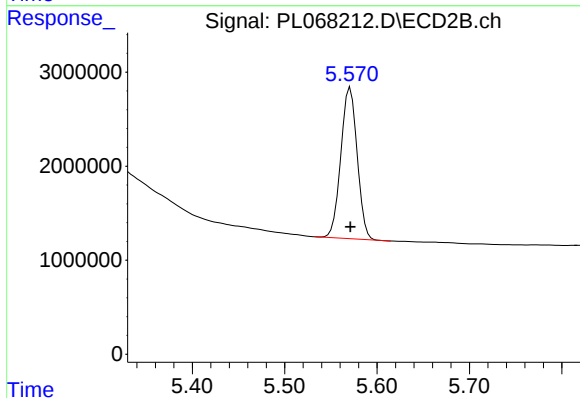


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 19725024
Conc: 19.33 ng/ml

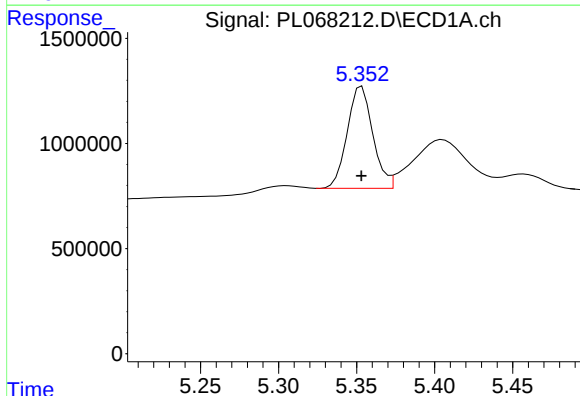


#2 alpha-BHC

R.T.: 5.353 min
Delta R.T.: 0.000 min
Response: 5518100
Conc: 9.43 ng/ml

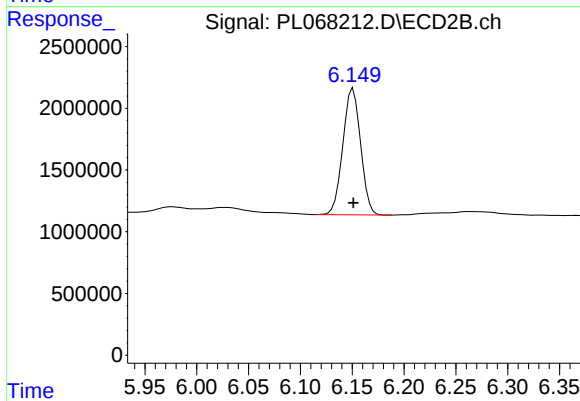

#2 alpha-BHC


R.T.: 6.151 min
Delta R.T.: 0.000 min
Response: 12195493
Conc: 8.97 ng/ml

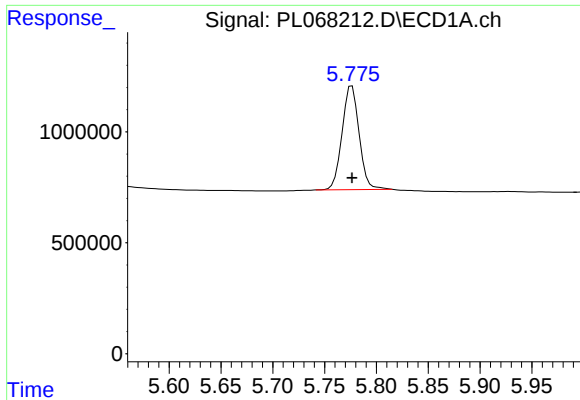

#3 gamma-BHC (Lindane)


R.T.: 5.776 min
Delta R.T.: 0.000 min
Response: 5363603
Conc: 9.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

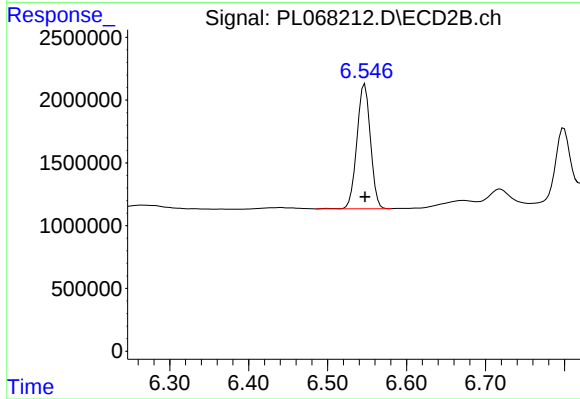


#3 gamma-BHC (Lindane)

R.T.: 6.547 min
Delta R.T.: 0.000 min
Response: 11843374
Conc: 9.18 ng/ml

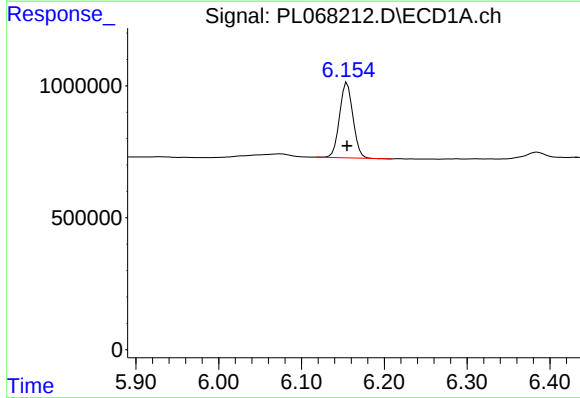


#6 beta-BHC

R.T.: 6.155 min
Delta R.T.: 0.000 min
Response: 3198336
Conc: 10.93 ng/ml

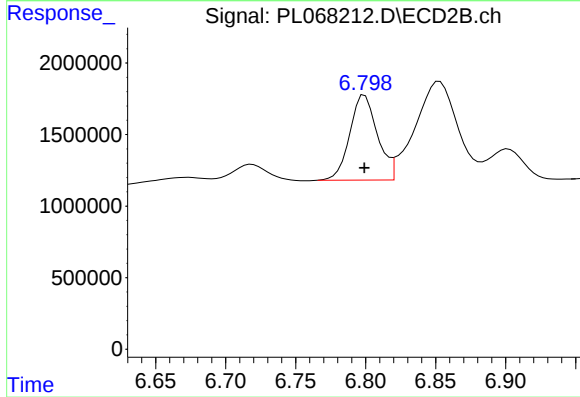

#6 beta-BHC


R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 8188287
Conc: 11.59 ng/ml

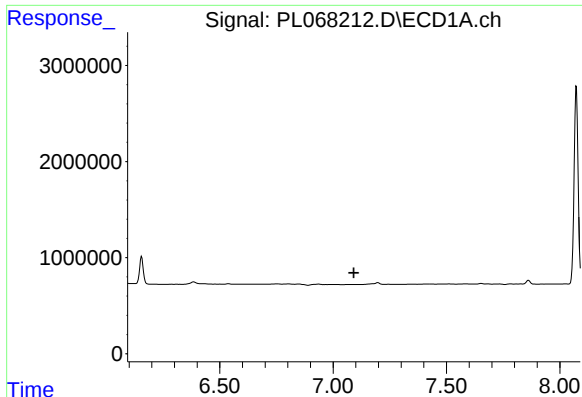

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.091 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PEM

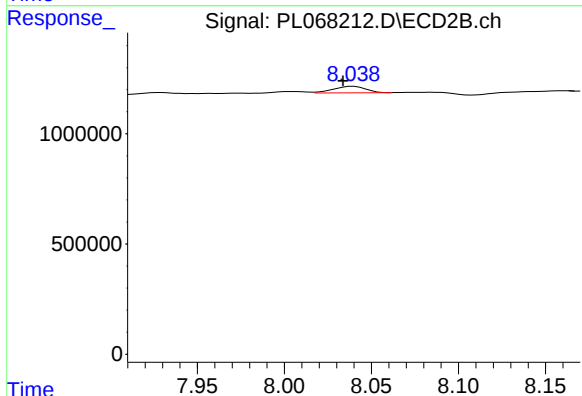


#8 Heptachlor epoxide

R.T.: 8.040 min
Delta R.T.: 0.006 min
Response: 379912
Conc: 0.34 ng/ml

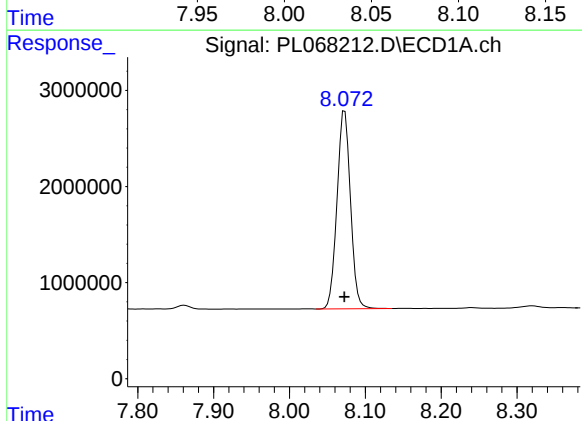


#14 Endrin

R.T.: 8.073 min
Delta R.T.: 0.000 min
Response: 25448392
Conc: 50.89 ng/ml

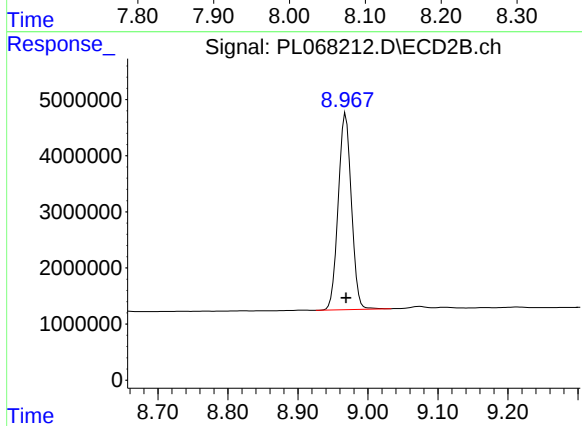

#14 Endrin


R.T.: 8.968 min
Delta R.T.: 0.000 min
Response: 45622740
Conc: 51.02 ng/ml

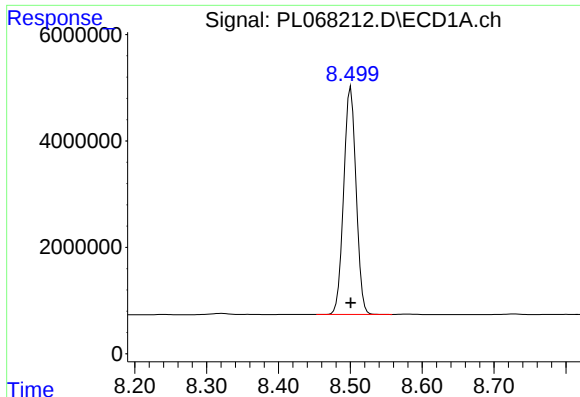

#17 4,4'-DDT


R.T.: 8.501 min
Delta R.T.: 0.000 min
Response: 51176274
Conc: 102.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

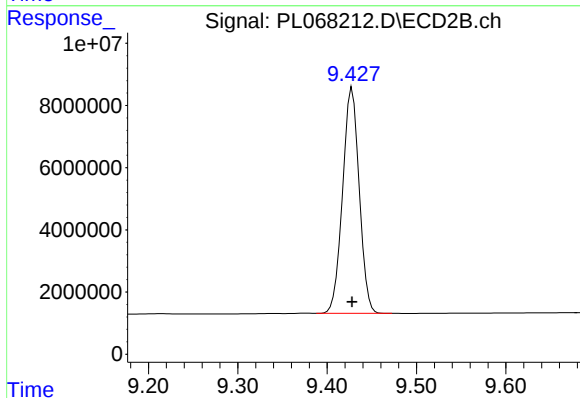


#17 4,4'-DDT

R.T.: 9.428 min
Delta R.T.: 0.000 min
Response: 93680097
Conc: 99.25 ng/ml

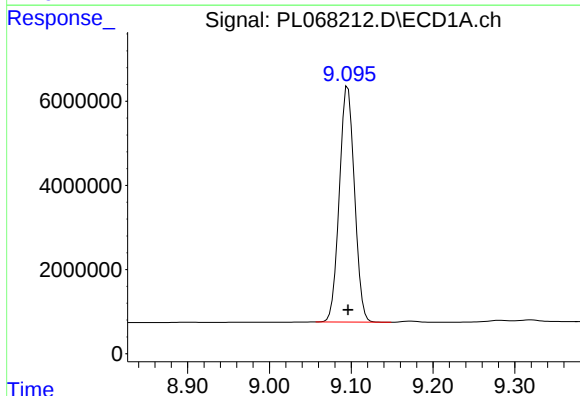


#20 Methoxychlor

R.T.: 9.096 min
Delta R.T.: 0.000 min
Response: 71713350
Conc: 229.26 ng/ml

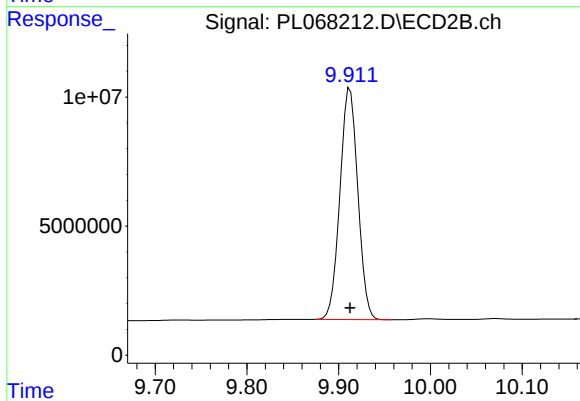

#20 Methoxychlor


R.T.: 9.912 min
Delta R.T.: 0.000 min
Response: 121636402
Conc: 239.42 ng/ml

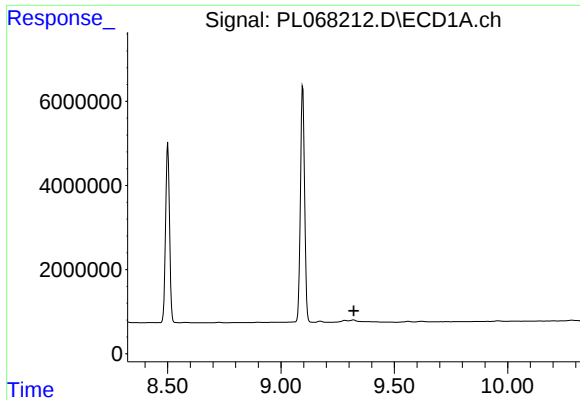

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.322 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PEM

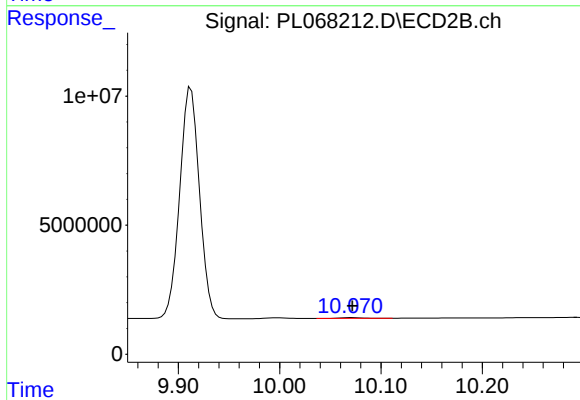


#21 Endrin ketone

R.T.: 10.072 min
Delta R.T.: 0.000 min
Response: 444743
Conc: 0.45 ng/ml

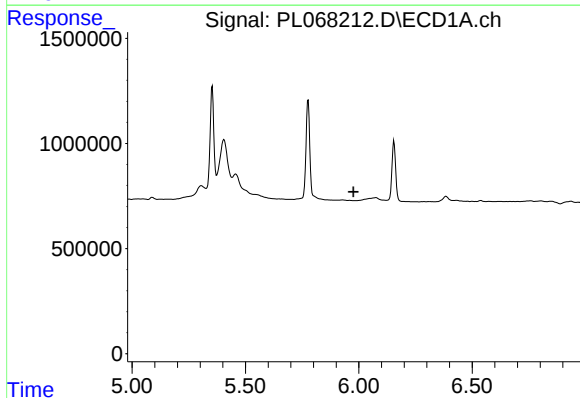


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.977 min
Response: 0
Conc: N.D.

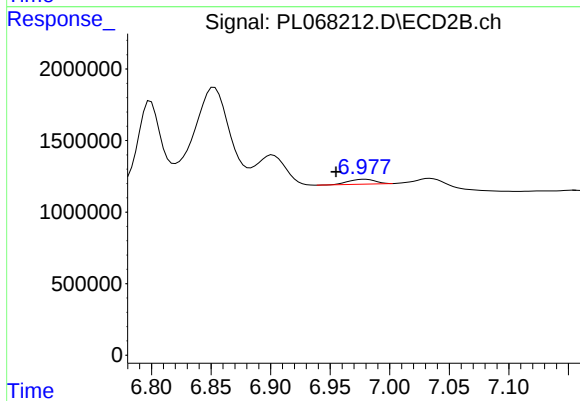

#23 Chlordane-1


R.T.: 6.979 min
Delta R.T.: 0.024 min
Response: 534723
Conc: 13.90 ng/ml

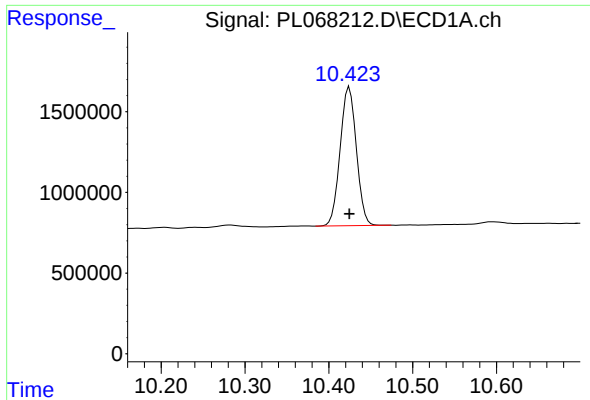

#28 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: 0.000 min
Response: 11567132
Conc: 20.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

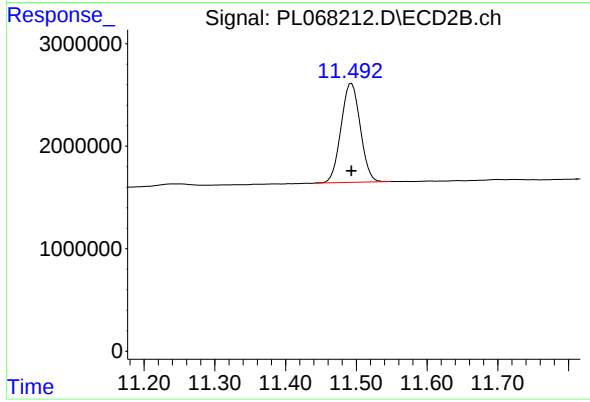

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 18270640
Conc: 20.48 ng/ml