

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
 Data File : PL068219.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2021 20:45
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 02:36:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 02:36:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.646	5.571	57655121	116.5E6	103.558	104.021
28)	SA Decachlor...	10.424	11.493	57264780	94573710	96.630	98.658
Target Compounds							
23)	Chlordane-1	5.977	6.955	16331153	40450278	1034.570	1051.181
24)	Chlordane-2	6.667	7.547	21563448	43919979	976.558	1001.452
25)	Chlordane-3	7.369	8.304	60716195	174.9E6	1059.994	1072.492
26)	Chlordane-4	7.438	8.386	63886738	207.7E6	1049.721	1052.666
27)	Chlordane-5	8.388	9.274	22705675	36036872	1057.072	1029.091



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
Data File : PL068219.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2021 20:45
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 02:36:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 02:36:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

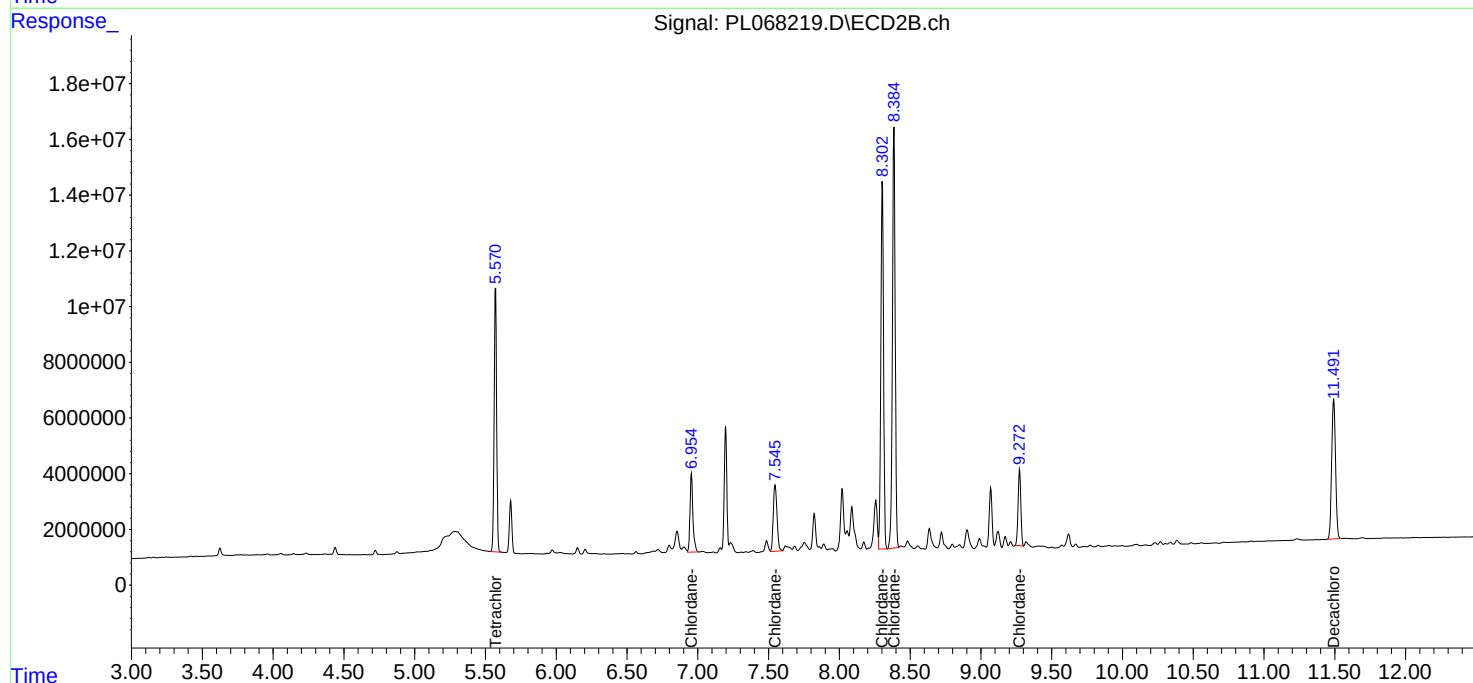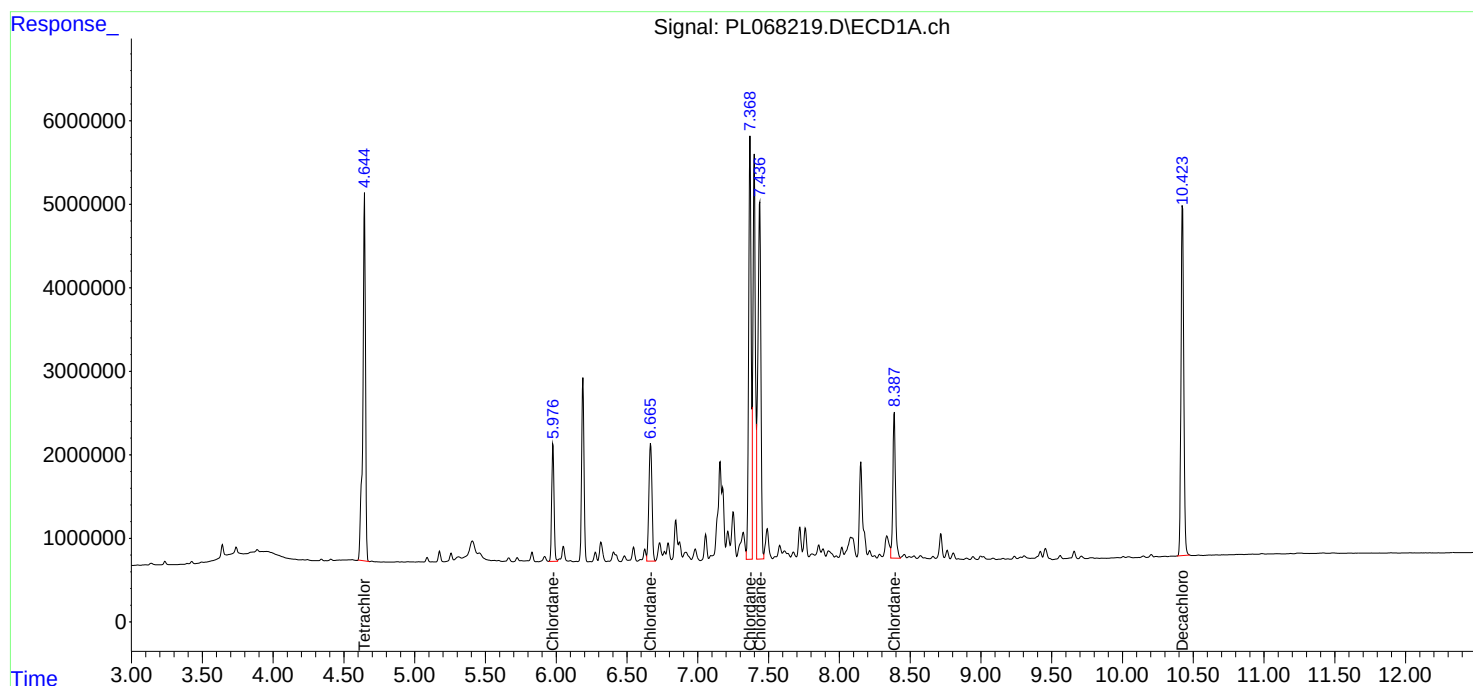


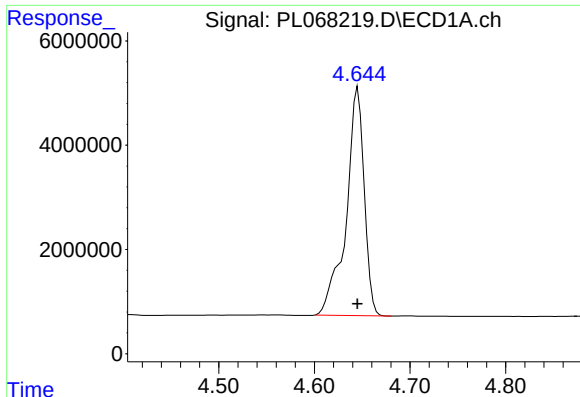

#1 Tetrachloro-m-xylene


R.T.: 4.646 min
Delta R.T.: 0.000 min
Response: 57655121
Conc: 103.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

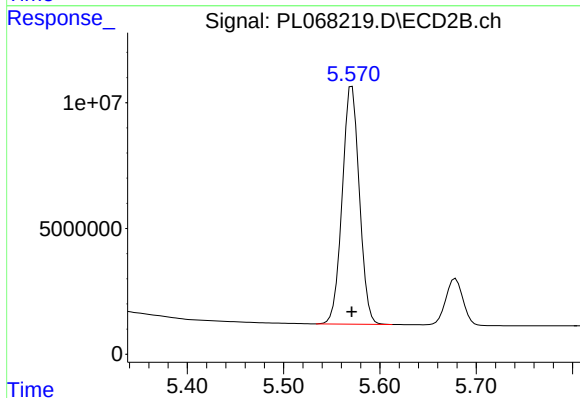


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 116492909
Conc: 104.02 ng/ml

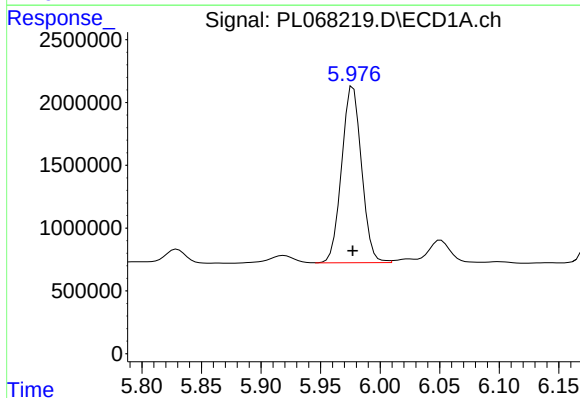


#23 Chlordane-1

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 16331153
Conc: 1034.57 ng/ml

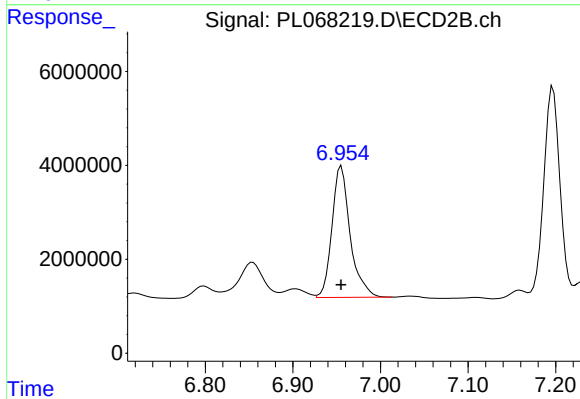

#23 Chlordane-1


R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 40450278
Conc: 1051.18 ng/ml

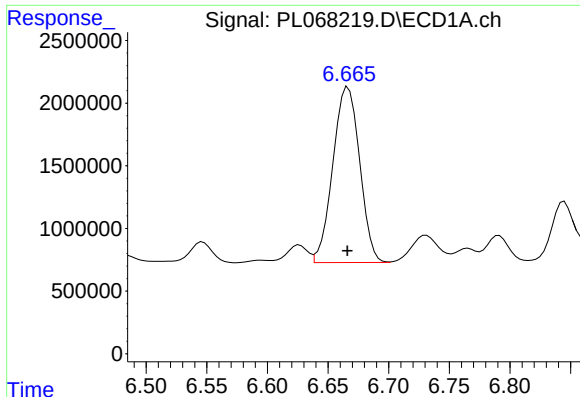

#24 Chlordane-2


R.T.: 6.667 min
Delta R.T.: 0.000 min
Response: 21563448
Conc: 976.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

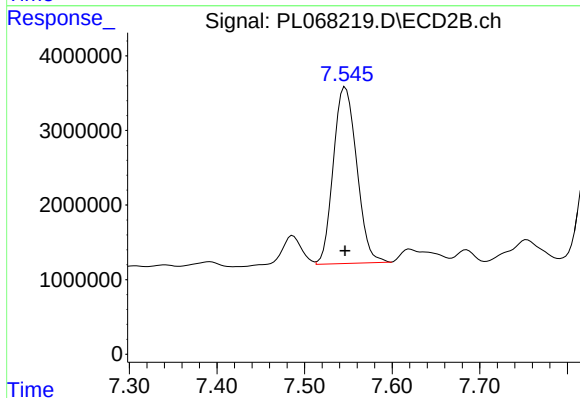


#24 Chlordane-2

R.T.: 7.547 min
Delta R.T.: 0.000 min
Response: 43919979
Conc: 1001.45 ng/ml

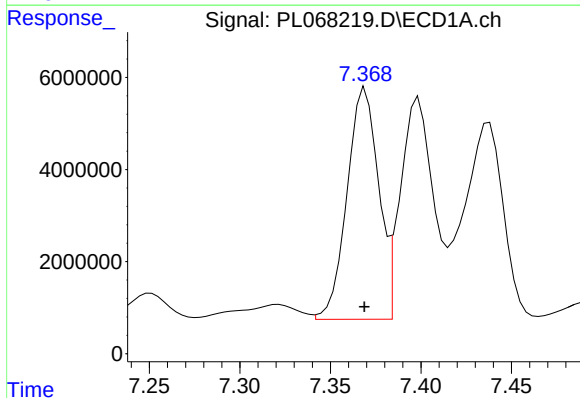


#25 Chlordane-3

R.T.: 7.369 min
Delta R.T.: 0.000 min
Response: 60716195
Conc: 1059.99 ng/ml

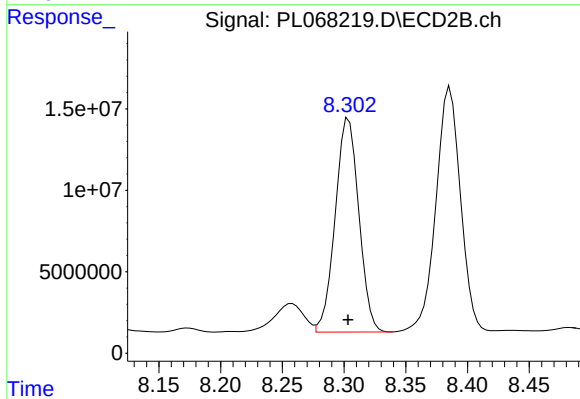

#25 Chlordane-3


R.T.: 8.304 min
Delta R.T.: 0.000 min
Response: 174948455
Conc: 1072.49 ng/ml

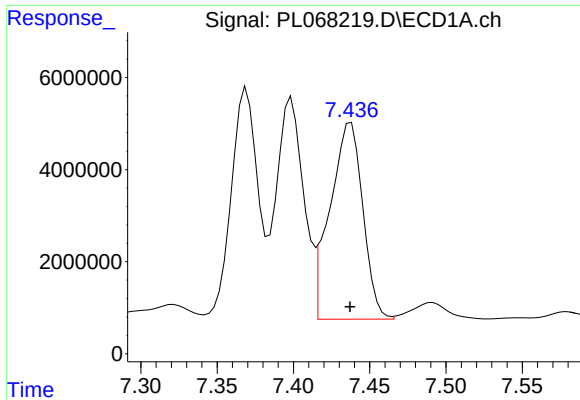

#26 Chlordane-4


R.T.: 7.438 min
Delta R.T.: 0.000 min
Response: 63886738
Conc: 1049.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

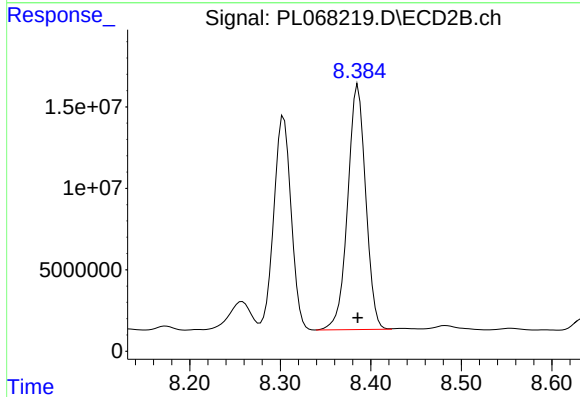


#26 Chlordane-4

R.T.: 8.386 min
Delta R.T.: 0.000 min
Response: 207738677
Conc: 1052.67 ng/ml

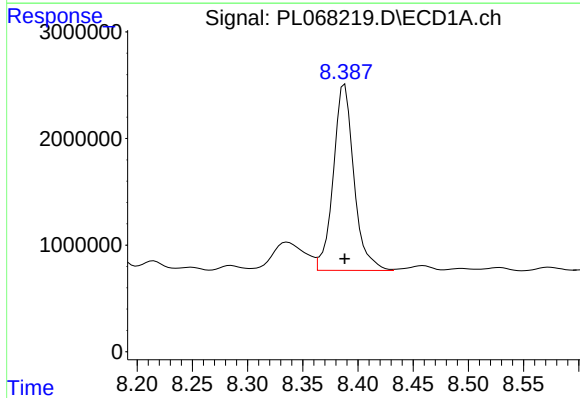


#27 Chlordane-5

R.T.: 8.388 min
Delta R.T.: 0.000 min
Response: 22705675
Conc: 1057.07 ng/ml

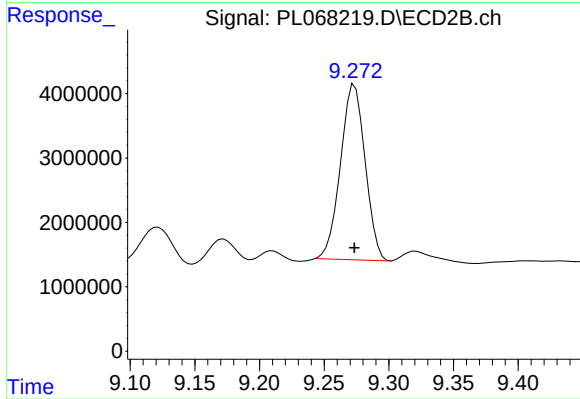

#27 Chlordane-5


R.T.: 9.274 min
Delta R.T.: 0.000 min
Response: 36036872
Conc: 1029.09 ng/ml

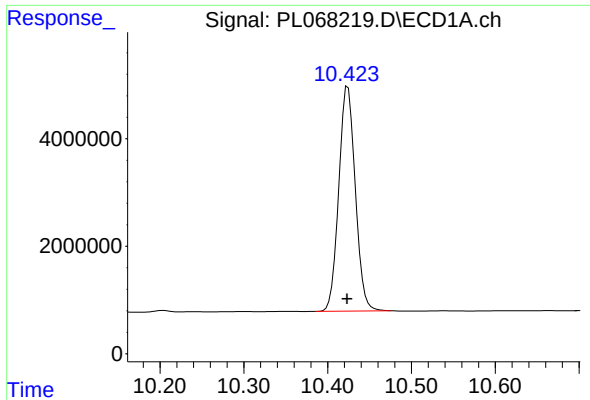

#28 Decachlorobiphenyl

R.T.: 10.424 min
Delta R.T.: 0.000 min
Response: 57264780
Conc: 96.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

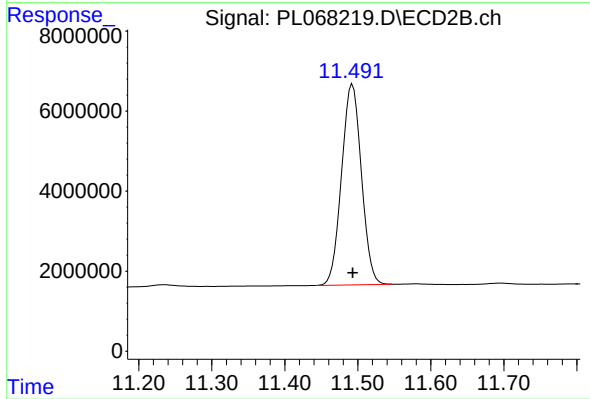

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 94573710
Conc: 98.66 ng/ml