

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
 Data File : PL068222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2021 21:35
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 02:37:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 02:36:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.571	14499253	28866624	26.043	25.776
28)	SA Decachlor...	10.424	11.492	16198757	25774730	27.334	26.888
Target Compounds							
23)	Chlordane-1	5.977	6.955	4213661	9978339	266.933	259.307
24)	Chlordane-2	6.666	7.546	6080389	11574890	275.367	263.928
25)	Chlordane-3	7.368	8.303	14688488	41413552	256.434	253.879
26)	Chlordane-4	7.438	8.386	15693620	50647758	257.861	256.645
27)	Chlordane-5	8.388	9.273	5654848	9014648	263.264	257.428


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
Data File : PL068222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2021 21:35
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 02:37:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 02:36:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

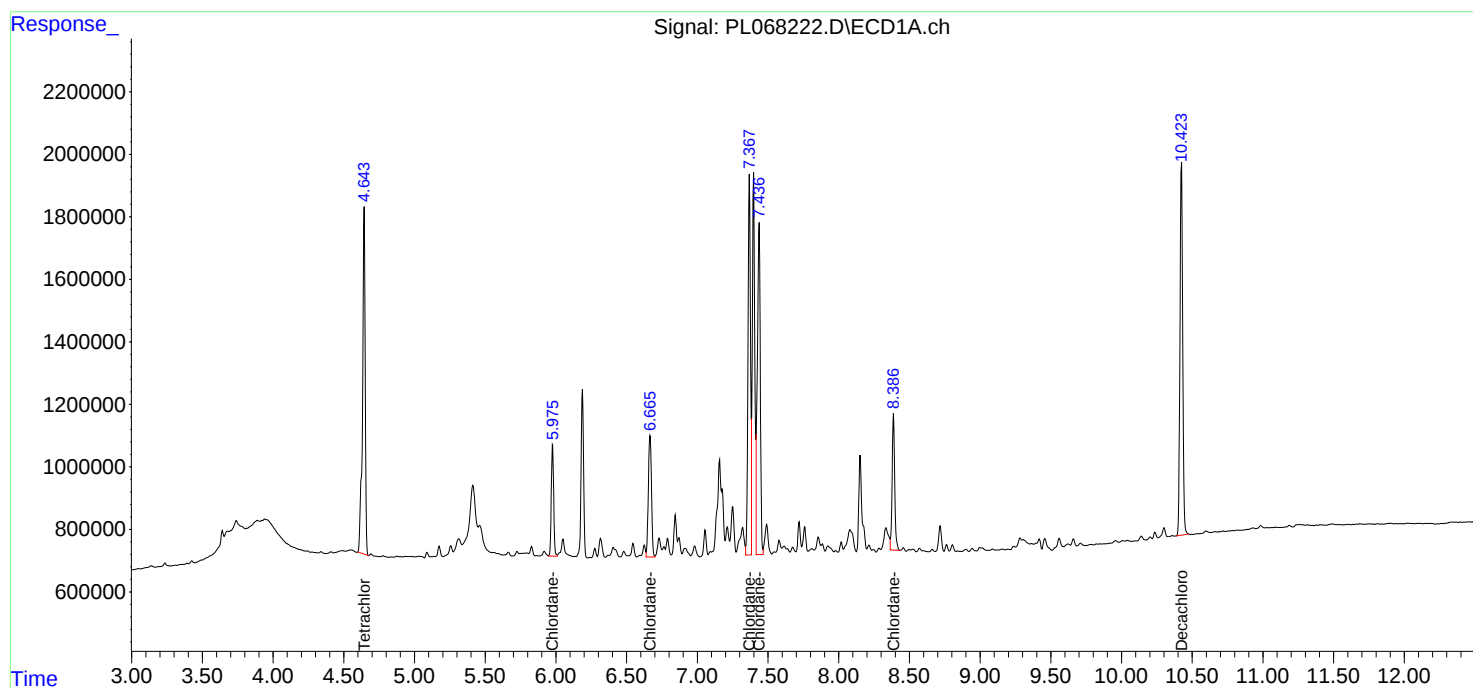


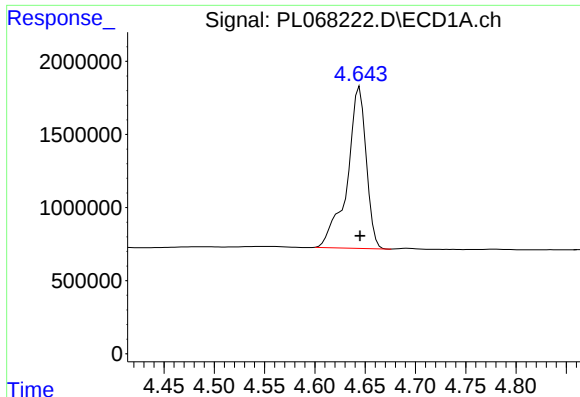

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 14499253
Conc: 26.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

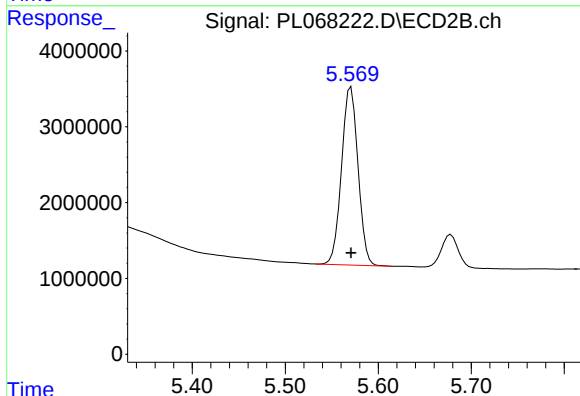


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 28866624
Conc: 25.78 ng/ml

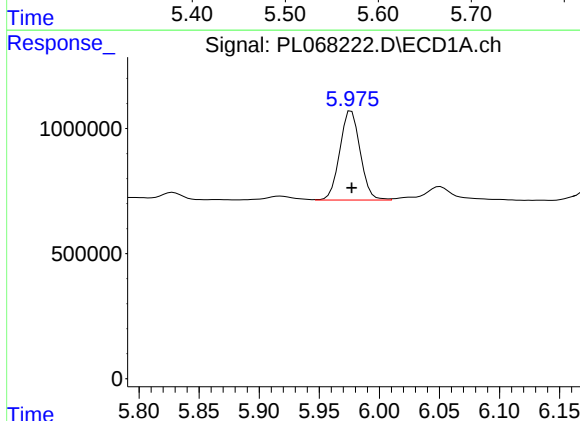


#23 Chlordane-1

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 4213661
Conc: 266.93 ng/ml

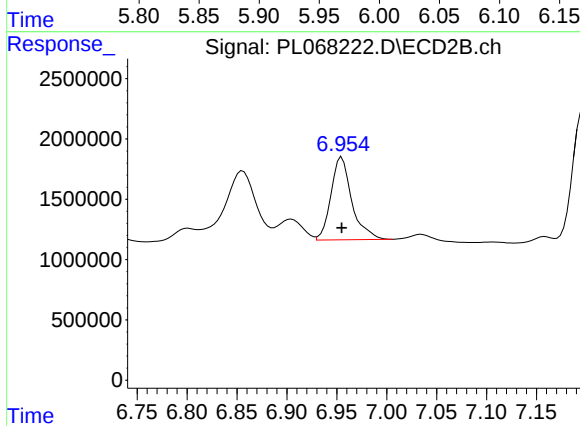

#23 Chlordane-1


R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 9978339
Conc: 259.31 ng/ml

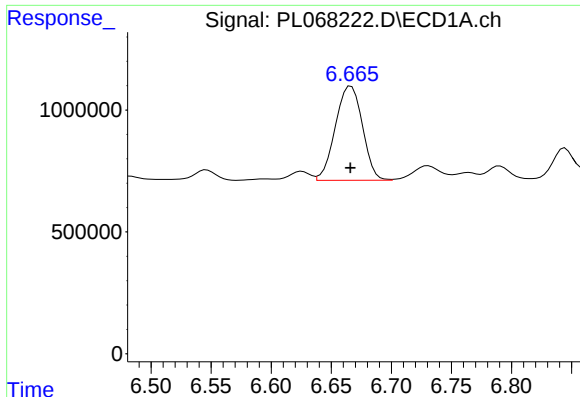

#24 Chlordane-2


R.T.: 6.666 min
Delta R.T.: 0.000 min
Response: 6080389
Conc: 275.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

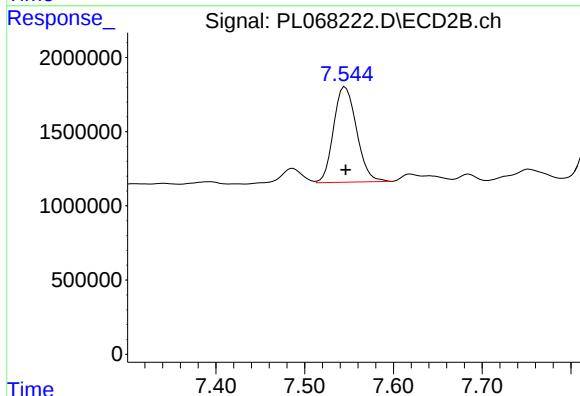


#24 Chlordane-2

R.T.: 7.546 min
Delta R.T.: 0.000 min
Response: 11574890
Conc: 263.93 ng/ml

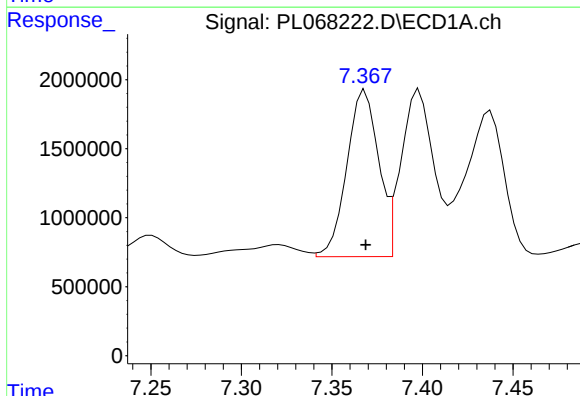


#25 Chlordane-3

R.T.: 7.368 min
Delta R.T.: 0.000 min
Response: 14688488
Conc: 256.43 ng/ml

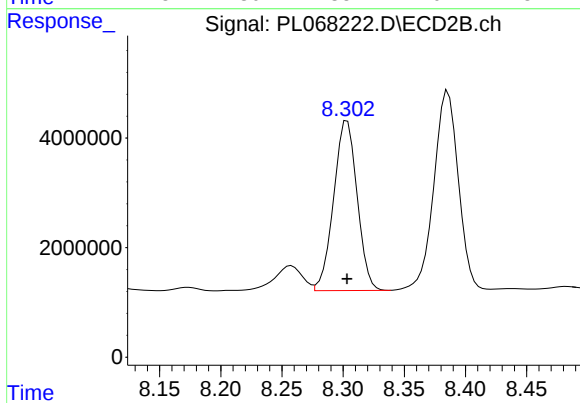

#25 Chlordane-3


R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 41413552
Conc: 253.88 ng/ml

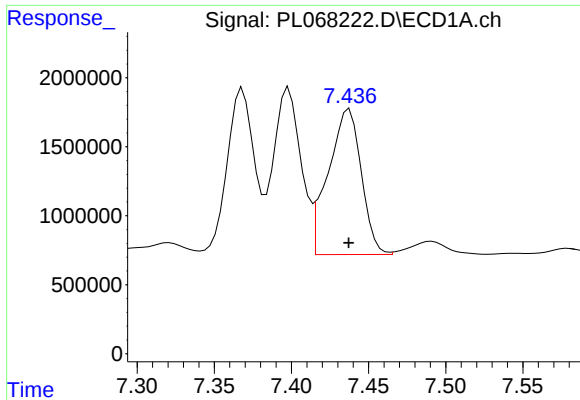

#26 Chlordane-4


R.T.: 7.438 min
Delta R.T.: 0.000 min
Response: 15693620
Conc: 257.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

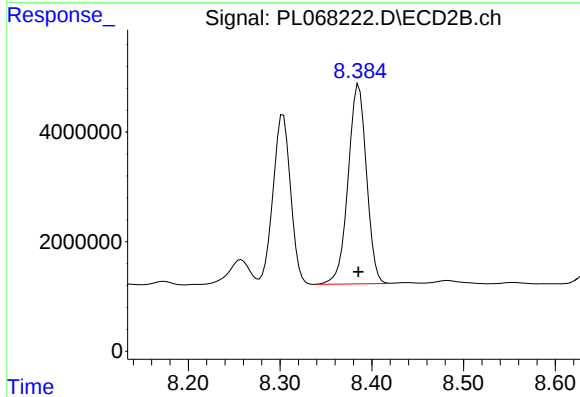


#26 Chlordane-4

R.T.: 8.386 min
Delta R.T.: 0.000 min
Response: 50647758
Conc: 256.65 ng/ml

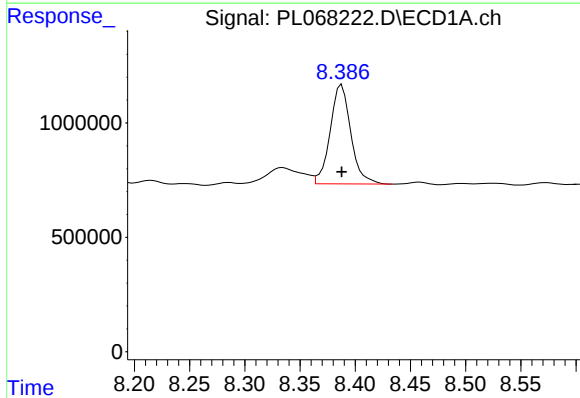


#27 Chlordane-5

R.T.: 8.388 min
Delta R.T.: 0.000 min
Response: 5654848
Conc: 263.26 ng/ml

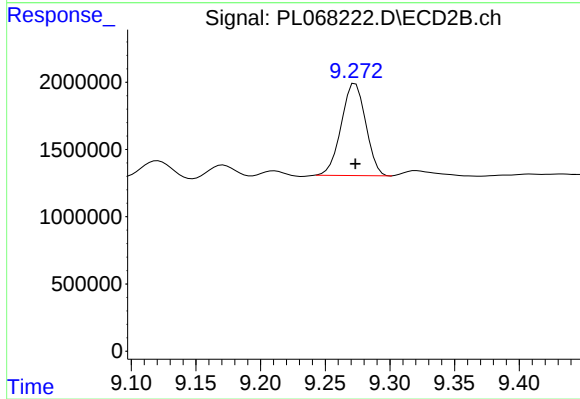

#27 Chlordane-5


R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 9014648
Conc: 257.43 ng/ml

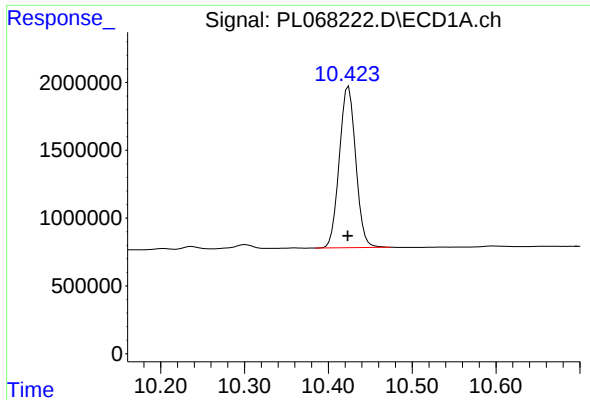

#28 Decachlorobiphenyl

R.T.: 10.424 min
Delta R.T.: 0.000 min
Response: 16198757
Conc: 27.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

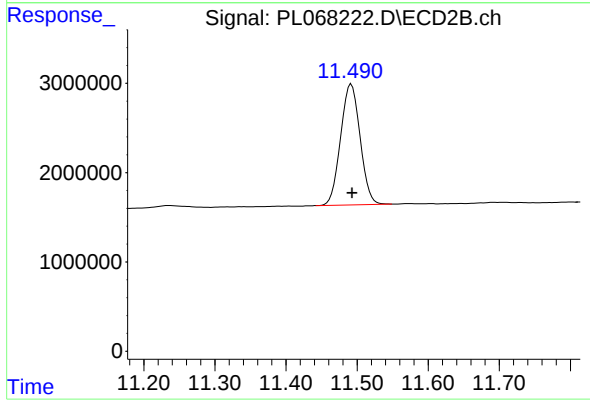

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: -0.001 min
Response: 25774730
Conc: 26.89 ng/ml