

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
 Data File : PL068223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2021 21:52
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 02:37:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 02:36:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.571	4364211	8636167	7.839	7.712
28)	SA Decachlor...	10.424	11.493	5375071	8534860	9.070	8.903
Target Compounds							
23)	Chlordane-1	5.977	6.955	1243258	2991073	78.760	77.729
24)	Chlordane-2	6.666	7.546	1893946	3498294	85.772	79.767
25)	Chlordane-3	7.368	8.303	4386471	12454717	76.580	76.352
26)	Chlordane-4	7.437	8.386	4653534	15380691	76.462	77.938
27)	Chlordane-5	8.388	9.273	1810370	2651269	84.282	75.711


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
Data File : PL068223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2021 21:52
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 02:37:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 02:36:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

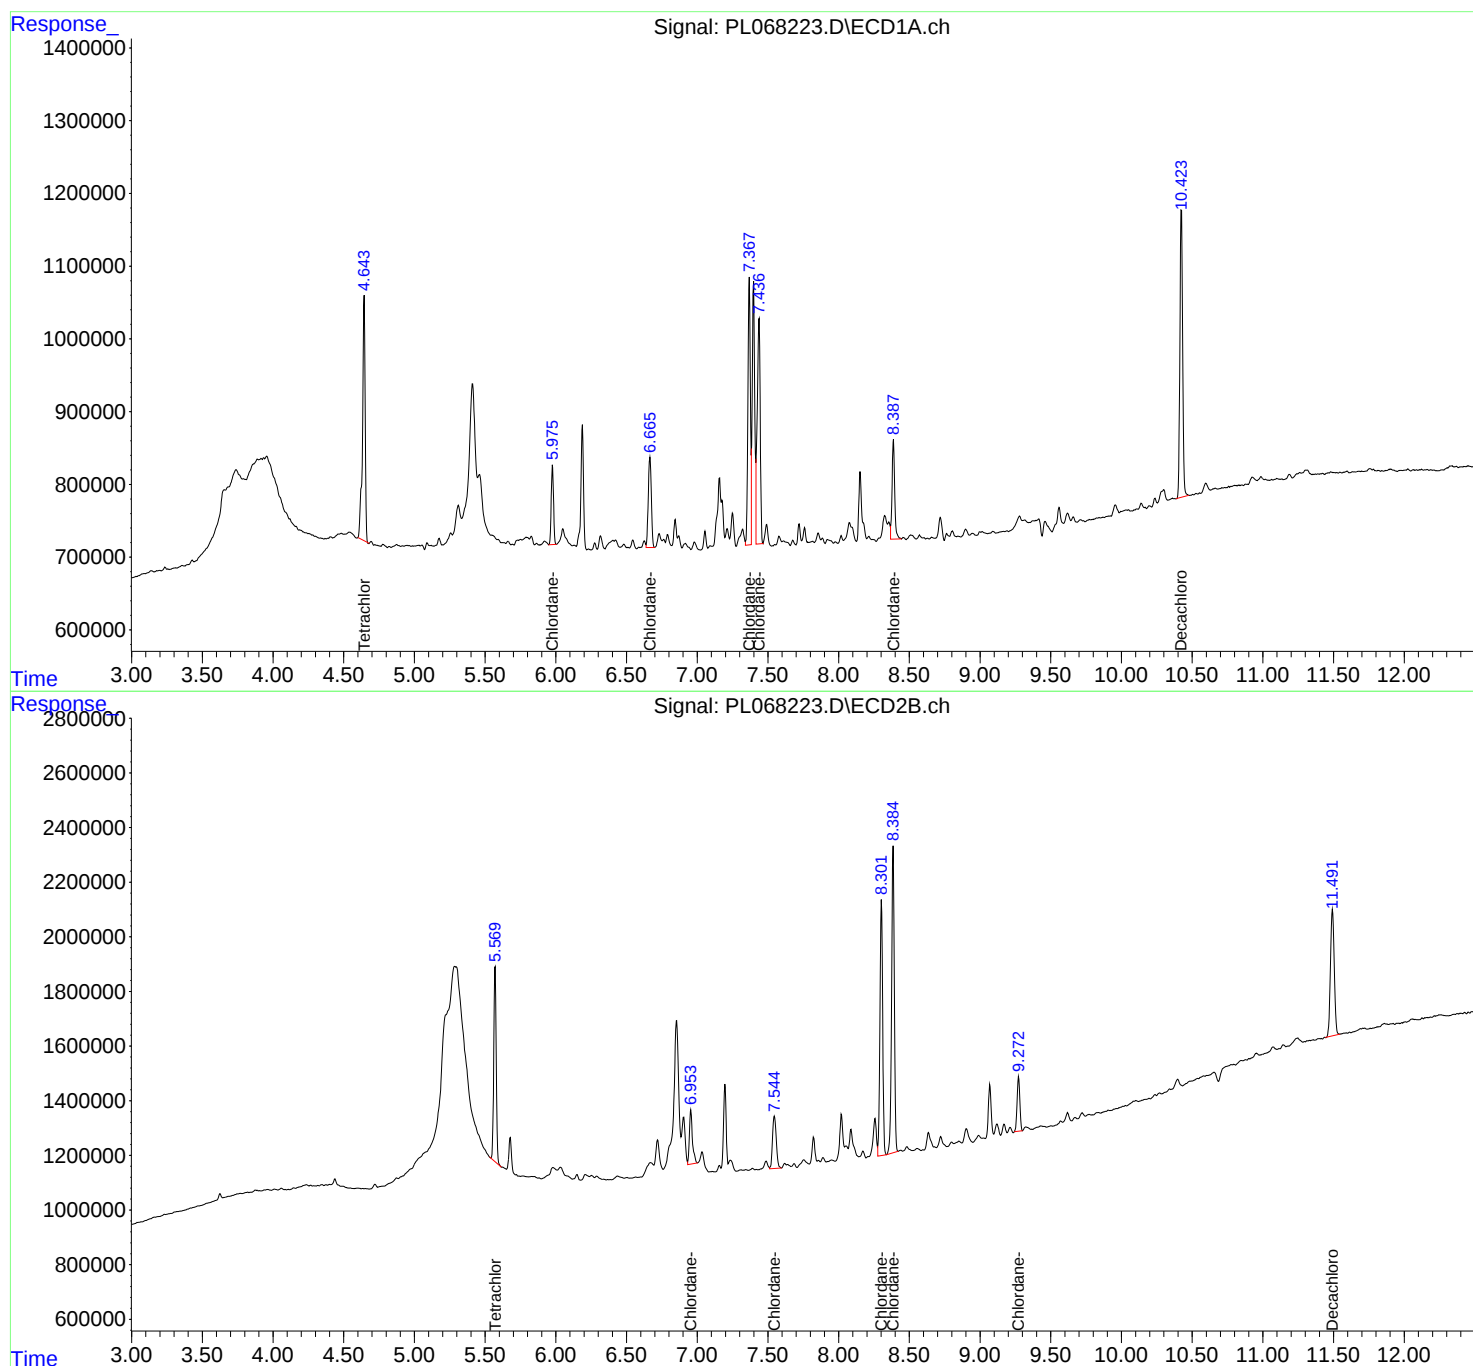


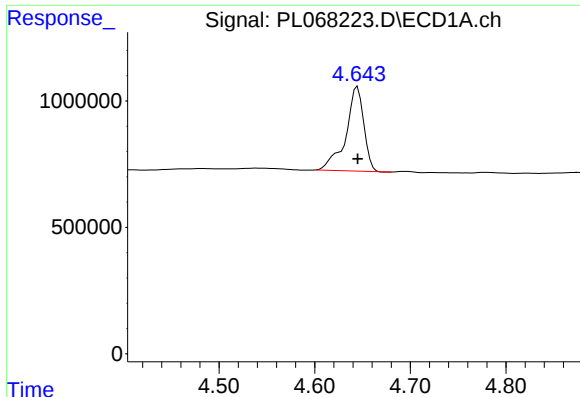

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 4364211
Conc: 7.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

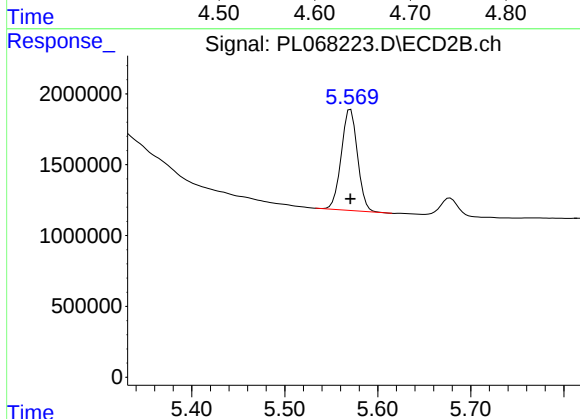


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 8636167
Conc: 7.71 ng/ml

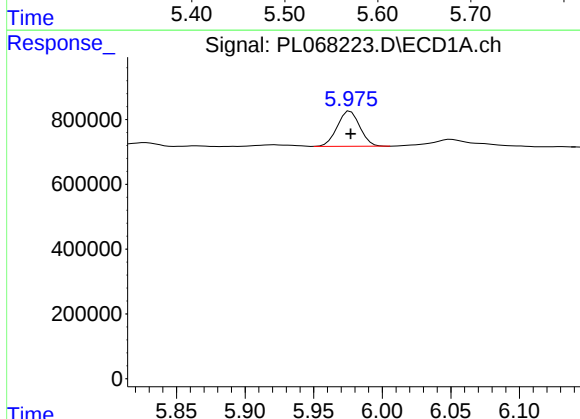


#23 Chlordane-1

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 1243258
Conc: 78.76 ng/ml

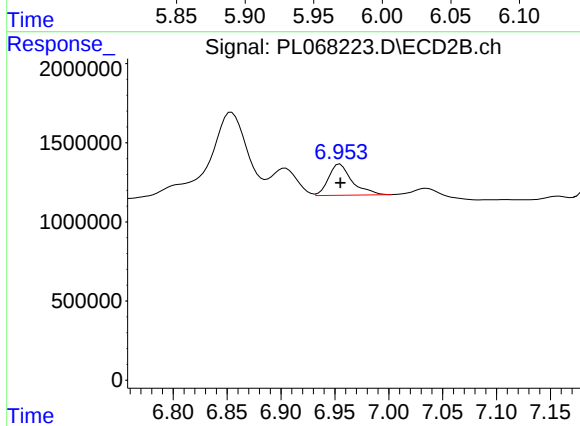

#23 Chlordane-1


R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 2991073
Conc: 77.73 ng/ml

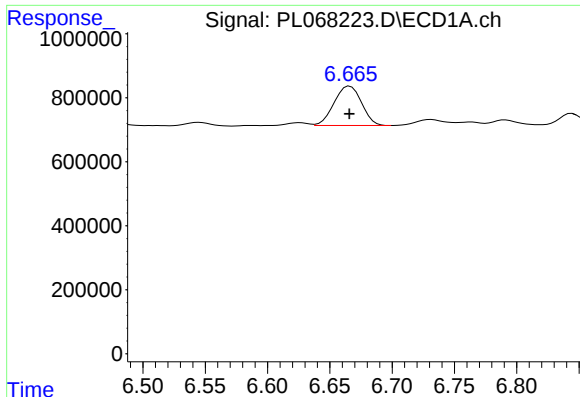

#24 Chlordane-2


R.T.: 6.666 min
Delta R.T.: 0.000 min
Response: 1893946
Conc: 85.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

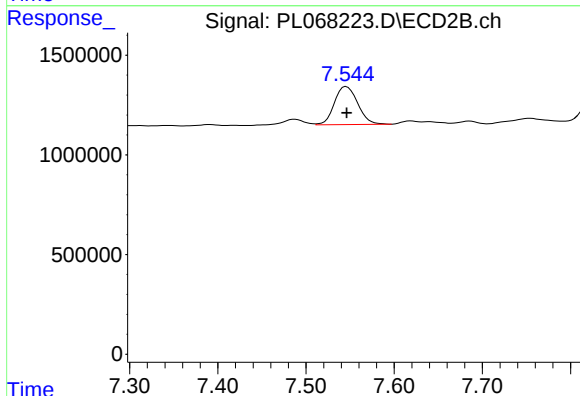


#24 Chlordane-2

R.T.: 7.546 min
Delta R.T.: 0.000 min
Response: 3498294
Conc: 79.77 ng/ml

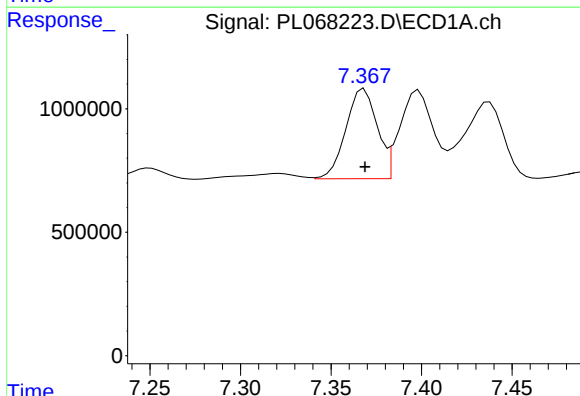


#25 Chlordane-3

R.T.: 7.368 min
Delta R.T.: 0.000 min
Response: 4386471
Conc: 76.58 ng/ml

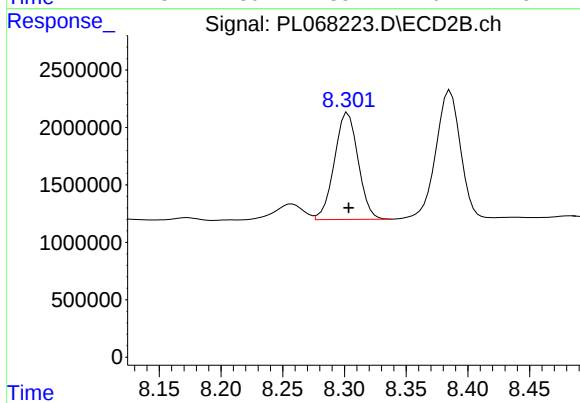

#25 Chlordane-3


R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 12454717
Conc: 76.35 ng/ml

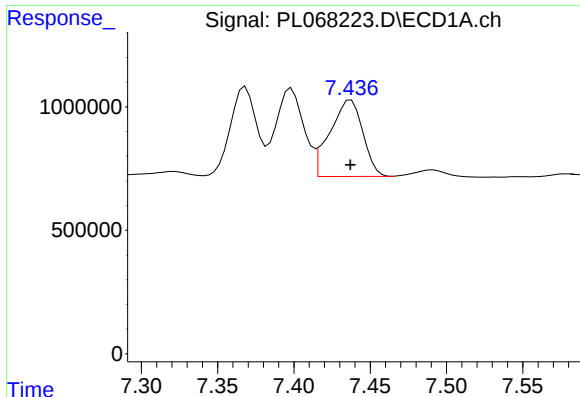

#26 Chlordane-4


R.T.: 7.437 min
Delta R.T.: 0.000 min
Response: 4653534
Conc: 76.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

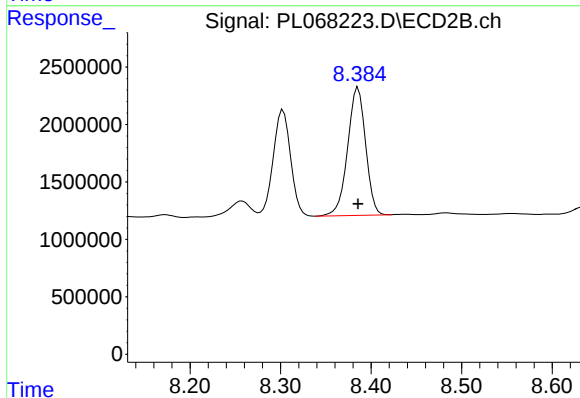


#26 Chlordane-4

R.T.: 8.386 min
Delta R.T.: 0.000 min
Response: 15380691
Conc: 77.94 ng/ml

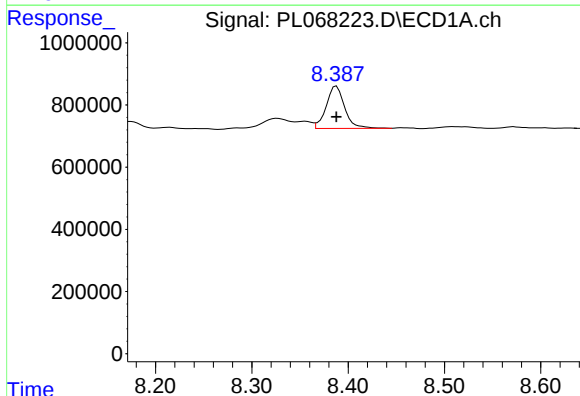


#27 Chlordane-5

R.T.: 8.388 min
Delta R.T.: 0.000 min
Response: 1810370
Conc: 84.28 ng/ml

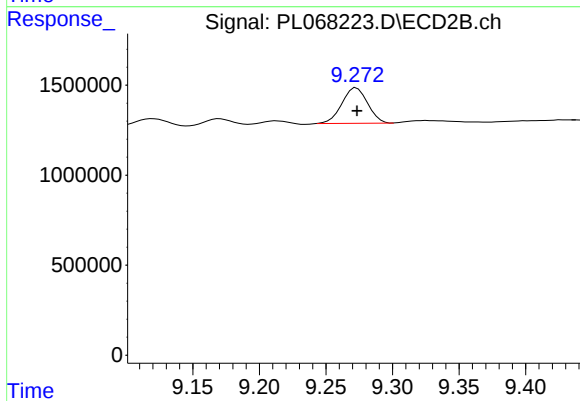

#27 Chlordane-5


R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 2651269
Conc: 75.71 ng/ml

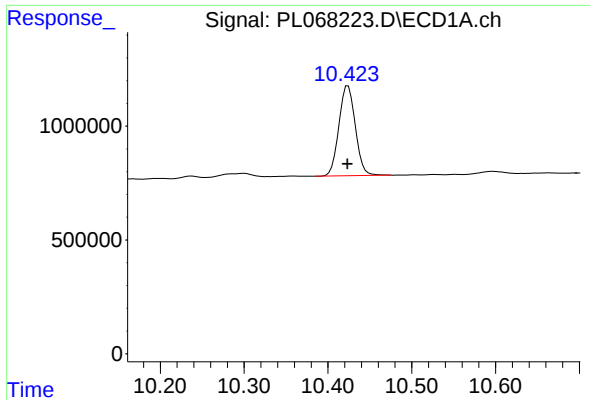

#28 Decachlorobiphenyl

R.T.: 10.424 min
Delta R.T.: 0.000 min
Response: 5375071
Conc: 9.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

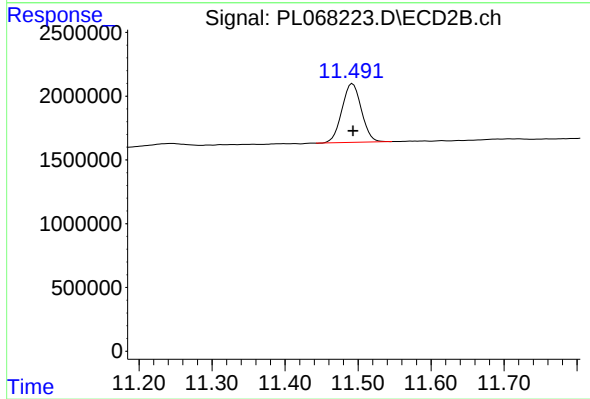

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 8534860
Conc: 8.90 ng/ml