

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
 Data File : PL068241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 02:50
 Operator : AR\AJ
 Sample : M3076-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210587-AMENDED-COM-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 04:21:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 03:26:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.571	8754903	20560580	20.399	20.149
28)	SA Decachlor...	10.424	11.493	8062788	14168364	14.336	15.884
Target Compounds							
3)	MA gamma-BHC...	0.000	6.518f	0	367680	N.D.	0.285 #
8)	B Heptachlo...	0.000	8.033	0	299264	N.D.	0.265 #
15)	B Endosulfa...	0.000	9.219f	0	589667	N.D.	0.651 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
Data File : PL068241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 02:50
Operator : AR\AJ
Sample : M3076-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20210587-AMENDED-COM-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 04:21:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 03:26:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

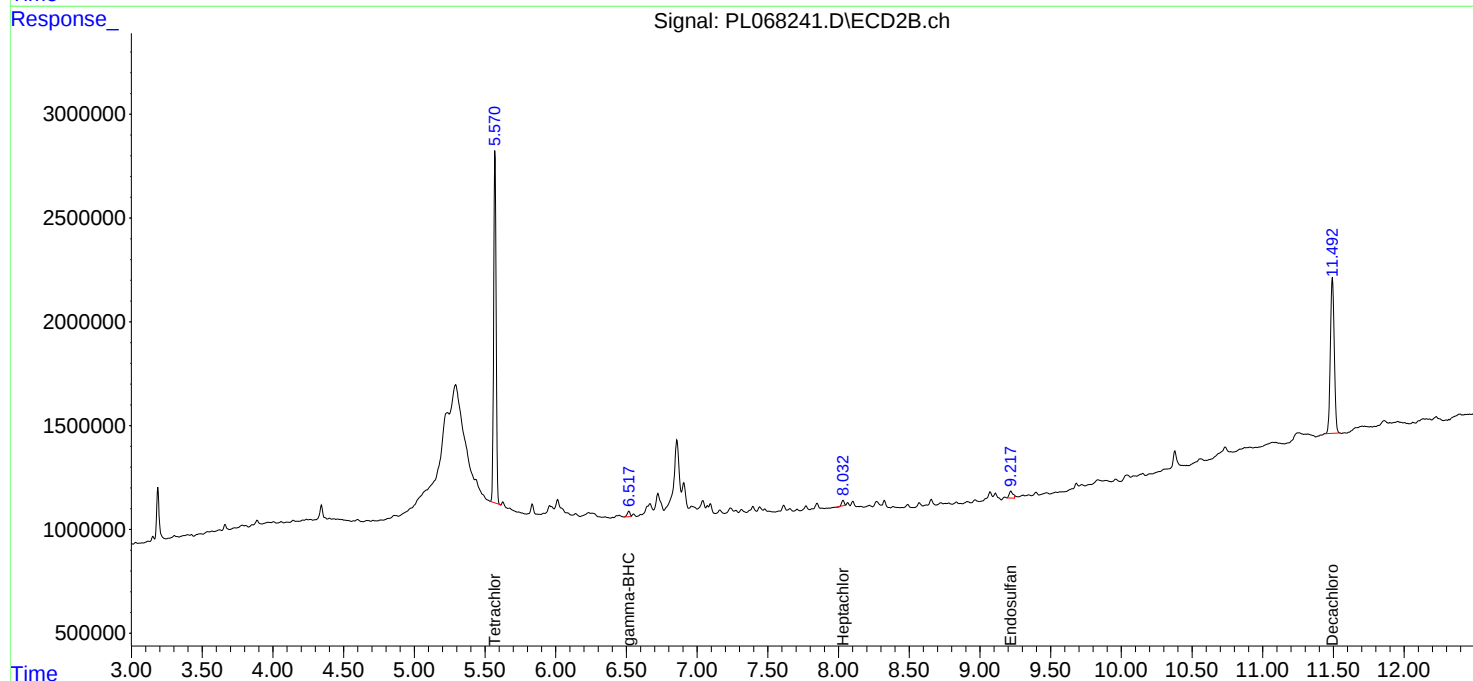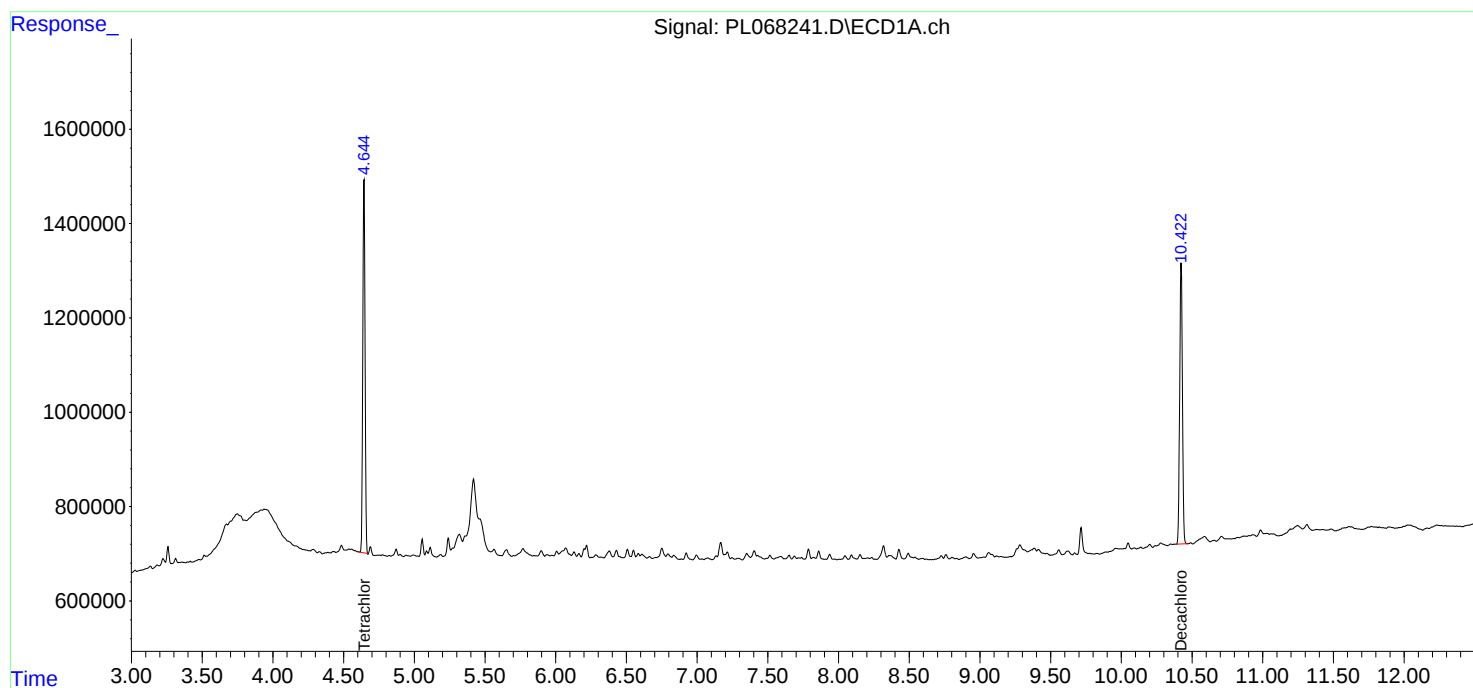


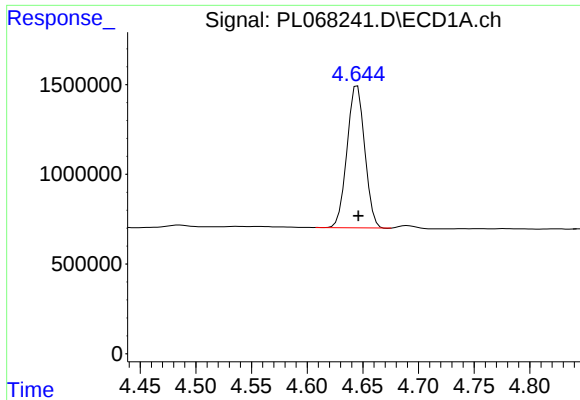

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 8754903
Conc: 20.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210587-AMENDED-COM-1

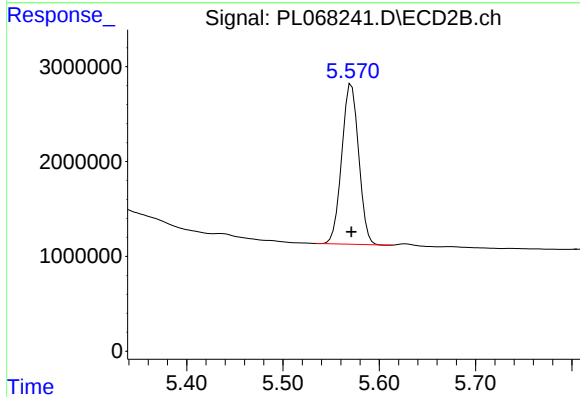


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 20560580
Conc: 20.15 ng/ml

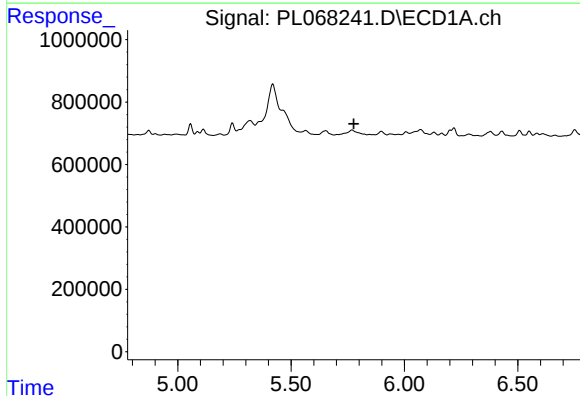


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.777 min
Response: 0
Conc: N.D.

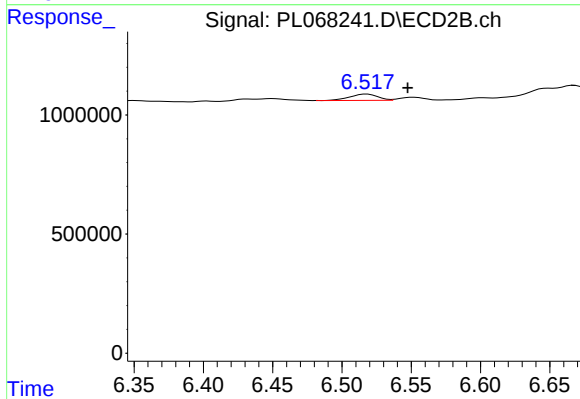

#3 gamma-BHC (Lindane)


R.T.: 6.518 min
Delta R.T.: -0.030 min
Response: 367680
Conc: 0.28 ng/ml

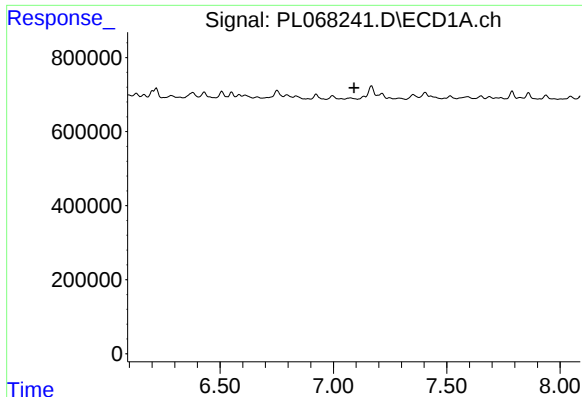

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210587-AMENDED-COM-1

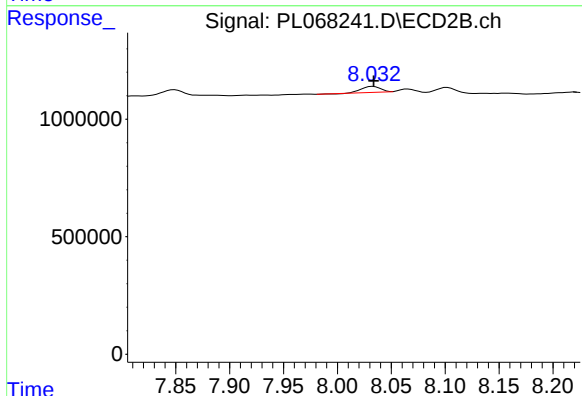


#8 Heptachlor epoxide

R.T.: 8.033 min
Delta R.T.: 0.000 min
Response: 299264
Conc: 0.26 ng/ml

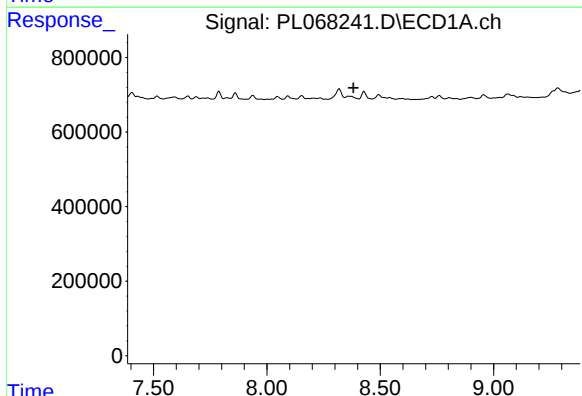


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

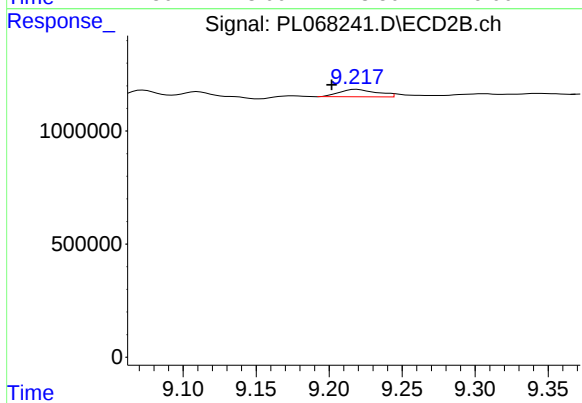

#15 Endosulfan II


R.T.: 9.219 min
Delta R.T.: 0.017 min
Response: 589667
Conc: 0.65 ng/ml

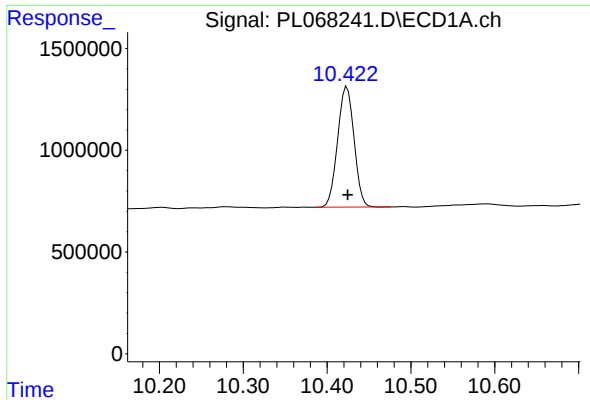

#28 Decachlorobiphenyl

R.T.: 10.424 min
Delta R.T.: 0.000 min
Response: 8062788
Conc: 14.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210587-AMENDED-COM-1

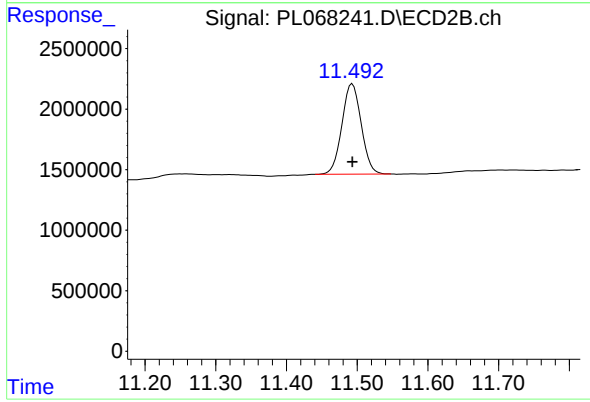

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 14168364
Conc: 15.88 ng/ml