

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
 Data File : PL068221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2021 21:18
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 02:48:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 02:48:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.571	27912062	55994693	50.000	50.000
28)	SA Decachlor...	10.423	11.493	29631056	47929995	50.000	50.000
Target Compounds							
23)	Chlordane-1	5.977	6.955	7892727	19240405	500.000	500.000
24)	Chlordane-2	6.666	7.546	11040535	21928155	500.000	500.000
25)	Chlordane-3	7.369	8.303	28639888	81561636	500.000	500.000
26)	Chlordane-4	7.437	8.386	30430340	98672637	500.000	500.000
27)	Chlordane-5	8.388	9.273	10739892	17509076	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
Data File : PL068221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2021 21:18
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 02:48:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 02:48:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

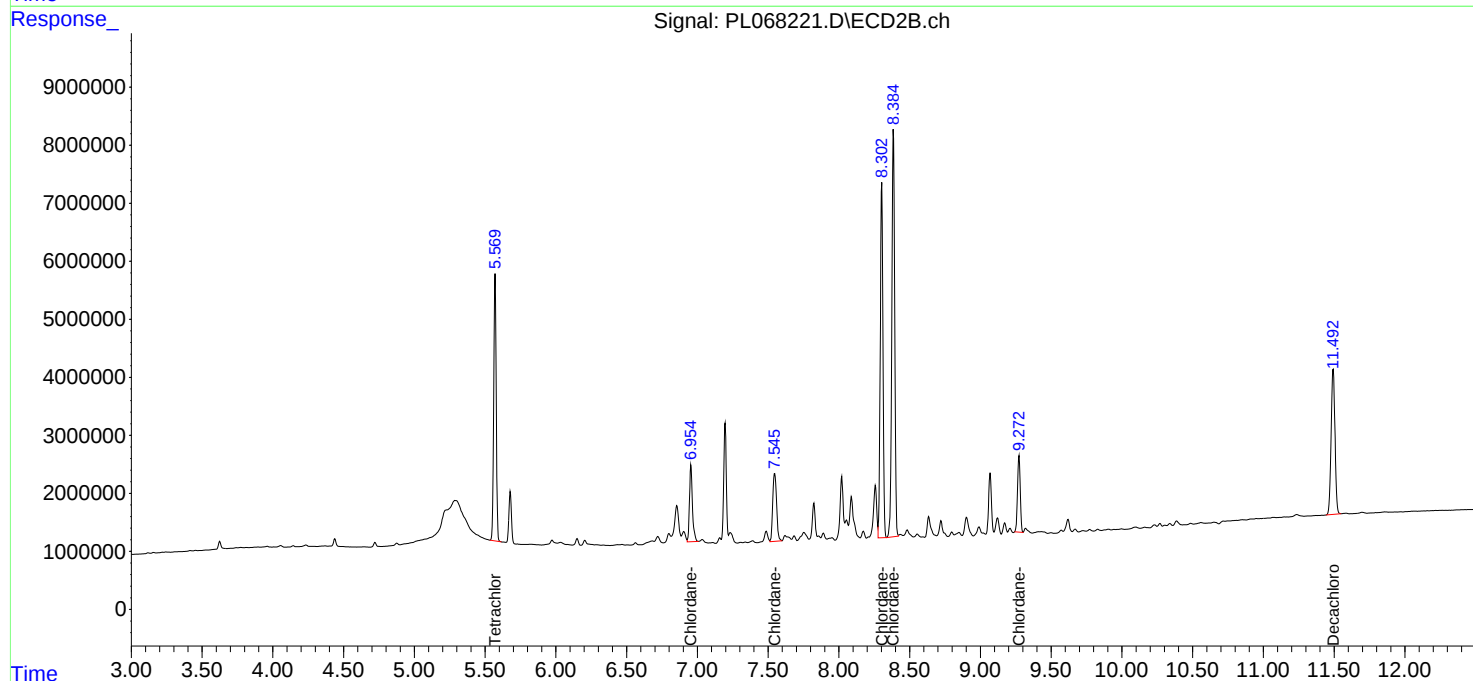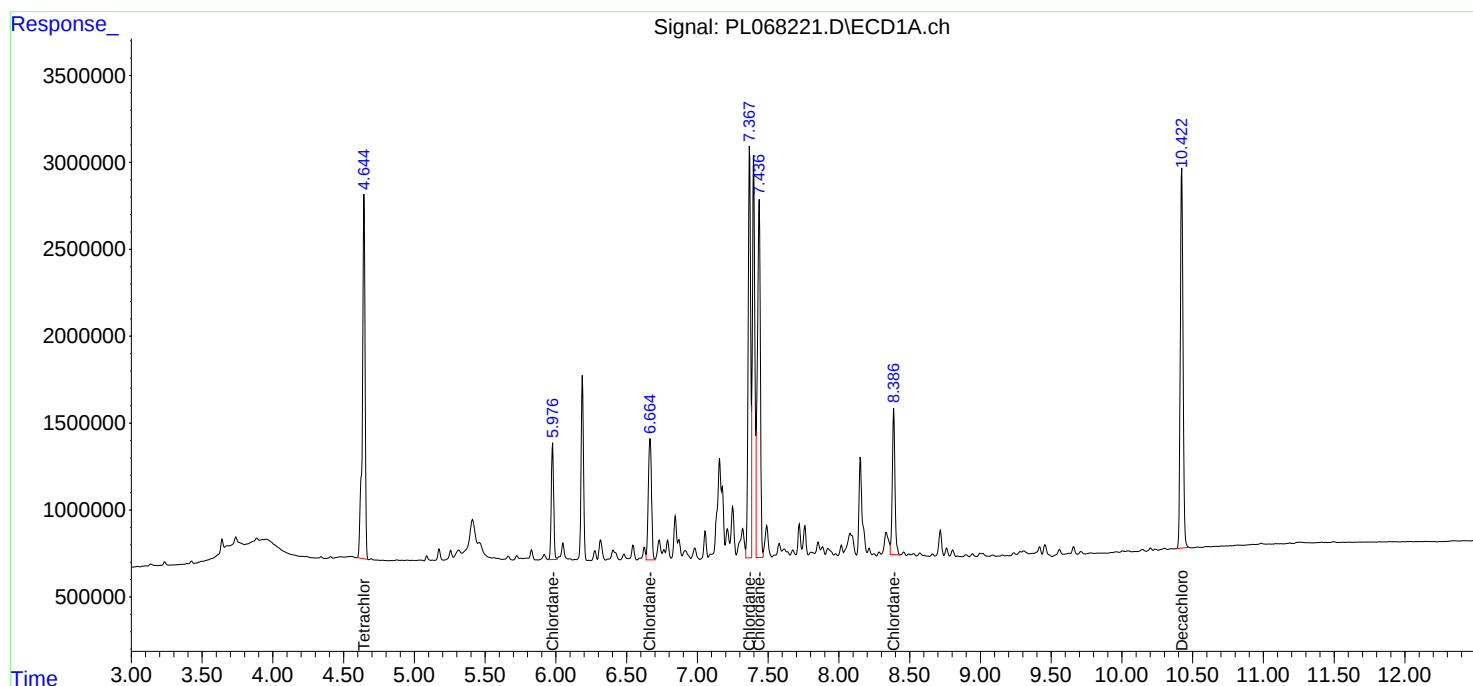


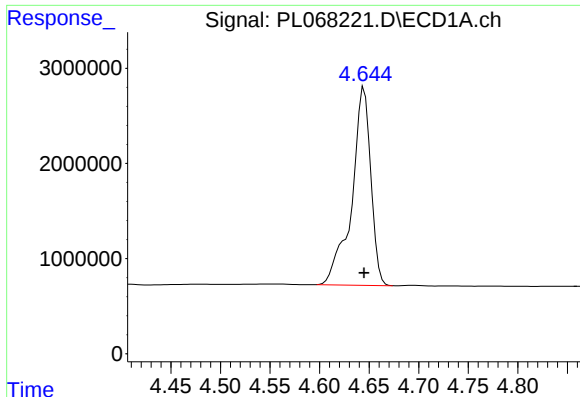

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 27912062
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

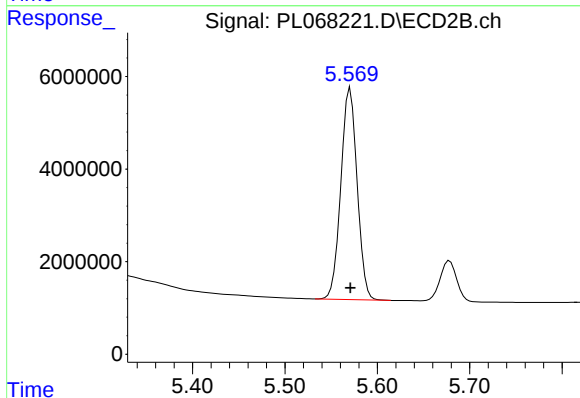


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 55994693
Conc: 50.00 ng/ml

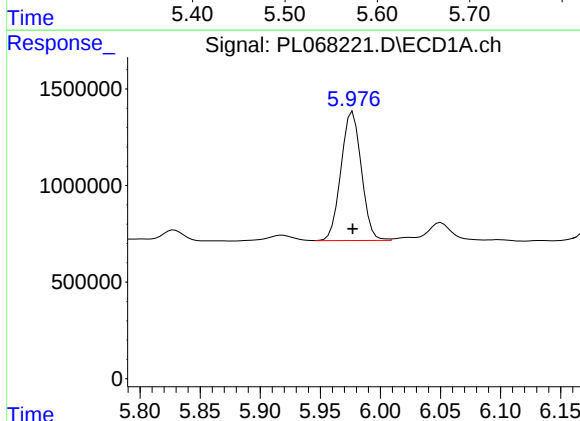


#23 Chlordane-1

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 7892727
Conc: 500.00 ng/ml

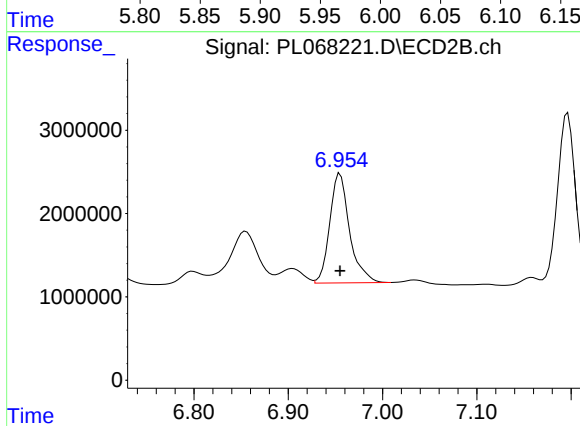

#23 Chlordane-1


R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 19240405
Conc: 500.00 ng/ml

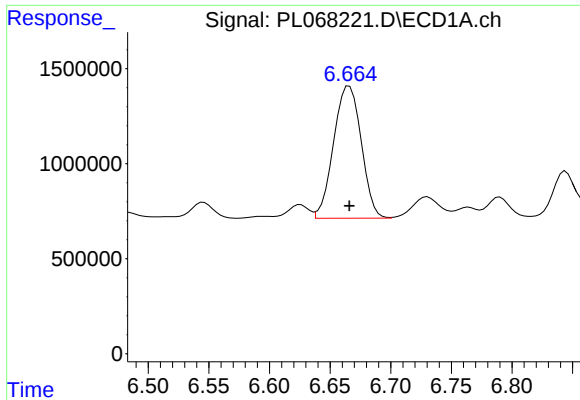

#24 Chlordane-2


R.T.: 6.666 min
Delta R.T.: 0.000 min
Response: 11040535
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

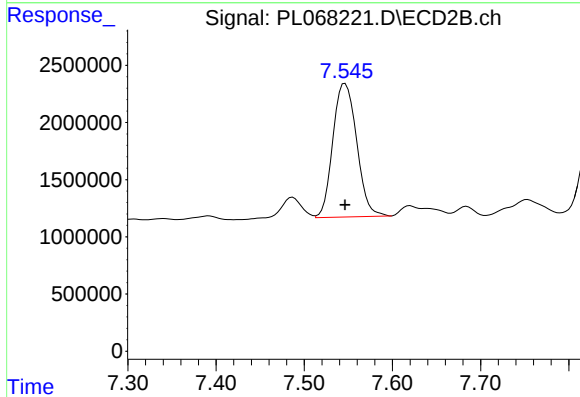


#24 Chlordane-2

R.T.: 7.546 min
Delta R.T.: 0.000 min
Response: 21928155
Conc: 500.00 ng/ml

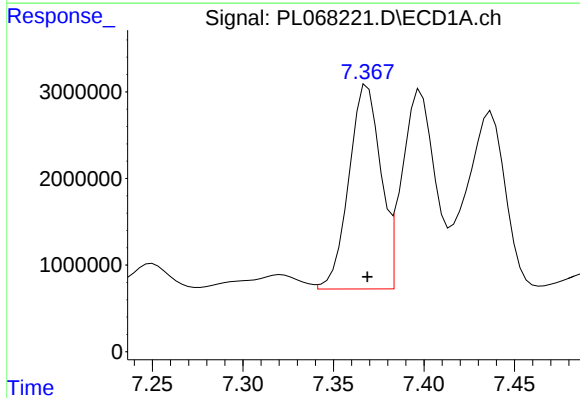


#25 Chlordane-3

R.T.: 7.369 min
Delta R.T.: 0.000 min
Response: 28639888
Conc: 500.00 ng/ml

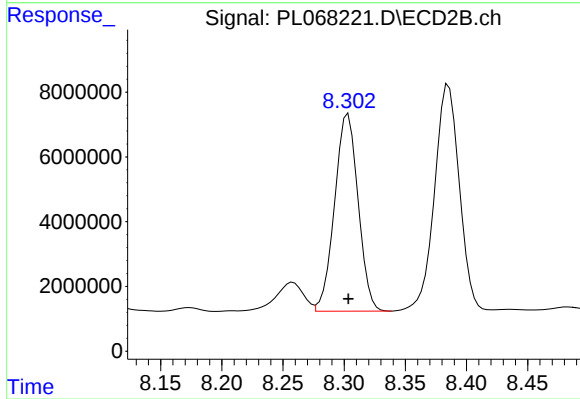

#25 Chlordane-3


R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 81561636
Conc: 500.00 ng/ml

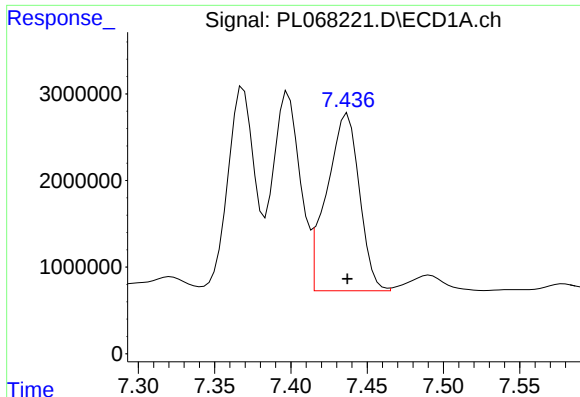

#26 Chlordane-4


R.T.: 7.437 min
Delta R.T.: 0.000 min
Response: 30430340
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

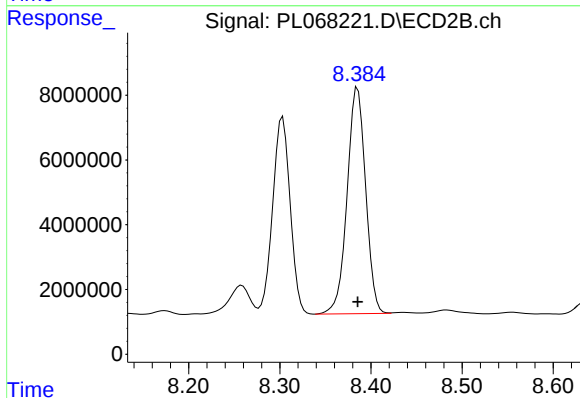


#26 Chlordane-4

R.T.: 8.386 min
Delta R.T.: 0.000 min
Response: 98672637
Conc: 500.00 ng/ml

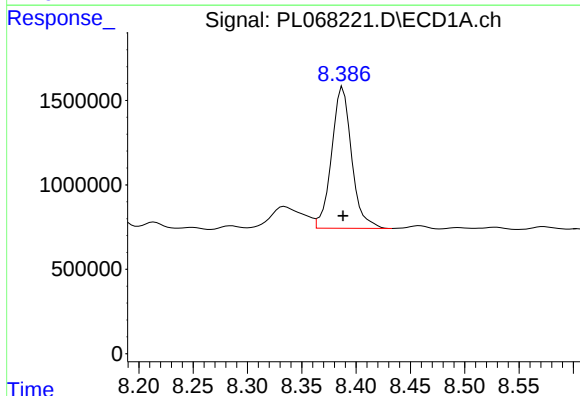


#27 Chlordane-5

R.T.: 8.388 min
Delta R.T.: 0.000 min
Response: 10739892
Conc: 500.00 ng/ml

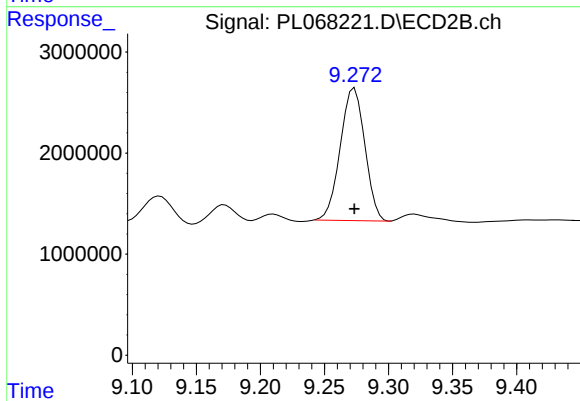

#27 Chlordane-5


R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 17509076
Conc: 500.00 ng/ml

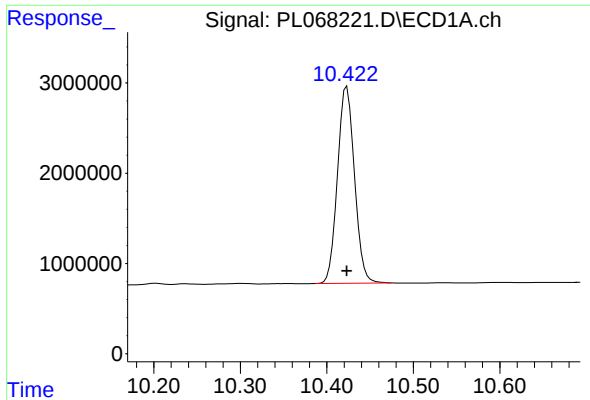

#28 Decachlorobiphenyl

R.T.: 10.423 min
Delta R.T.: 0.000 min
Response: 29631056
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

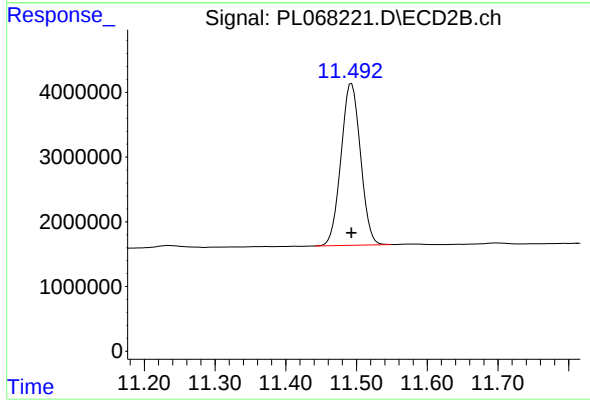

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 47929995
Conc: 50.00 ng/ml