

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
 Data File : PL068230.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2021 23:48
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL071921CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 03:50:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 03:26:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.571	27391294	55142046	63.822	54.038
28)	SA Decachlor...	10.424	11.493	28929598	47296083	51.438	53.023
Target Compounds							
23)	Chlordane-1	5.977	6.955	7841771	19125554	496.772	497.015
24)	Chlordane-2	6.666	7.546	10877969	21928797	492.638	500.015
25)	Chlordane-3	7.369	8.304	28065778	81450630	489.977	499.319
26)	Chlordane-4	7.437	8.386	29752110	98501025	488.856	499.130
27)	Chlordane-5	8.389	9.274	10436677	17438753	485.884	497.992



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
Data File : PL068230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2021 23:48
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL071921CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 03:50:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 03:26:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

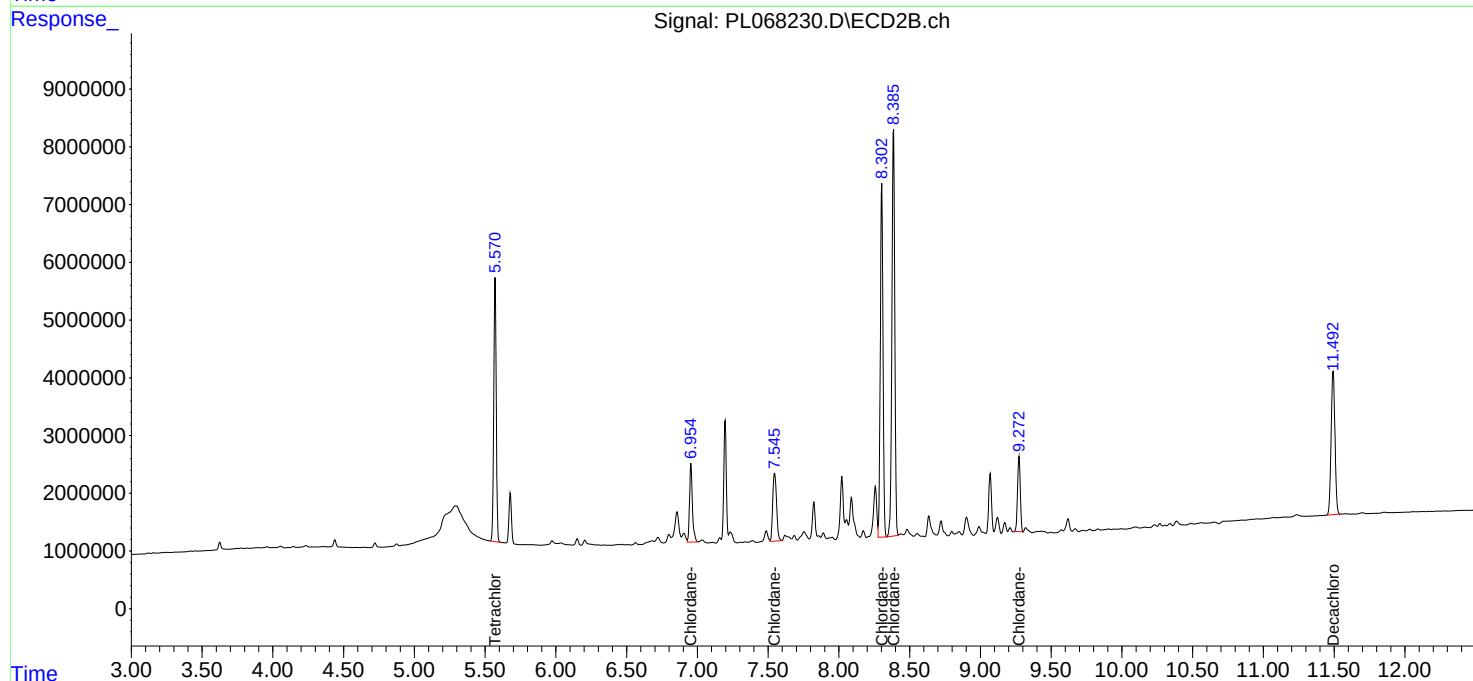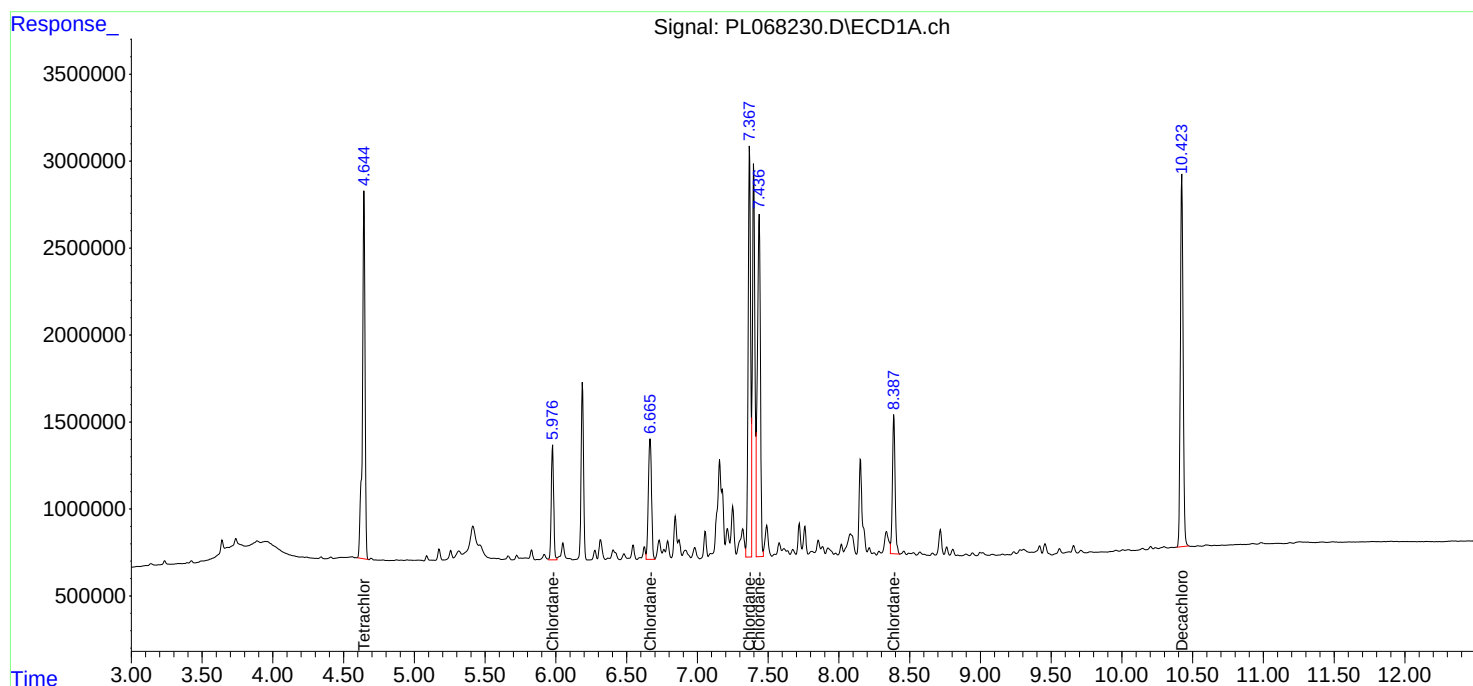


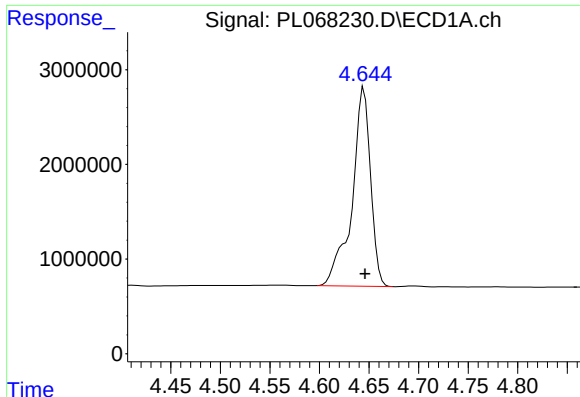

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: -0.001 min
Response: 27391294
Conc: 63.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL071921CHLOR

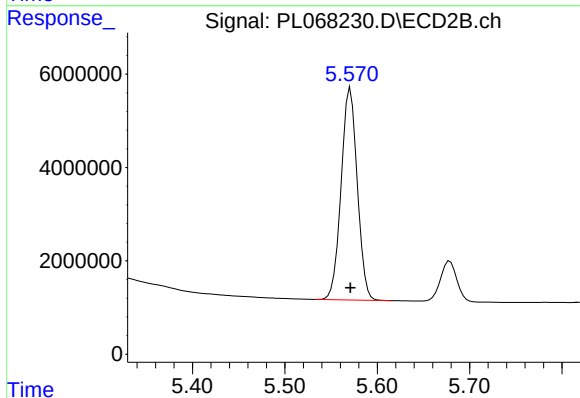


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 55142046
Conc: 54.04 ng/ml

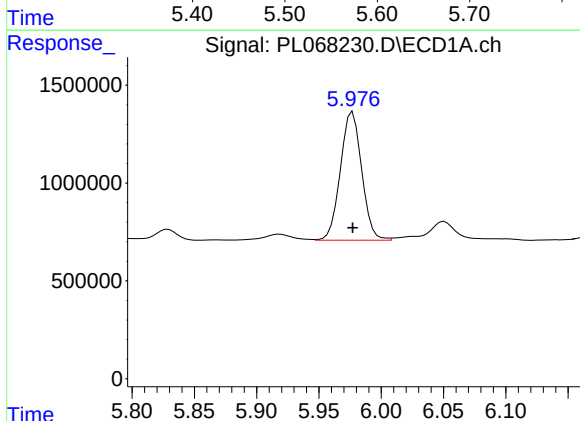


#23 Chlordane-1

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 7841771
Conc: 496.77 ng/ml

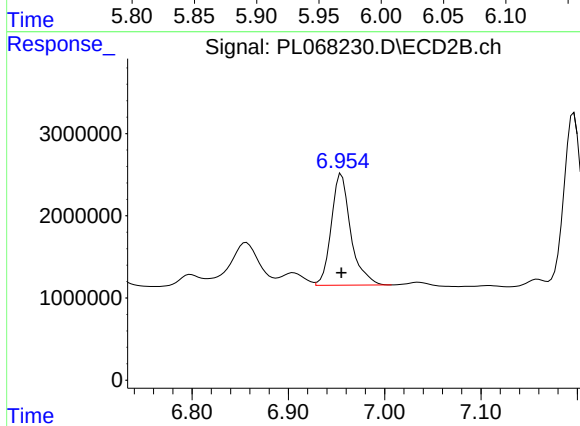

#23 Chlordane-1


R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 19125554
Conc: 497.02 ng/ml

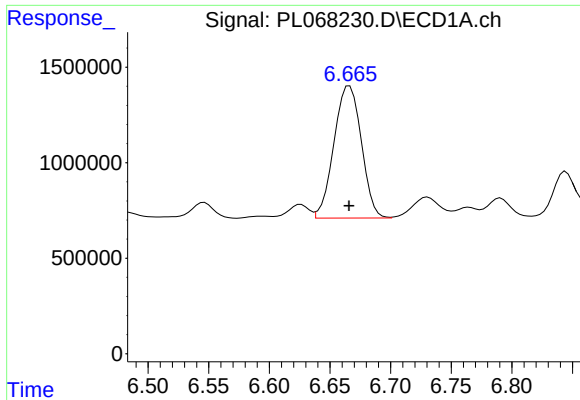

#24 Chlordane-2


R.T.: 6.666 min
Delta R.T.: 0.000 min
Response: 10877969
Conc: 492.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL071921CHLOR

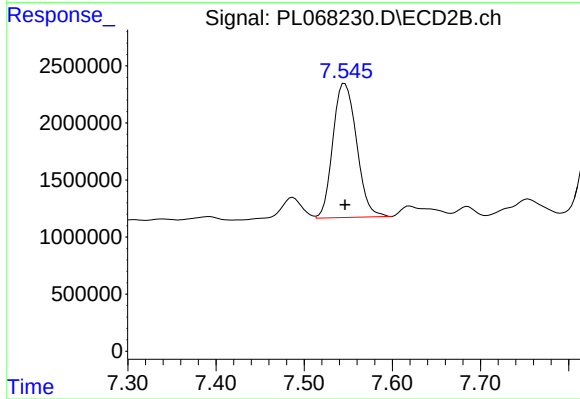


#24 Chlordane-2

R.T.: 7.546 min
Delta R.T.: 0.000 min
Response: 21928797
Conc: 500.01 ng/ml

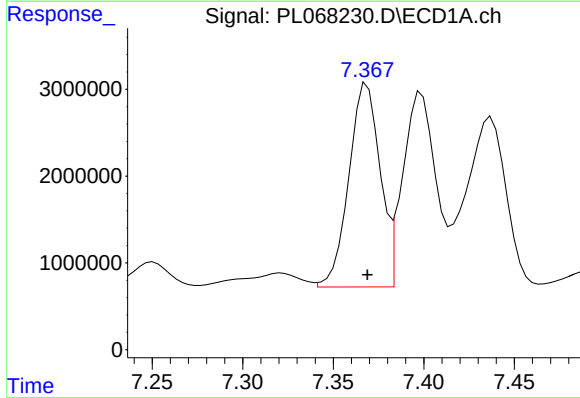


#25 Chlordane-3

R.T.: 7.369 min
Delta R.T.: 0.000 min
Response: 28065778
Conc: 489.98 ng/ml

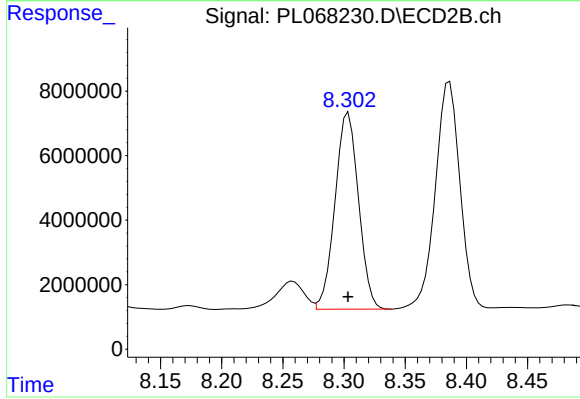

#25 Chlordane-3


R.T.: 8.304 min
Delta R.T.: 0.000 min
Response: 81450630
Conc: 499.32 ng/ml

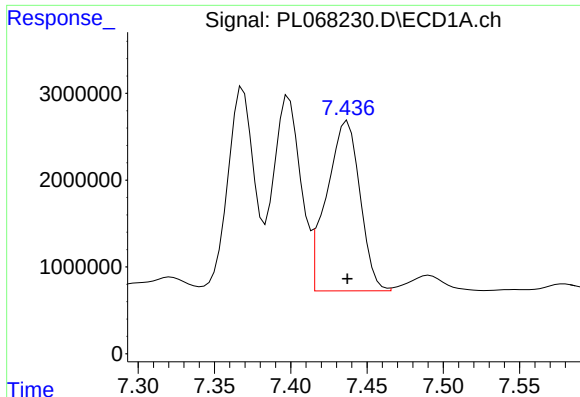

#26 Chlordane-4


R.T.: 7.437 min
Delta R.T.: 0.000 min
Response: 29752110
Conc: 488.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL071921CHLOR

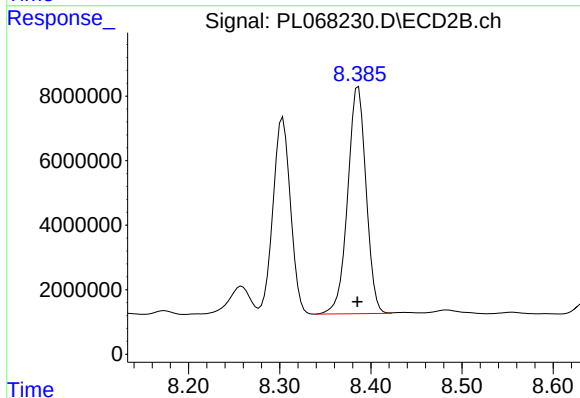


#26 Chlordane-4

R.T.: 8.386 min
Delta R.T.: 0.000 min
Response: 98501025
Conc: 499.13 ng/ml

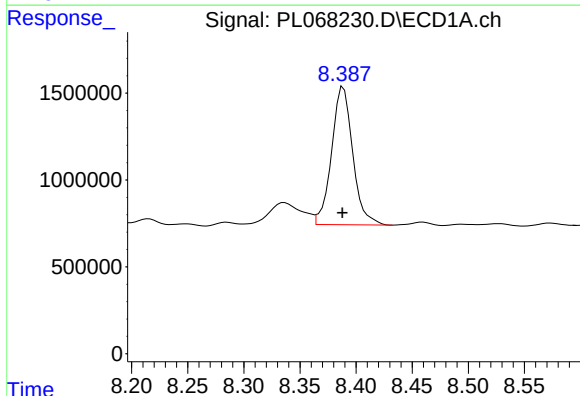


#27 Chlordane-5

R.T.: 8.389 min
Delta R.T.: 0.000 min
Response: 10436677
Conc: 485.88 ng/ml

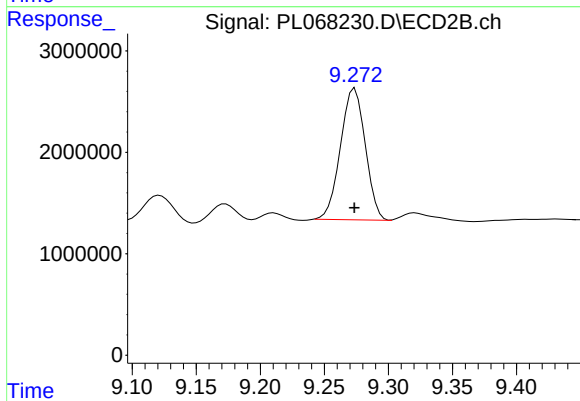

#27 Chlordane-5


R.T.: 9.274 min
Delta R.T.: 0.000 min
Response: 17438753
Conc: 497.99 ng/ml

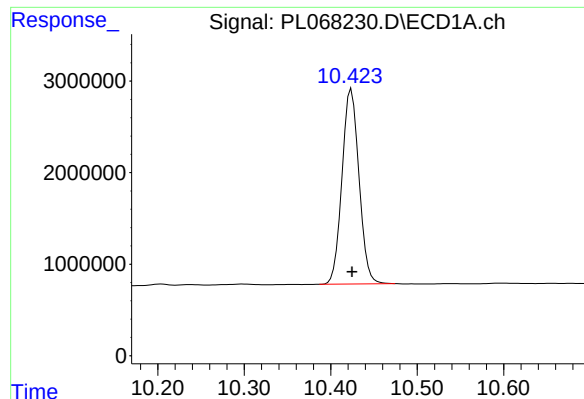

#28 Decachlorobiphenyl

R.T.: 10.424 min
Delta R.T.: 0.000 min
Response: 28929598
Conc: 51.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL071921CHLOR

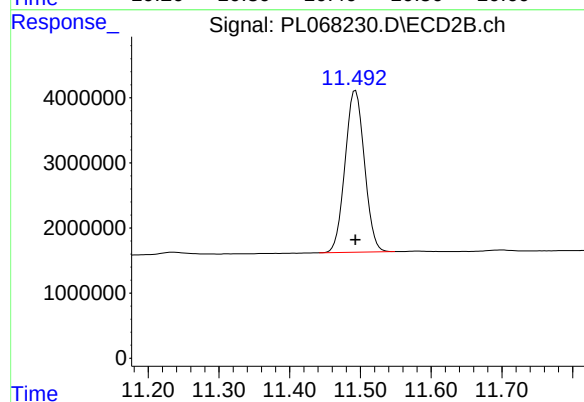

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 47296083
Conc: 53.02 ng/ml