

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
 Data File : PL068240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 02:33
 Operator : AR\AJ
 Sample : M3074-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-071621

Manual Integrations
 APPROVED

Ankita
 7/20/2021 2:59:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 09:58:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 03:26:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.645	5.571	6391198	14309089	14.892	14.023
28) SA Decachlor...	10.425	11.493	7803951	13061708	13.876	14.643
Target Compounds						
10) B gamma-Chl...	7.366	8.302	280682	400376	0.489m	0.356 #
11) B alpha-Chl...	7.436	8.386	306848	869231	0.534m	0.773 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
Data File : PL068240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 02:33
Operator : AR\AJ
Sample : M3074-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleID :
OK-02-071621


Manual Integrations
APPROVED

Ankita
7/20/2021 2:59:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 09:58:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 03:26:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

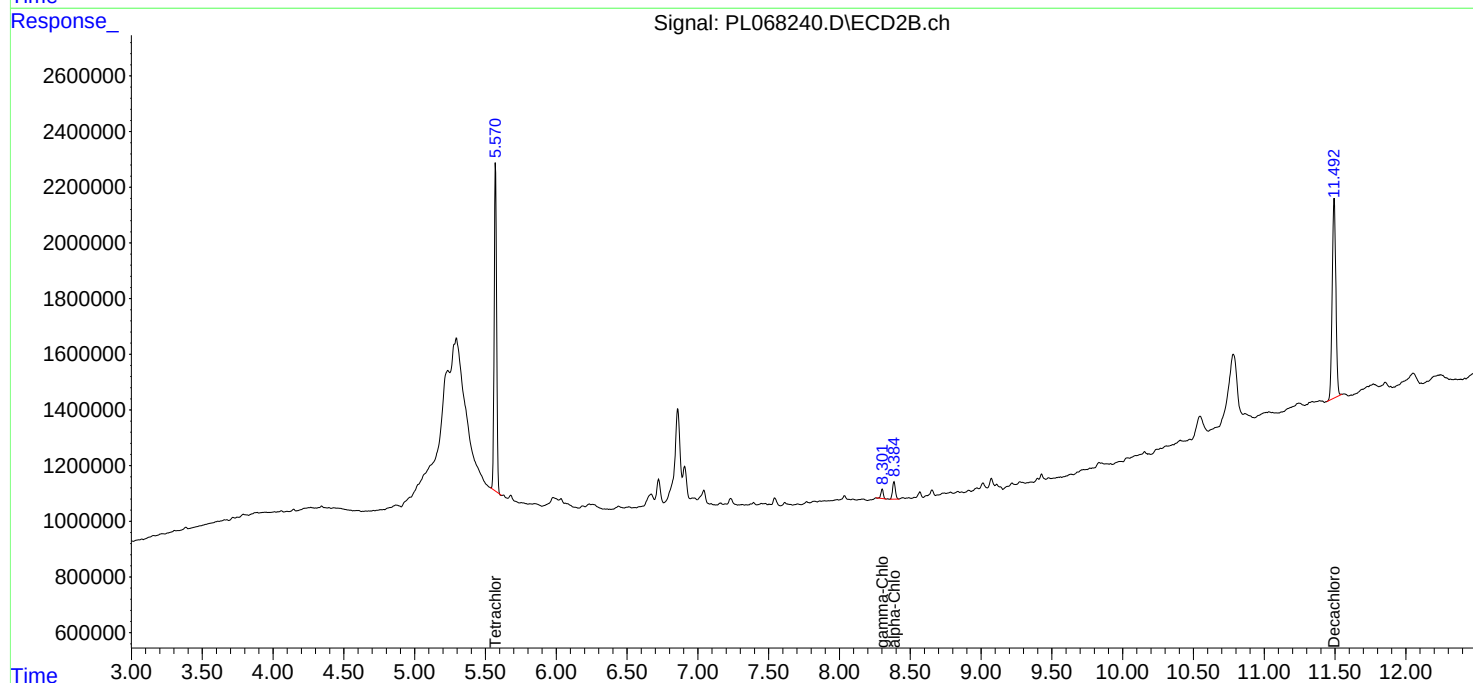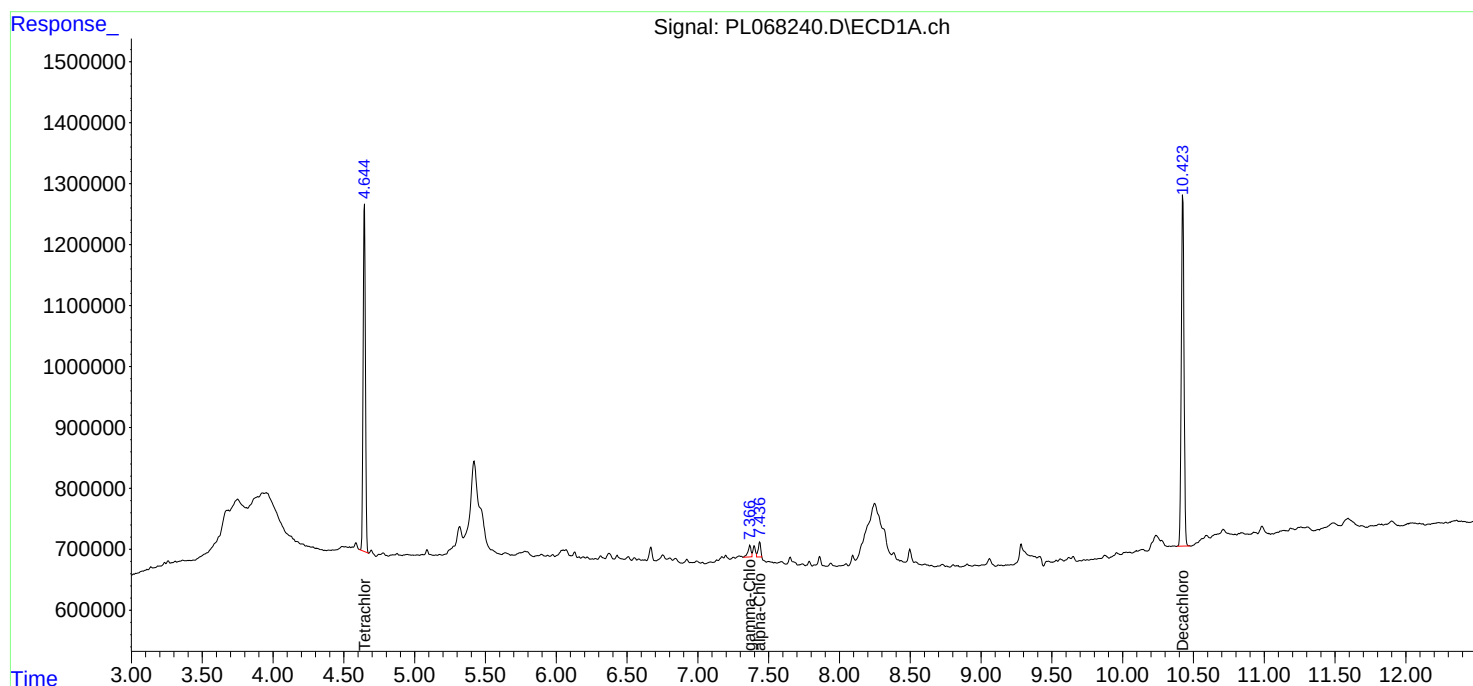

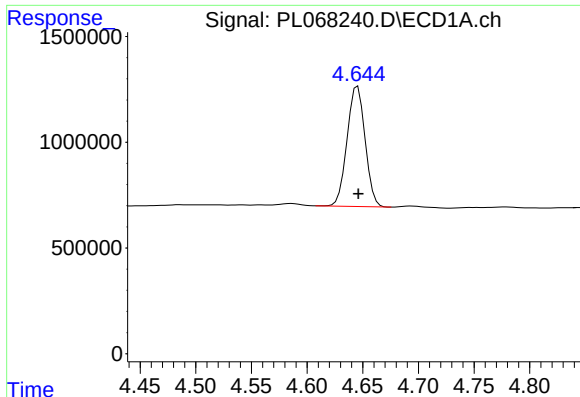


#1 Tetrachloro-m-xylene

R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 6391198
Conc: 14.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-071621


Manual Integrations
APPROVED

Ankita
7/20/2021 2:59:57 PM

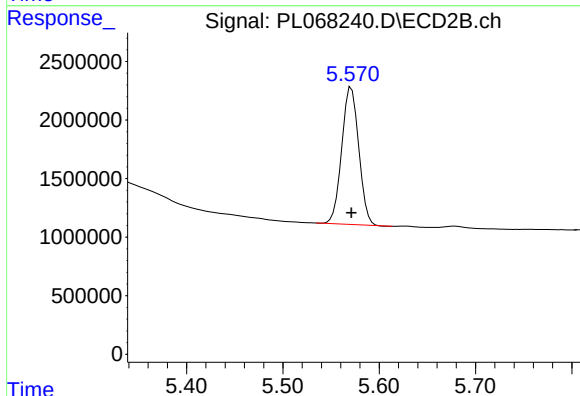


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 14309089
Conc: 14.02 ng/ml

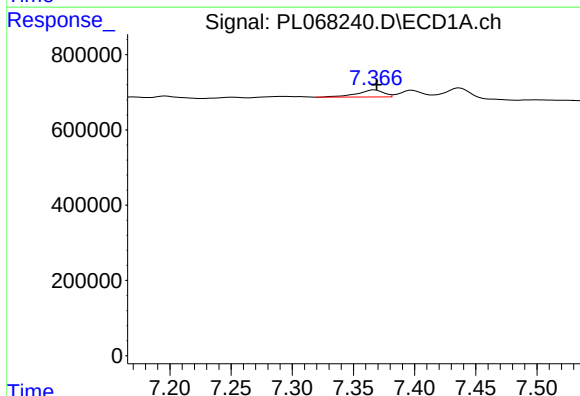


#10 gamma-Chlordane

R.T.: 7.366 min
Delta R.T.: -0.003 min
Response: 280682
Conc: 0.49 ng/ml m

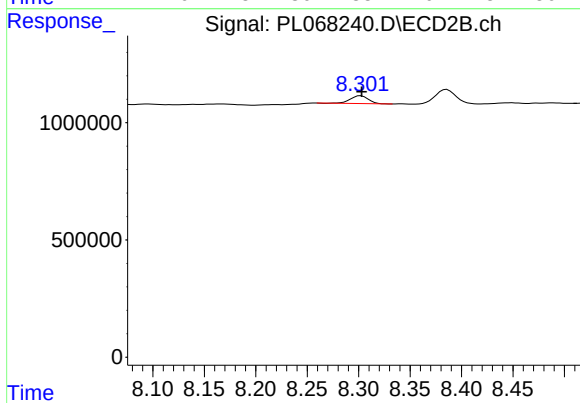

#10 gamma-Chlordane

R.T.: 8.302 min
Delta R.T.: 0.000 min
Response: 400376
Conc: 0.36 ng/ml

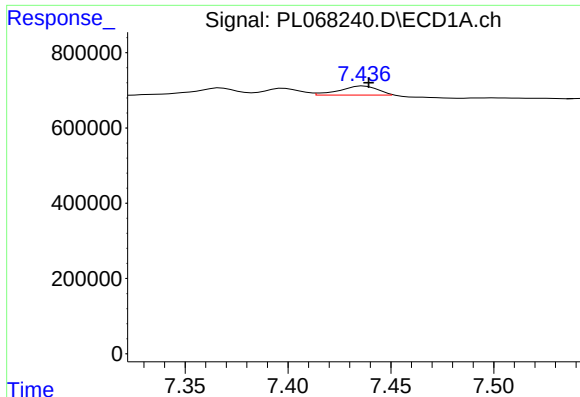


#11 alpha-Chlordane

R.T.: 7.436 min
Delta R.T.: -0.003 min
Response: 306848
Conc: 0.53 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OK-02-071621


Manual Integrations
APPROVED

Ankita
7/20/2021 2:59:57 PM

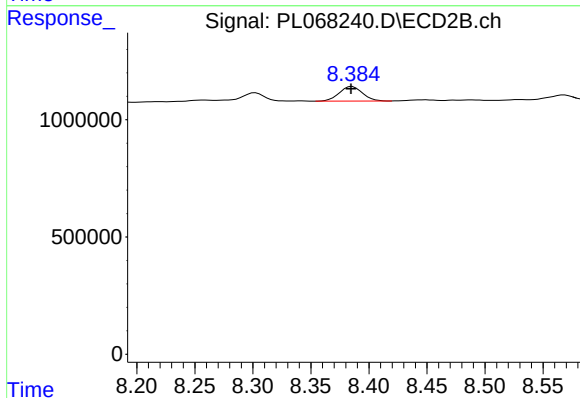


#11 alpha-Chlordane

R.T.: 8.386 min
Delta R.T.: 0.001 min
Response: 869231
Conc: 0.77 ng/ml

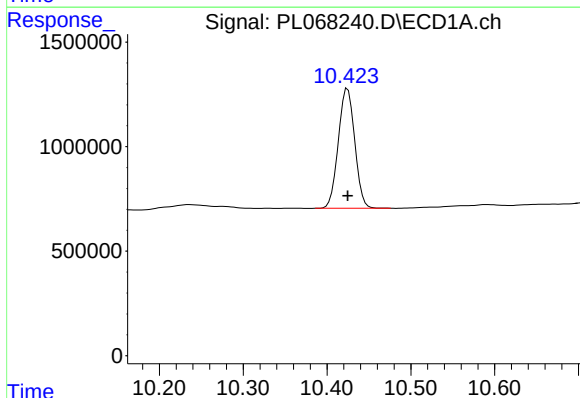

#28 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: 0.000 min
Response: 7803951
Conc: 13.88 ng/ml

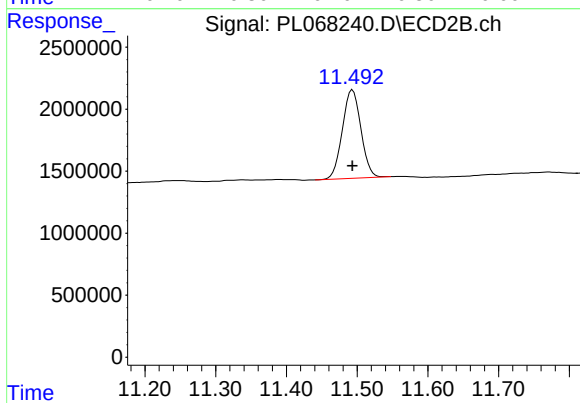

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 13061708
Conc: 14.64 ng/ml