

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
 Data File : PL068253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2021 06:09
 Operator : AR\AJ
 Sample : M3065-01RE 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-071521

Manual Integrations
 APPROVED

mohammad
 7/20/2021 10:06:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 07:23:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 03:26:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.644	5.569	1133274	2072614	2.641	2.031m
28) SA Decachlor...	10.423	11.490	1466716	3135500	2.608	3.515m#
Target Compounds						
16) A 4,4'-DDD	8.229	9.105	419878	1760596	0.940m	2.068 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071921\
Data File : PL068253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2021 06:09
Operator : AR\AJ
Sample : M3065-01RE 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TR-04-071521


Manual Integrations
APPROVED

mohammad
7/20/2021 10:06:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 07:23:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 03:26:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

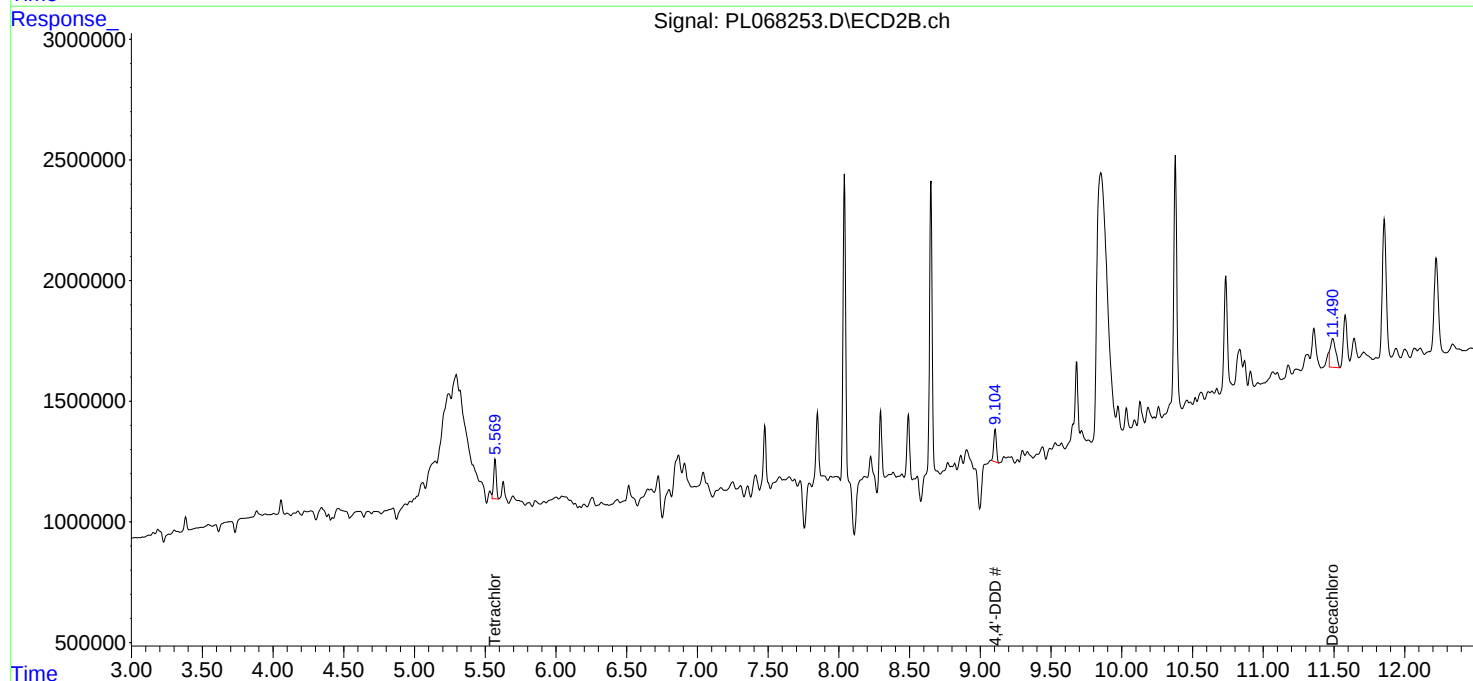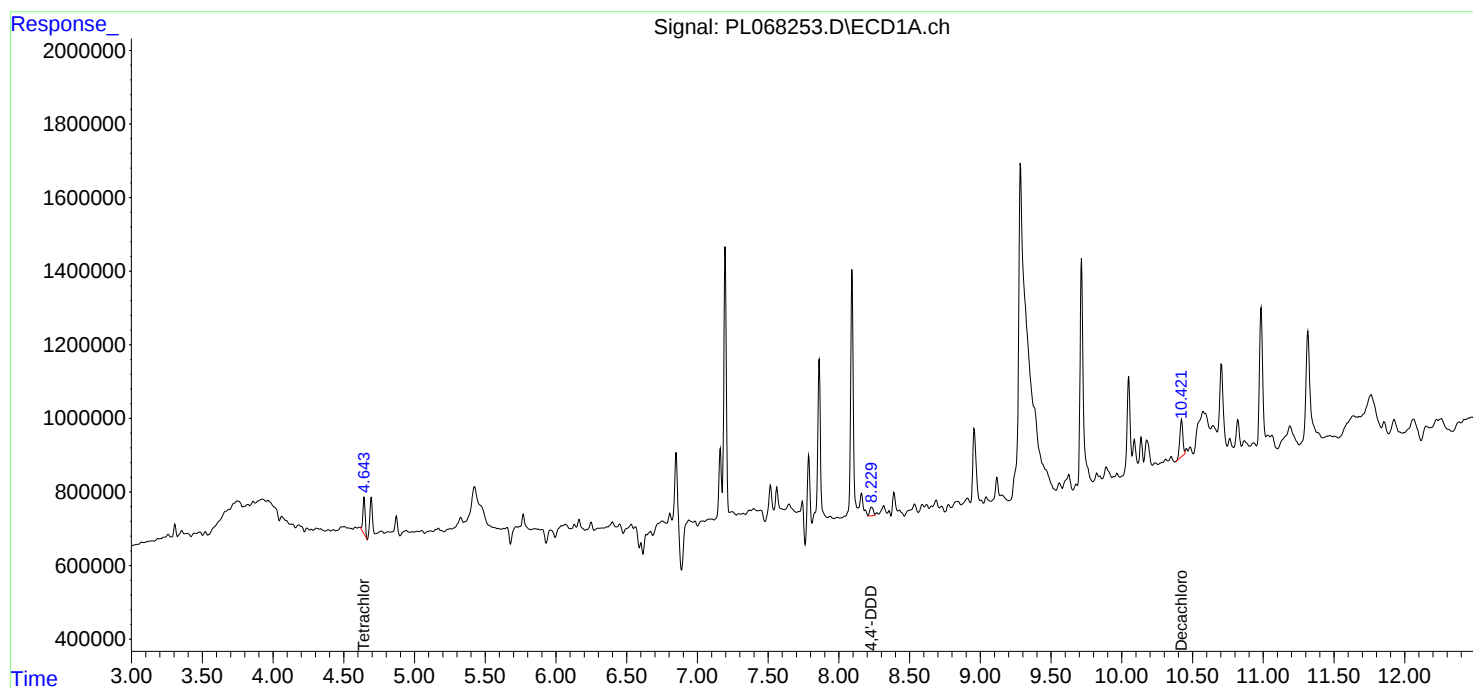

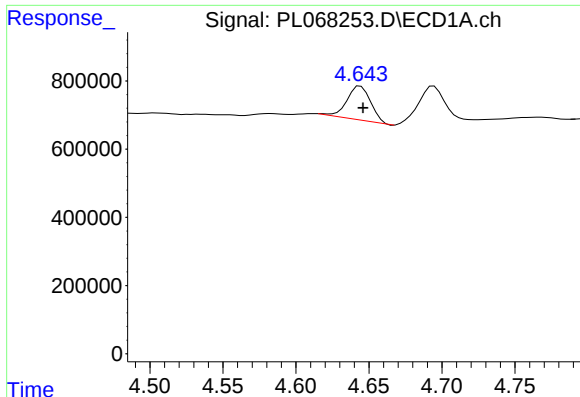


#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: -0.002 min
Response: 1133274
Conc: 2.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-071521


Manual Integrations
APPROVED

mohammad
7/20/2021 10:06:47 AM

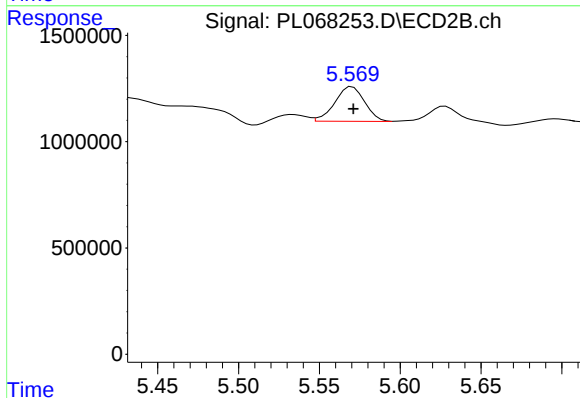


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 2072614
Conc: 2.03 ng/ml m

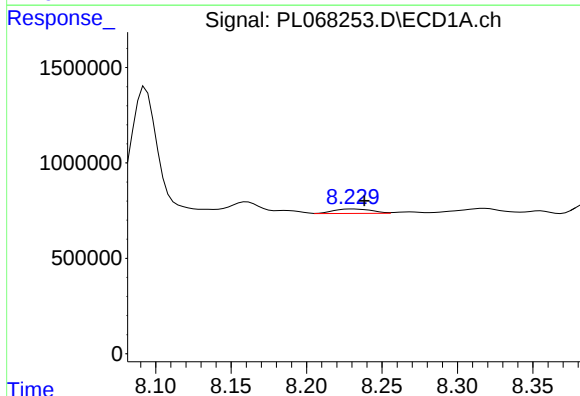


#16 4,4'-DDD

R.T.: 8.229 min
Delta R.T.: -0.010 min
Response: 419878
Conc: 0.94 ng/ml m

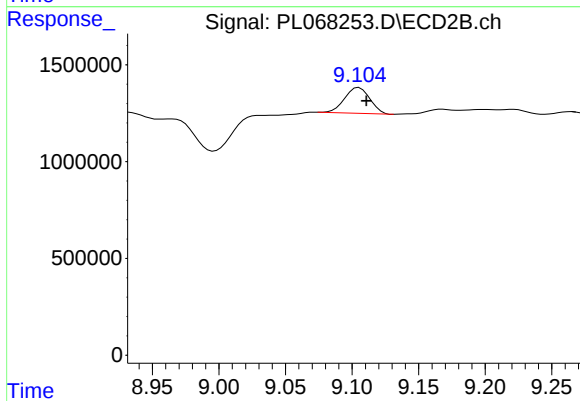

#16 4,4'-DDD

R.T.: 9.105 min
Delta R.T.: -0.006 min
Response: 1760596
Conc: 2.07 ng/ml

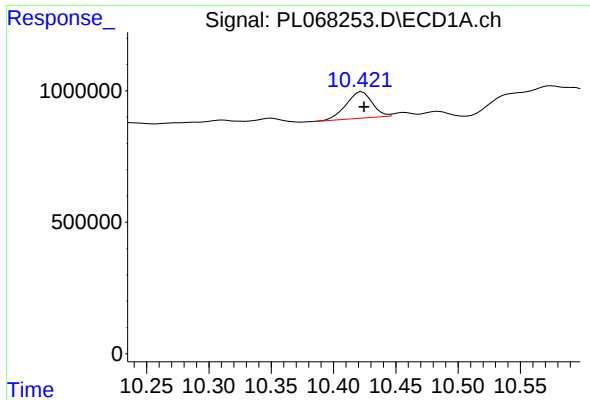


#28 Decachlorobiphenyl

R.T.: 10.423 min
Delta R.T.: -0.002 min
Response: 1466716
Conc: 2.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-071521

Manual Integrations
APPROVED

mohammad
7/20/2021 10:06:47 AM

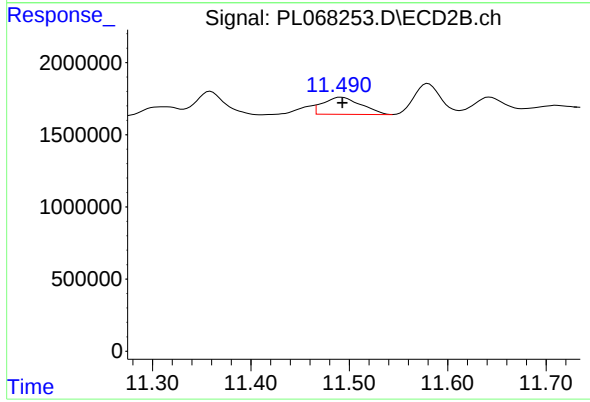

#28 Decachlorobiphenyl

R.T.: 11.490 min
Delta R.T.: -0.003 min
Response: 3135500
Conc: 3.52 ng/ml m