

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072020\
 Data File : PL060018.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2020 10:15
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 16:41:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	0.000	5.202	0	32409787	N.D.	9.634 #
9) A	Endosulfan I	0.000	6.232f	0	1577225	N.D.	0.591 #
15) B	Endosulfa...	6.305	0.000	2682635	0	1.606	N.D. #
17) MA	4,4'-DDT	0.000	7.125f	0	8150019	N.D.	4.139 #
18) B	Endrin al...	6.469	7.076f	4331810	1121745	3.037	0.516 #
24)	Chlordane-2	0.000	5.468	0	20106696	N.D.	175.489 #
26)	Chlordane-4	0.000	6.232f	0	1577225	N.D.	3.407 #
27)	Chlordane-5	6.305	7.000	2682635	2833484	47.279	36.483



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072020\
Data File : PL060018.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2020 10:15
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 16:41:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

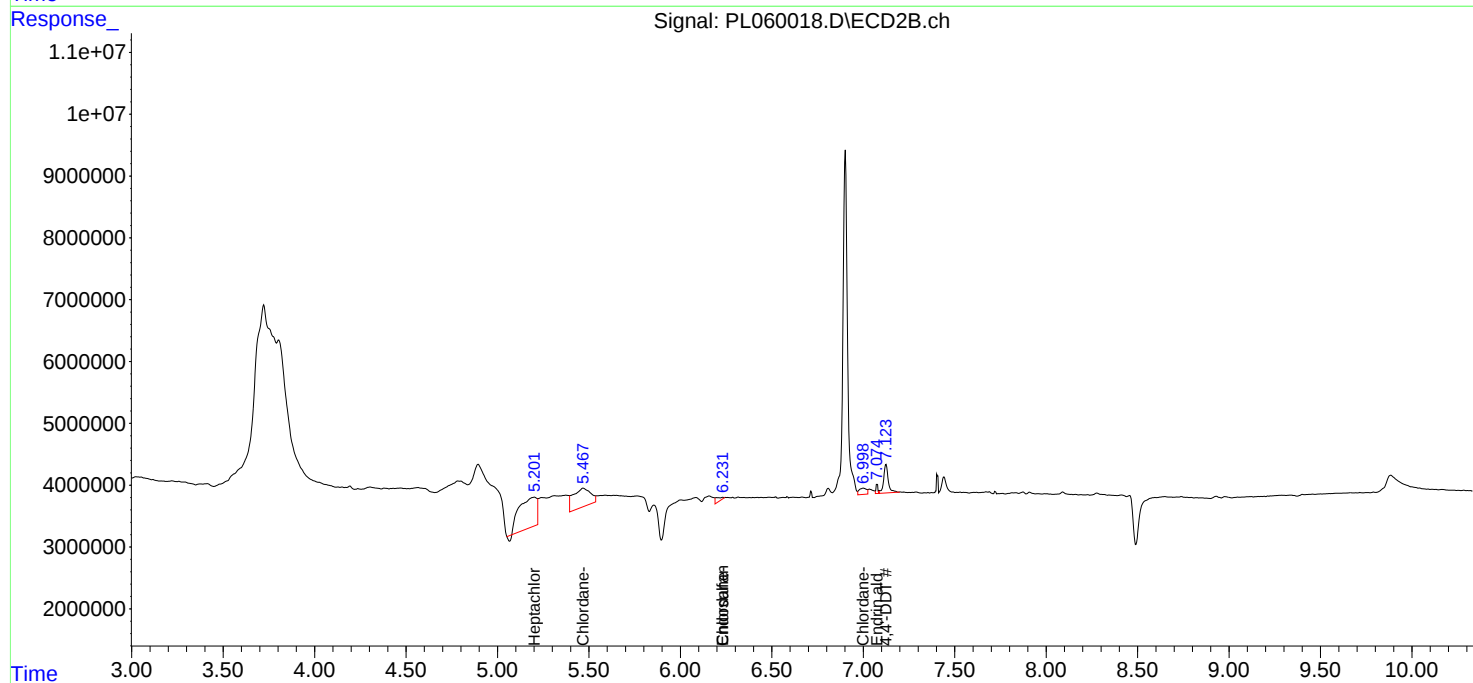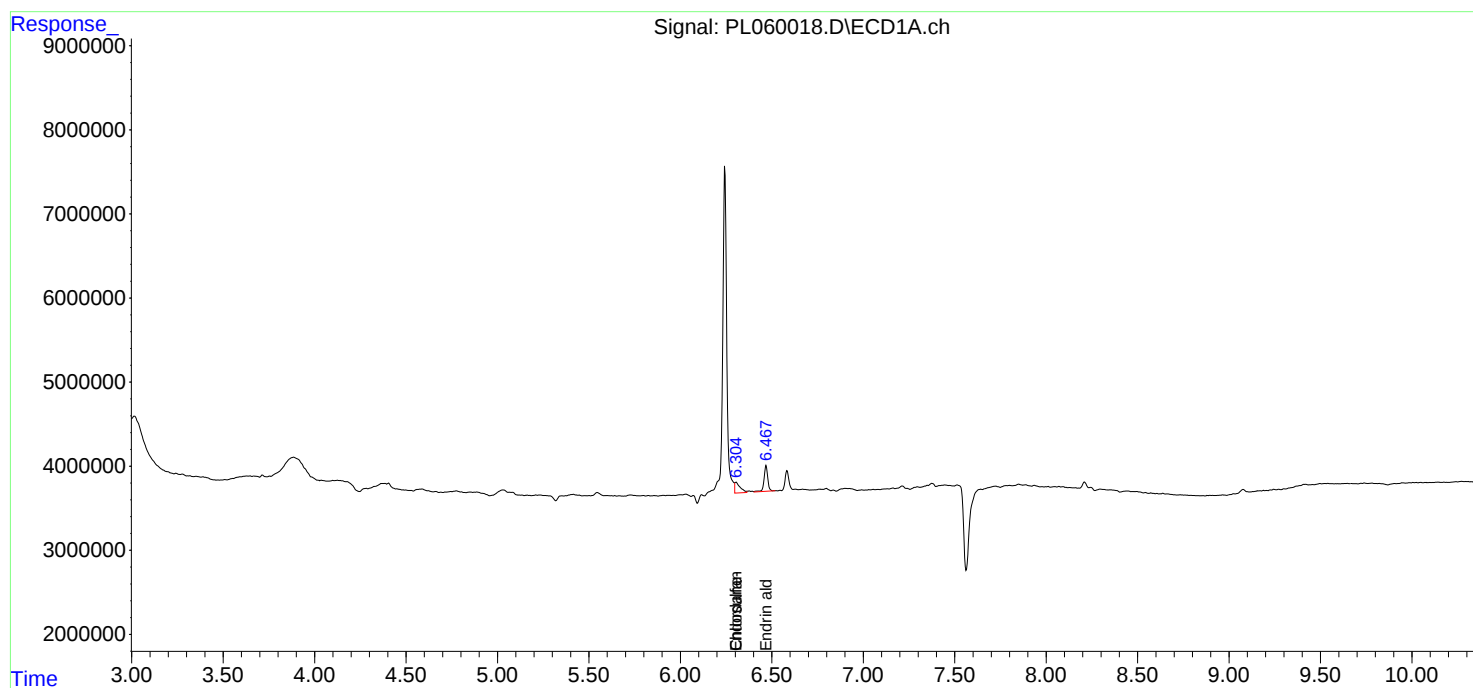


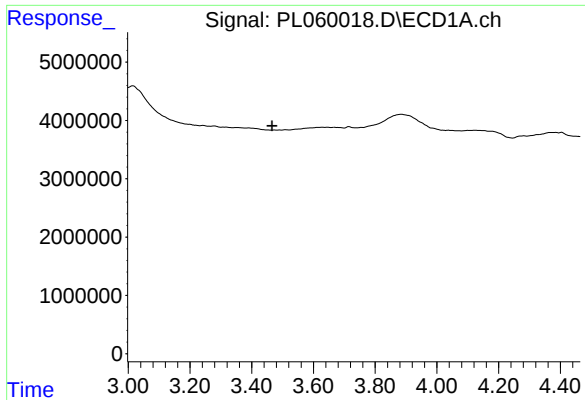

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.466 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

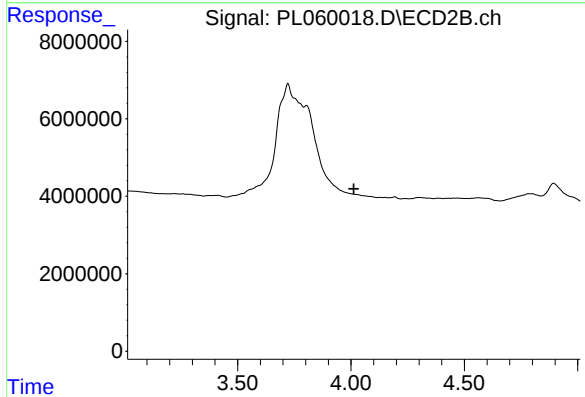


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.012 min
Response: 0
Conc: N.D.

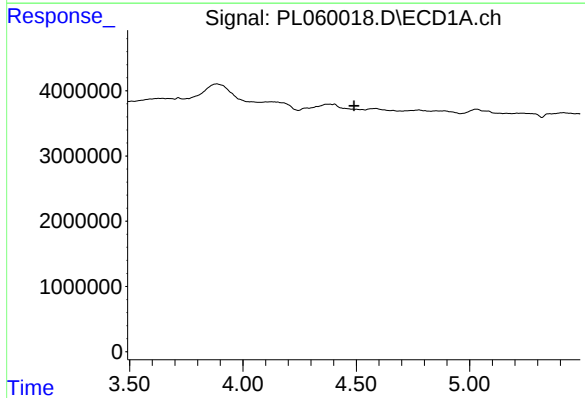


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

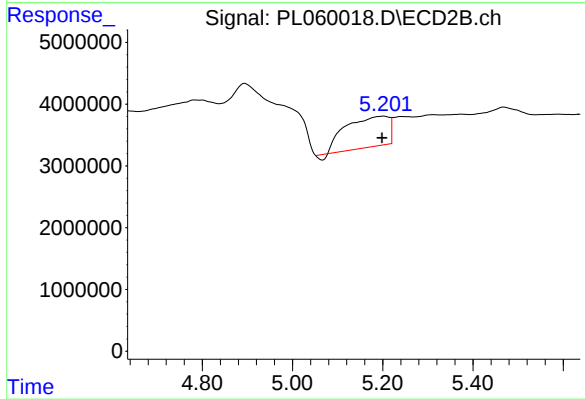

#4 Heptachlor


R.T.: 5.202 min
Delta R.T.: 0.004 min
Response: 32409787
Conc: 9.63 ng/ml

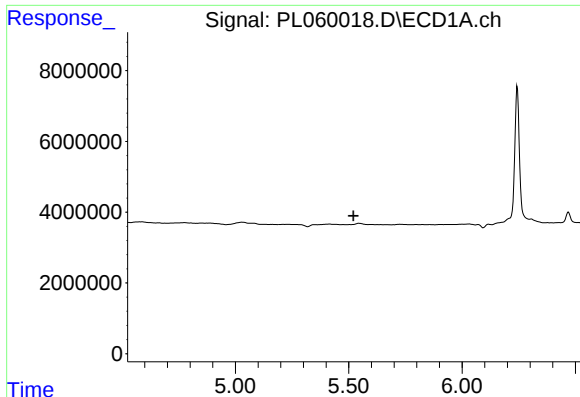

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

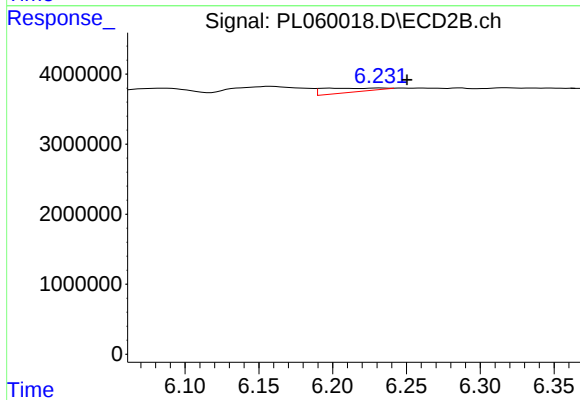


#9 Endosulfan I

R.T.: 6.232 min
Delta R.T.: -0.018 min
Response: 1577225
Conc: 0.59 ng/ml

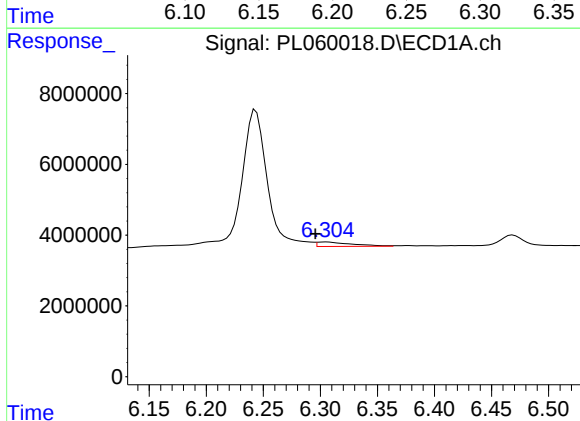


#15 Endosulfan II

R.T.: 6.305 min
Delta R.T.: 0.010 min
Response: 2682635
Conc: 1.61 ng/ml

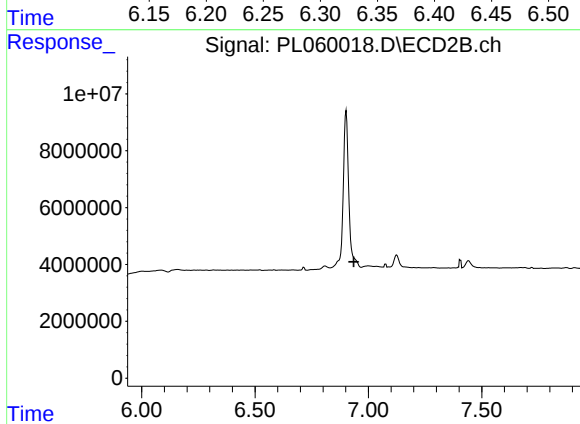

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.936 min
Response: 0
Conc: N.D.

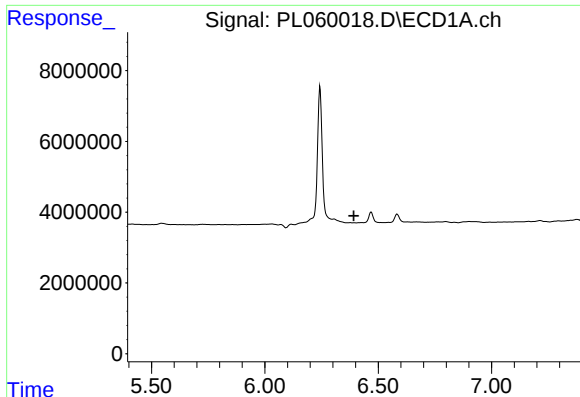

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

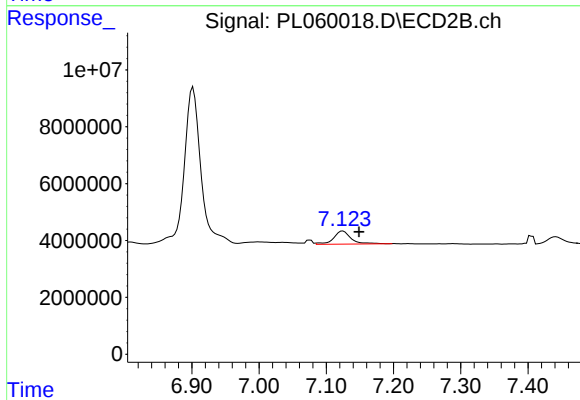


#17 4,4'-DDT

R.T.: 7.125 min
Delta R.T.: -0.024 min
Response: 8150019
Conc: 4.14 ng/ml

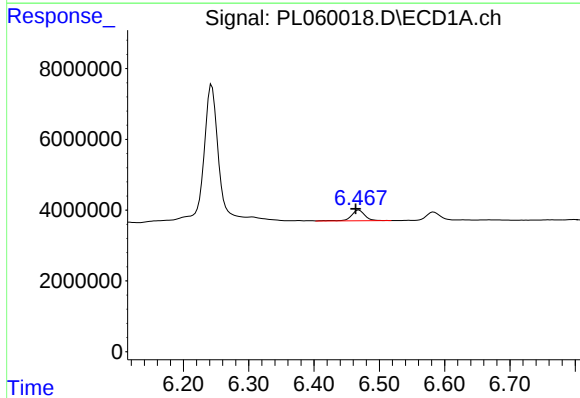


#18 Endrin aldehyde

R.T.: 6.469 min
Delta R.T.: 0.005 min
Response: 4331810
Conc: 3.04 ng/ml

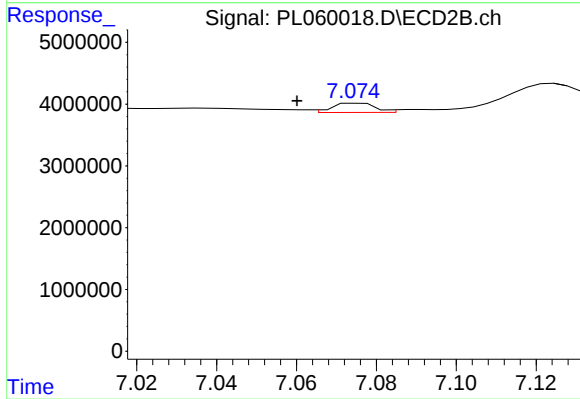

#18 Endrin aldehyde


R.T.: 7.076 min
Delta R.T.: 0.016 min
Response: 1121745
Conc: 0.52 ng/ml

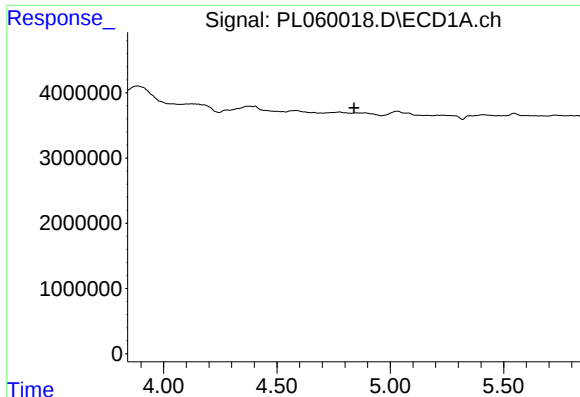

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.840 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

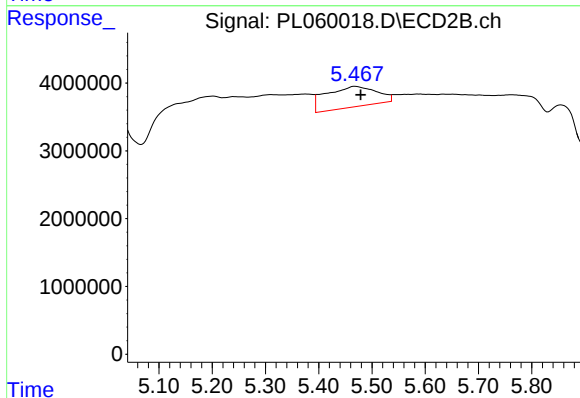


#24 Chlordane-2

R.T.: 5.468 min
Delta R.T.: -0.011 min
Response: 20106696
Conc: 175.49 ng/ml

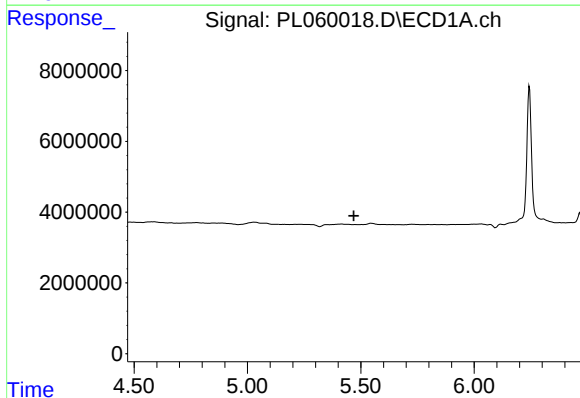


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

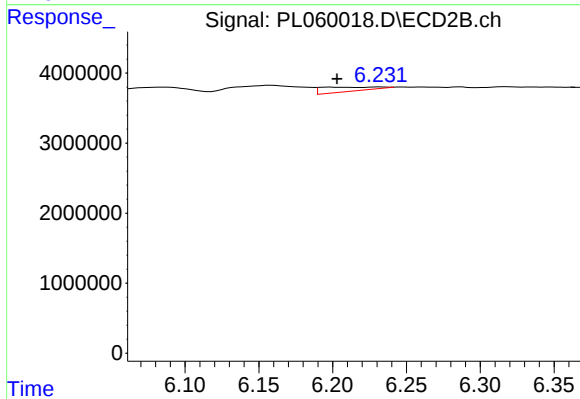

#26 Chlordane-4


R.T.: 6.232 min
Delta R.T.: 0.029 min
Response: 1577225
Conc: 3.41 ng/ml

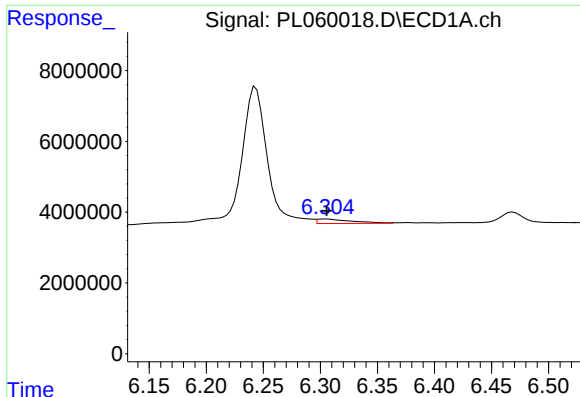

#27 Chlordane-5


R.T.: 6.305 min
Delta R.T.: 0.000 min
Response: 2682635
Conc: 47.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

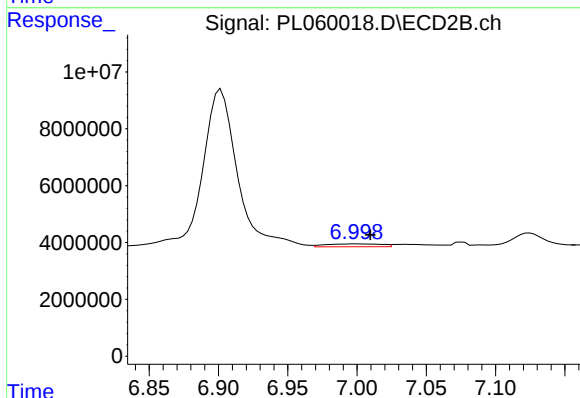


#27 Chlordane-5

R.T.: 7.000 min
Delta R.T.: -0.010 min
Response: 2833484
Conc: 36.48 ng/ml

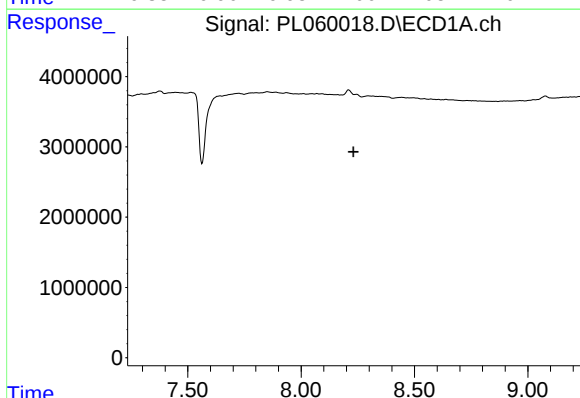

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.231 min
Response: 0
Conc: N.D.

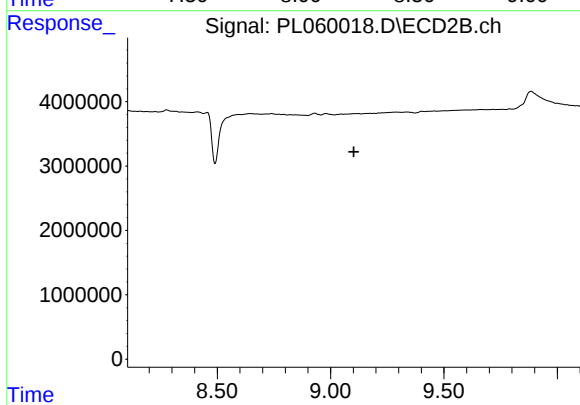

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.103 min
Response: 0
Conc: N.D.