

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072020\
 Data File : PL060022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2020 12:38
 Operator : DD\AJ
 Sample : PB130295BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 16:45:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.012	41411630	57986714	21.410	21.880
28)	SA Decachlor...	8.228	9.104	36503892	35694142	22.190	17.067
Target Compounds							
4)	MA Heptachlor	0.000	5.201	0	5488837	N.D.	1.632 #
9)	A Endosulfan I	0.000	6.250	0	1698024	N.D.	0.637 #
10)	B gamma-Chl...	0.000	6.099f	0	3662601	N.D.	1.279 #
18)	B Endrin al...	6.470	0.000	1069323	0	0.750	N.D. #
25)	Chlordane-3	0.000	6.099f	0	3662601	N.D.	9.466 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072020\
Data File : PL060022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2020 12:38
Operator : DD\AJ
Sample : PB130295BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 16:45:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

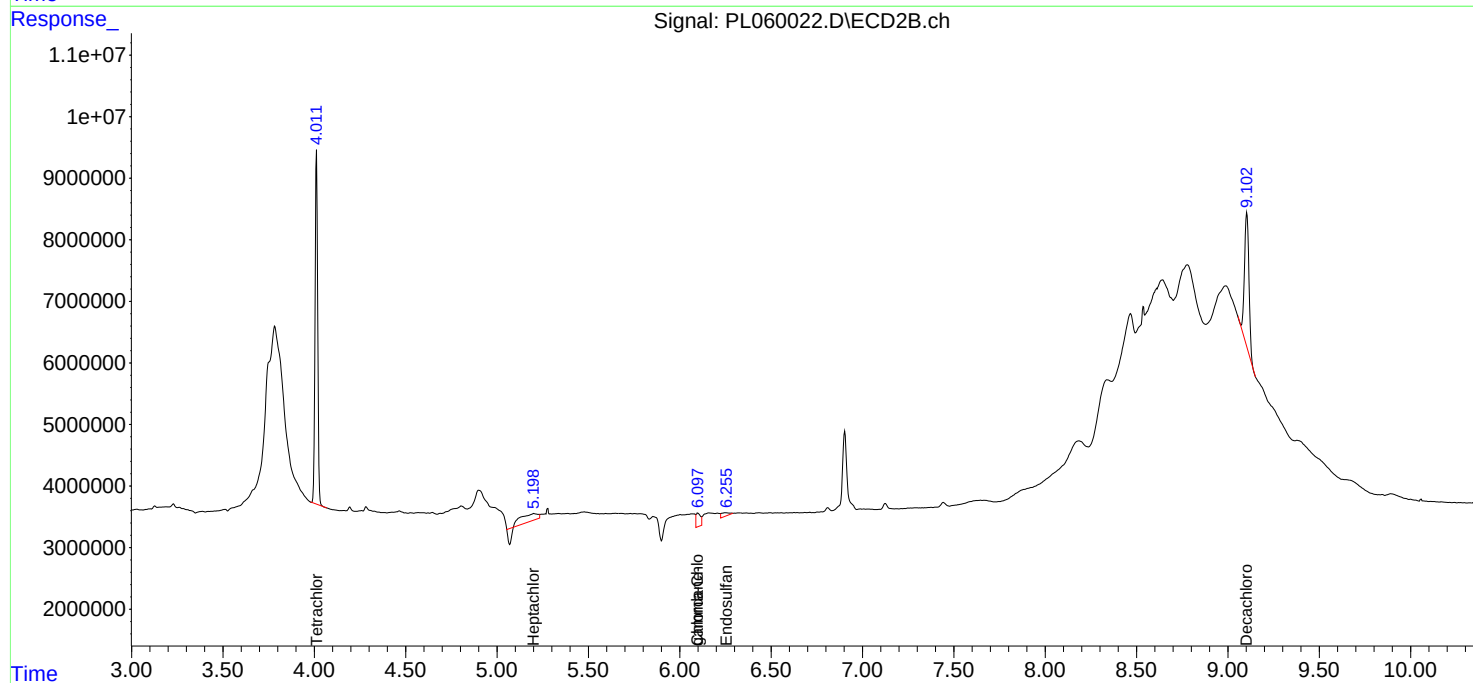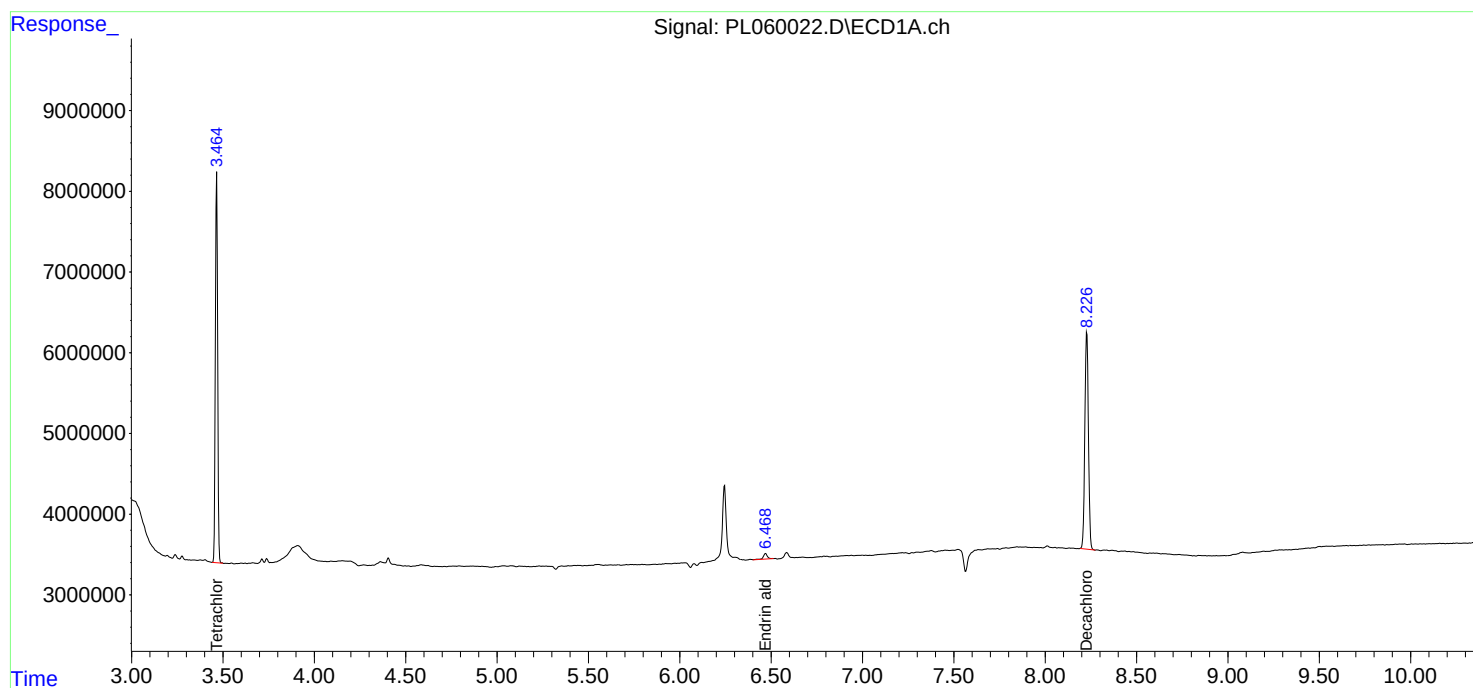


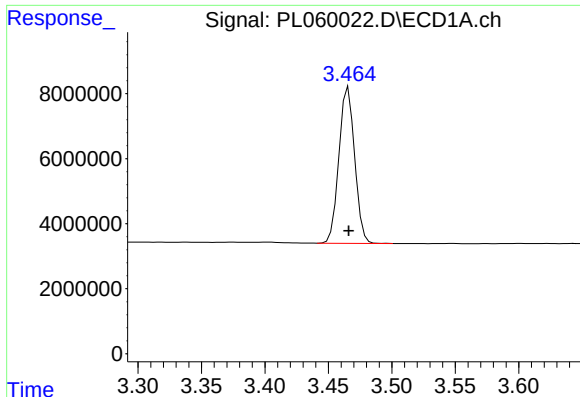

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 41411630
Conc: 21.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

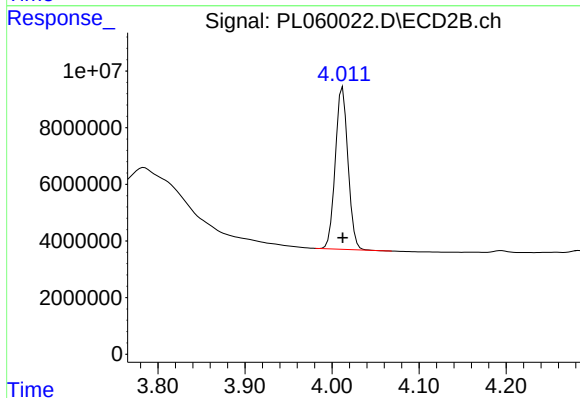


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 57986714
Conc: 21.88 ng/ml

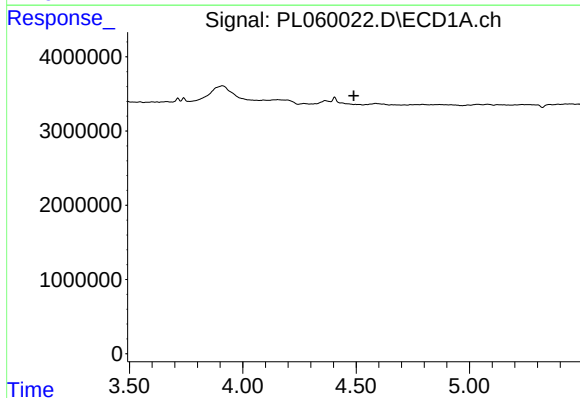


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

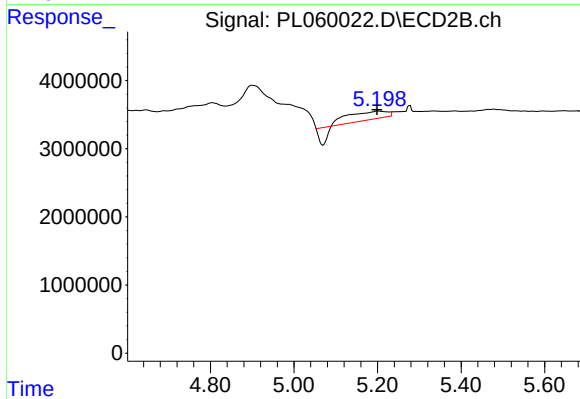

#4 Heptachlor


R.T.: 5.201 min
Delta R.T.: 0.003 min
Response: 5488837
Conc: 1.63 ng/ml

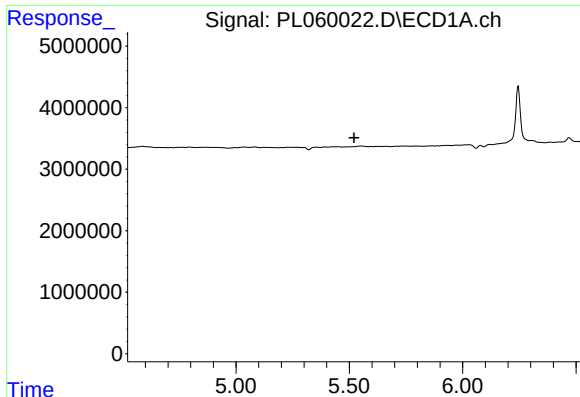

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

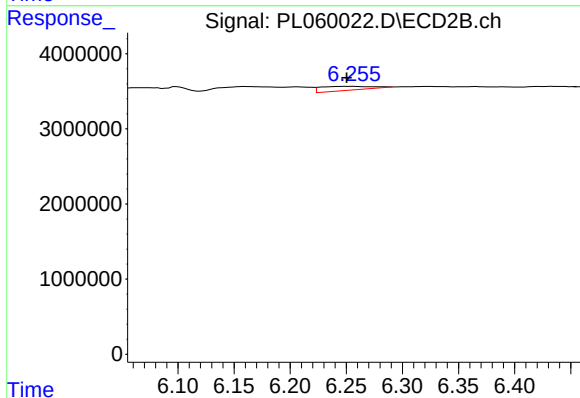


#9 Endosulfan I

R.T.: 6.250 min
Delta R.T.: 0.000 min
Response: 1698024
Conc: 0.64 ng/ml

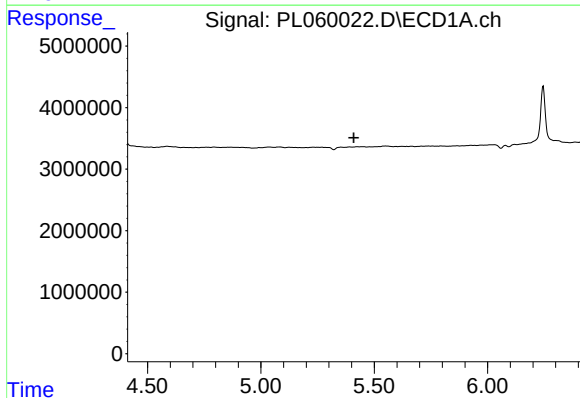


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.410 min
Response: 0
Conc: N.D.

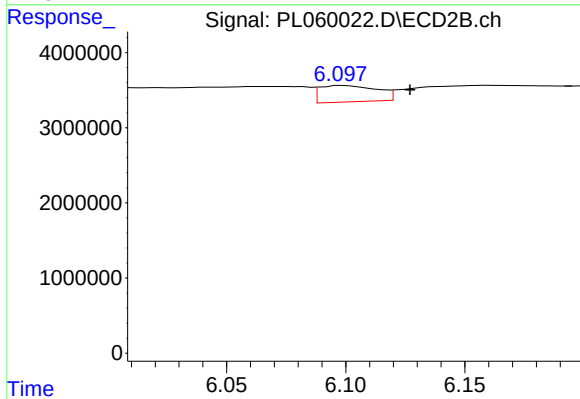

#10 gamma-Chlordane


R.T.: 6.099 min
Delta R.T.: -0.028 min
Response: 3662601
Conc: 1.28 ng/ml

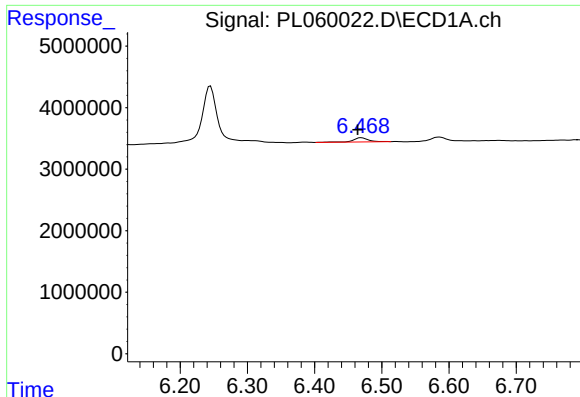

#18 Endrin aldehyde


R.T.: 6.470 min
Delta R.T.: 0.006 min
Response: 1069323
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

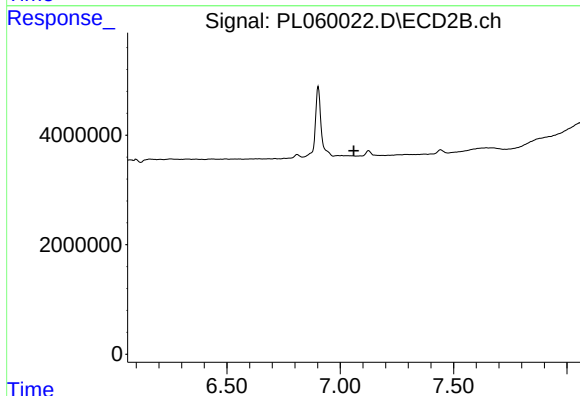


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

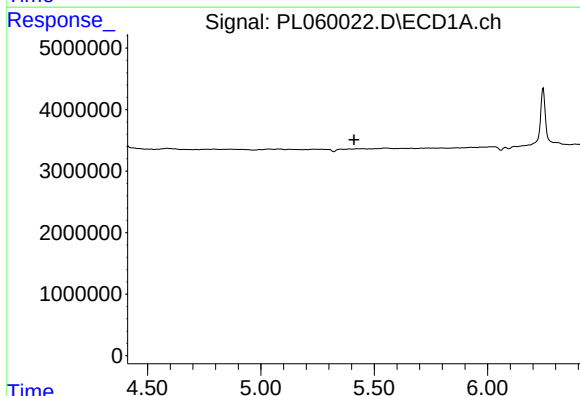


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.411 min
Response: 0
Conc: N.D.

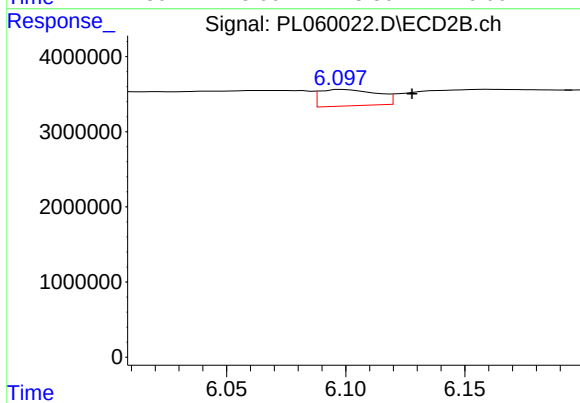

#25 Chlordane-3


R.T.: 6.099 min
Delta R.T.: -0.029 min
Response: 3662601
Conc: 9.47 ng/ml

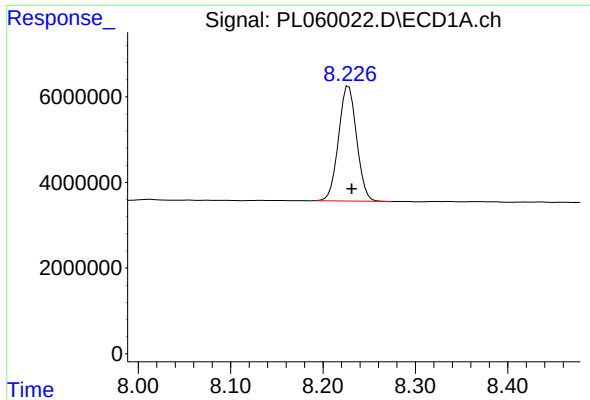

#28 Decachlorobiphenyl

R.T.: 8.228 min
Delta R.T.: -0.003 min
Response: 36503892
Conc: 22.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

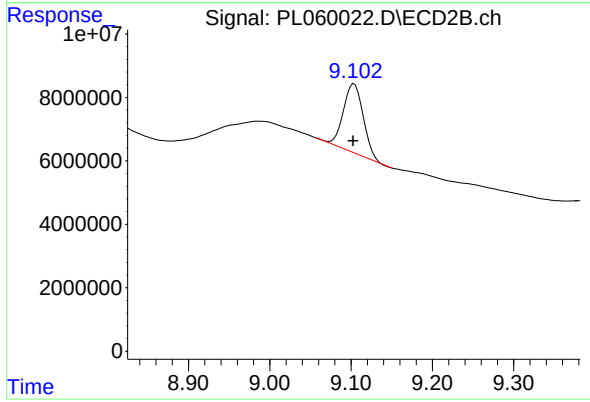

#28 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: 0.000 min
Response: 35694142
Conc: 17.07 ng/ml