

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072020\
 Data File : PL060033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2020 15:17
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 16:57:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.011	39988458	55380633	20.674	20.897
28)	SA Decachlor...	8.225	9.101	32523025	41044999	19.770	19.626
Target Compounds							
4)	MA Heptachlor	0.000	5.199	0	5691129	N.D.	1.692 #
9)	A Endosulfan I	0.000	6.238	0	1199346	N.D.	0.450 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072020\
Data File : PL060033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2020 15:17
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 16:57:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

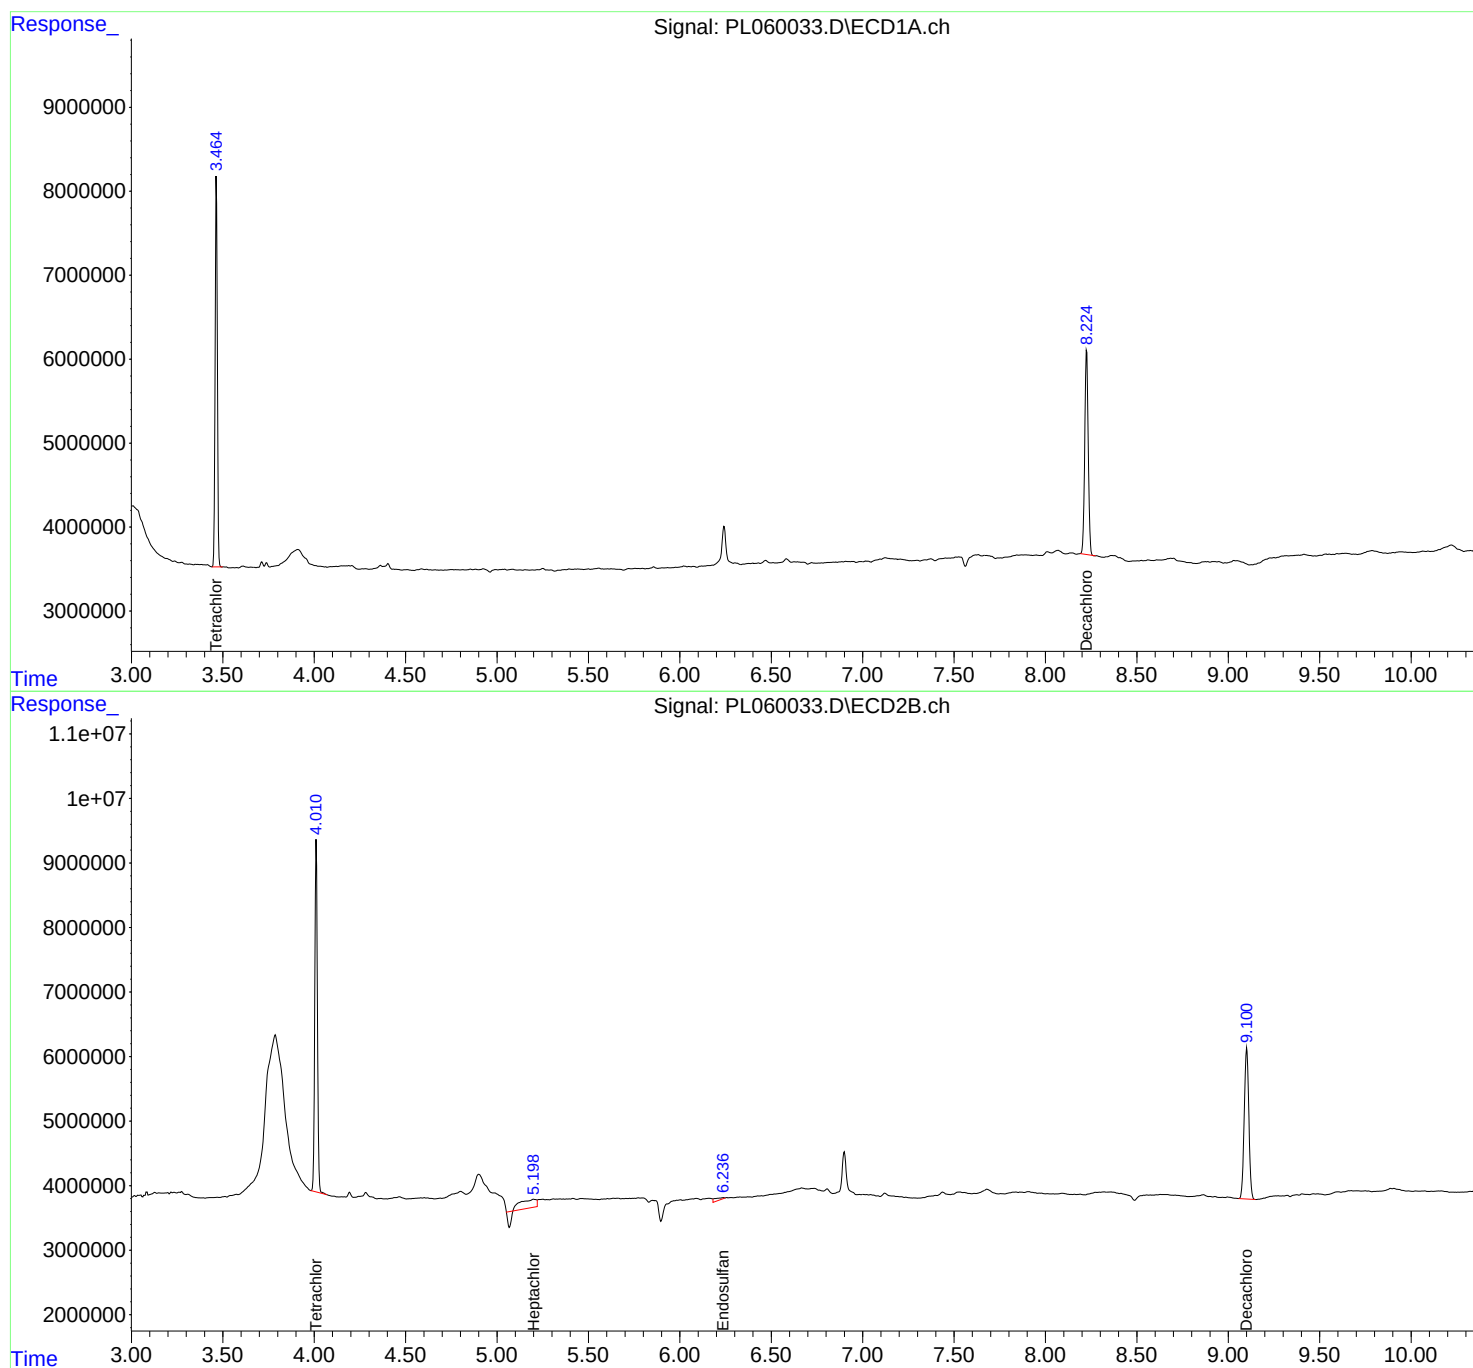


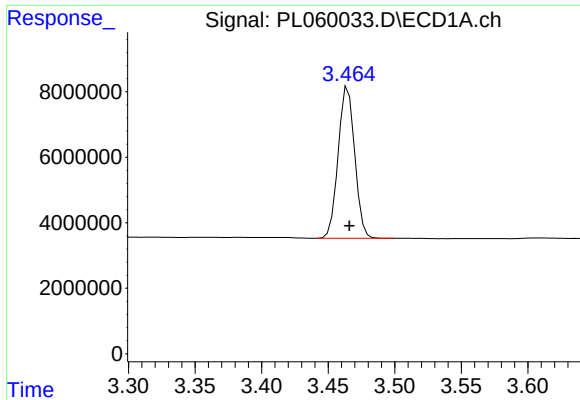

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: -0.001 min
Response: 39988458
Conc: 20.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

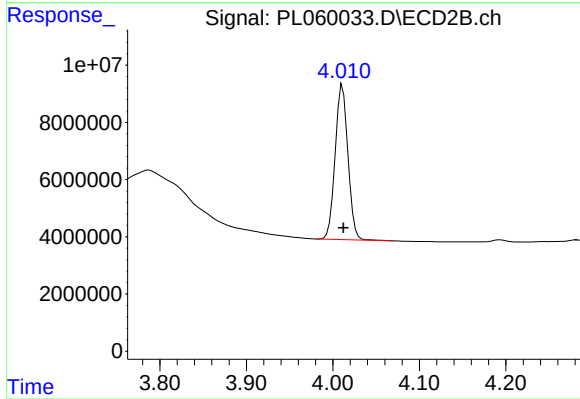


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.001 min
Response: 55380633
Conc: 20.90 ng/ml

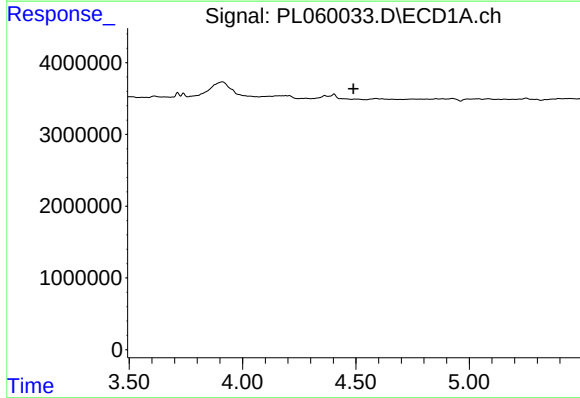


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

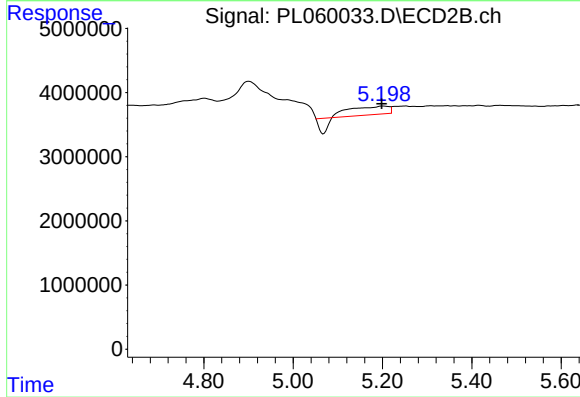

#4 Heptachlor


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 5691129
Conc: 1.69 ng/ml

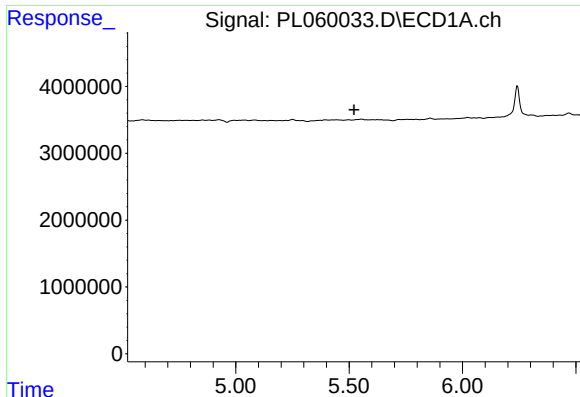

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

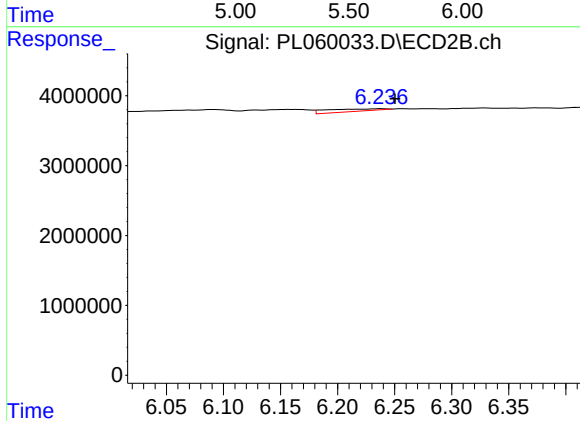


#9 Endosulfan I

R.T.: 6.238 min
Delta R.T.: -0.012 min
Response: 1199346
Conc: 0.45 ng/ml

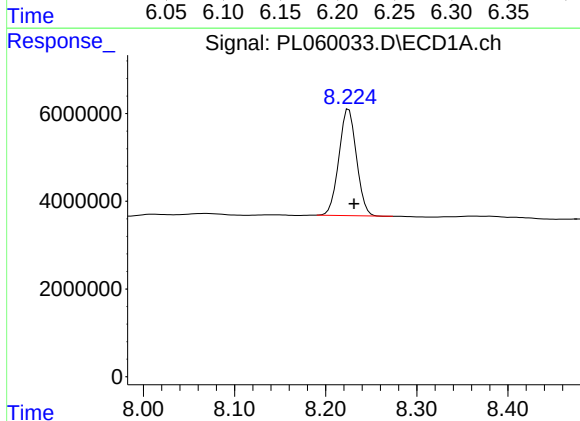

#28 Decachlorobiphenyl

R.T.: 8.225 min
Delta R.T.: -0.006 min
Response: 32523025
Conc: 19.77 ng/ml

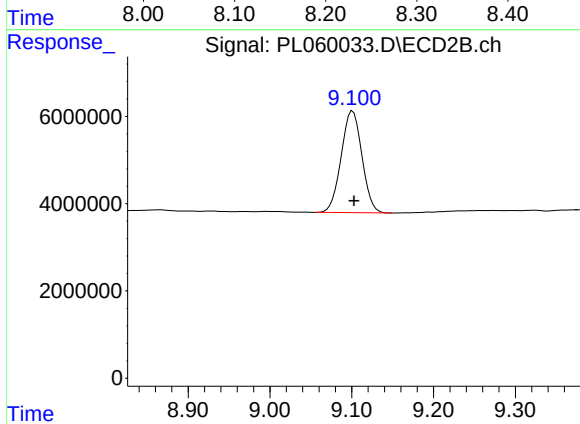

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: -0.002 min
Response: 41044999
Conc: 19.63 ng/ml